
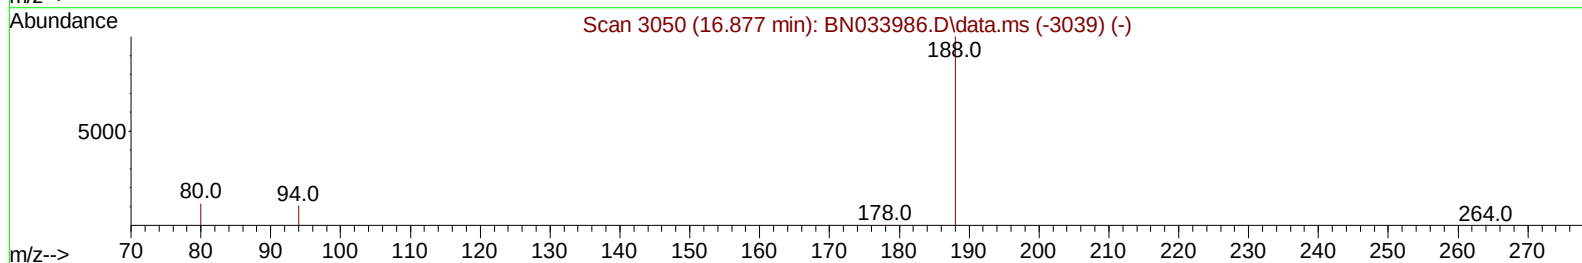
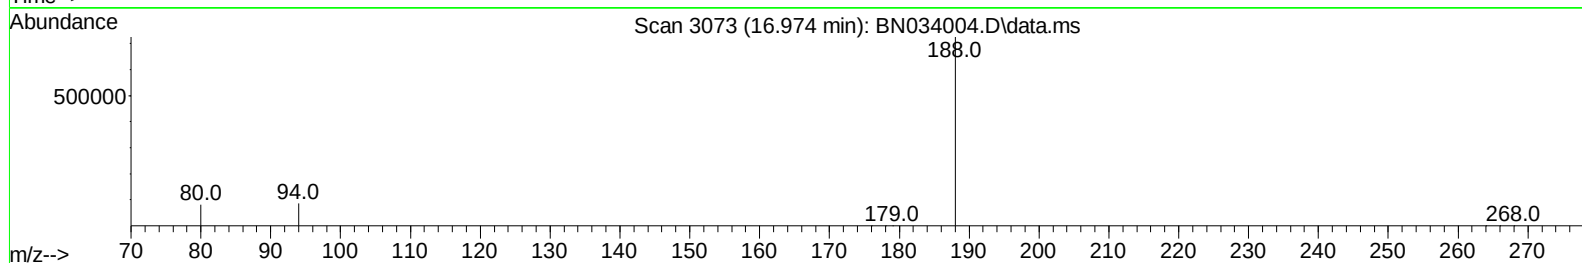


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

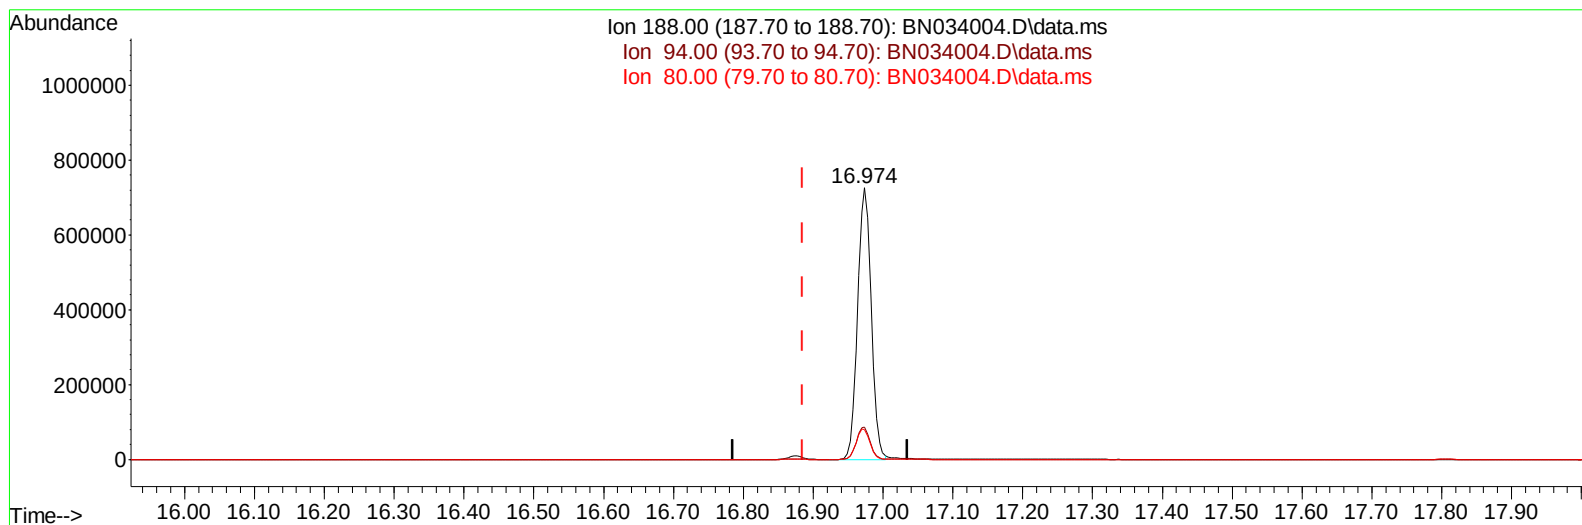

TIC: BN034004.D\data.ms

(13) Phenanthrene-d10 (I)




16.974min (+ 0.089) 0.40 ng/u1

response 983423

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.82
80.00	11.50	11.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

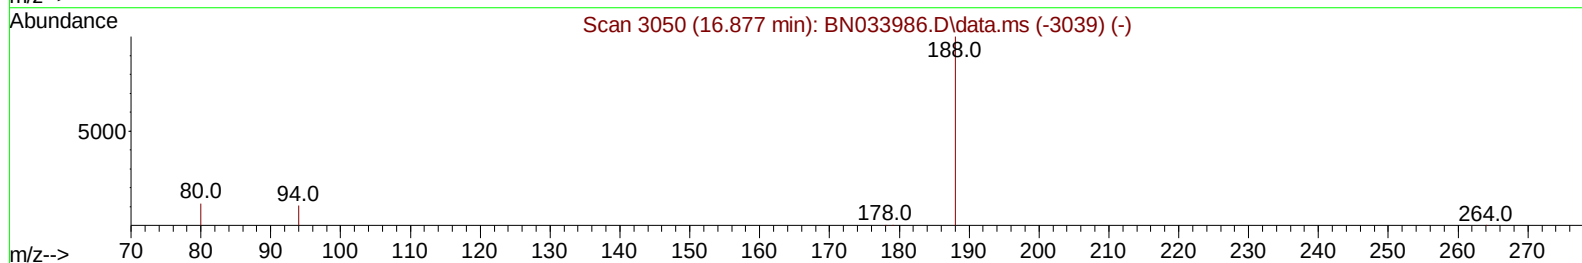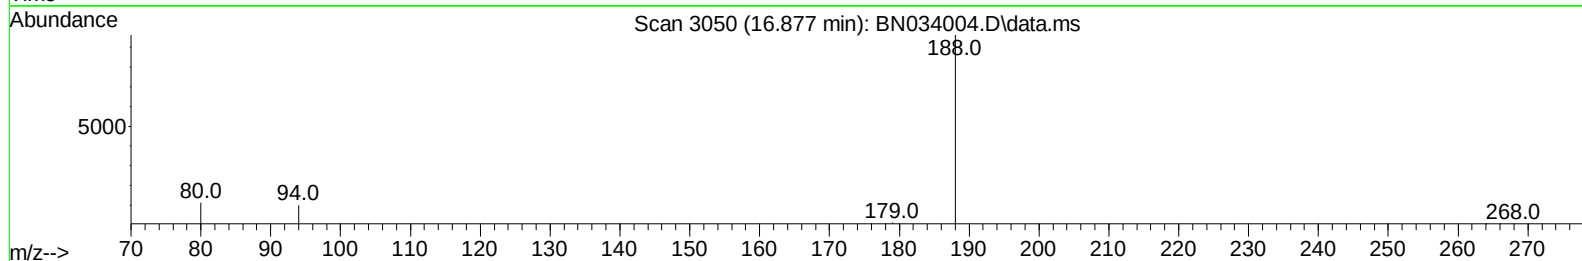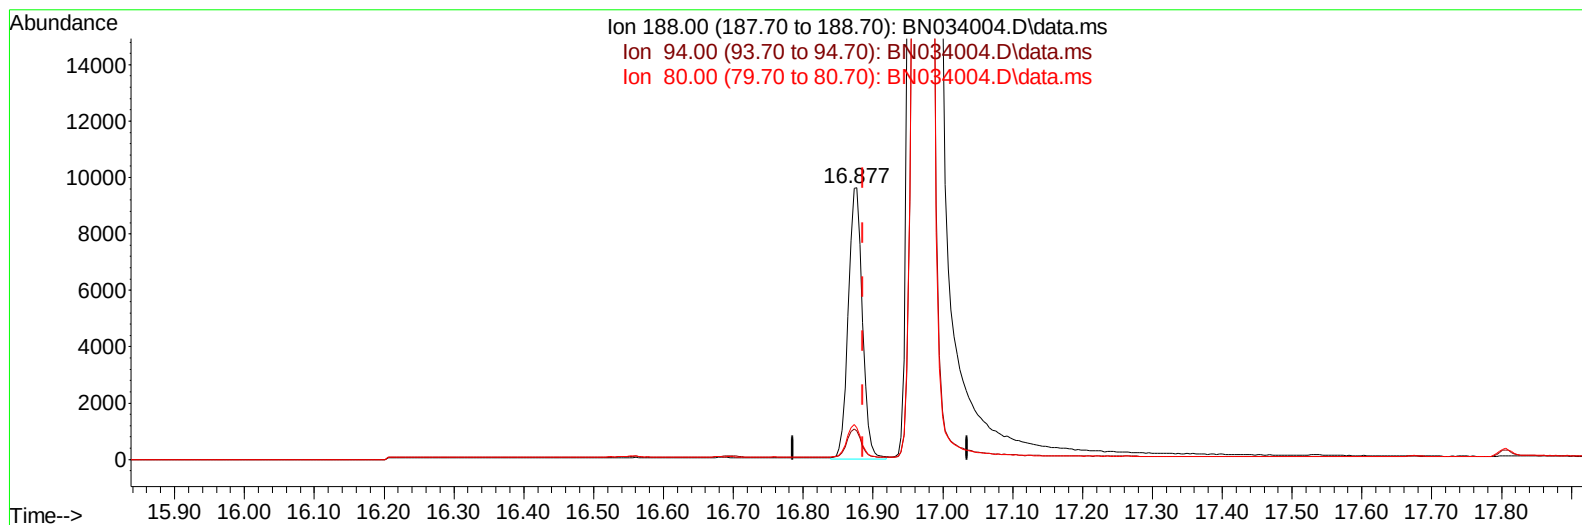

TIC: BN034004.D\data.ms

(13) Phenanthrene-d10 (I)




16.877min (-0.008) 0.40 ng/ul m

response 13485

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	10.48
80.00	11.50	11.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

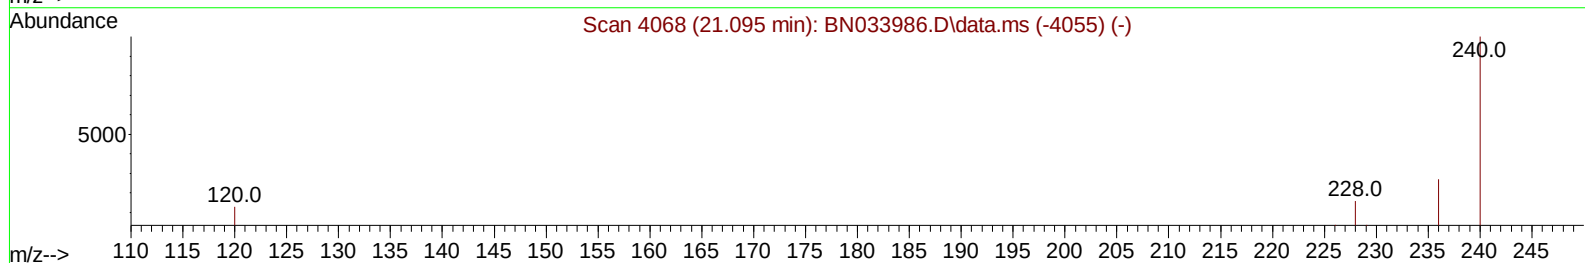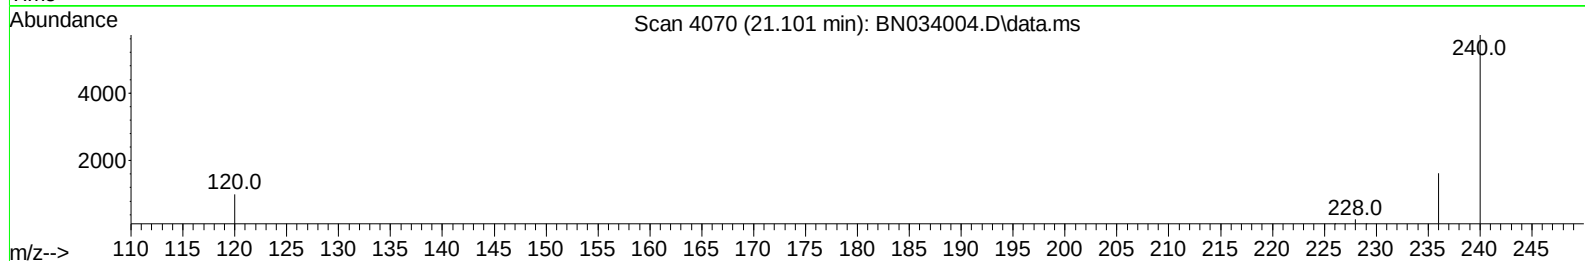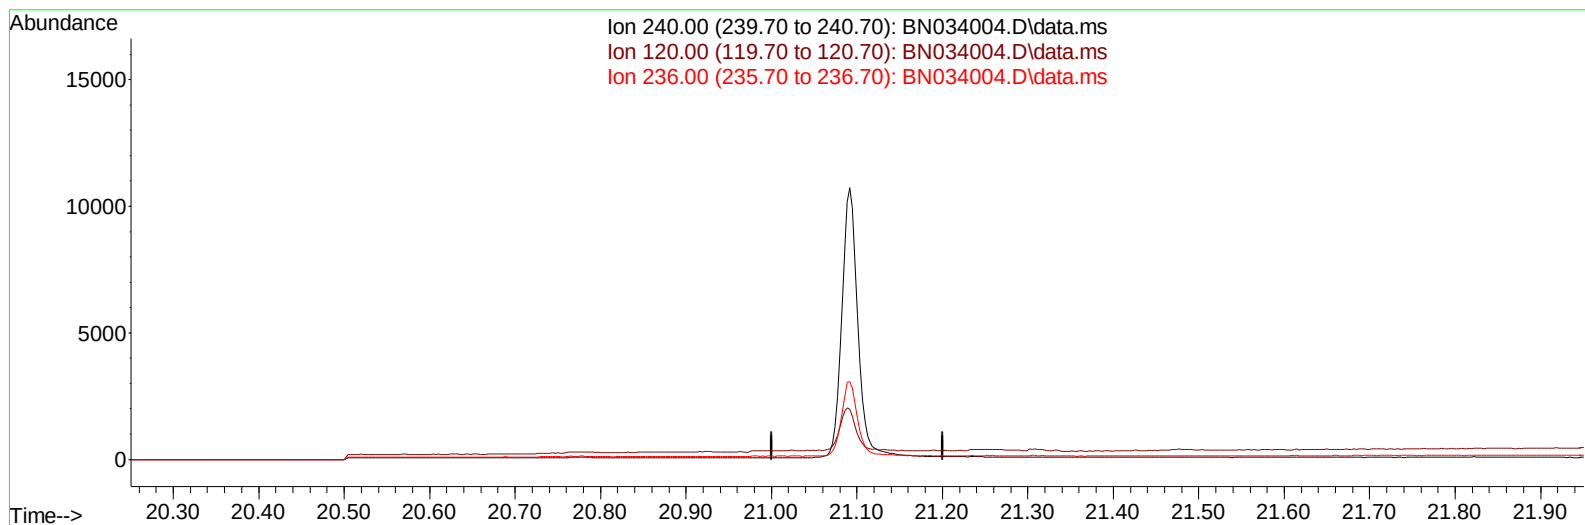

TIC: BN034004.D\data.ms

(17) Chrysene-d12




21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

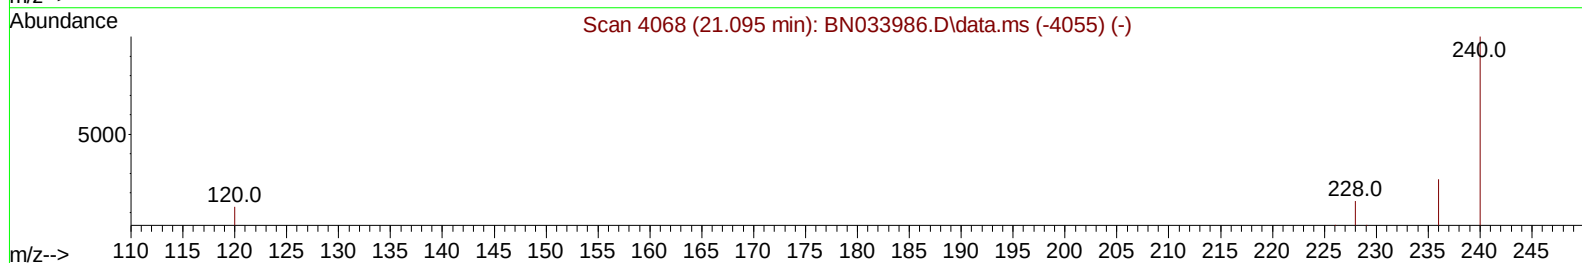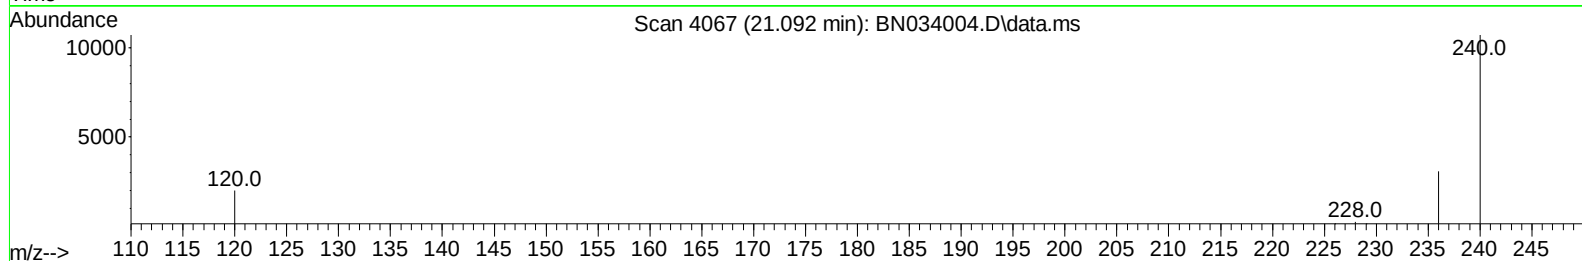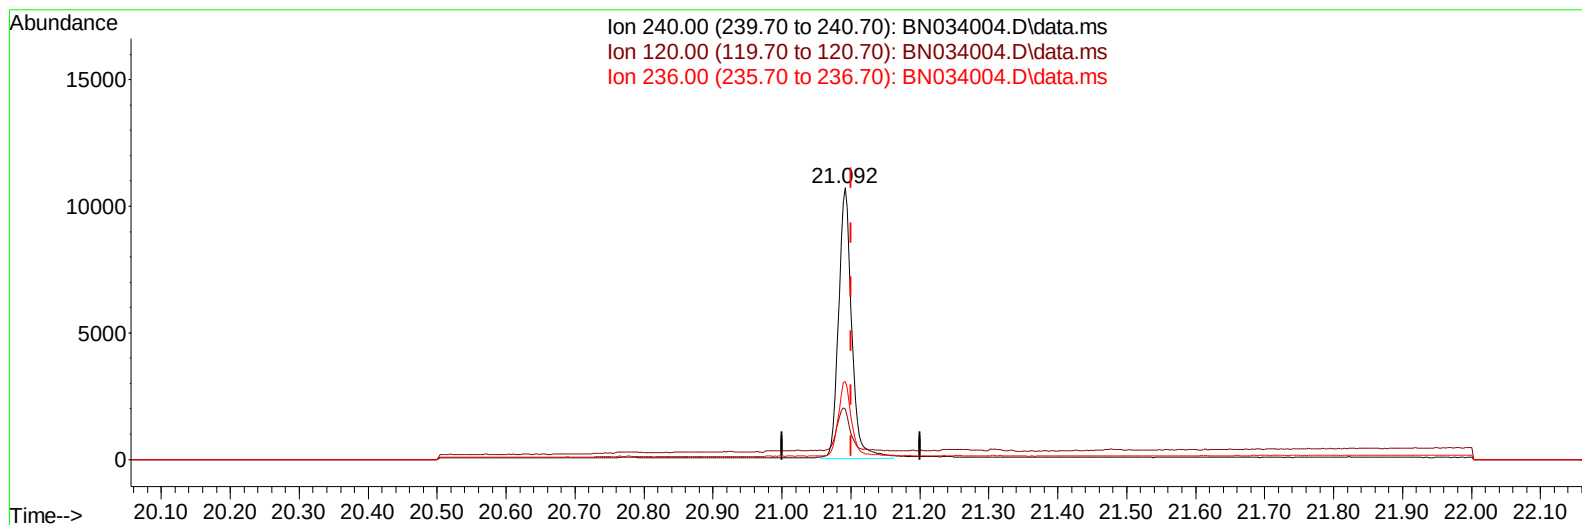

TIC: BN034004.D\data.ms

(17) Chrysene-d12




21.092min (-0.009) 0.40 ng/ul m

response 14213

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	18.58
236.00	28.30	28.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

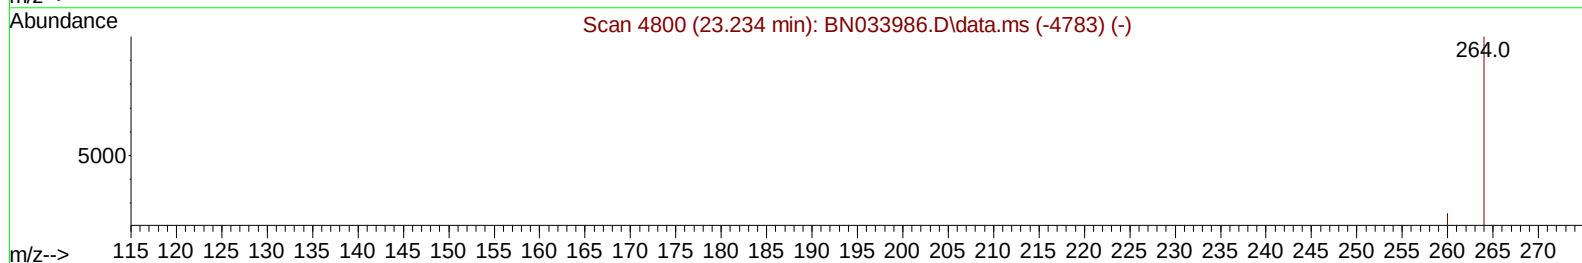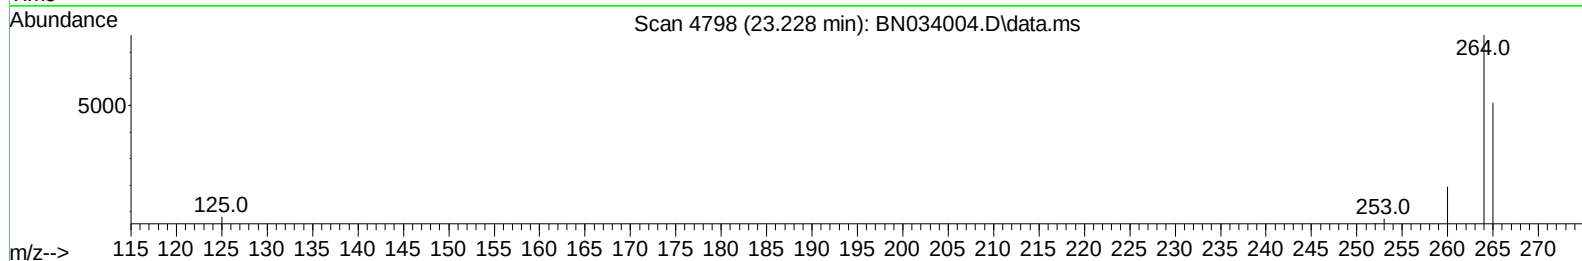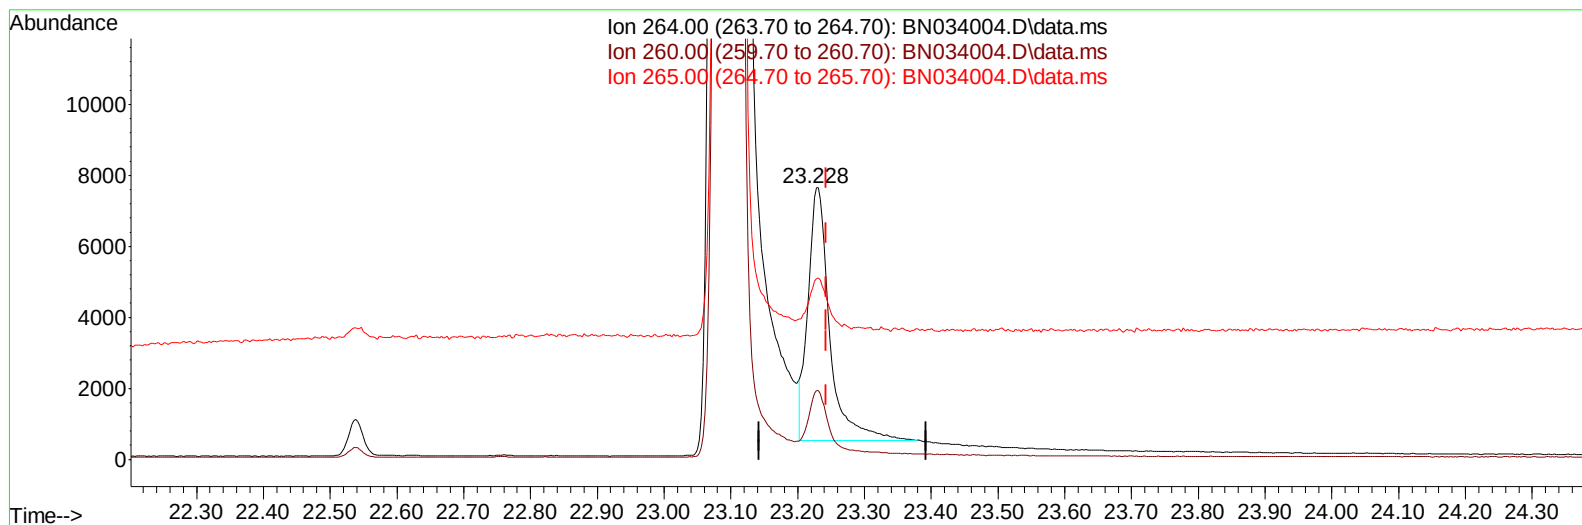

TIC: BN034004.D\data.ms

(23) Perylene-d12 (I)




23.228min (-0.015) 0.40 ng/u1

response 16324

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.29
265.00	73.30	66.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

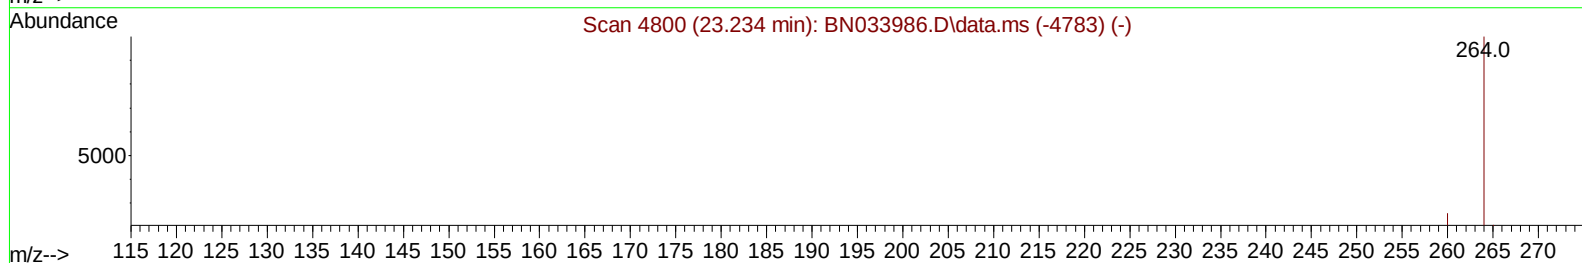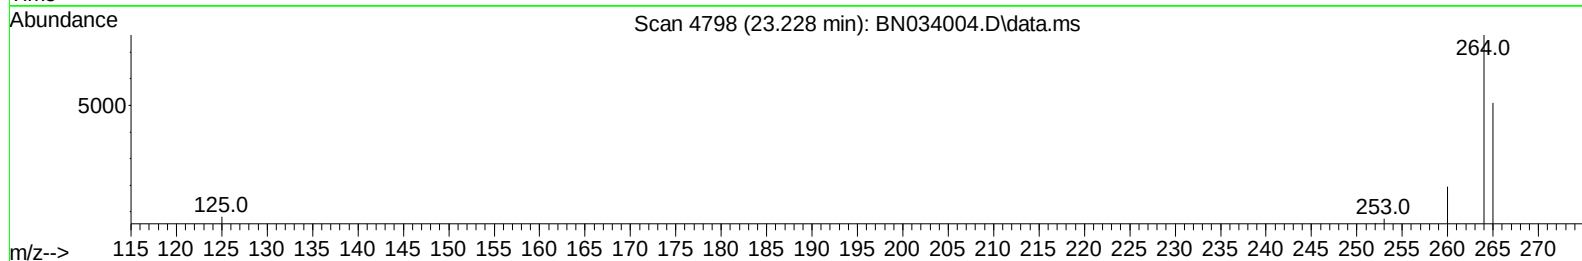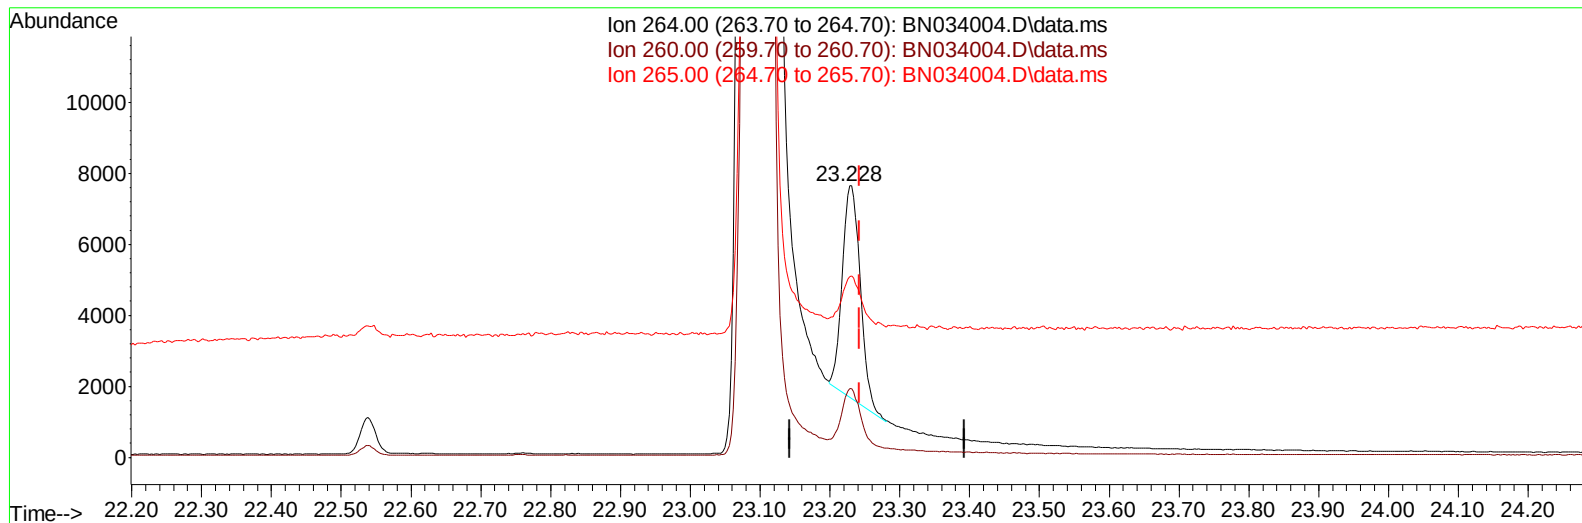

TIC: BN034004.D\data.ms

(23) Perylene-d12 (I)

23.228min (-0.015) 0.40 ng/ul m

response 10671

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.29
265.00	73.30	66.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034004.D
 Acq On : 17 Sep 2024 01:26
 Operator : JU/RC
 Sample : P3994-06
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4334	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	12131	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.119	164	7720	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.877	188	13485m	0.400	ng/ul	0.00
17) Chrysene-d12	21.092	240	14213m	0.400	ng/ul	0.00
23) Perylene-d12	23.228	264	10671m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	24907	5.590	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	4863	0.279	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	12252	0.289	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	1408	0.285	ng/ul#	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034004.D
Acq On : 17 Sep 2024 01:26
Operator : JU/RC
Sample : P3994-06
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Sep 17 01:52:51 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

