
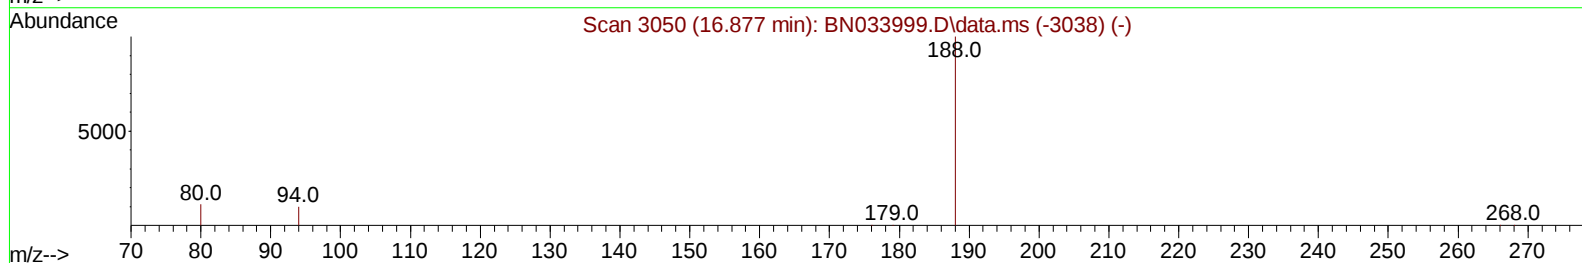
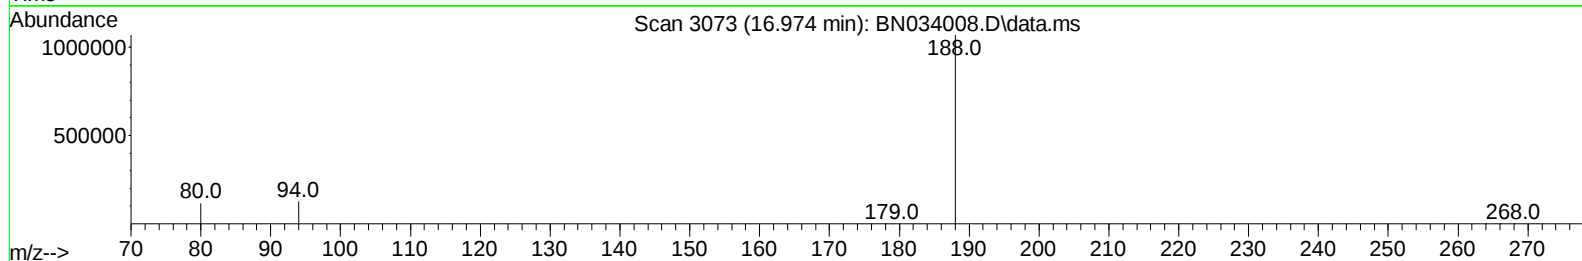


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

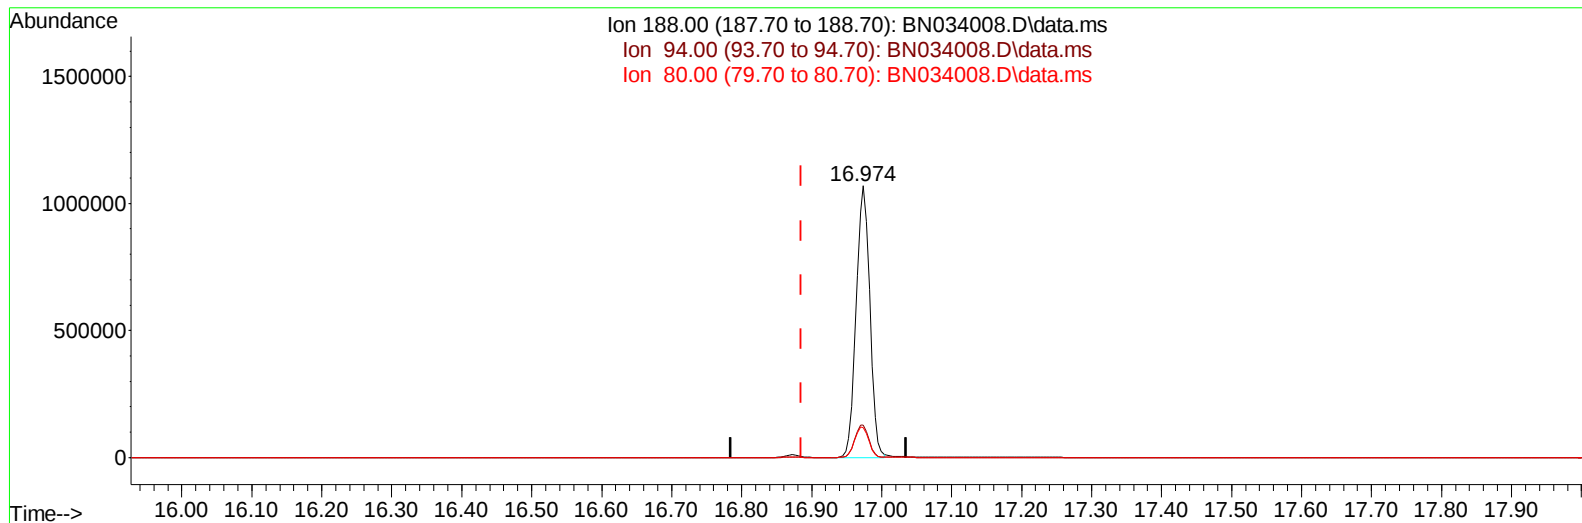




TIC: BN034008.D\data.ms

(13) Phenanthrene-d10 (I)**16.974min (+ 0.089) 0.40 ng/ul****response 1441503**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.82
80.00	11.50	10.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

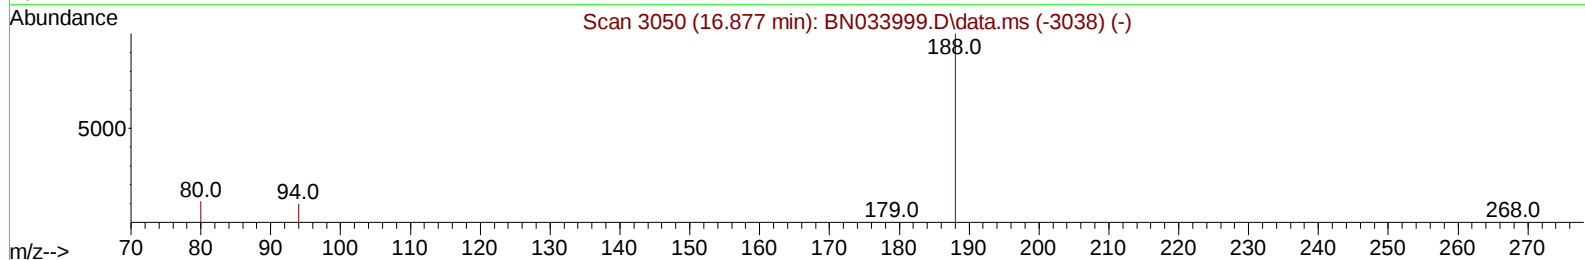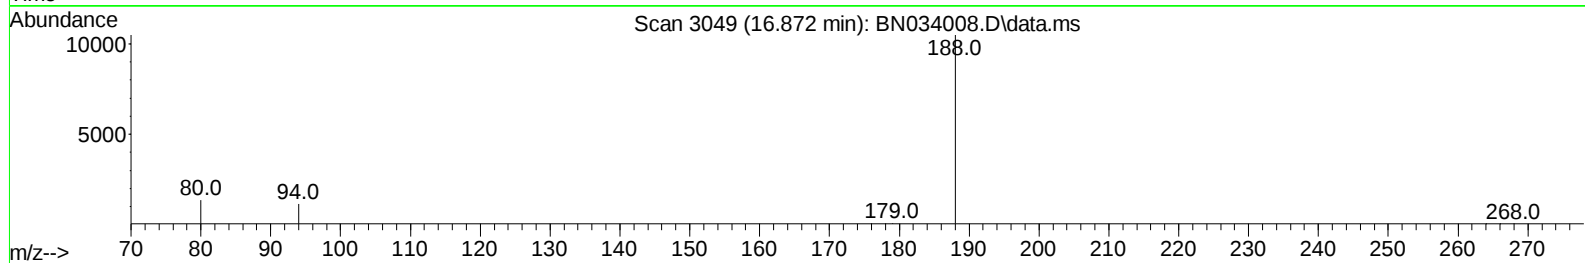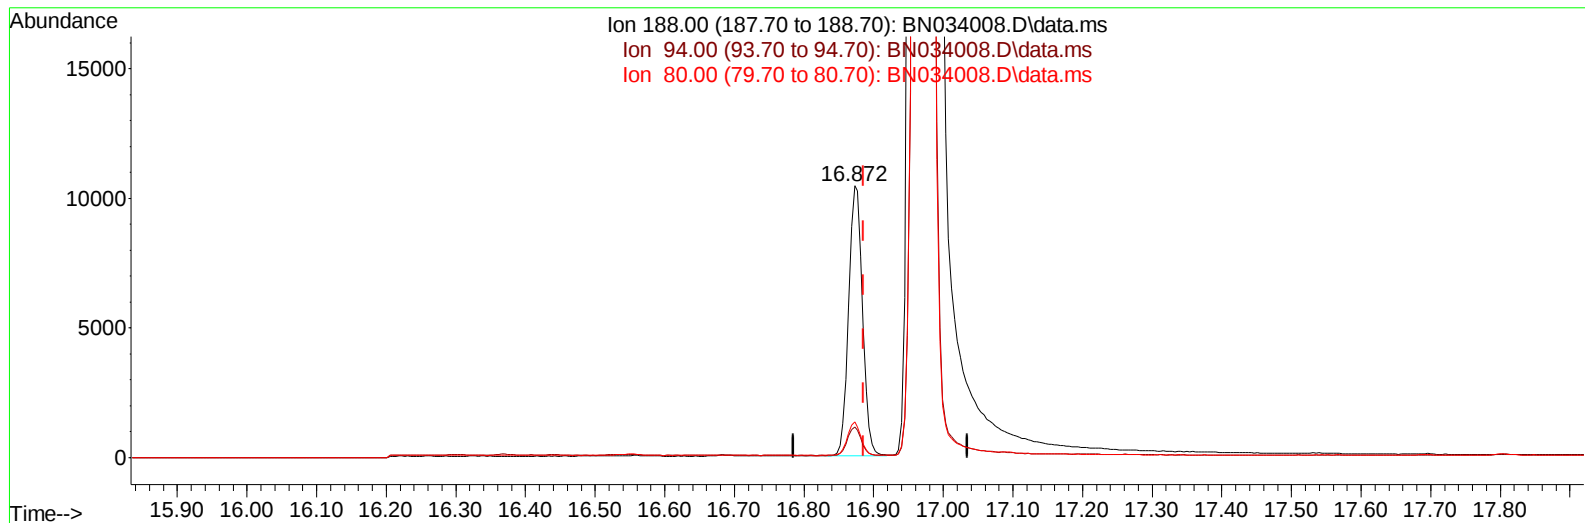




TIC: BN034008.D\data.ms

(13) Phenanthrene-d10 (I)**16.872min (-0.013) 0.40 ng/ul m****response 14487**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.12
80.00	11.50	13.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

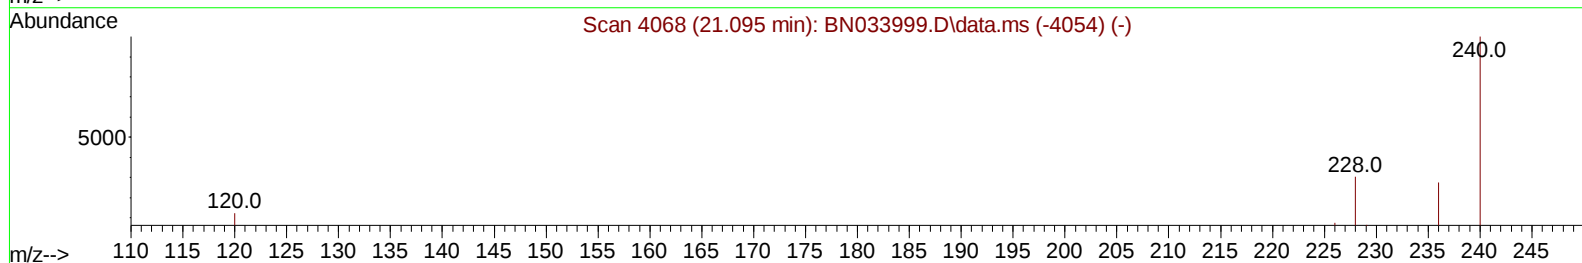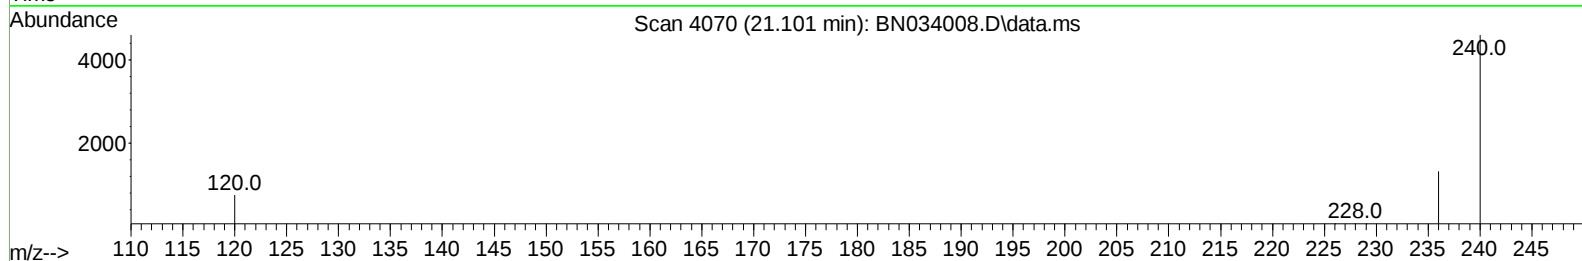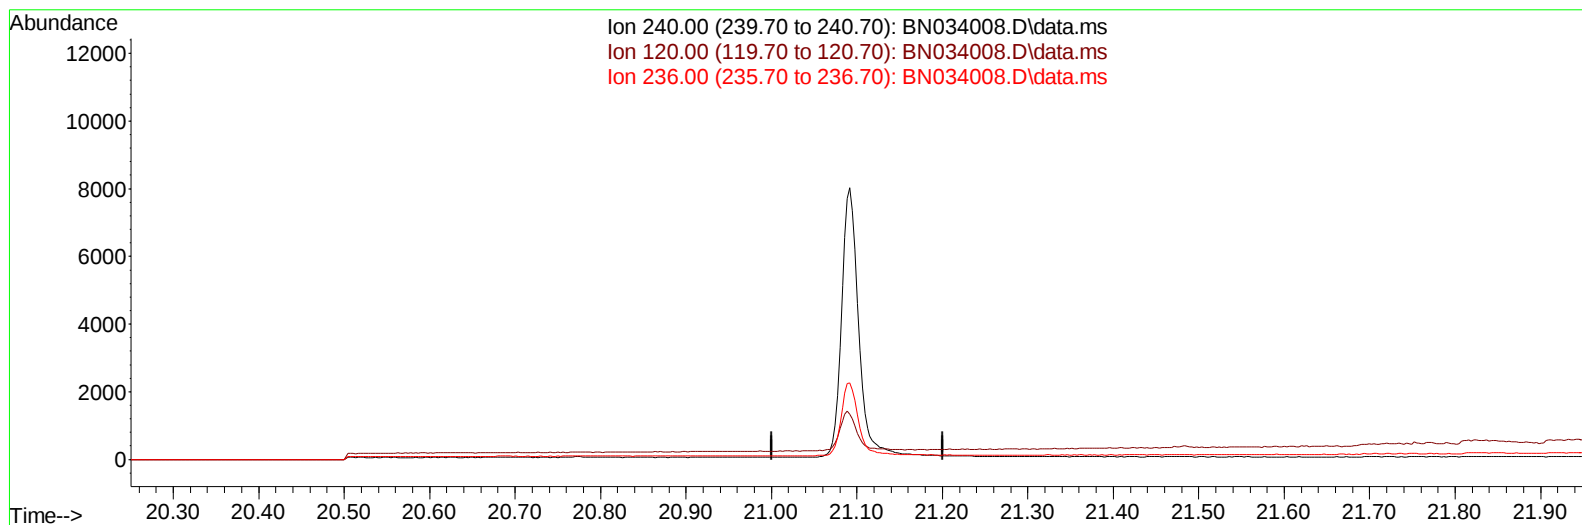

TIC: BN034008.D\data.ms

(17) Chrysene-d12




21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

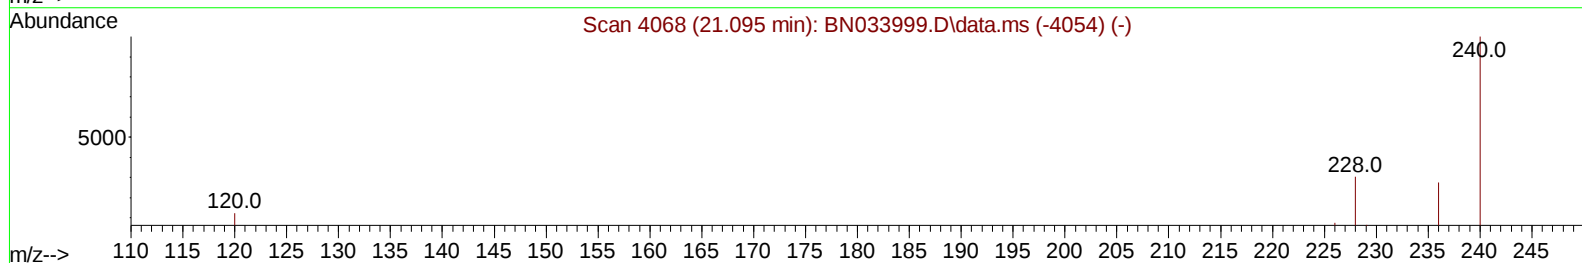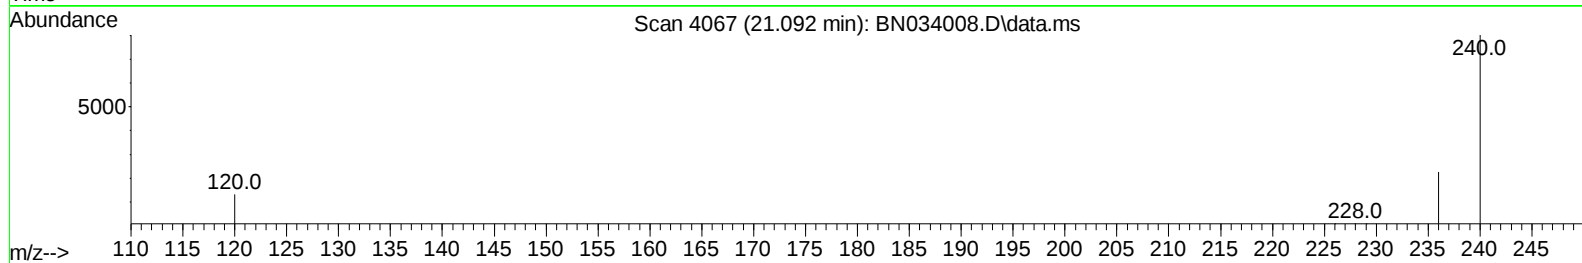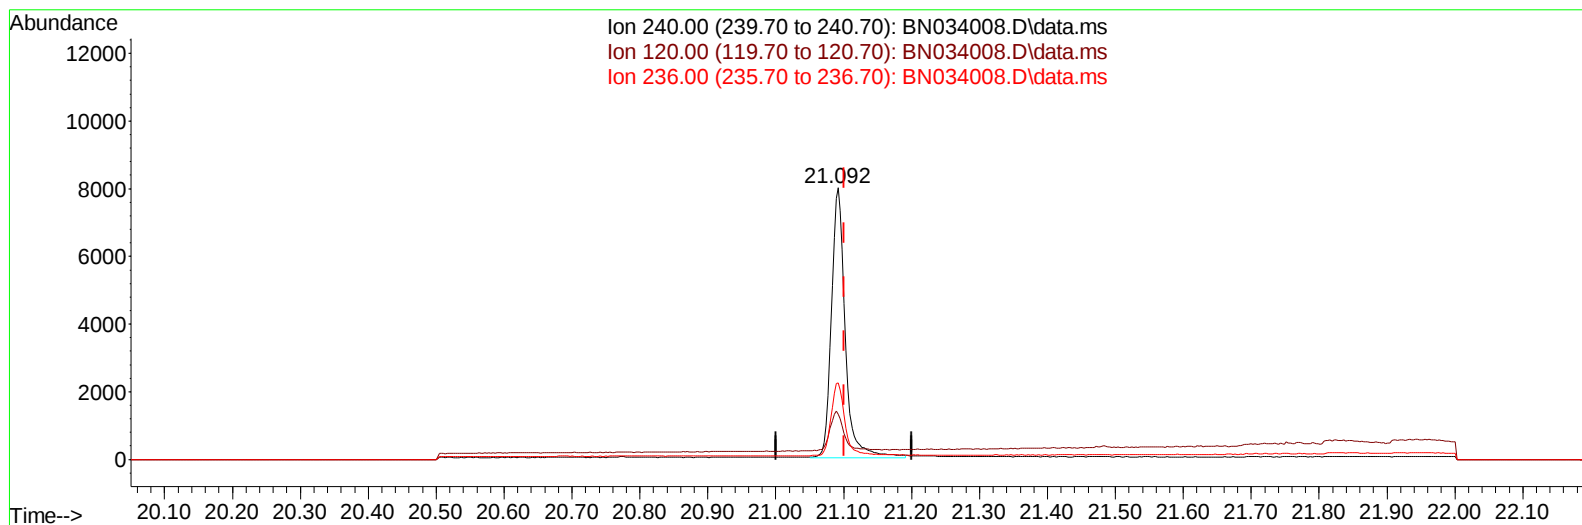

TIC: BN034008.D\data.ms

(17) Chrysene-d12




21.092min (-0.009) 0.40 ng/ul m

response 11299

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	16.58
236.00	28.30	28.10
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

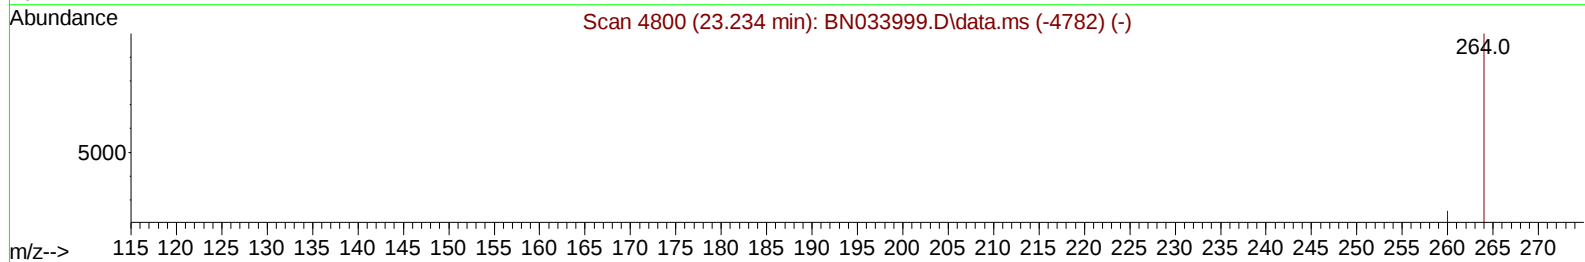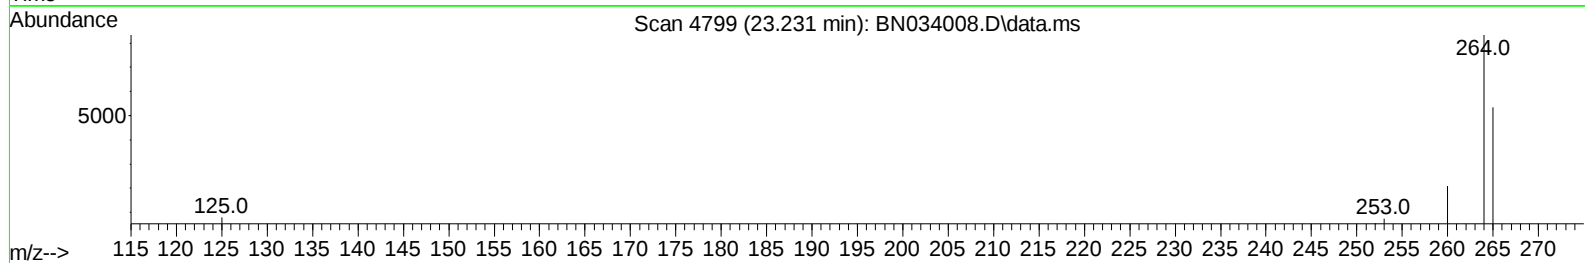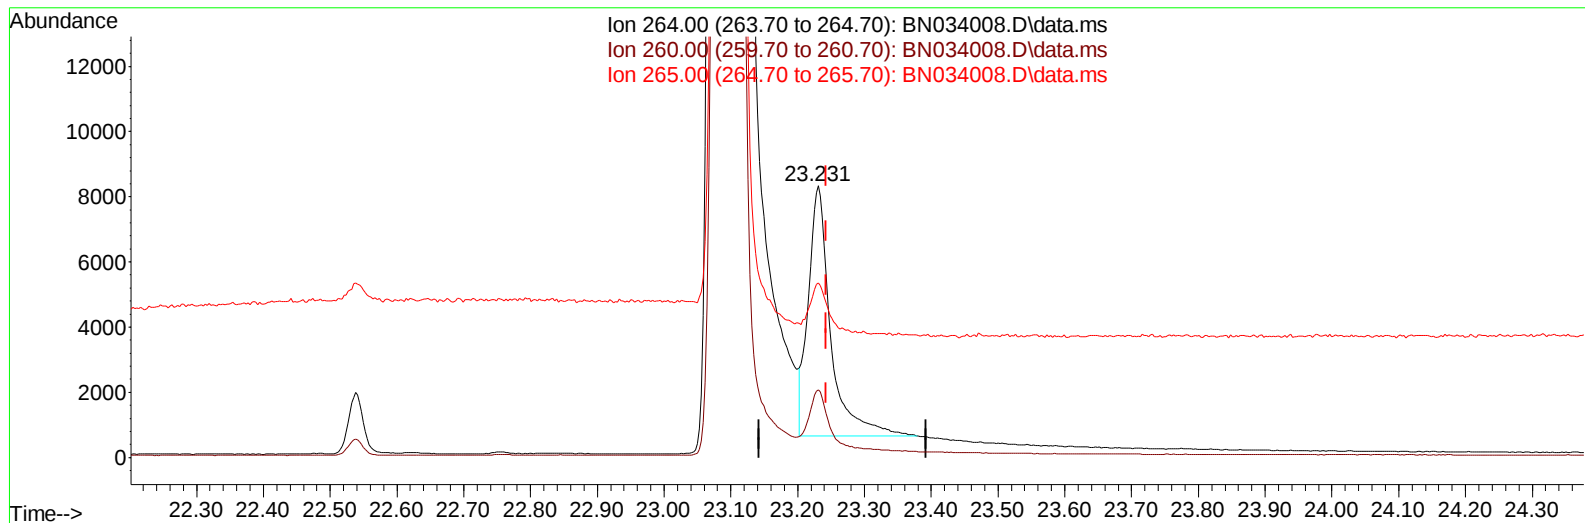

TIC: BN034008.D\data.ms

(23) Perylene-d12 (I)




23.231min (-0.012) 0.40 ng/ul

response 18069

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.01
265.00	73.30	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

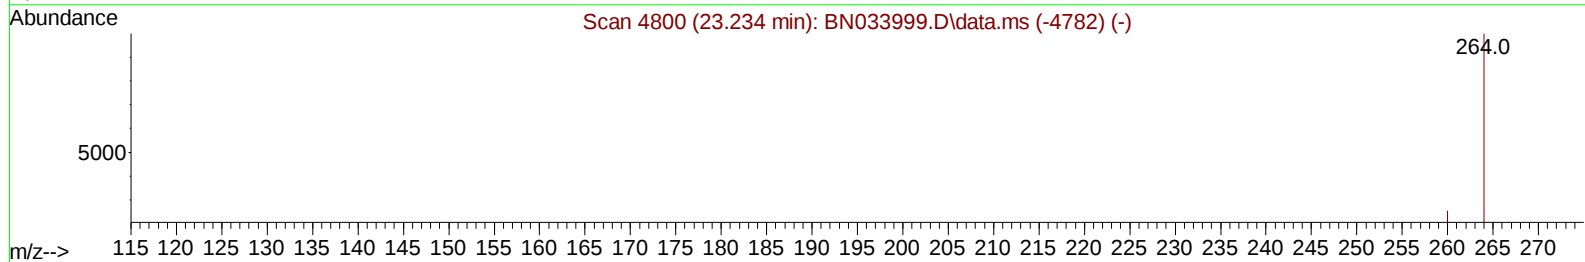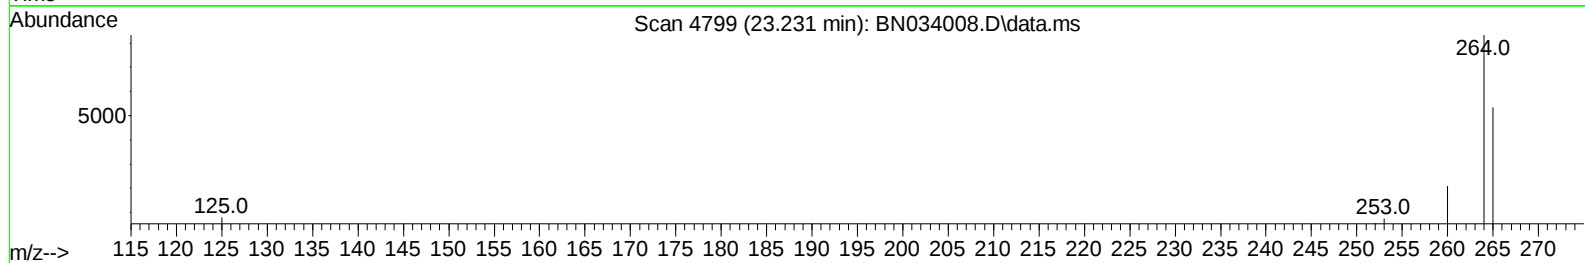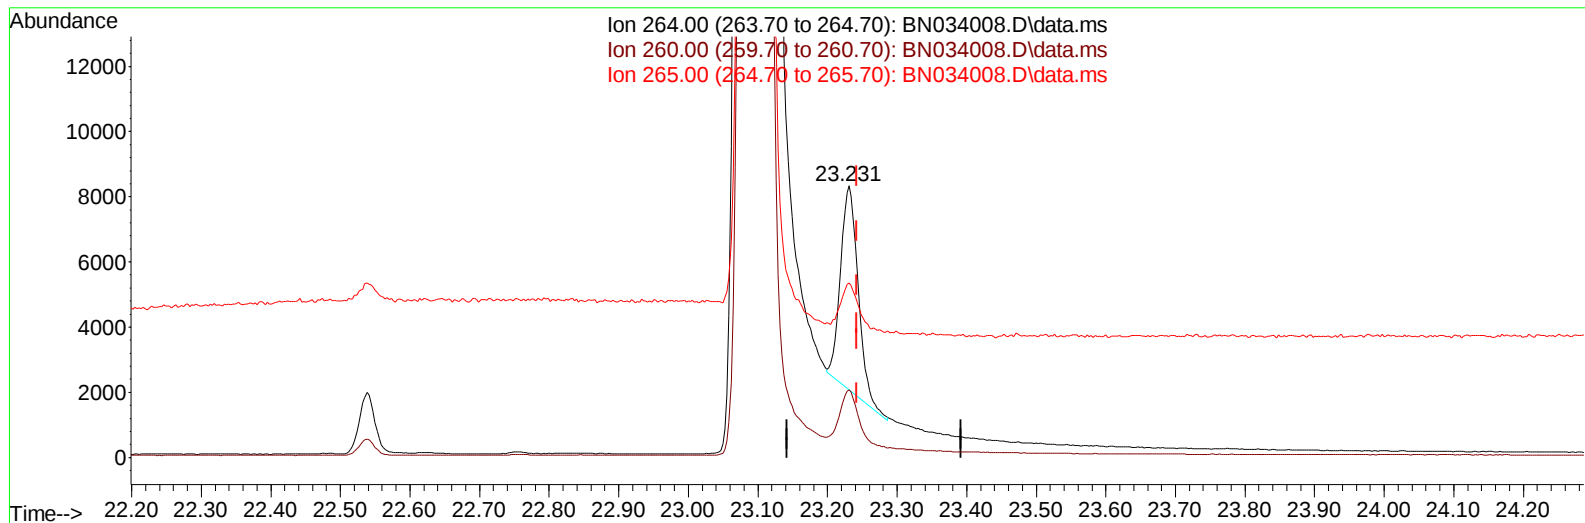

TIC: BN034008.D\data.ms

(23) Perylene-d12 (I)

23.231min (-0.012) 0.40 ng/ul m

response 10877

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.01
265.00	73.30	64.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034008.D
 Acq On : 17 Sep 2024 03:50
 Operator : JU/RC
 Sample : P3997-12
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.473	152	4628	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.228	136	13027	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.119	164	7070	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.872	188	14487m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.092	240	11299m	0.400	ng/ul	0.00
23) Perylene-d12	23.231	264	10877m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	30712	6.455	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	8121	0.435	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	17498	0.519	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034008.D
Acq On : 17 Sep 2024 03:50
Operator : JU/RC
Sample : P3997-12
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Sep 17 04:23:40 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

