
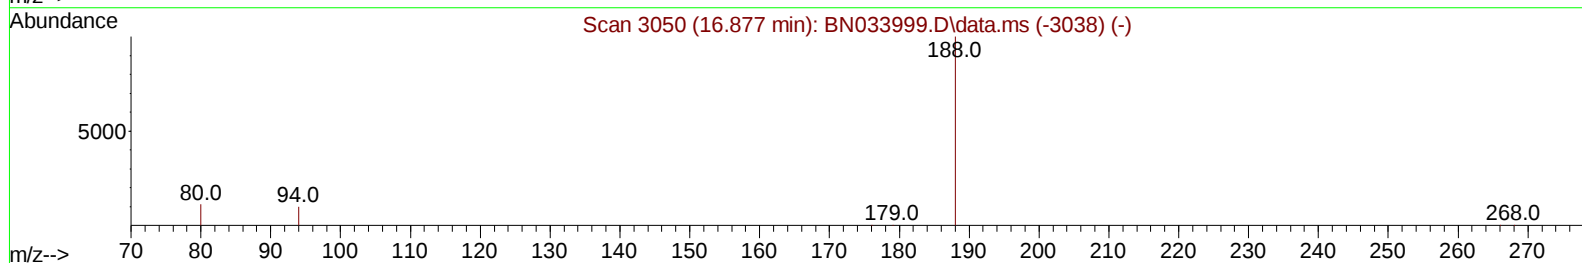
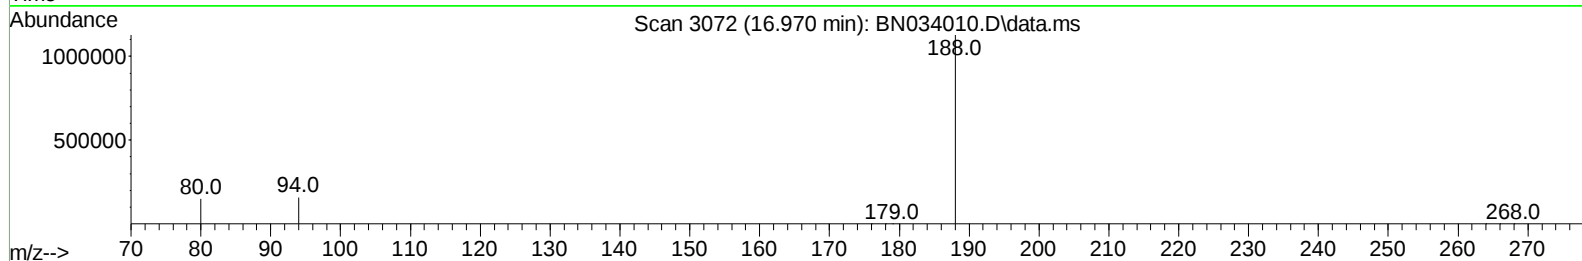


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

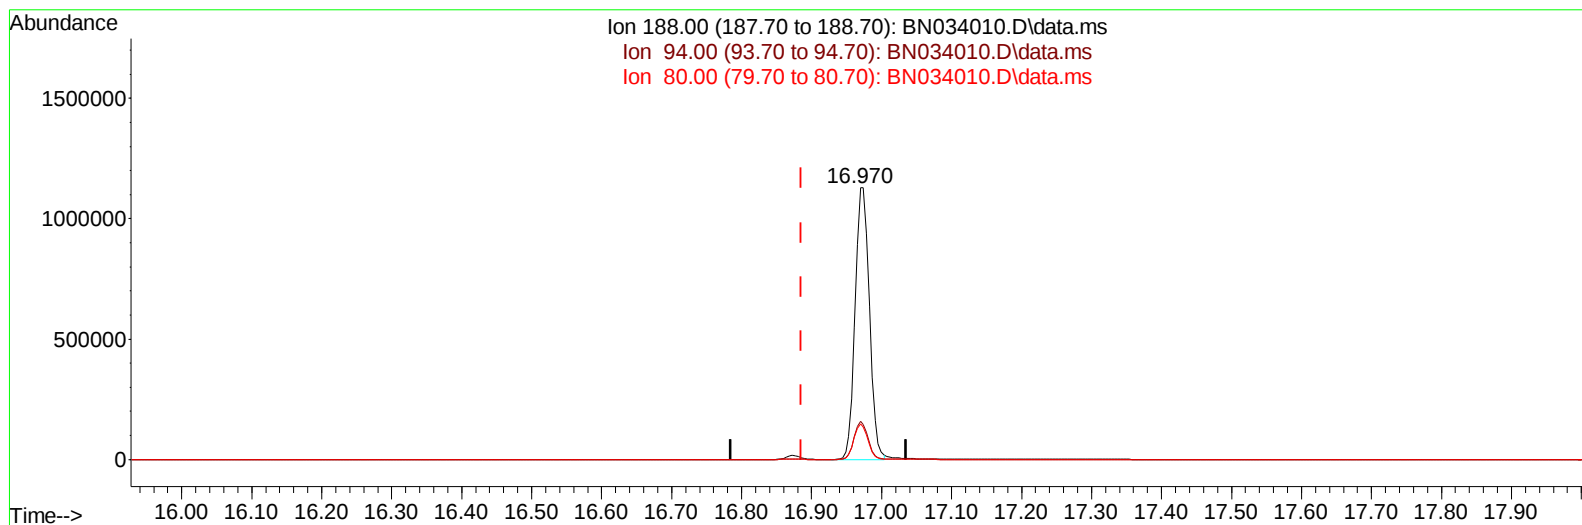

TIC: BN034010.D\data.ms

(13) Phenanthrene-d10 (I)




16.970min (+ 0.084) 0.40 ng/ul

response 1589314

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	14.03#
80.00	11.50	13.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

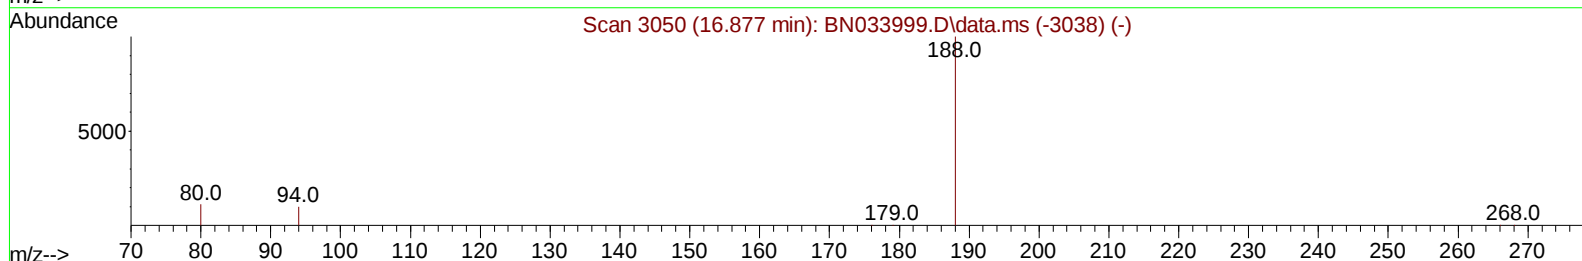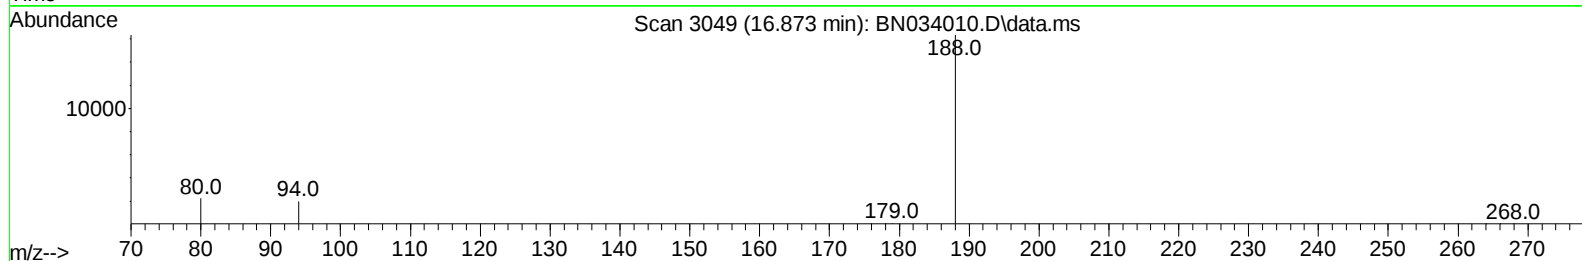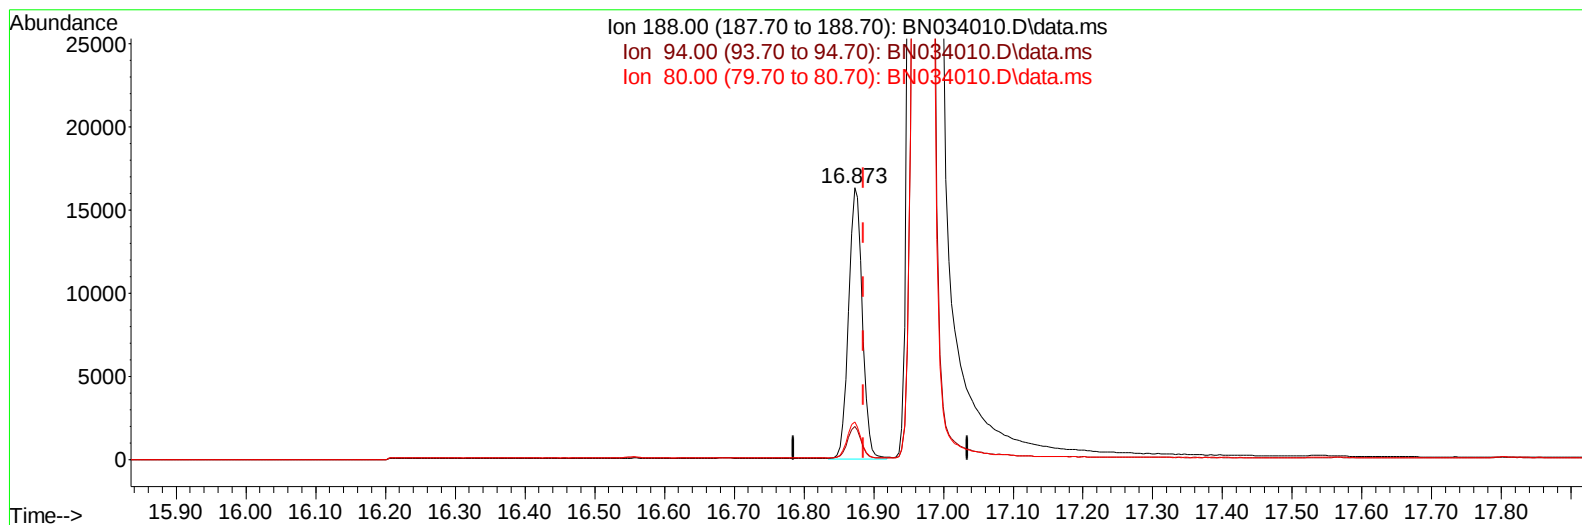

TIC: BN034010.D\data.ms

(13) Phenanthrene-d10 (I)




16.873min (-0.013) 0.40 ng/ul m

response 22308

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	12.19
80.00	11.50	13.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

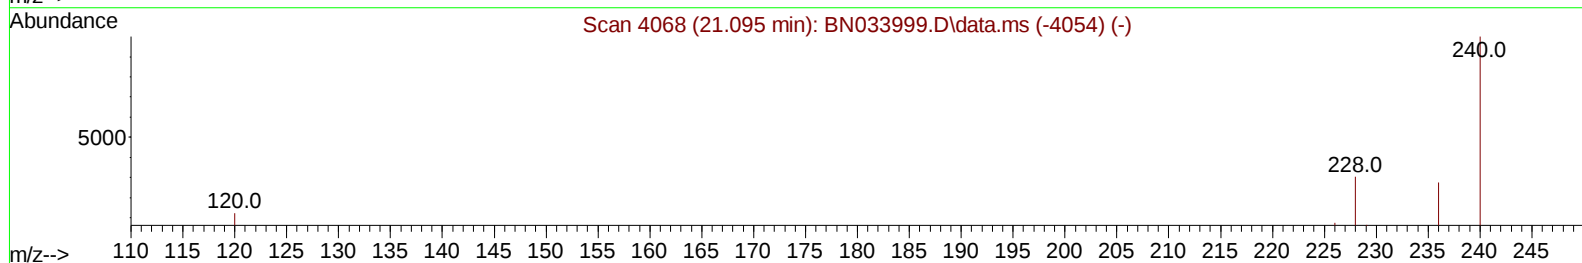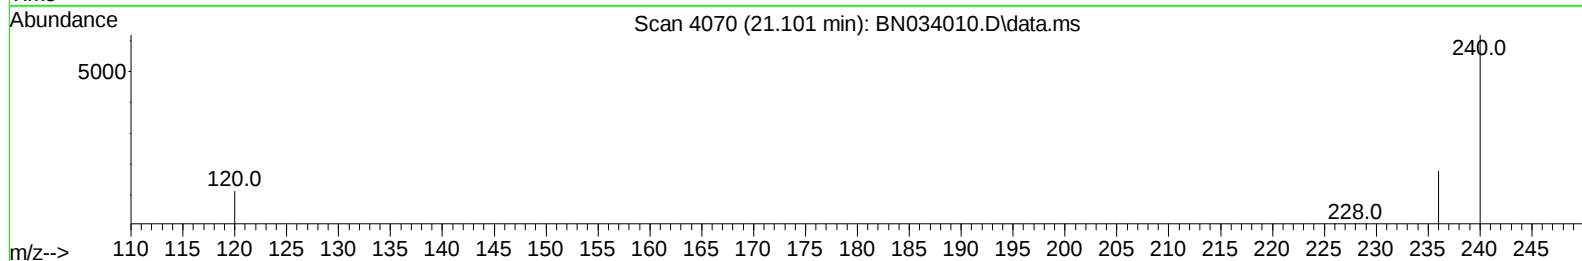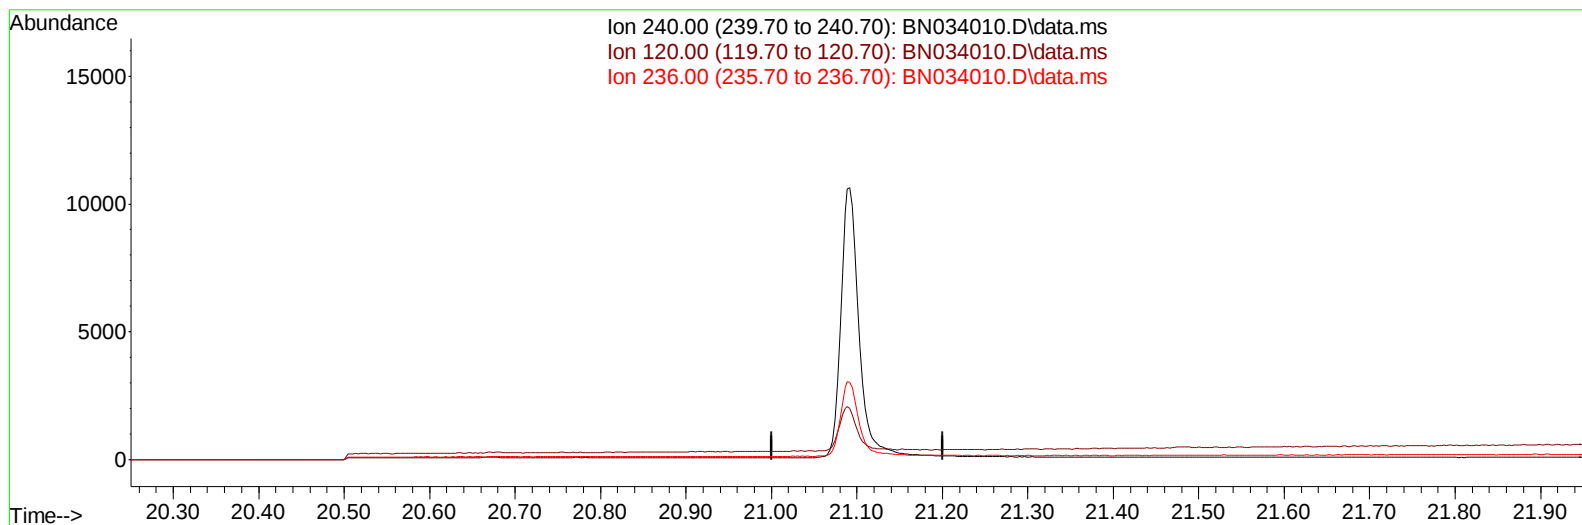

TIC: BN034010.D\data.ms

(17) Chrysene-d12




21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

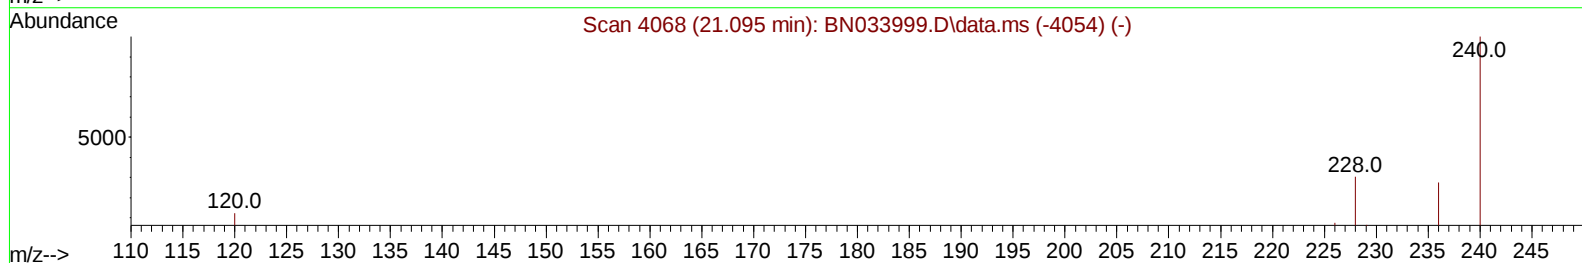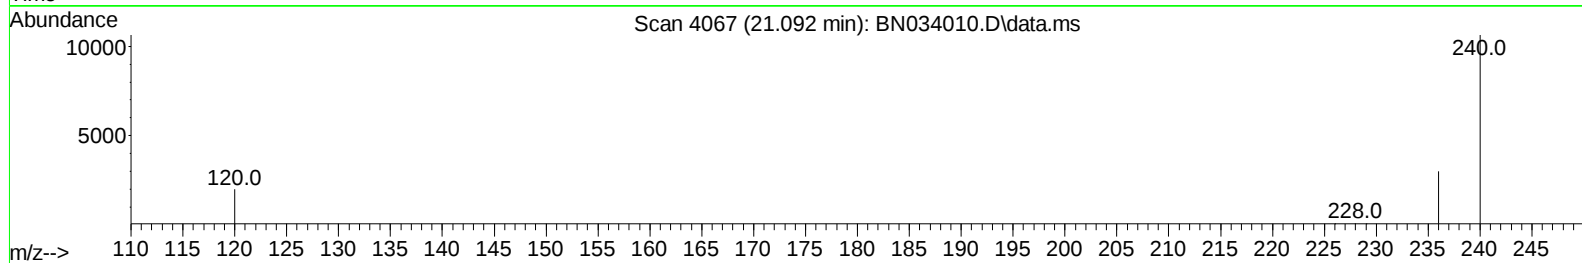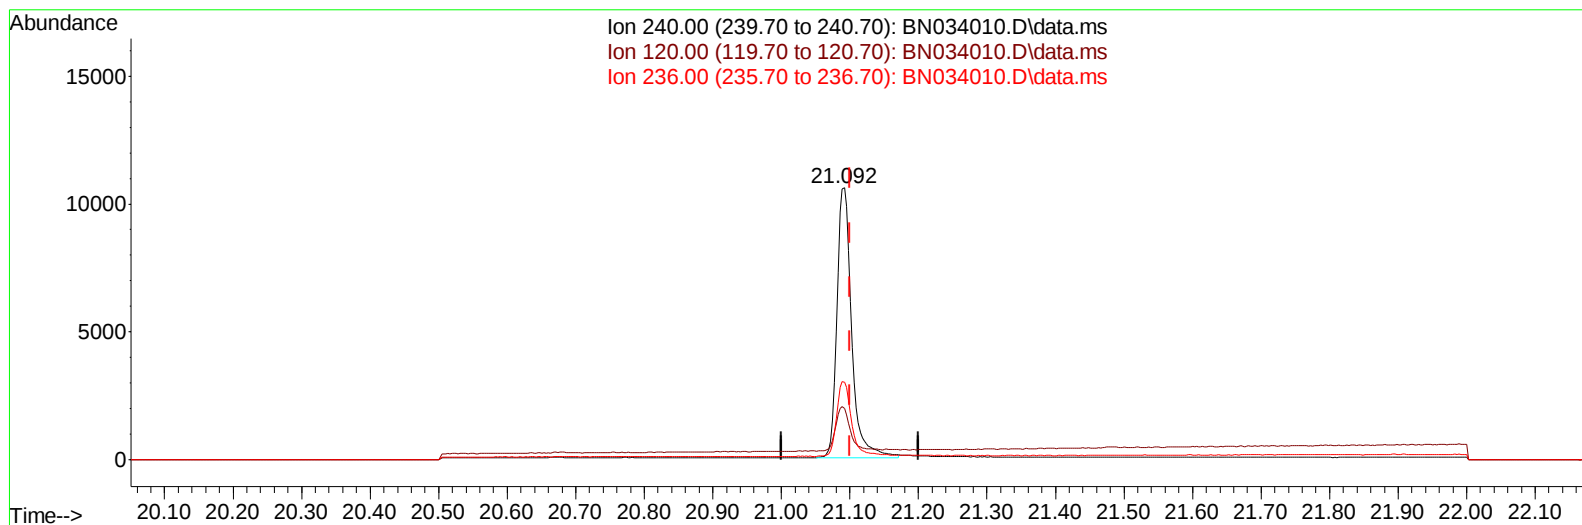

TIC: BN034010.D\data.ms

(17) Chrysene-d12




21.092min (-0.009) 0.40 ng/ul m

response 15801

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	18.81
236.00	28.30	28.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

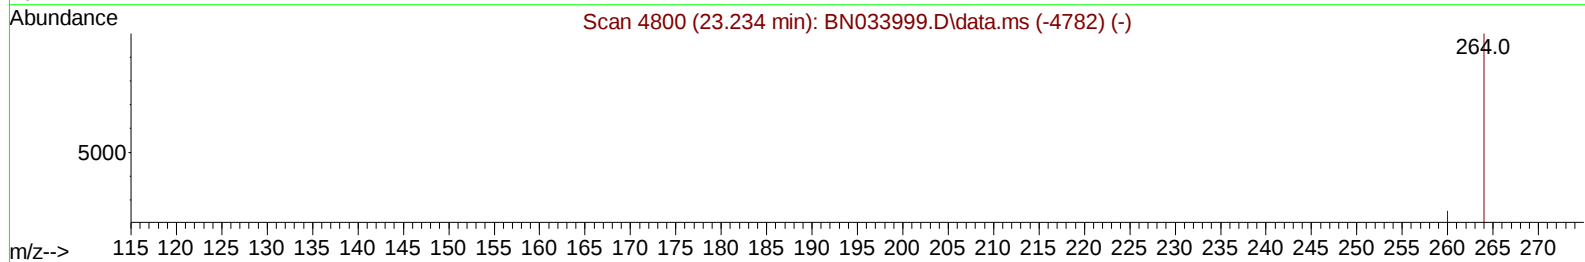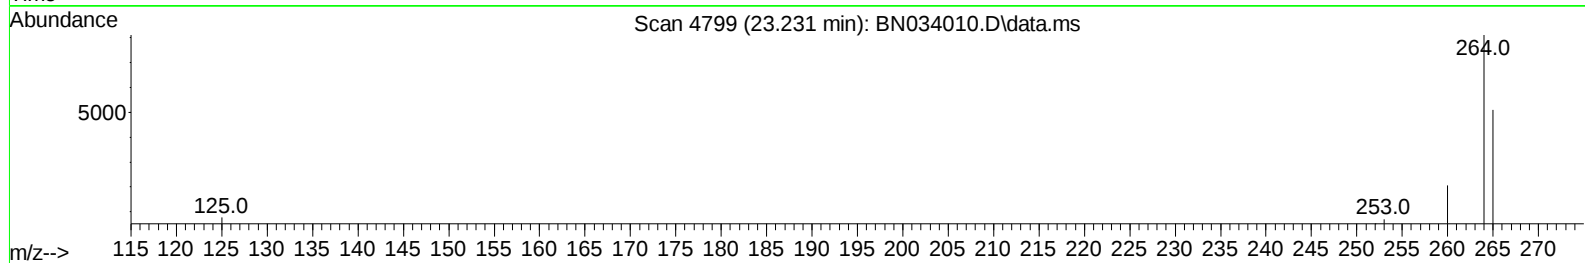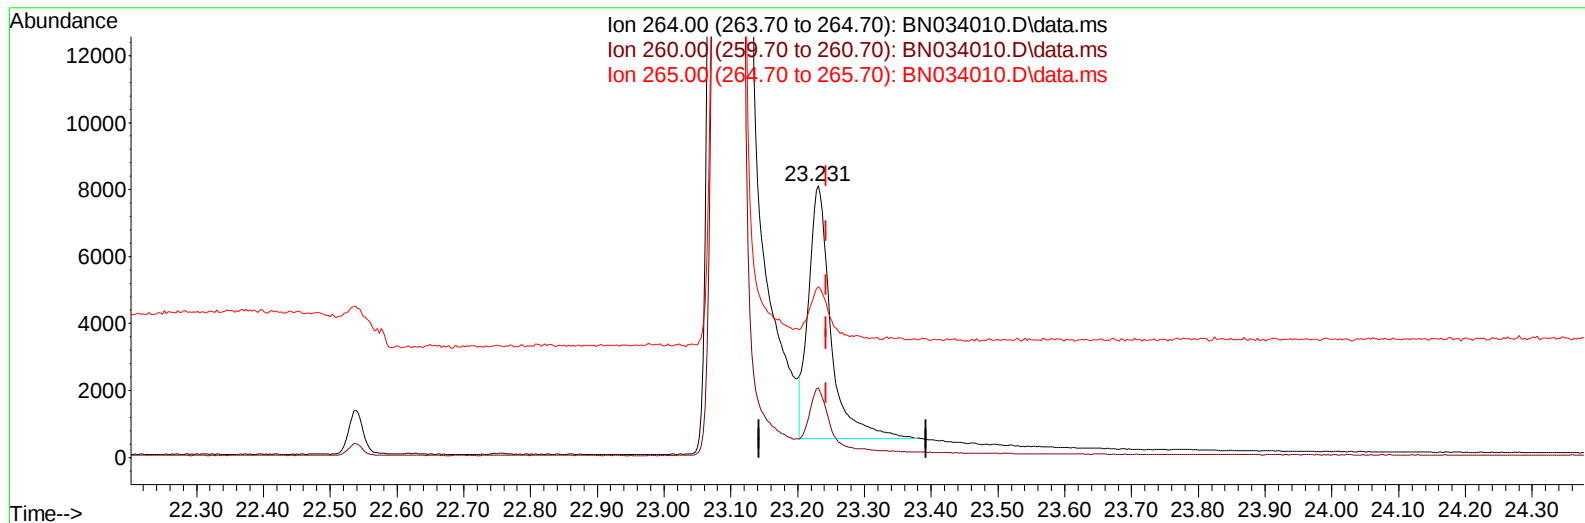

TIC: BN034010.D\data.ms

(23) Perylene-d12 (I)




23.231min (-0.012) 0.40 ng/ul

response 17822

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.51
265.00	73.30	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

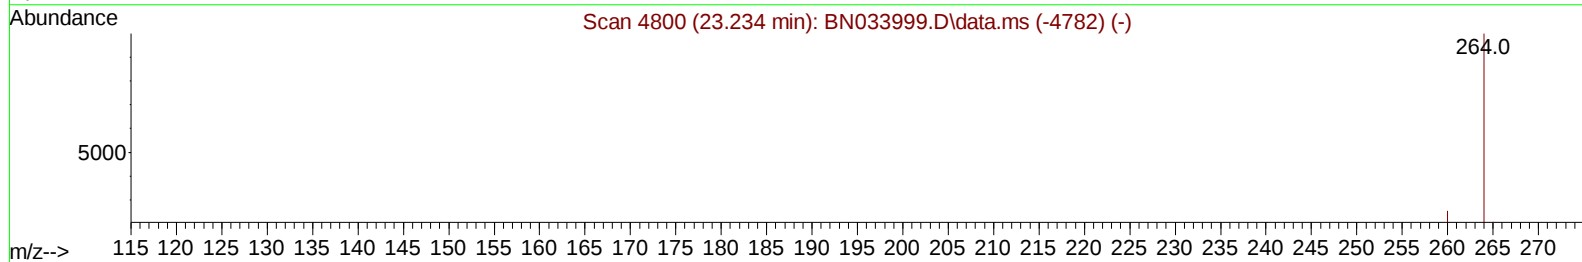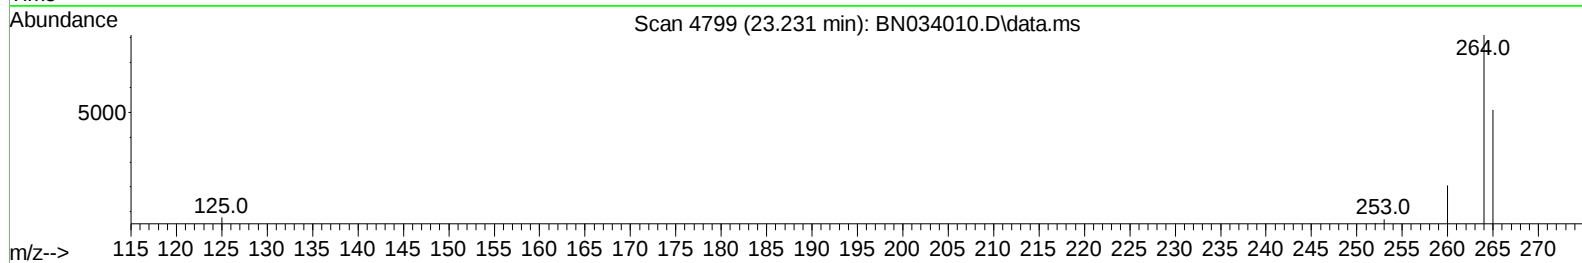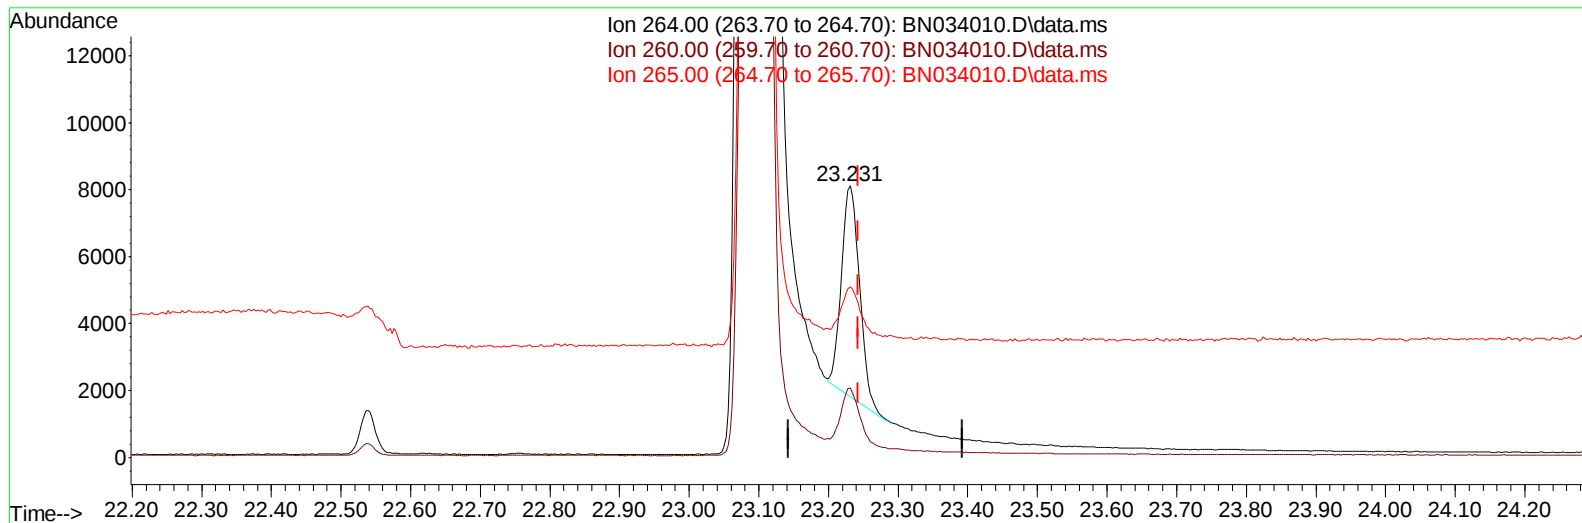

TIC: BN034010.D\data.ms

(23) Perylene-d12 (I)

23.231min (-0.012) 0.40 ng/ul m

response 11391

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	25.51
265.00	73.30	62.83
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034010.D
 Acq On : 17 Sep 2024 05:02
 Operator : JU/RC
 Sample : P3997-14
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.473	152	8069	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.228	136	21988	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.119	164	10984	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.873	188	22308m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.092	240	15801m	0.400	ng/ul	0.00
23) Perylene-d12	23.231	264	11391m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.093	96	28002	3.376	ng/ul	-0.01
6) 2-Methylnaphthalene-d10	11.834	152	8905	0.282	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	19436	0.413	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034010.D
Acq On : 17 Sep 2024 05:02
Operator : JU/RC
Sample : P3997-14
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Sep 17 05:28:53 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

