
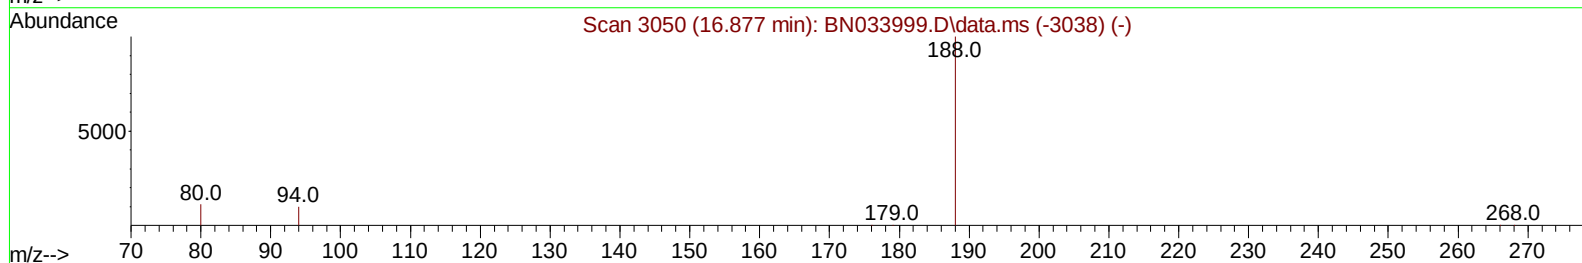
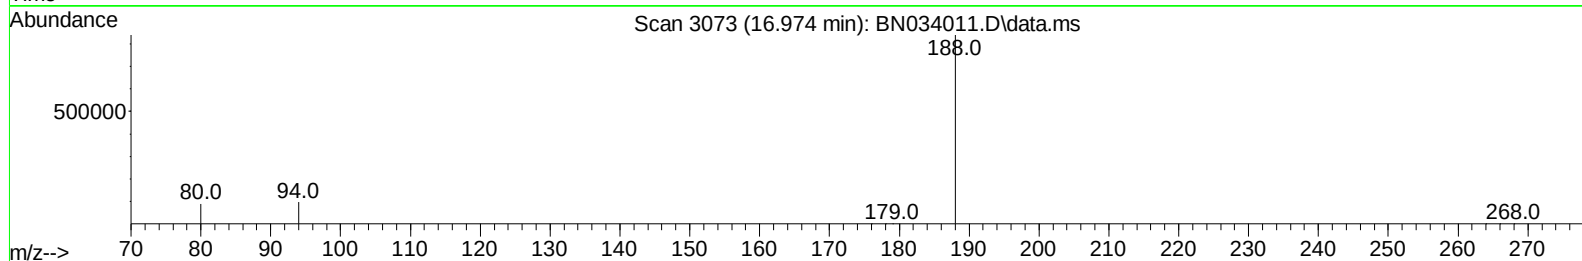


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

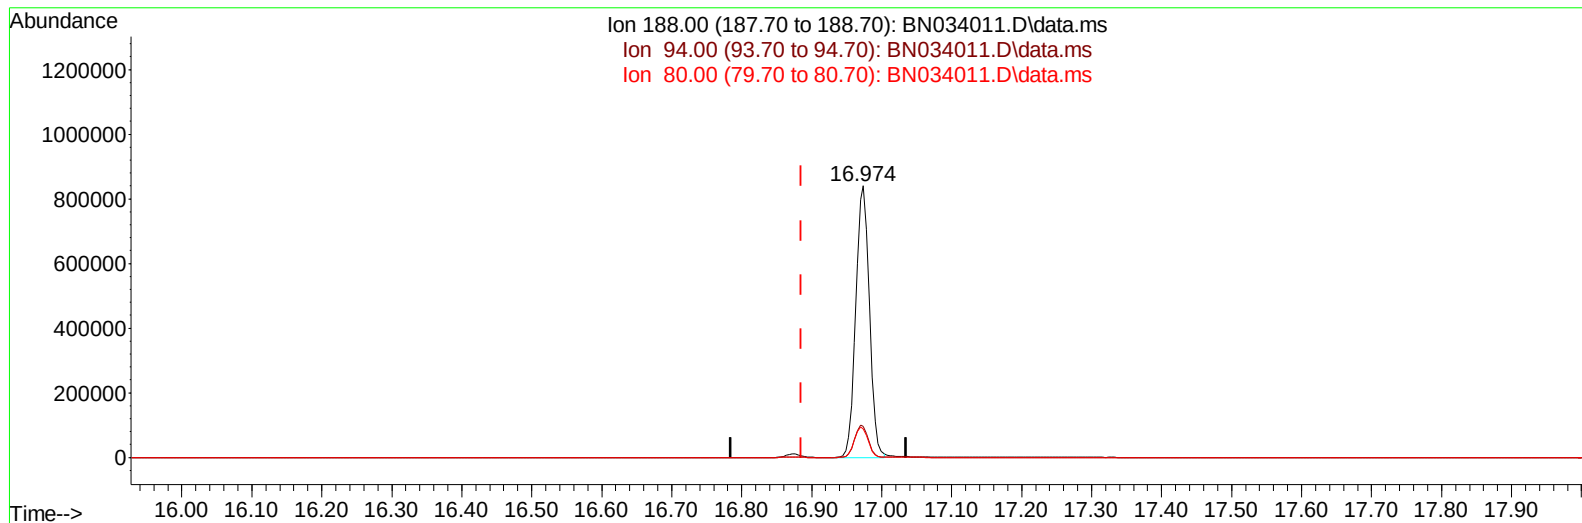

TIC: BN034011.D\data.ms

(13) Phenanthrene-d10 (I)




16.974min (+ 0.089) 0.40 ng/u1

response 1126570

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.48
80.00	11.50	10.61
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

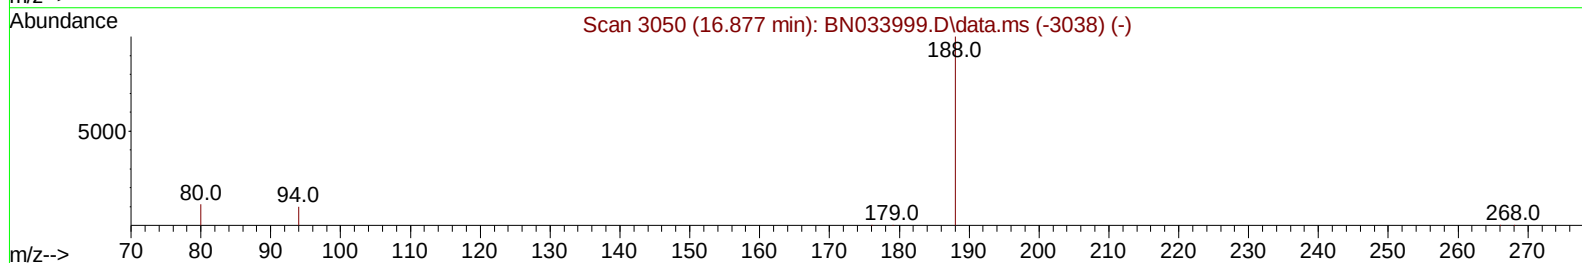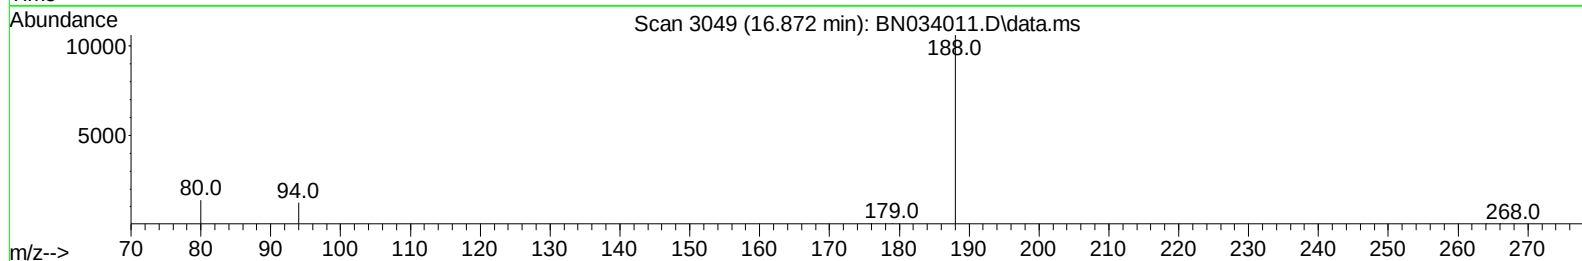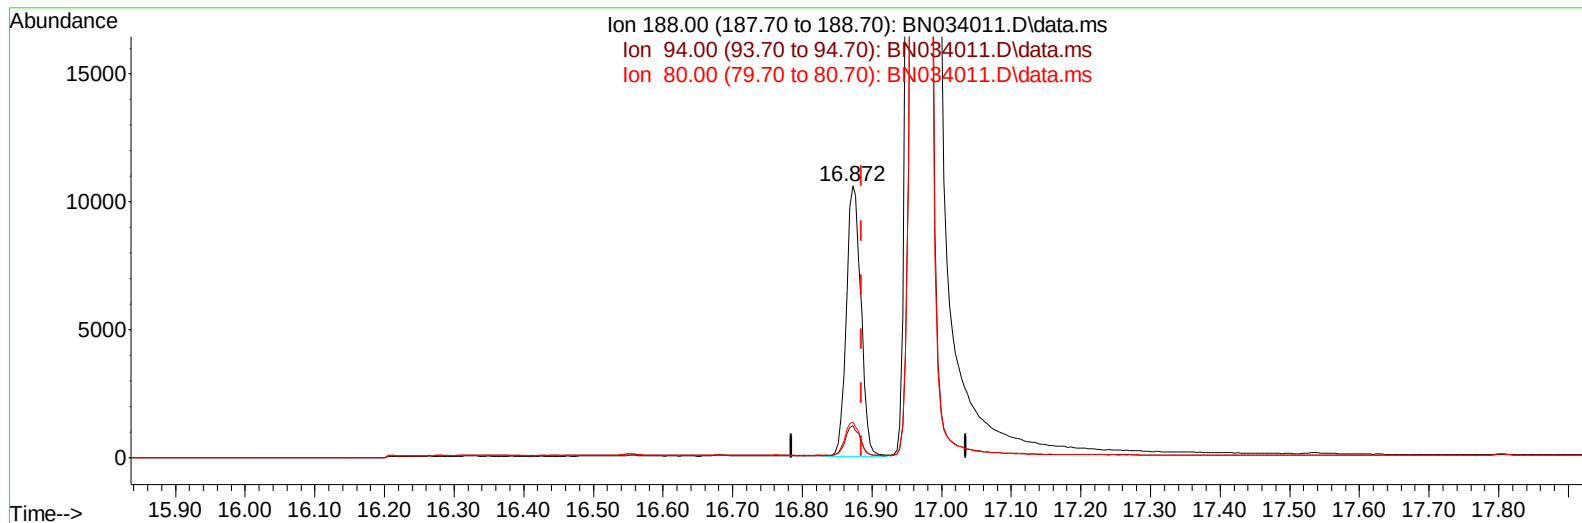




TIC: BN034011.D\data.ms

(13) Phenanthrene-d10 (I)**16.872min (-0.013) 0.40 ng/ul m****response 15420**

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	10.30	11.63
80.00	11.50	13.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

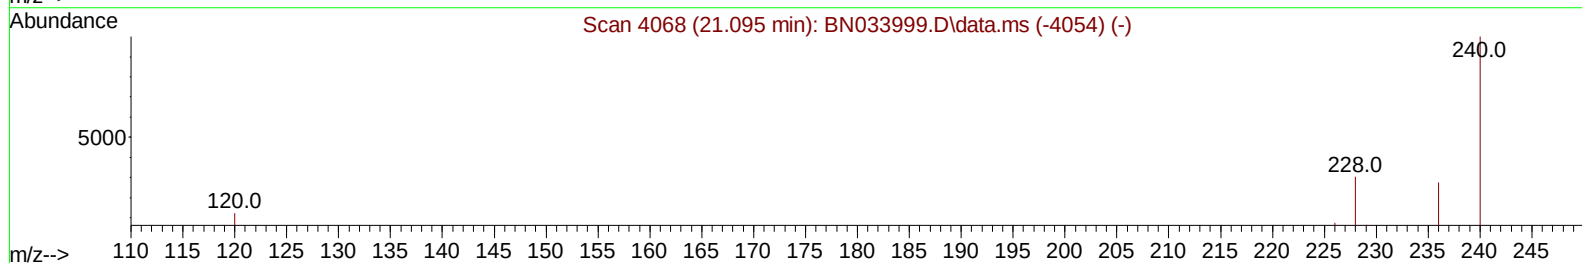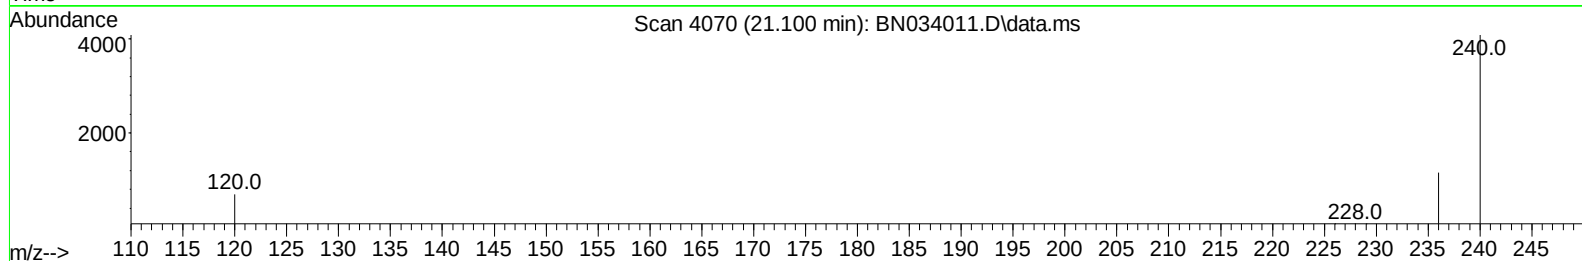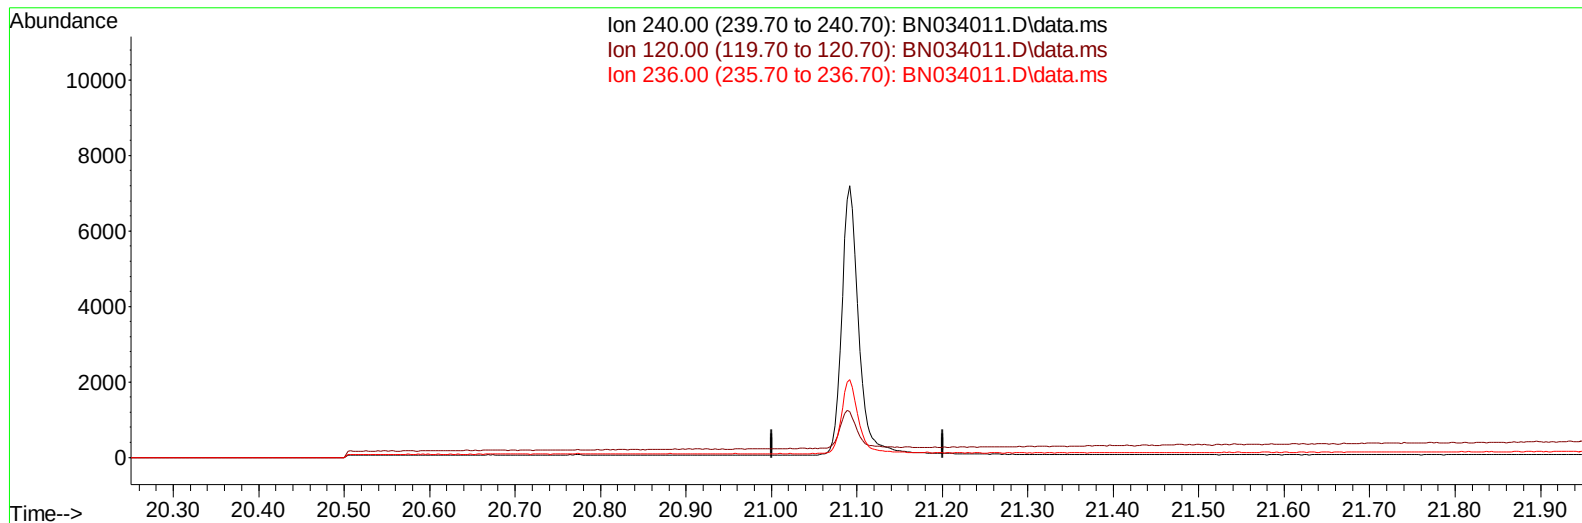

TIC: BN034011.D\data.ms

(17) Chrysene-d12




21.101min (-21.101) 0.00 ng/u1

response 0

Ion	Exp%	Act%
240.00	100.00	0.00
120.00	16.40	0.00#
236.00	28.30	0.00#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

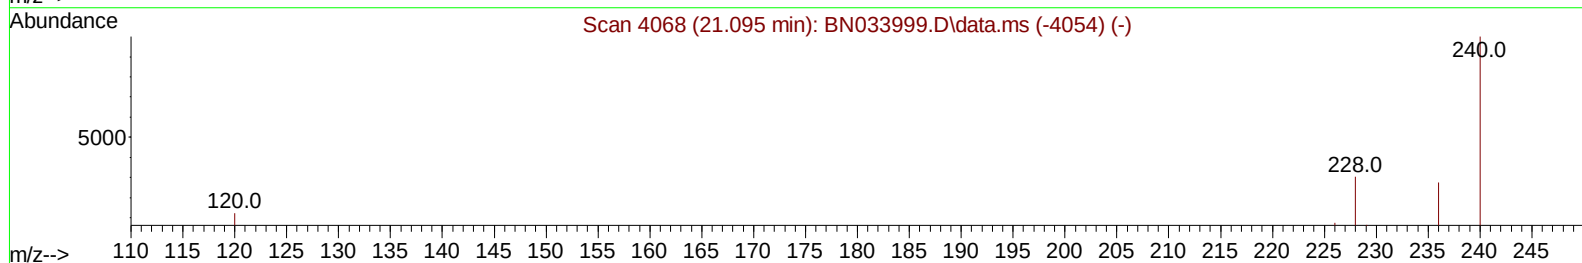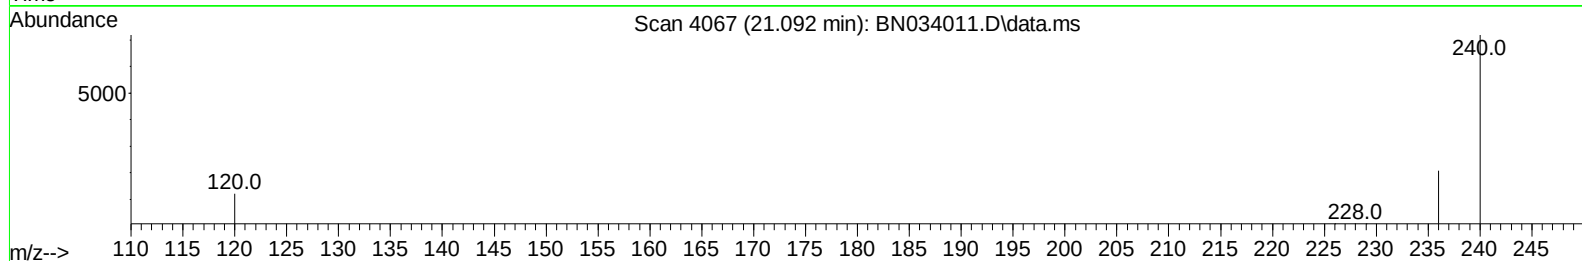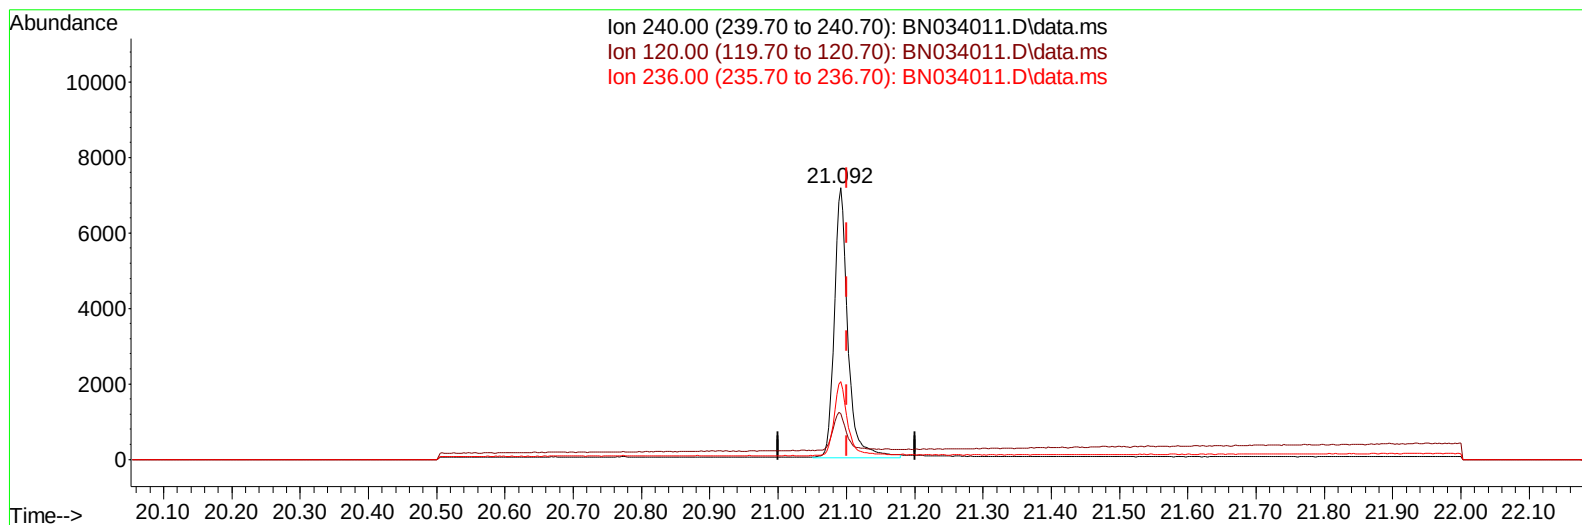

TIC: BN034011.D\data.ms

(17) Chrysene-d12




21.092min (-0.009) 0.40 ng/ul m

response 10056

Ion	Exp%	Act%
240.00	100.00	100.00
120.00	16.40	16.91
236.00	28.30	28.68
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

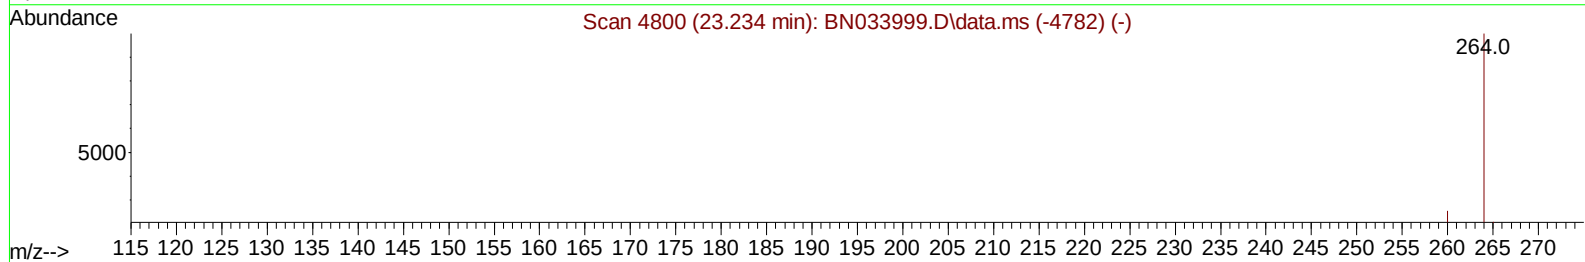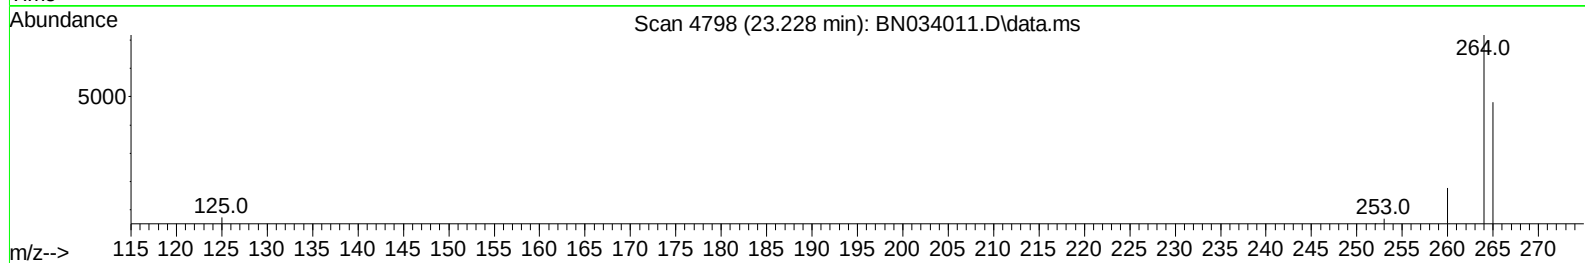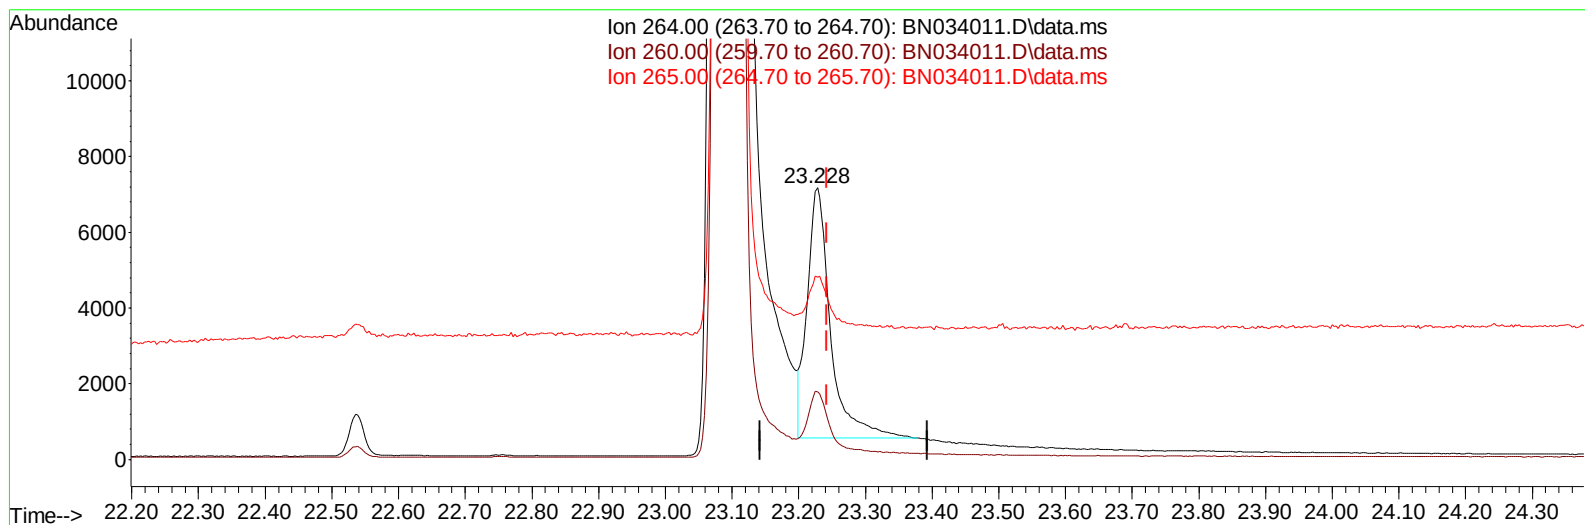

TIC: BN034011.D\data.ms

(23) Perylene-d12 (I)




23.228min (-0.015) 0.40 ng/ul

response 16049

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	24.92
265.00	73.30	66.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

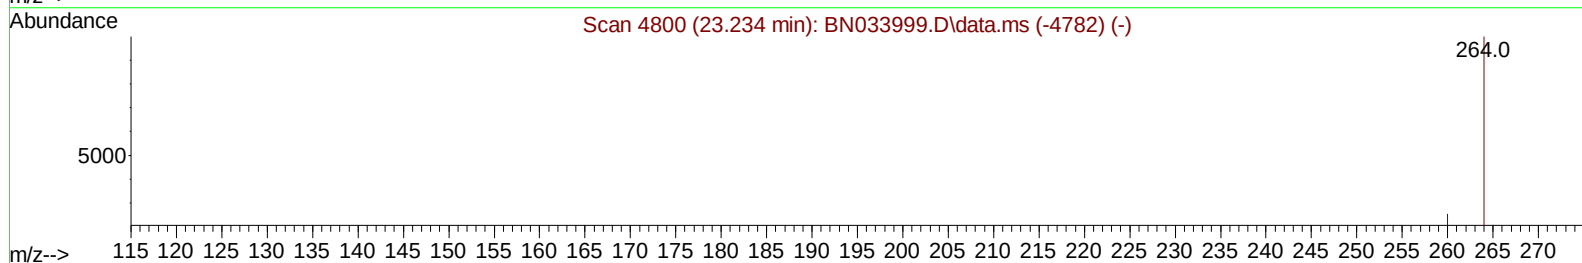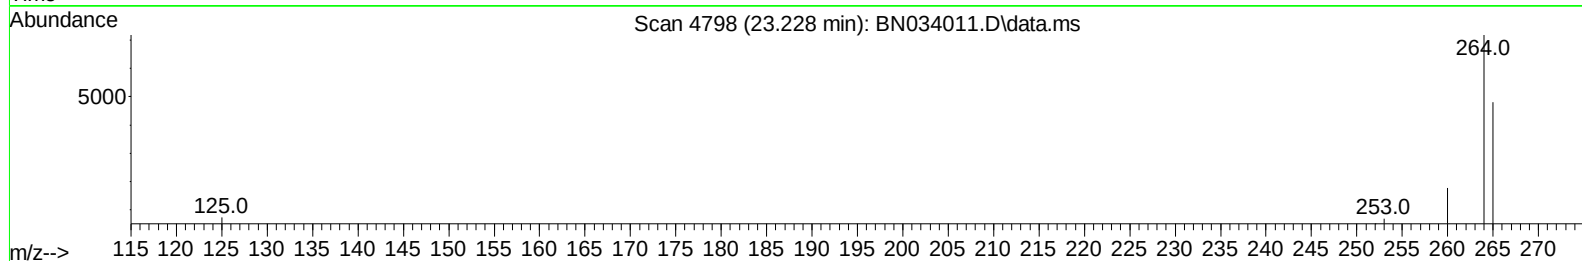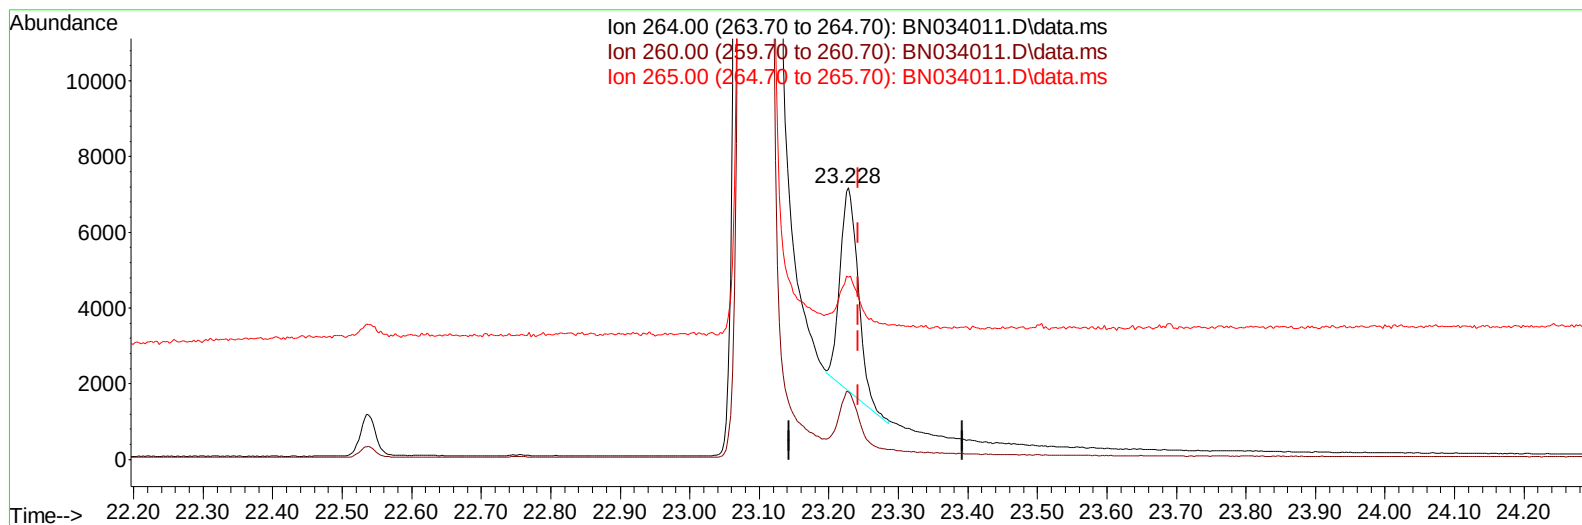

TIC: BN034011.D\data.ms

(23) Perylene-d12 (I)

23.228min (-0.015) 0.40 ng/ul m

response 9684

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.60	24.92
265.00	73.30	66.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034011.D
 Acq On : 17 Sep 2024 05:38
 Operator : JU/RC
 Sample : P3997-15
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.473	152	4596	0.400	ng/ul	-0.01
4) Naphthalene-d8	10.228	136	12701	0.400	ng/ul	-0.02
9) Acenaphthene-d10	14.119	164	6500	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.872	188	15420m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.092	240	10056m	0.400	ng/ul	0.00
23) Perylene-d12	23.228	264	9684m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	30352	6.424	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	6184	0.339	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	13398	0.447	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034011.D
Acq On : 17 Sep 2024 05:38
Operator : JU/RC
Sample : P3997-15
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Sep 17 07:01:34 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

