

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN033991.D
 Acq On : 16 Sep 2024 17:01
 Operator : JU/RC
 Sample : P3864-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BH7N3

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/17/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 16 18:39:15 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4702	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	12897	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.123	164	6513	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.877	188	13288m	0.400	ng/ul	0.00
17) Chrysene-d12	21.097	240	10003m	0.400	ng/ul	0.00
23) Perylene-d12	23.243	264	9621m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	30322	6.273	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	6354	0.343	ng/ul	-0.01
18) Fluoranthene-d10	18.920	212	12240	0.410	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.131	88	4687	0.874	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN033991.D
Acq On : 16 Sep 2024 17:01
Operator : JU/RC
Sample : P3864-01
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BH7N3

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 16 18:39:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

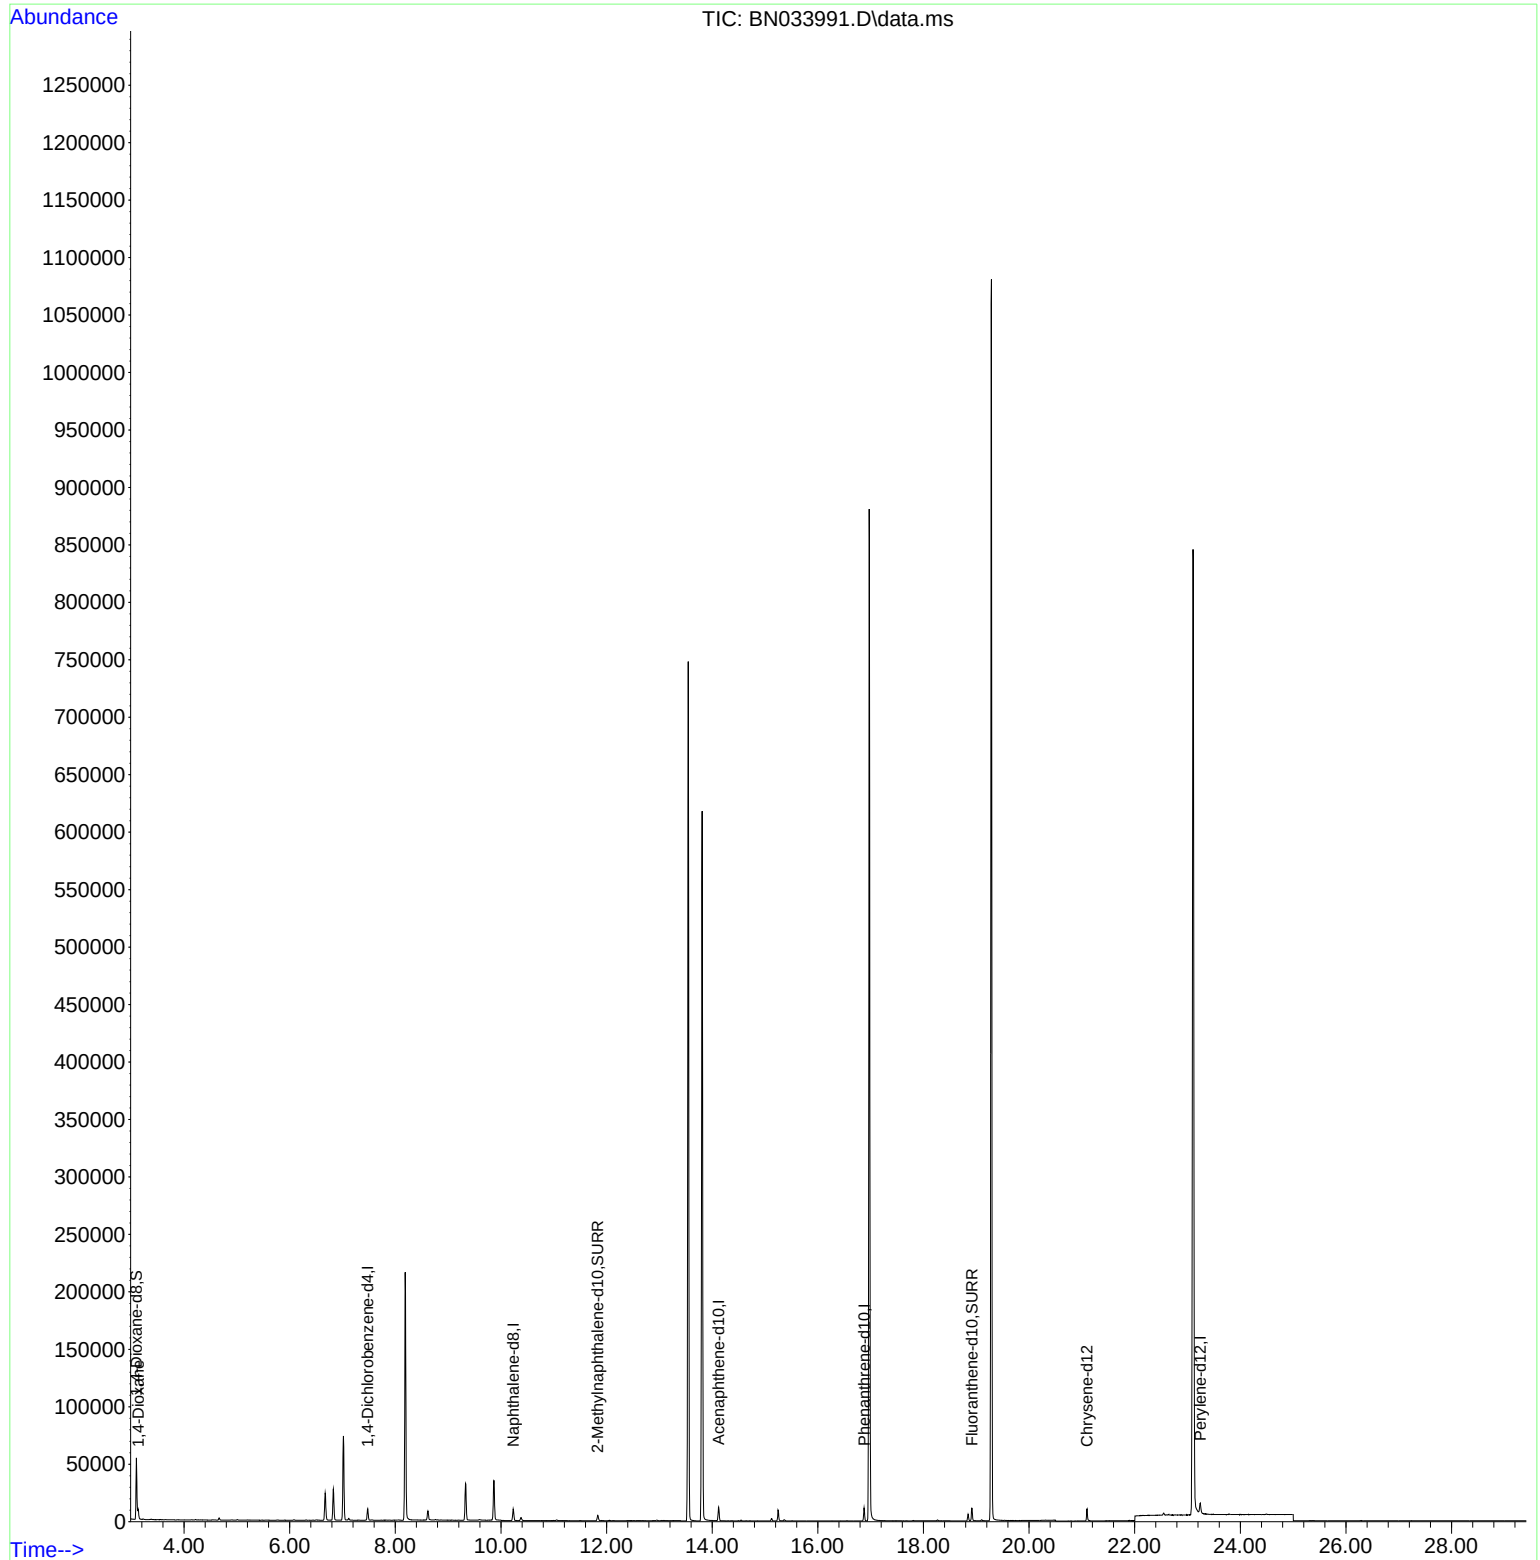

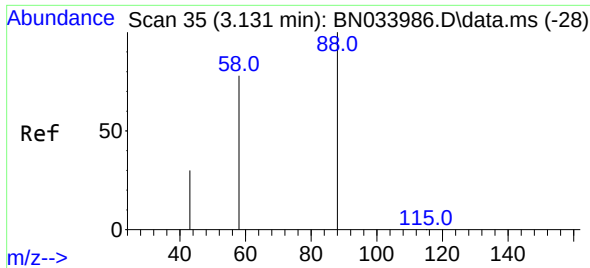

#2
1,4-Dioxane
Concen: 0.874 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN033991.D
Acq: 16 Sep 2024 17:01

Instrument :
BNA_N
ClientSampleId :
BH7N3

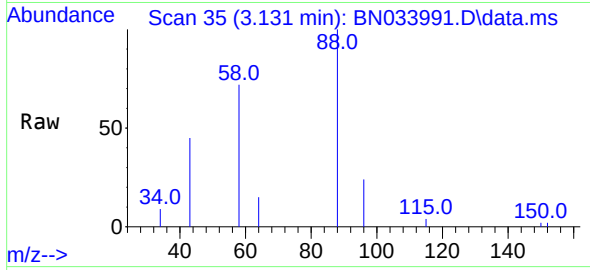

Tgt Ion: 88 Resp: 468
Ion Ratio Lower Upper
88 100
43 44.8 47.0 70.4
58 72.2 53.0 79.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

