

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034003.D
 Acq On : 17 Sep 2024 00:50
 Operator : JU/RC
 Sample : P3994-05
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B21

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/17/2024
 Supervised By :mohammad ahmed 09/17/2024

Quant Time: Sep 17 01:16:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4069	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	11332	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.119	164	6052	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.877	188	12697m	0.400	ng/ul	0.00
17) Chrysene-d12	21.095	240	10029m	0.400	ng/ul	0.00
23) Perylene-d12	23.234	264	9681m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.089	96	52595m	12.573	ng/ul	-0.02
6) 2-Methylnaphthalene-d10	11.834	152	5147	0.317	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	12538	0.419	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.131	88	24904	5.365	ng/ul#	79

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034003.D
Acq On : 17 Sep 2024 00:50
Operator : JU/RC
Sample : P3994-05
Misc :
ALS Vial : 19 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
C0B21

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024


Quant Time: Sep 17 01:16:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

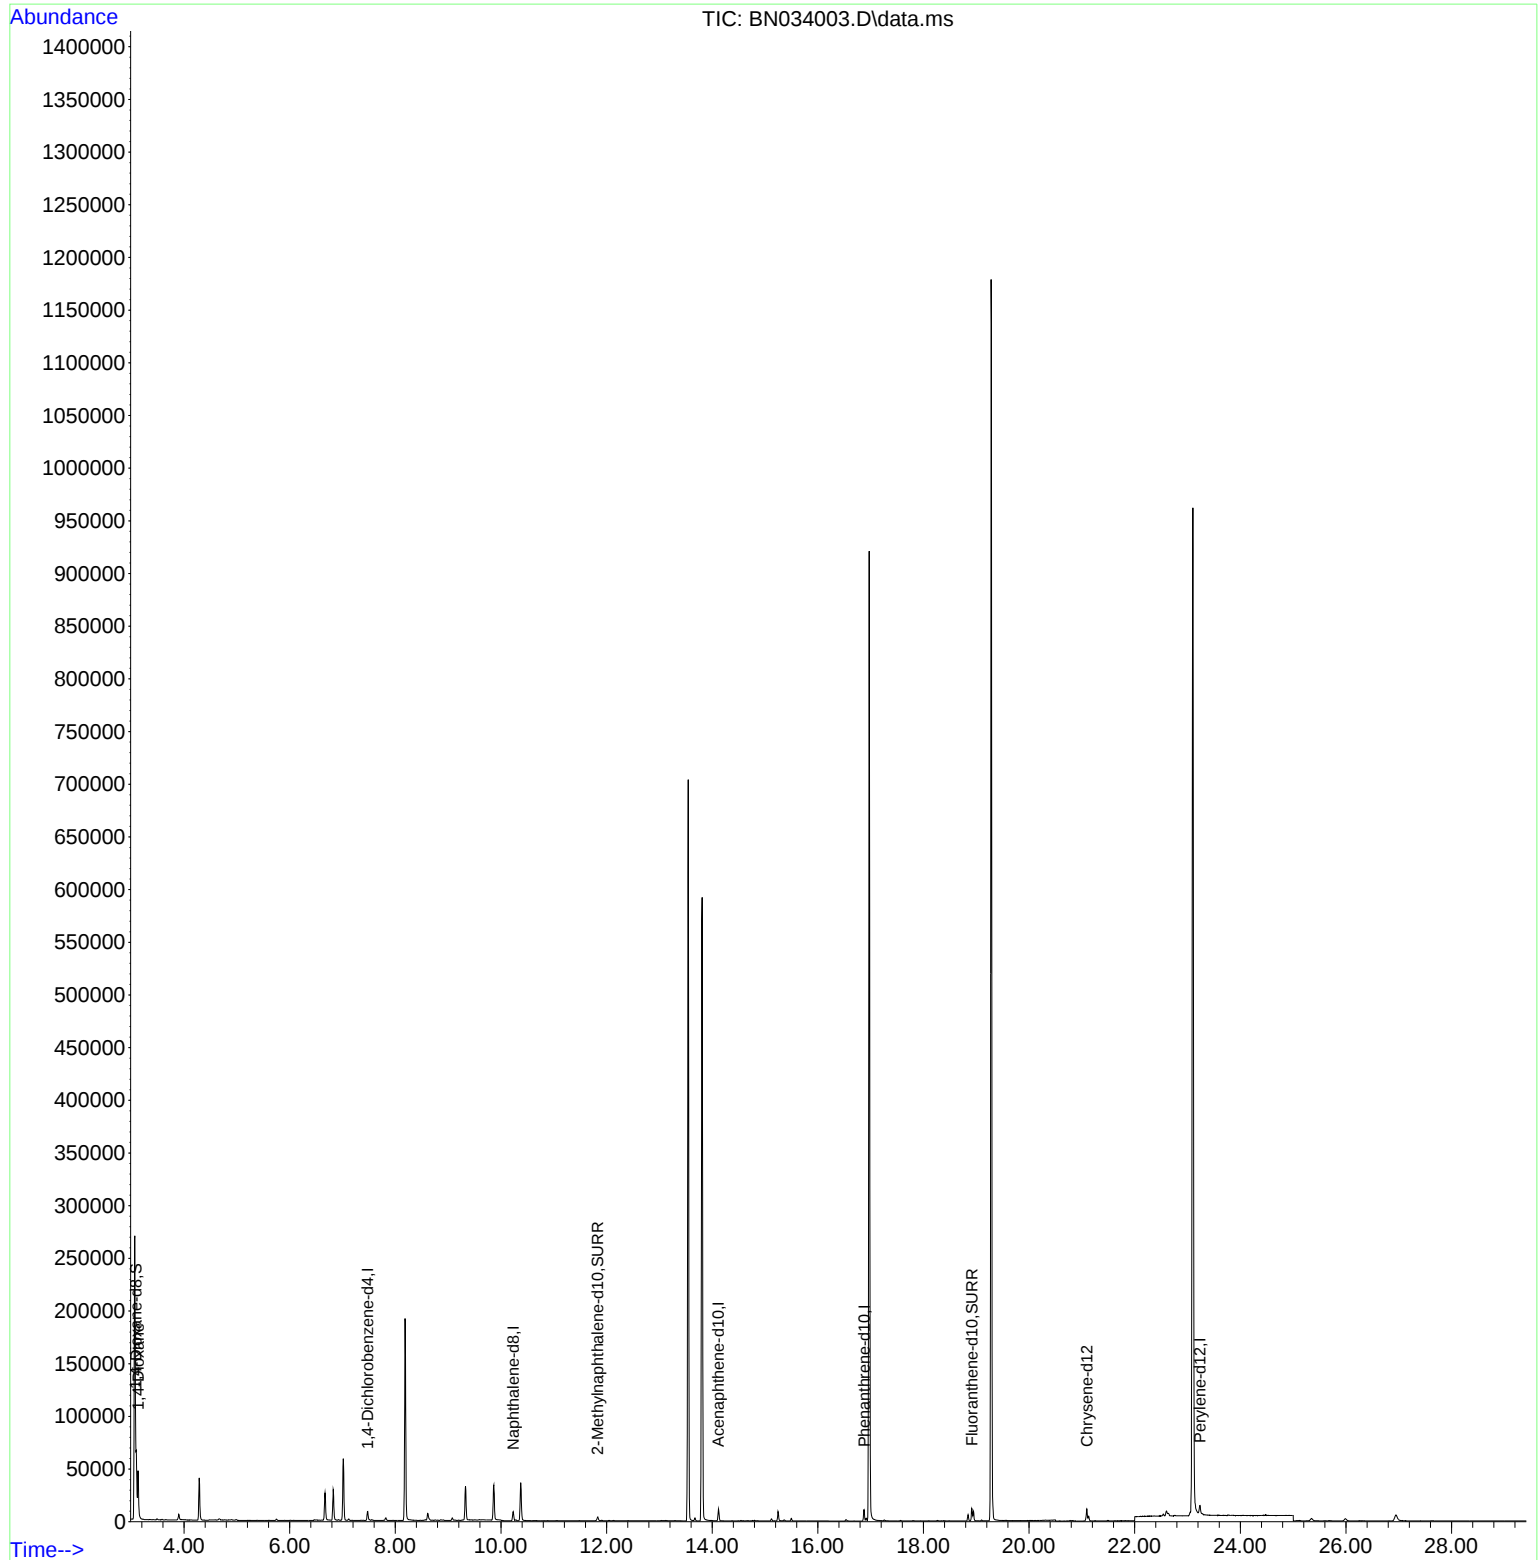

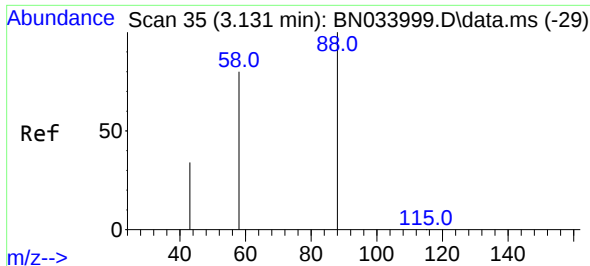

#2
1,4-Dioxane
Concen: 5.365 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN034003.D
Acq: 17 Sep 2024 00:50

Instrument :
BNA_N
ClientSampleId :
C0B21

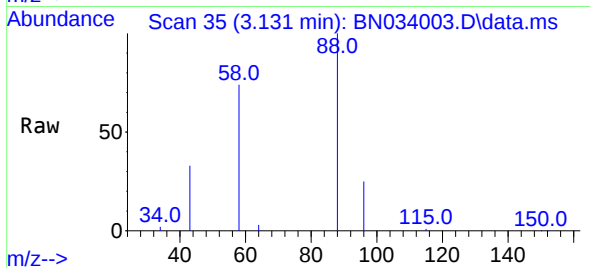

Tgt Ion: 88 Resp: 24904
Ion Ratio Lower Upper
88 100
43 33.0 47.0 70.4
58 74.0 53.0 79.4

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/17/2024
Supervised By :mohammad ahmed 09/17/2024

