

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034005.D
 Acq On : 17 Sep 2024 02:02
 Operator : JU/RC
 Sample : P3994-07
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0B27

Quant Time: Sep 17 02:32:28 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.477	152	4508	0.400	ng/ul	0.00
4) Naphthalene-d8	10.233	136	12512	0.400	ng/ul	-0.01
9) Acenaphthene-d10	14.119	164	6509	0.400	ng/ul	-0.01
13) Phenanthrene-d10	16.872	188	13391m	0.400	ng/ul	-0.01
17) Chrysene-d12	21.092	240	10600m	0.400	ng/ul	0.00
23) Perylene-d12	23.231	264	10286m	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	26587	5.737	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.834	152	5099	0.284	ng/ul	-0.01
18) Fluoranthene-d10	18.915	212	12969	0.410	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.127	88	61962	12.049	ng/ul#	76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034005.D
Acq On : 17 Sep 2024 02:02
Operator : JU/RC
Sample : P3994-07
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0B27

Quant Time: Sep 17 02:32:28 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

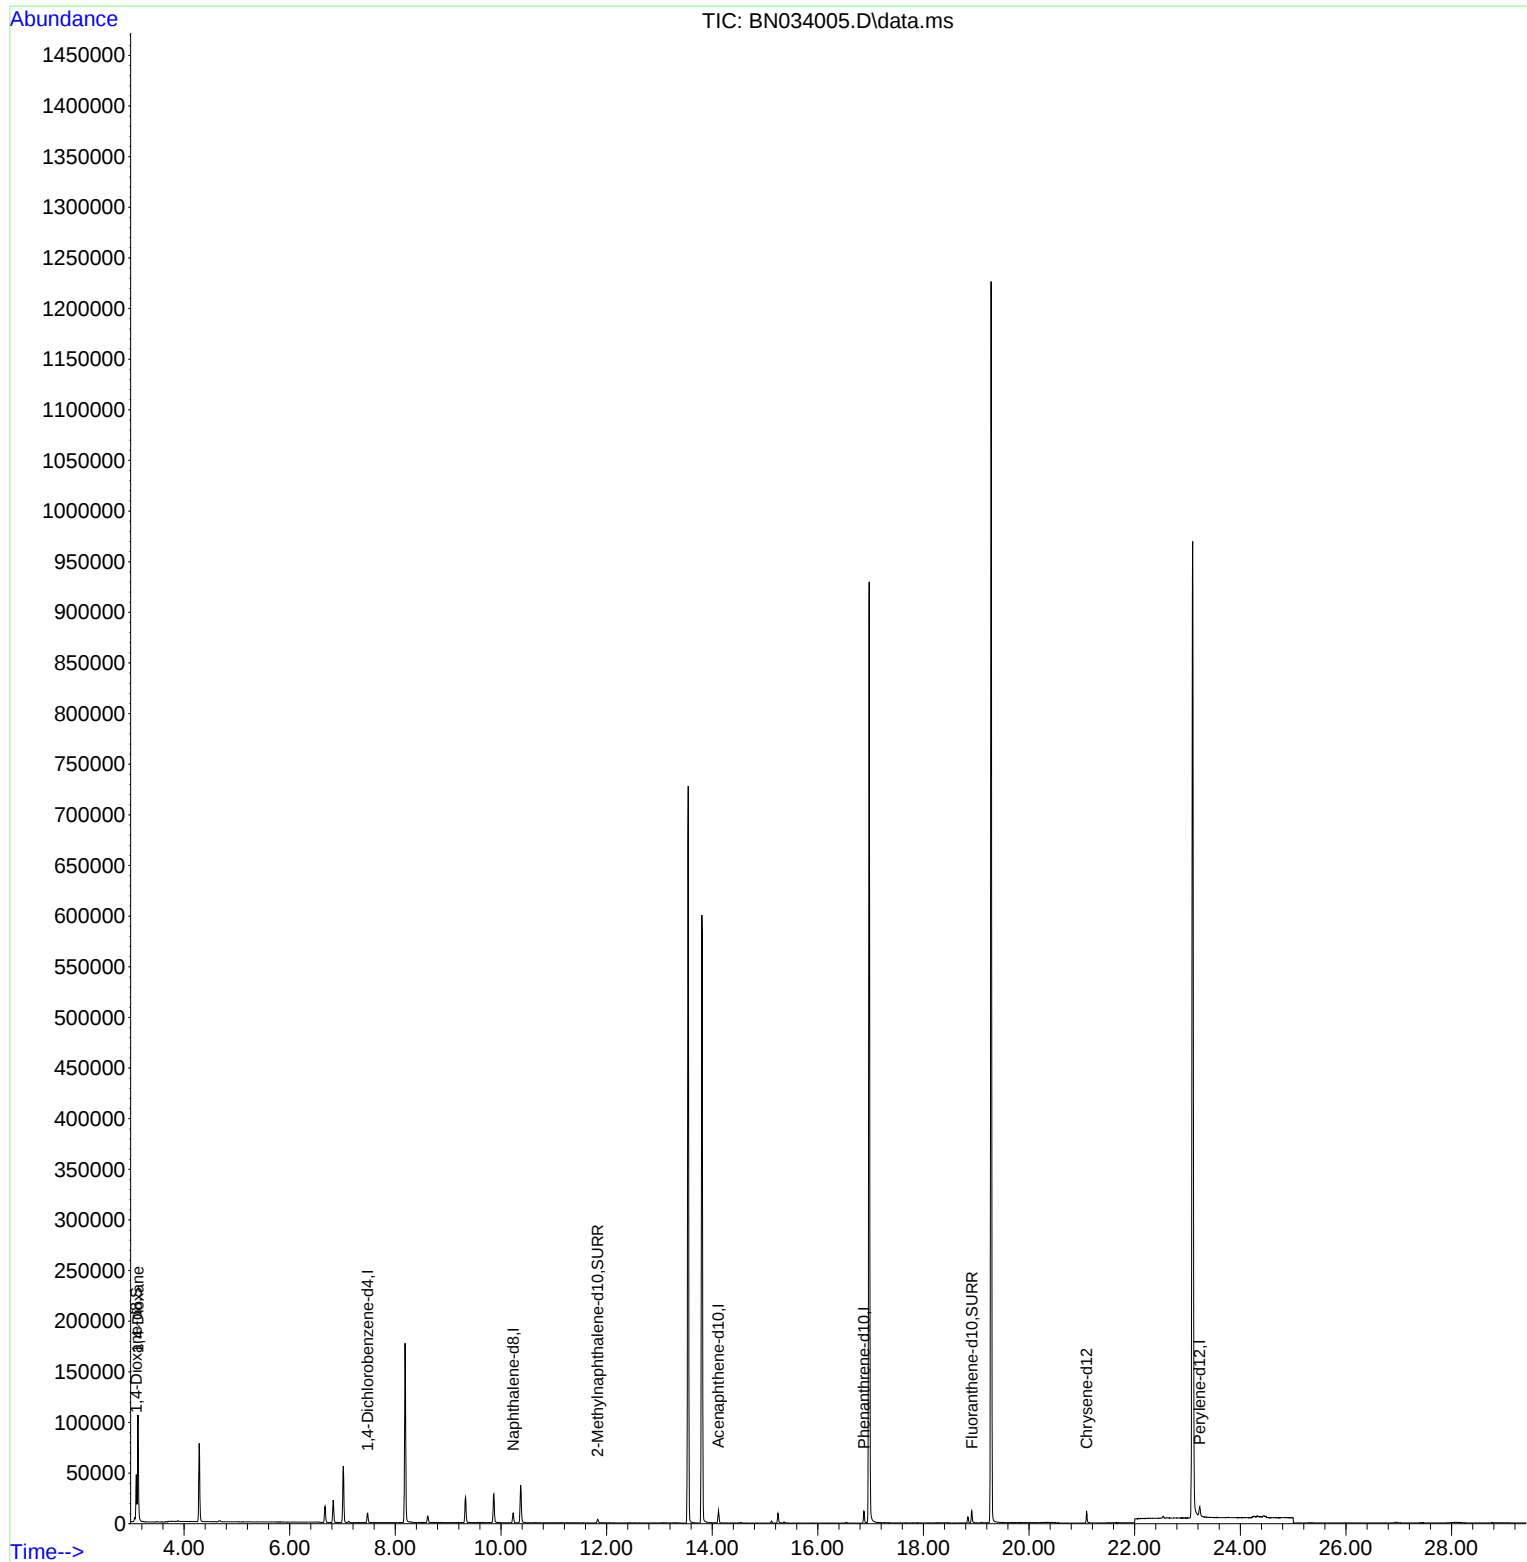


Abundance Scan 35 (3.131 min): BN033999.D\data.ms (-29)

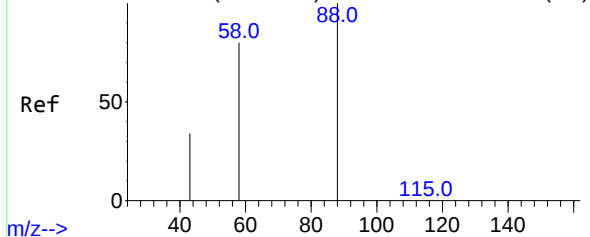


m/z-->

Abundance Scan 34 (3.127 min): BN034005.D\data.ms

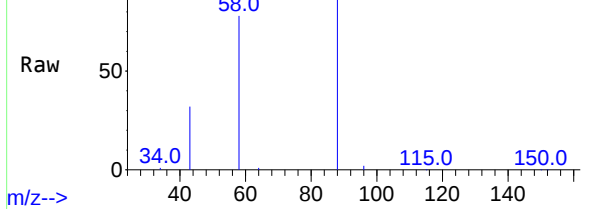

m/z-->

Abundance Scan 34 (3.127 min): BN034005.D\data.ms (-12)

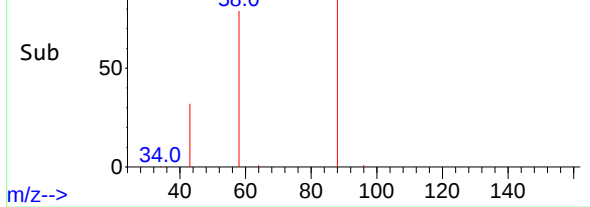

m/z-->

#2
1,4-Dioxane
Concen: 12.049 ng/ul
RT: 3.127 min Scan# 34
Delta R.T. -0.008 min
Lab File: BN034005.D
Acq: 17 Sep 2024 02:02

Instrument :
BNA_N
ClientSampleId :
C0B27

Tgt Ion: 88 Resp: 61962
Ion Ratio Lower Upper
88 100
43 32.3 47.0 70.4#
58 78.0 53.0 79.4

