

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
 Data File : BN034007.D
 Acq On : 17 Sep 2024 03:14
 Operator : JU/RC
 Sample : P3994-11
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 C0AS3

Quant Time: Sep 17 03:37:43 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sun Sep 15 01:52:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.473	152	4558	0.400	ng/u1	-0.01
4) Naphthalene-d8	10.228	136	12985	0.400	ng/u1	#-0.02
9) Acenaphthene-d10	14.119	164	28397	0.400	ng/u1	#-0.01
13) Phenanthrene-d10	16.872	188	16287m	0.400	ng/u1	-0.01
17) Chrysene-d12	21.089	240	13001m	0.400	ng/u1	-0.01
23) Perylene-d12	23.228	264	12265m	0.400	ng/u1	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.097	96	29649	6.327	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.828	152	10725	0.576	ng/u1	-0.02
18) Fluoranthene-d10	18.915	212	19841m	0.512	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.131	88	4479	0.861	ng/u1	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091624\
Data File : BN034007.D
Acq On : 17 Sep 2024 03:14
Operator : JU/RC
Sample : P3994-11
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
C0AS3

Quant Time: Sep 17 03:37:43 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN082724.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sun Sep 15 01:52:43 2024
Response via : Initial Calibration

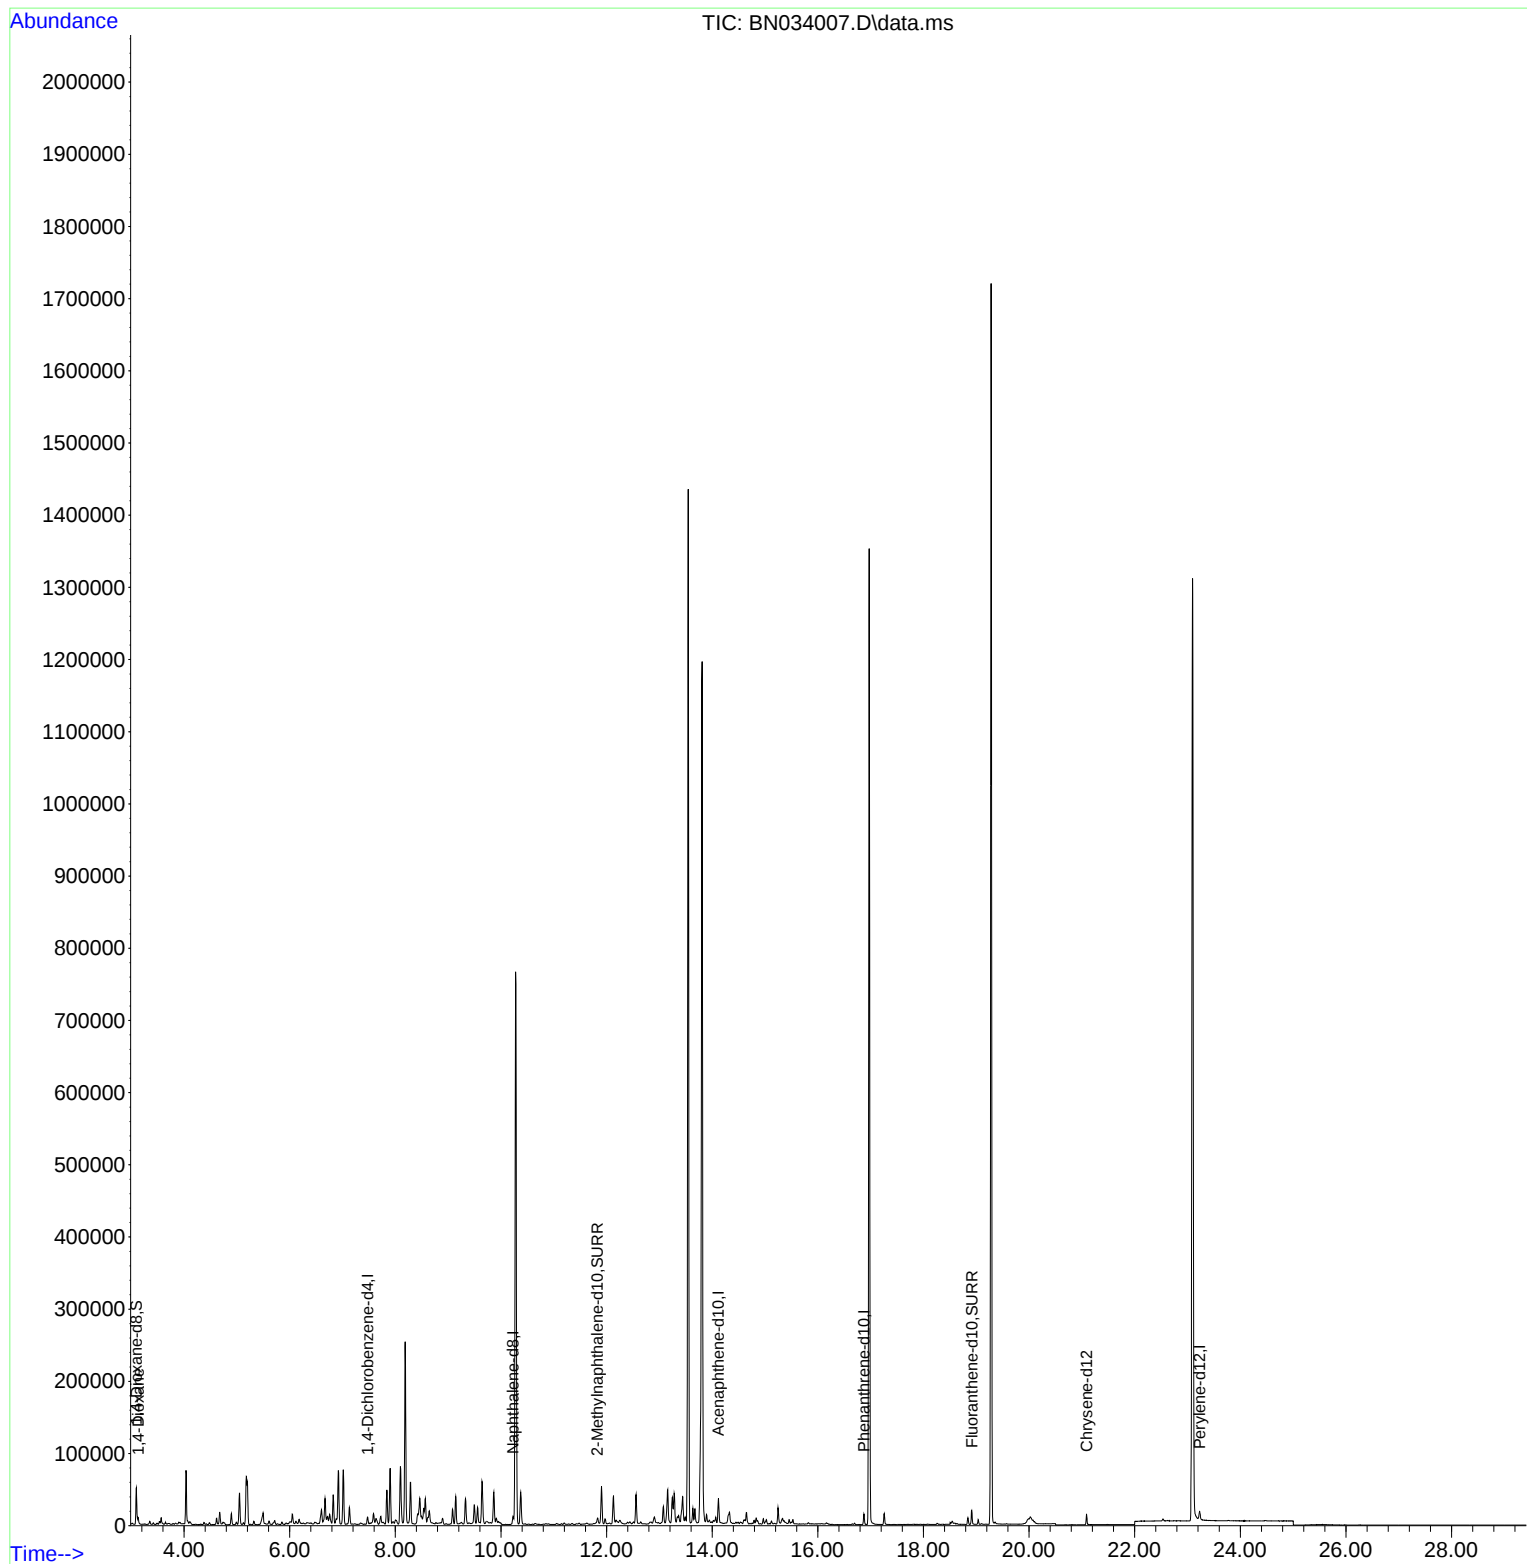

Abundance Scan 35 (3.131 min): BN033999.D\data.ms (-29)

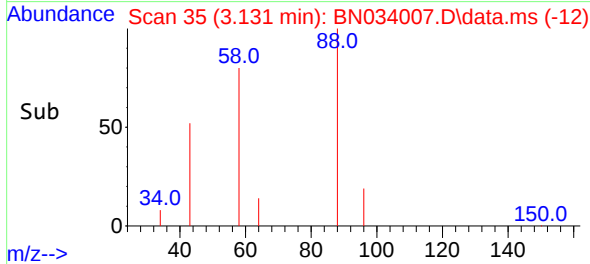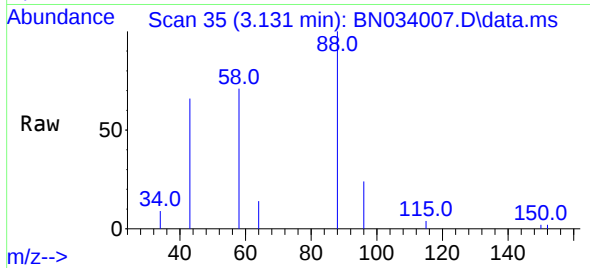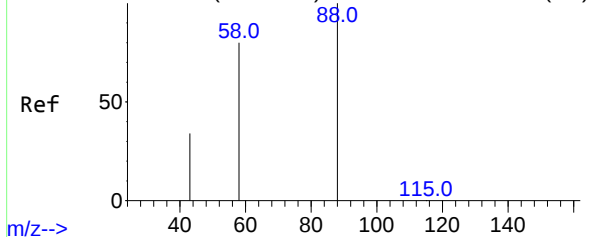

#2
1,4-Dioxane
Concen: 0.861 ng/ul
RT: 3.131 min Scan# 31
Delta R.T. -0.004 min
Lab File: BN034007.D
Acq: 17 Sep 2024 03:14

Instrument :
BNA_N
ClientSampleId :
C0AS3

Tgt Ion:	88	Resp:	4479
Ion	Ratio	Lower	Upper
88	100		
43	65.9	47.0	70.4
58	70.9	53.0	79.4

