

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
 Data File : BN037725.D
 Acq On : 16 Sep 2025 10:13
 Operator : RC/JU
 Sample : PB169520BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK520

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.263	26	30	38	rBV	74228	102320	1.68%	0.170%
2	3.675	95	100	124	rBV	999657	1511837	24.81%	2.510%
3	4.016	153	158	168	rVB2	38789	57120	0.94%	0.095%
4	6.987	656	663	675	rBV	1111007	1744586	28.63%	2.897%
5	7.163	686	693	704	rVB	897674	1391189	22.83%	2.310%
6	7.363	720	727	739	rBV	1151116	1805501	29.63%	2.998%
7	7.840	800	808	815	rBV	948094	1520203	24.95%	2.524%
8	8.540	919	927	941	rBV	1303565	2112341	34.67%	3.507%
9	8.993	997	1004	1013	rBV	1012619	1621617	26.61%	2.693%
10	9.104	1019	1023	1030	rVB5	4999	8266	0.14%	0.014%
11	9.722	1120	1128	1137	rBV	678202	1093472	17.95%	1.816%
12	10.257	1211	1219	1230	rBV	1218972	2014361	33.06%	3.345%
13	10.645	1276	1285	1293	rBV	1220654	2022708	33.20%	3.358%
14	10.769	1298	1306	1321	rBV	1242502	2169388	35.60%	3.602%
15	11.287	1390	1394	1398	rBV2	6983	9914	0.16%	0.016%
16	12.239	1550	1556	1561	rVB2	21953	35248	0.58%	0.059%
17	13.481	1760	1767	1772	rBV2	20561	30382	0.50%	0.050%
18	13.904	1832	1839	1845	rBV	1878765	2641315	43.35%	4.386%
19	14.186	1877	1887	1896	rBV	2446093	3547151	58.21%	5.890%
20	14.492	1931	1939	1948	rBV	1689436	2458348	40.34%	4.082%
21	14.669	1962	1969	1982	rBV	977583	1376725	22.59%	2.286%
22	15.486	2101	2108	2115	rBV	2979279	4181470	68.62%	6.943%
23	15.592	2119	2126	2141	rVV	580976	796523	13.07%	1.323%
24	15.728	2145	2149	2154	rVB3	11989	16831	0.28%	0.028%
25	17.022	2366	2369	2374	rBV2	6658	10325	0.17%	0.017%
26	17.239	2399	2406	2413	rBV2	2009242	2739116	44.95%	4.548%
27	17.339	2416	2423	2431	rBV	3369675	4545031	74.59%	7.547%
28	18.145	2557	2560	2563	rBV4	5196	6438	0.11%	0.011%
29	19.198	2734	2739	2743	rBV2	37634	51711	0.85%	0.086%
30	19.263	2746	2750	2756	rVV	35462	46905	0.77%	0.078%
31	19.345	2760	2764	2768	rVB	40307	46377	0.76%	0.077%
32	19.474	2782	2786	2793	rBV	41945	58727	0.96%	0.098%
33	19.586	2799	2805	2807	rBV	86617	109315	1.79%	0.182%
34	19.627	2807	2812	2821	rVV	3794357	5270233	86.49%	8.751%
35	19.692	2821	2823	2829	rVB7	13312	20223	0.33%	0.034%
36	20.421	2945	2947	2952	rVB5	19376	17524	0.29%	0.029%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037725.D
Acq On : 16 Sep 2025 10:13
Operator : RC/JU
Sample : PB169520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION

37	20.627	2978	2982	2987	rBV2	50193	62145	1.02%	0.103%
38	21.492	3122	3129	3137	rBV	2119653	3227775	52.97%	5.359%
39	24.368	3608	3618	3636	rVB	2427804	6093358	100.00%	10.117%
40	24.574	3644	3653	3666	rVB	1488515	3652609	59.94%	6.065%




Sum of corrected areas: 60226628

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037725.D
Acq On : 16 Sep 2025 10:13
Operator : RC/JU
Sample : PB169520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

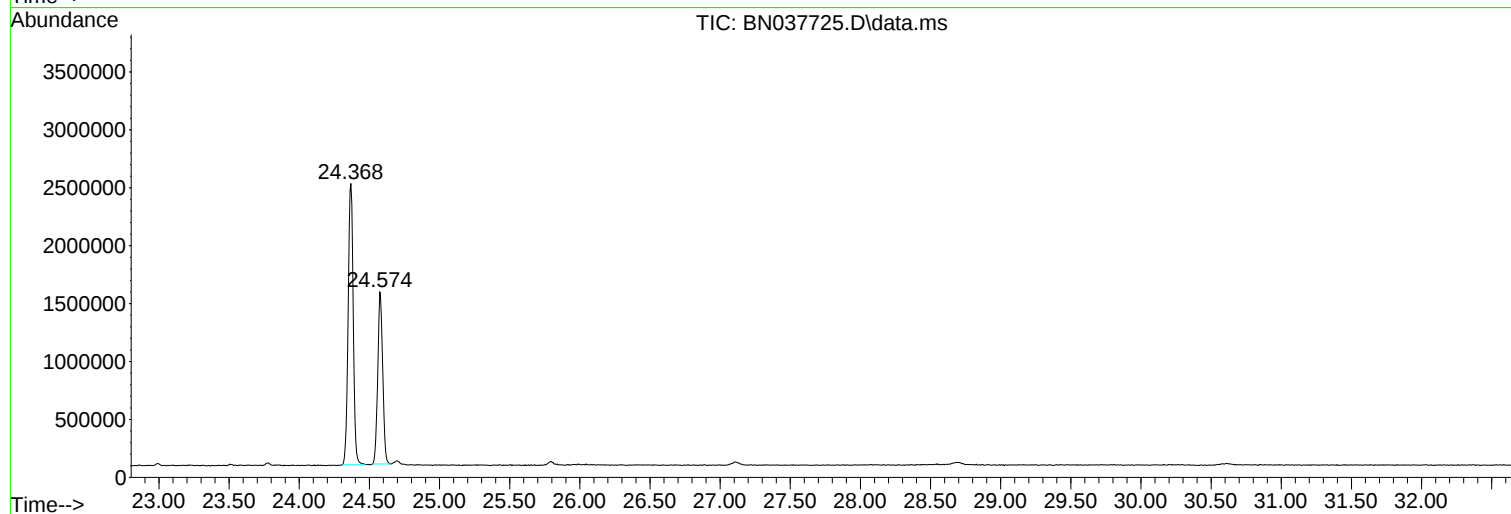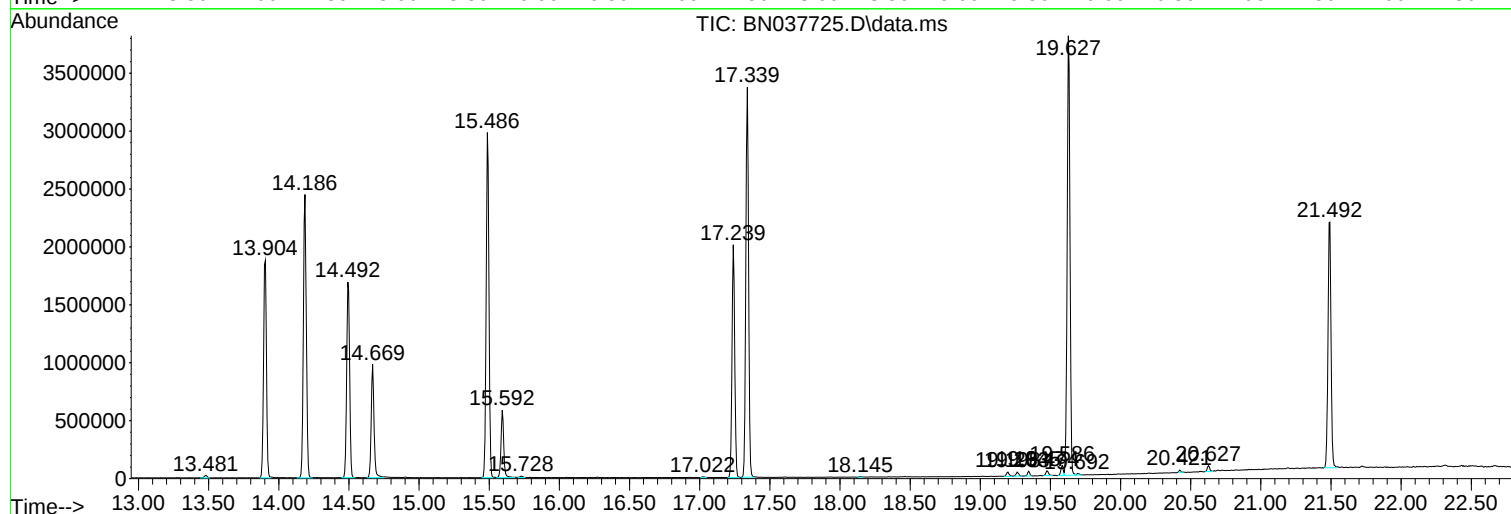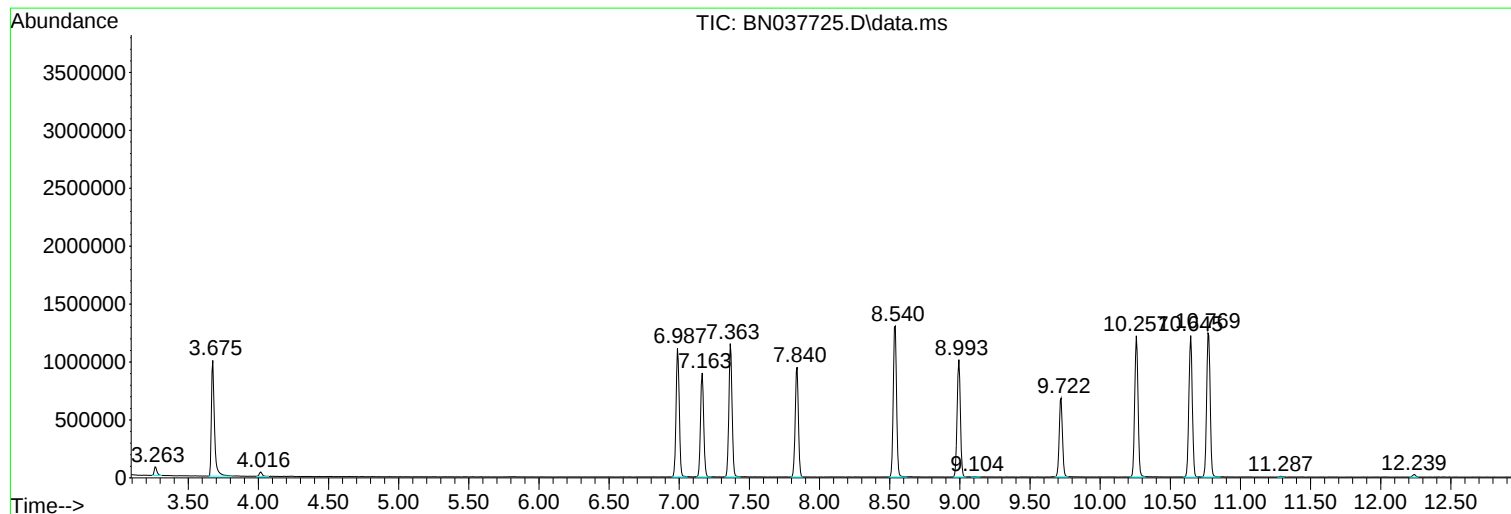

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037725.D
Acq On : 16 Sep 2025 10:13
Operator : RC/JU
Sample : PB169520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037725.D
Acq On : 16 Sep 2025 10:13
Operator : RC/JU
Sample : PB169520BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK520

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
