

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
 Data File : BN037729.D
 Acq On : 16 Sep 2025 12:50
 Operator : RC/JU
 Sample : PB169522BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK522

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037729.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.264	25	30	35	rBV	66275	85883	2.08%	0.182%
2	3.670	94	99	113	rBV	893167	1252650	30.35%	2.653%
3	4.011	151	157	164	rBV	28830	44369	1.08%	0.094%
4	4.228	189	194	199	rVB6	4039	6780	0.16%	0.014%
5	6.987	655	663	673	rBV	931974	1435637	34.78%	3.041%
6	7.158	683	692	701	rBV	752860	1186853	28.76%	2.514%
7	7.363	717	727	737	rBV	968228	1514533	36.70%	3.208%
8	7.834	799	807	815	rVB	849250	1324622	32.09%	2.806%
9	8.534	919	926	938	rBV	1124944	1764426	42.75%	3.737%
10	8.987	996	1003	1014	rBV	825475	1360377	32.96%	2.881%
11	9.105	1019	1023	1027	rVB4	3288	4571	0.11%	0.010%
12	9.716	1118	1127	1138	rBV	554498	870085	21.08%	1.843%
13	10.257	1211	1219	1234	rBV	1009674	1684907	40.82%	3.569%
14	10.646	1277	1285	1294	rBV	1033068	1760741	42.66%	3.730%
15	10.769	1298	1306	1315	rBV	1084538	1803654	43.70%	3.820%
16	11.293	1390	1395	1401	rVB3	5058	9223	0.22%	0.020%
17	12.234	1551	1555	1561	rVB	17649	26987	0.65%	0.057%
18	13.481	1760	1767	1772	rBV	17344	24451	0.59%	0.052%
19	13.898	1832	1838	1847	rBV	1549903	2121713	51.41%	4.494%
20	14.187	1880	1887	1895	rBV	1958010	2963092	71.79%	6.276%
21	14.492	1932	1939	1946	rVB	1460915	2085979	50.54%	4.418%
22	14.669	1958	1969	1983	rBV	686653	990742	24.00%	2.099%
23	15.487	2101	2108	2116	rBV	2471524	3438009	83.30%	7.282%
24	15.592	2120	2126	2134	rBV	401967	540635	13.10%	1.145%
25	15.728	2146	2149	2155	rVB3	10630	13716	0.33%	0.029%
26	16.275	2237	2242	2247	rBV6	2551	4379	0.11%	0.009%
27	17.022	2364	2369	2375	rBV4	5280	7942	0.19%	0.017%
28	17.239	2400	2406	2413	rBV2	1575094	2149348	52.08%	4.553%
29	17.339	2416	2423	2435	rVV	2579903	3558114	86.21%	7.537%
30	18.145	2556	2560	2565	rBV5	4803	7007	0.17%	0.015%
31	19.198	2734	2739	2745	rBV	26457	35660	0.86%	0.076%
32	19.263	2746	2750	2756	rVB2	24503	30773	0.75%	0.065%
33	19.345	2760	2764	2767	rBV2	26242	28608	0.69%	0.061%
34	19.428	2775	2778	2781	rBV4	5030	6540	0.16%	0.014%
35	19.475	2781	2786	2792	rBV	48259	73613	1.78%	0.156%
36	19.580	2800	2804	2807	rBV	58242	71783	1.74%	0.152%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037729.D
Acq On : 16 Sep 2025 12:50
Operator : RC/JU
Sample : PB169522BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK522

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION

37	19.627	2807	2812	2821	rVV	2925519	3940382	95.47%	8.346%
38	19.698	2821	2824	2829	rVB6	9632	15610	0.38%	0.033%
39	20.627	2978	2982	2988	rBV3	35337	50916	1.23%	0.108%
40	21.486	3122	3128	3137	rBV2	1557291	2292579	55.55%	4.856%
41	24.363	3608	3617	3634	rVB	1631565	4127326	100.00%	8.742%
42	24.574	3644	3653	3665	rBV2	1006834	2495942	60.47%	5.287%




Sum of corrected areas: 47211157

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037729.D
Acq On : 16 Sep 2025 12:50
Operator : RC/JU
Sample : PB169522BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

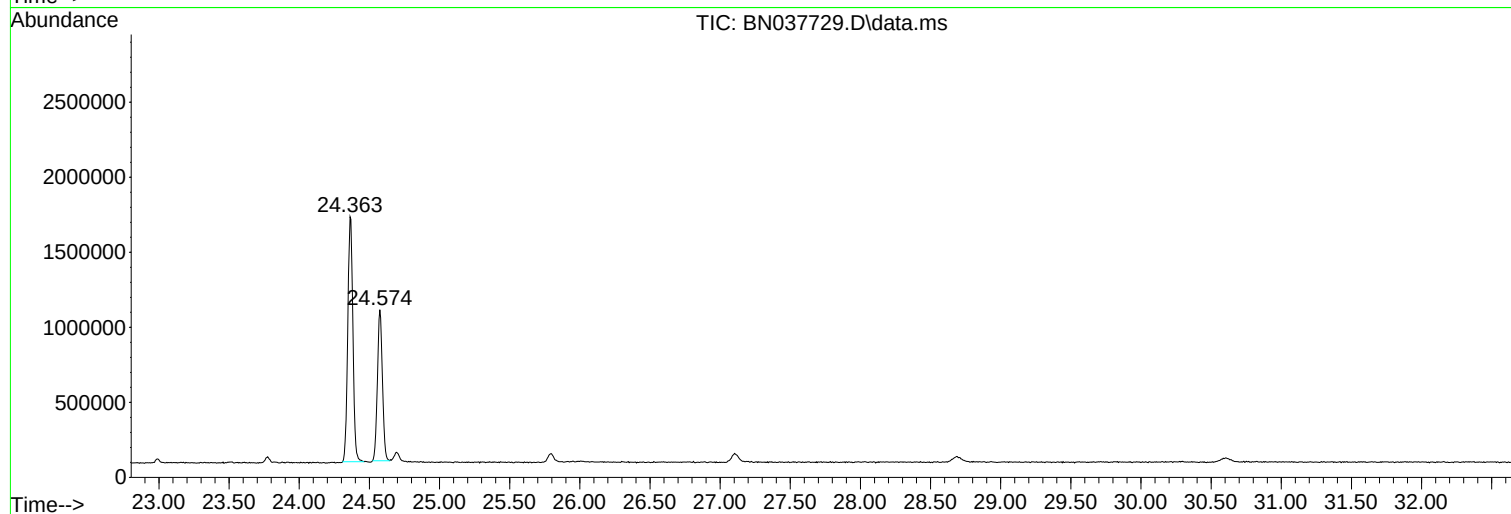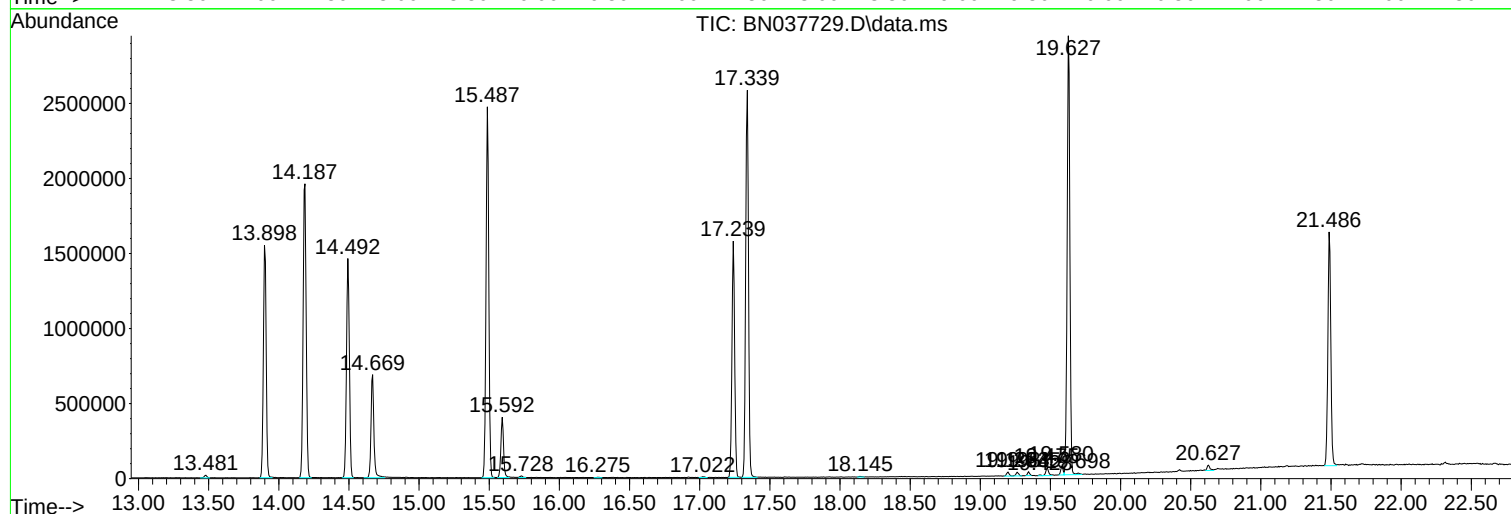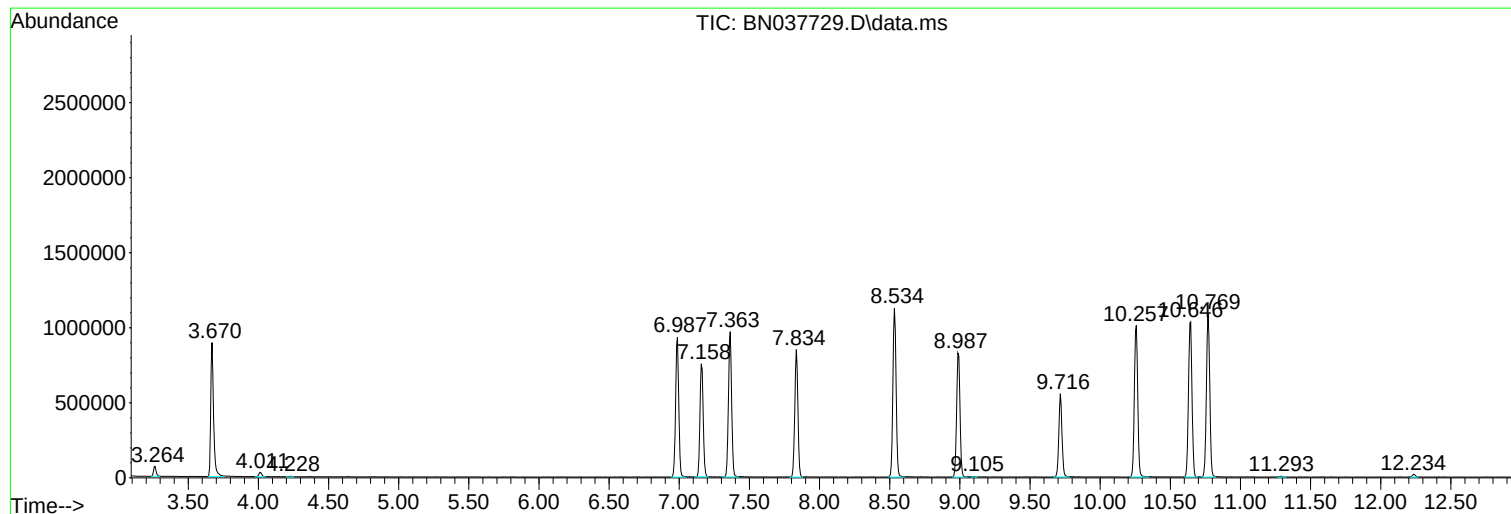

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037729.D
Acq On : 16 Sep 2025 12:50
Operator : RC/JU
Sample : PB169522BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037729.D
Acq On : 16 Sep 2025 12:50
Operator : RC/JU
Sample : PB169522BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK522

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------