

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
 Data File : BN037730.D
 Acq On : 16 Sep 2025 13:29
 Operator : RC/JU
 Sample : PB169524BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK524

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037730.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	40	rVB	61155	85043	2.16%	0.194%
2	3.670	94	99	114	rBV	839696	1182734	30.07%	2.700%
3	4.011	152	157	164	rVB	29827	41054	1.04%	0.094%
4	6.987	655	663	673	rBV	866232	1333586	33.90%	3.045%
5	7.158	684	692	702	rBV	724414	1117968	28.42%	2.553%
6	7.364	720	727	735	rBV	904812	1414336	35.96%	3.229%
7	7.834	800	807	814	rBV	788176	1210490	30.77%	2.764%
8	8.534	919	926	936	rBV	1044793	1631119	41.47%	3.724%
9	8.987	996	1003	1013	rBV	765123	1265826	32.18%	2.890%
10	9.099	1017	1022	1025	rBV5	3624	5688	0.14%	0.013%
11	9.716	1120	1127	1141	rBV	493655	787894	20.03%	1.799%
12	10.257	1210	1219	1231	rBV	956570	1563945	39.76%	3.571%
13	10.640	1277	1284	1292	rVB	942788	1599428	40.66%	3.652%
14	10.769	1298	1306	1316	rBV	990468	1664524	42.32%	3.801%
15	11.287	1389	1394	1398	rBV4	5383	7657	0.19%	0.017%
16	12.234	1551	1555	1562	rBV3	15050	24925	0.63%	0.057%
17	13.475	1760	1766	1772	rBV3	15064	21349	0.54%	0.049%
18	13.898	1831	1838	1844	rBV	1432508	1958092	49.78%	4.471%
19	14.181	1879	1886	1895	rBV	1805388	2725938	69.30%	6.224%
20	14.493	1932	1939	1947	rBV	1327406	1882174	47.85%	4.298%
21	14.669	1961	1969	1987	rBV	632552	926061	23.54%	2.114%
22	14.910	2004	2010	2012	rBV4	3476	5416	0.14%	0.012%
23	15.487	2101	2108	2115	rBV	2261815	3188724	81.06%	7.281%
24	15.592	2120	2126	2138	rBV	361048	502520	12.78%	1.147%
25	15.728	2145	2149	2154	rVB4	7231	10311	0.26%	0.024%
26	17.022	2366	2369	2373	rVB2	4447	5876	0.15%	0.013%
27	17.239	2400	2406	2416	rVB	1450683	1959621	49.82%	4.474%
28	17.339	2416	2423	2434	rBV	2441160	3325975	84.55%	7.594%
29	17.598	2461	2467	2468	rBV5	2836	5161	0.13%	0.012%
30	18.028	2535	2540	2543	rBV5	2680	4651	0.12%	0.011%
31	18.145	2558	2560	2564	rVB5	3619	4380	0.11%	0.010%
32	19.198	2735	2739	2743	rBV2	21925	30281	0.77%	0.069%
33	19.263	2746	2750	2755	rBV	20945	28899	0.73%	0.066%
34	19.345	2761	2764	2767	rBV2	21105	23933	0.61%	0.055%
35	19.475	2782	2786	2792	rBV	41261	57349	1.46%	0.131%
36	19.581	2800	2804	2807	rBV	52784	68046	1.73%	0.155%

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037730.D
Acq On : 16 Sep 2025 13:29
Operator : RC/JU
Sample : PB169524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK524

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Title : SVOA CALIBRATION

37	19.628	2807	2812	2820	rVV	2719000	3634289	92.39%	8.298%
38	19.698	2822	2824	2828	rVB5	9980	10100	0.26%	0.023%
39	20.422	2945	2947	2950	rBV3	10565	7762	0.20%	0.018%
40	20.628	2978	2982	2986	rBV4	32593	42194	1.07%	0.096%
41	21.492	3122	3129	3137	rBV	1409162	2158005	54.86%	4.927%
42	24.369	3608	3618	3633	rBV2	1573502	3933550	100.00%	8.981%
43	24.574	3644	3653	3666	rBV	945817	2340020	59.49%	5.343%




Sum of corrected areas: 43796894

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037730.D
Acq On : 16 Sep 2025 13:29
Operator : RC/JU
Sample : PB169524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

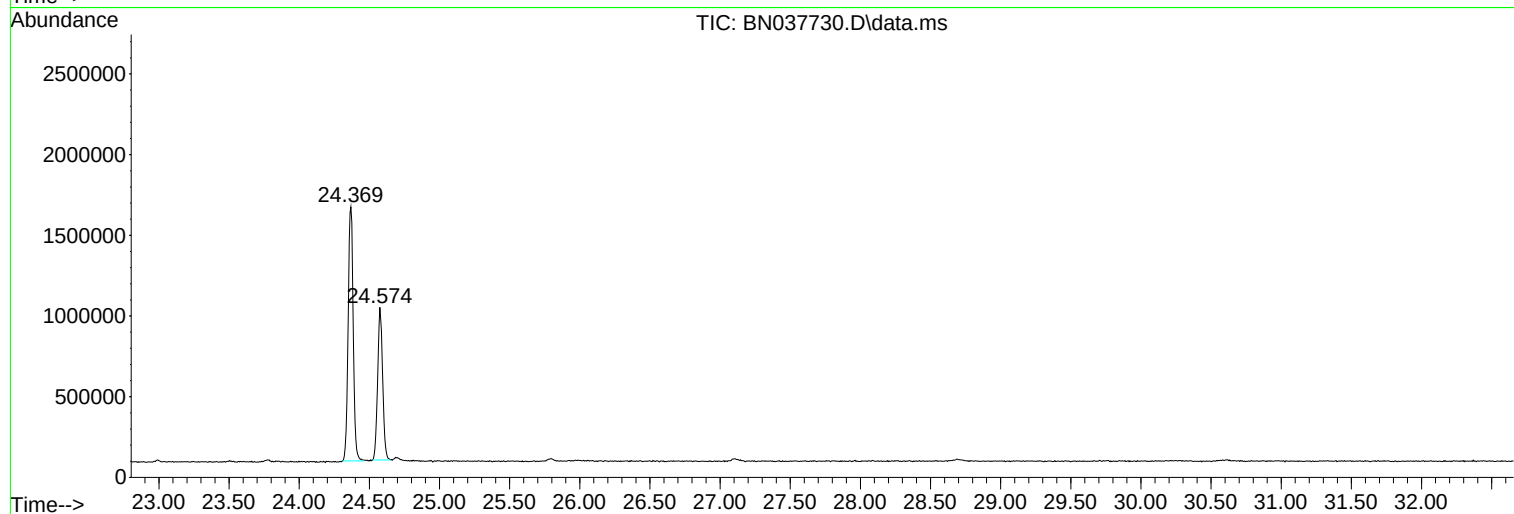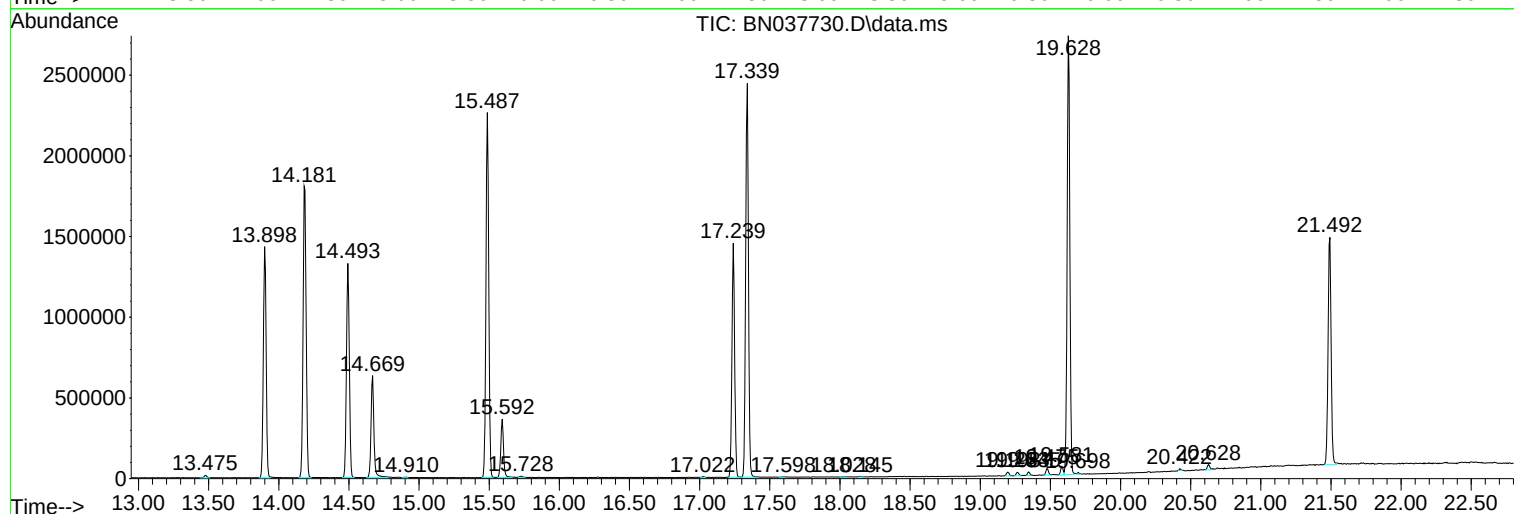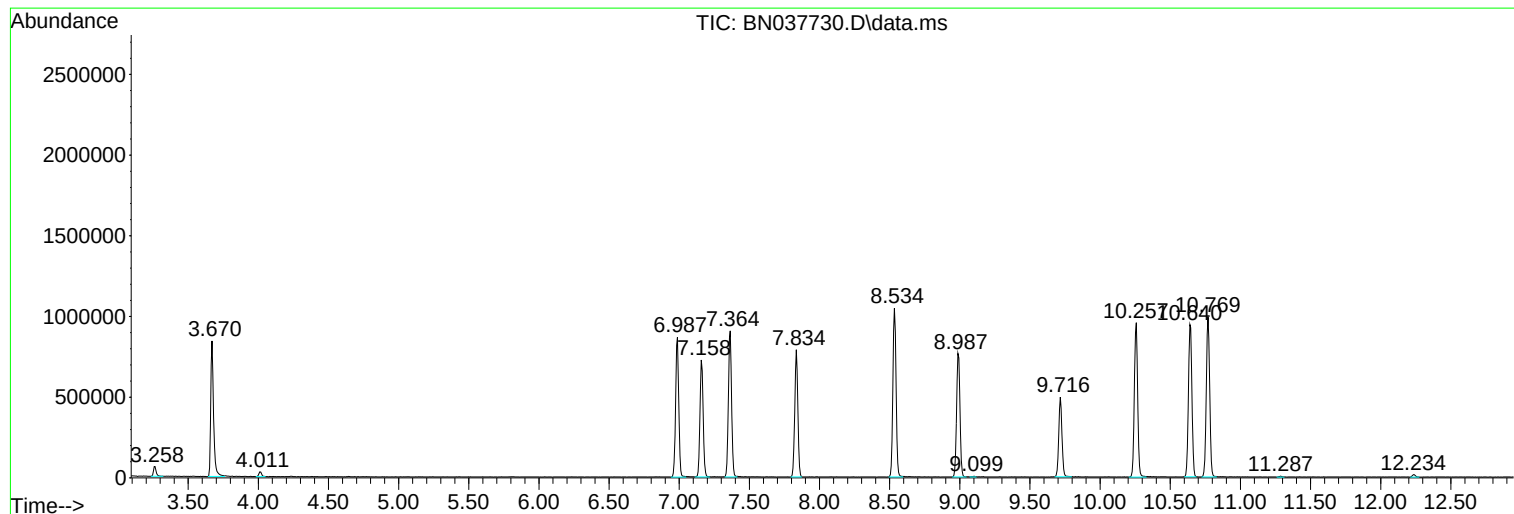

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037730.D
Acq On : 16 Sep 2025 13:29
Operator : RC/JU
Sample : PB169524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037730.D
Acq On : 16 Sep 2025 13:29
Operator : RC/JU
Sample : PB169524BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK524

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------