

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
 Data File : BN037731.D
 Acq On : 16 Sep 2025 14:09
 Operator : RC/JU
 Sample : PB169690BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK690

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BN037731.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	40	rVB	64064	88621	2.07%	0.210%
2	3.670	95	99	119	rBV	920191	1246291	29.13%	2.953%
3	4.011	151	157	162	rBV2	10995	16642	0.39%	0.039%
4	6.987	655	663	675	rBV	898635	1374888	32.14%	3.258%
5	7.158	681	692	703	rBV	719009	1116521	26.10%	2.645%
6	7.364	720	727	740	rBV	930669	1453476	33.97%	3.444%
7	7.834	800	807	814	rBV	597469	925163	21.63%	2.192%
8	8.534	919	926	937	rBV	1060615	1667271	38.97%	3.950%
9	8.858	977	981	986	rVB5	5260	7797	0.18%	0.018%
10	8.987	996	1003	1014	rBV	792802	1289067	30.13%	3.054%
11	9.716	1120	1127	1136	rBV	514652	810047	18.93%	1.919%
12	10.258	1211	1219	1230	rBV	967787	1579661	36.92%	3.743%
13	10.640	1277	1284	1296	rVB	741023	1212246	28.34%	2.872%
14	10.769	1298	1306	1322	rVV	1021247	1694020	39.60%	4.014%
15	12.234	1549	1555	1561	rBV	15202	25023	0.58%	0.059%
16	13.899	1832	1838	1845	rBV	1469413	1966431	45.96%	4.659%
17	14.187	1880	1887	1897	rBV	1859305	2735610	63.94%	6.482%
18	14.493	1933	1939	1947	rBV	1012708	1433328	33.50%	3.396%
19	14.669	1962	1969	1987	rBV	664003	967056	22.60%	2.291%
20	15.487	2098	2108	2115	rBV	2318760	3229130	75.48%	7.651%
21	15.593	2120	2126	2137	rBV	371841	514337	12.02%	1.219%
22	15.728	2144	2149	2154	rVB5	9566	14621	0.34%	0.035%
23	17.028	2366	2370	2375	rBV6	4376	6683	0.16%	0.016%
24	17.240	2399	2406	2414	rBV	1078547	1527443	35.70%	3.619%
25	17.340	2416	2423	2437	rVB	2375069	3375994	78.91%	7.999%
26	17.604	2464	2468	2473	rBV5	2796	4680	0.11%	0.011%
27	19.192	2734	2738	2743	rVB3	22093	31810	0.74%	0.075%
28	19.263	2746	2750	2755	rVB2	24762	32050	0.75%	0.076%
29	19.475	2782	2786	2792	rBV	66342	92996	2.17%	0.220%
30	19.628	2806	2812	2822	rBV	2849126	3780511	88.37%	8.958%
31	21.486	3122	3128	3137	rBV2	1184943	1759642	41.13%	4.169%
32	24.363	3608	3617	3631	rBV	1734619	4278196	100.00%	10.137%
33	24.574	3644	3653	3665	rVB	785150	1947428	45.52%	4.614%




Sum of corrected areas: 42204680

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037731.D
Acq On : 16 Sep 2025 14:09
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

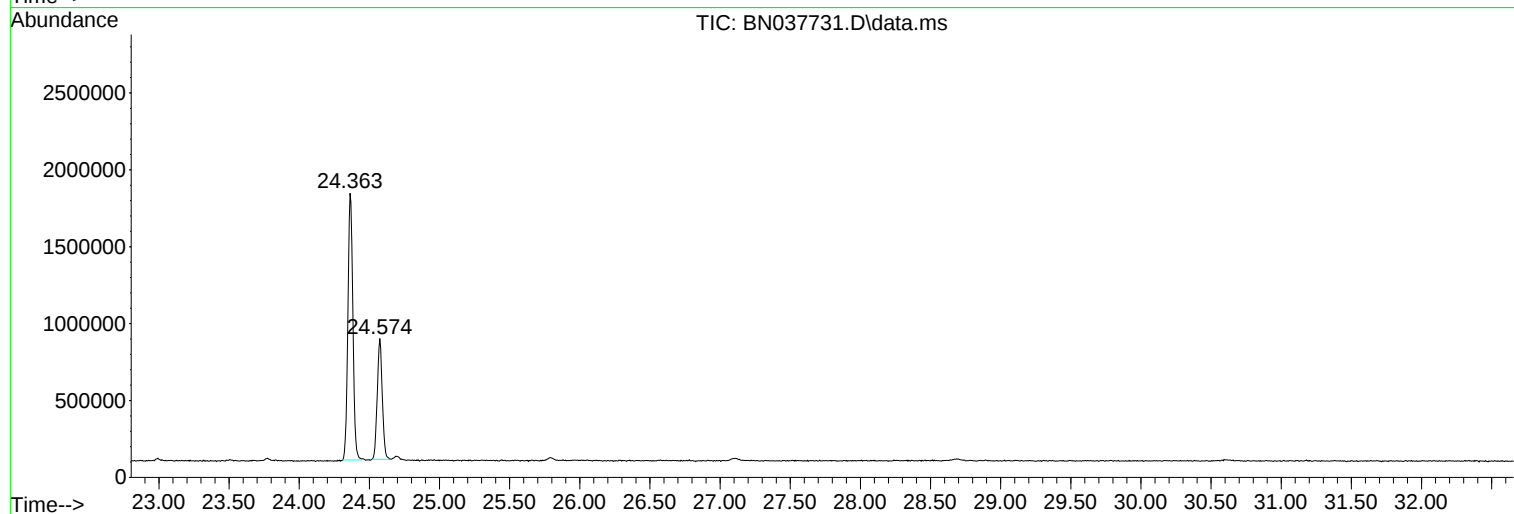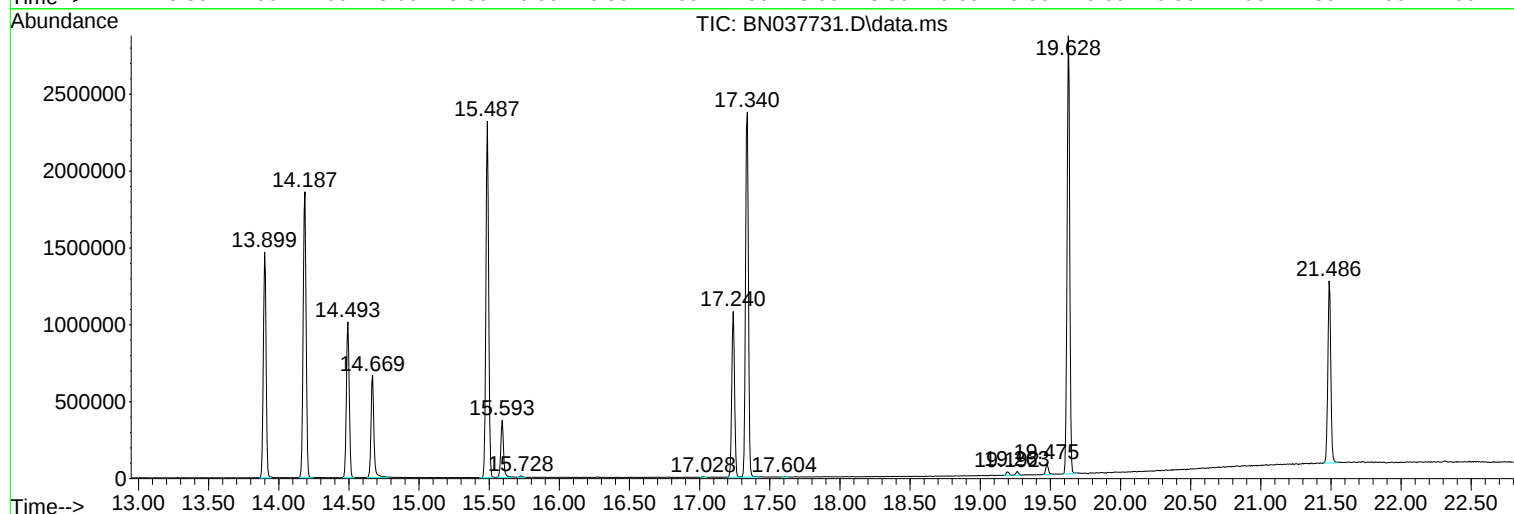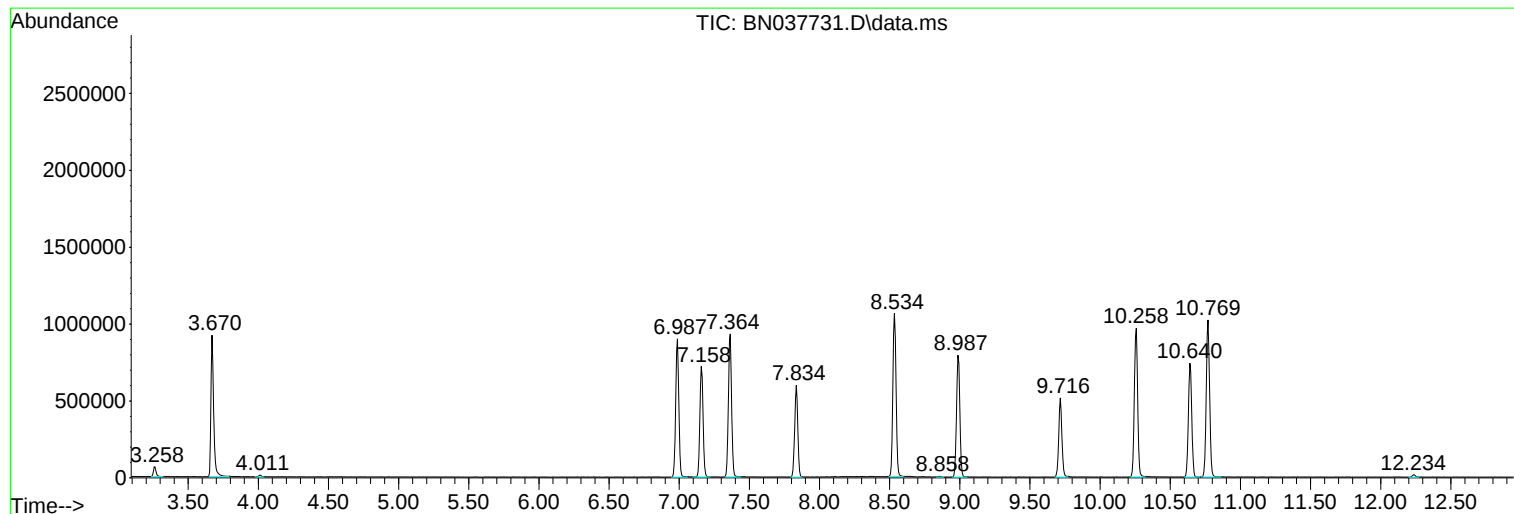

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037731.D
Acq On : 16 Sep 2025 14:09
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091625\
Data File : BN037731.D
Acq On : 16 Sep 2025 14:09
Operator : RC/JU
Sample : PB169690BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK690

Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-BN091225.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc