


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091720\
 Data File : BN011818.D
 Acq On : 17 Sep 2020 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 18 10:47:35 2020

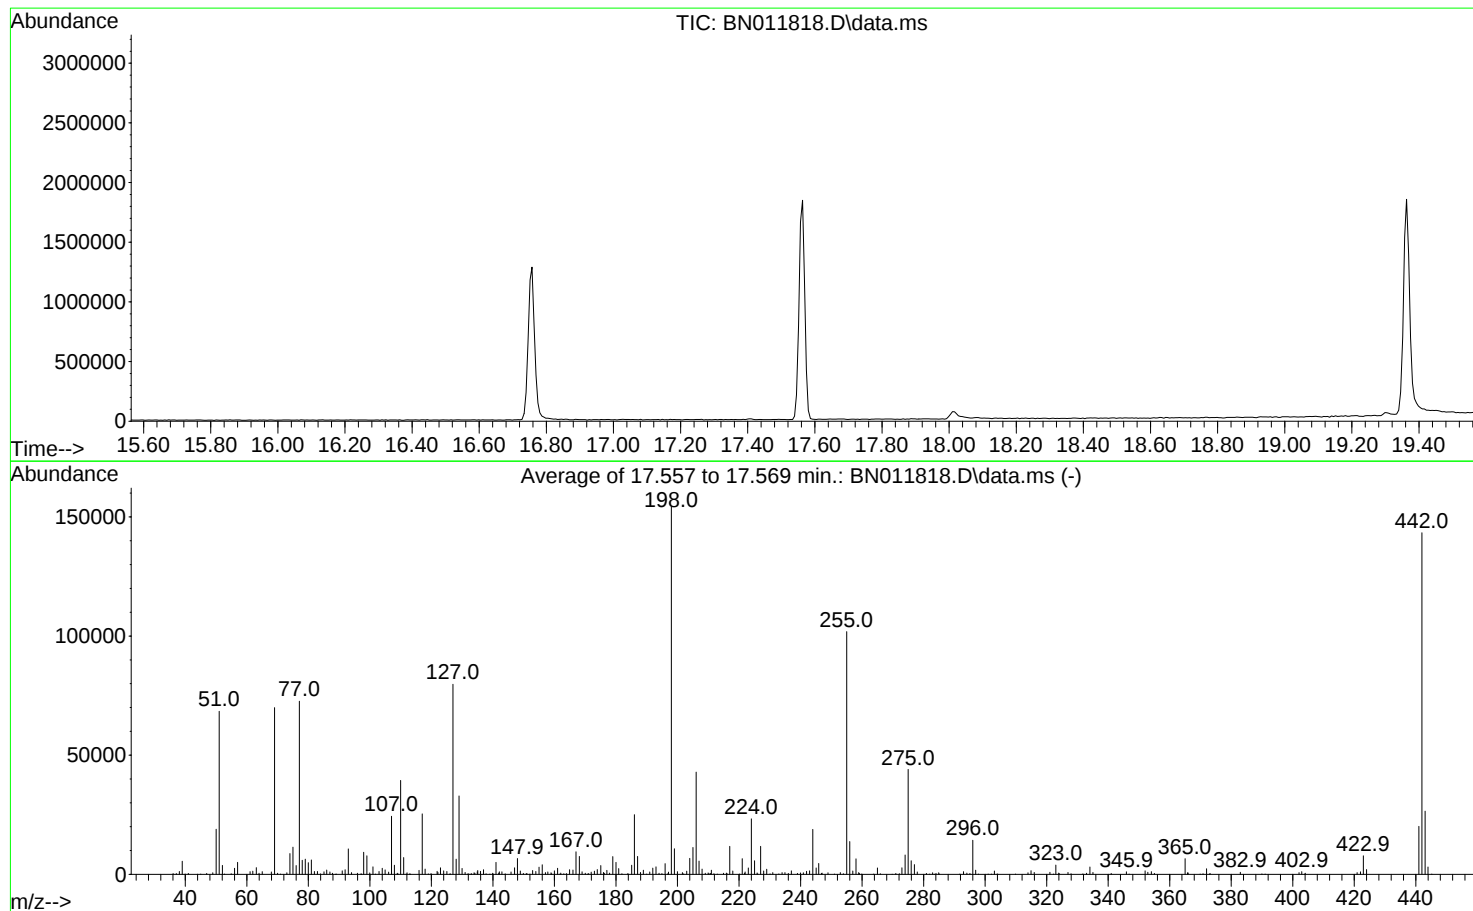

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.3	68437	PASS
68	69	0.00	2	1.5	1017	PASS
69	198	0.00	100	45.3	69941	PASS
70	69	0.00	2	0.7	460	PASS
127	198	10	80	51.7	79752	PASS
197	198	0.00	2	0.6	927	PASS
198	198	100	100	100.0	154357	PASS
199	198	5	9	6.9	10715	PASS
275	198	10	60	28.5	44019	PASS
365	198	1	100	4.3	6594	PASS
441	198	0.01	100	13.0	20143	PASS
442	198	50	100	92.9	143379	PASS
443	442	15	24	18.5	26544	PASS