

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016300.D
 Acq On : 17 Sep 2021 16:12
 Operator : CG/JU
 Sample : SSTDIC0.1
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDIC0.1

Quant Time: Sep 17 18:07:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 17:56:40 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	20676	0.400	ng	0.00
7) Naphthalene-d8	10.457	136	96588	0.400	ng	# 0.00
13) Acenaphthene-d10	14.307	164	55322	0.400	ng	0.00
19) Phenanthrene-d10	17.066	188	103794	0.400	ng	# 0.00
29) Chrysene-d12	21.259	240	102667	0.400	ng	# 0.00
35) Perylene-d12	23.522	264	101998	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.300	112	5447	0.103	ng	0.00
5) Phenol-d6	6.868	99	6629	0.100	ng	0.00
8) Nitrobenzene-d5	8.835	82	5797	0.075	ng	0.00
11) 2-Methylnaphthalene-d10	12.051	152	15189	0.101	ng	0.00
14) 2,4,6-Tribromophenol	15.804	330	1399	0.062	ng	0.00
15) 2-Fluorobiphenyl	12.936	172	22289	0.103	ng	0.00
27) Fluoranthene-d10	19.102	212	29886	0.098	ng	0.00
31) Terphenyl-d14	19.713	244	27166	0.105	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.299	88	733	0.100	ng	# 1
3) n-Nitrosodimethylamine	3.659	42	1476	0.097	ng	# 85
6) bis(2-Chloroethyl)ether	7.135	93	5751	0.106	ng	94
9) Naphthalene	10.508	128	26925	0.104	ng	# 93
10) Hexachlorobutadiene	10.799	225	4880	0.093	ng	# 99
12) 2-Methylnaphthalene	12.127	142	17756	0.102	ng	# 96
16) Acenaphthylene	14.027	152	25187	0.102	ng	99
17) Acenaphthene	14.370	154	15653	0.097	ng	100
18) Fluorene	15.360	166	19464	0.098	ng	99
20) 4,6-Dinitro-2-methylph...	15.448	198	174	0.030	ng	# 10
21) 4-Bromophenyl-phenylether	16.263	248	6007	0.108	ng	# 84
22) Hexachlorobenzene	16.372	284	5694	0.086	ng	# 91
23) Atrazine	16.543	200	5574	0.109	ng	# 96
24) Pentachlorophenol	16.713	266	1518	0.129	ng	98
25) Phenanthrene	17.102	178	29235	0.097	ng	97
26) Anthracene	17.188	178	28261	0.102	ng	99
28) Fluoranthene	19.132	202	34032	0.096	ng	99
30) Pyrene	19.495	202	35169	0.101	ng	99
32) Benzo(a)anthracene	21.248	228	34431	0.108	ng	99
33) Chrysene	21.302	228	33513	0.106	ng	99
34) Bis(2-ethylhexyl)phtha...	21.206	149	19060	0.097	ng	99
36) Indeno(1,2,3-cd)pyrene	25.819	276	32376	0.191	ng	99
37) Benzo(b)fluoranthene	22.841	252	34910	0.089	ng	# 88
38) Benzo(k)fluoranthene	22.889	252	32853	0.094	ng	# 82
39) Benzo(a)pyrene	23.423	252	30839	0.105	ng	# 86
40) Dibenzo(a,h)anthracene	25.846	278	27614	0.213	ng	# 92
41) Benzo(g,h,i)perylene	26.524	276	27158	0.193	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016300.D
Acq On : 17 Sep 2021 16:12
Operator : CG/JU
Sample : SSTDICC0.1
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1

Quant Time: Sep 17 18:07:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 17:56:40 2021
Response via : Initial Calibration




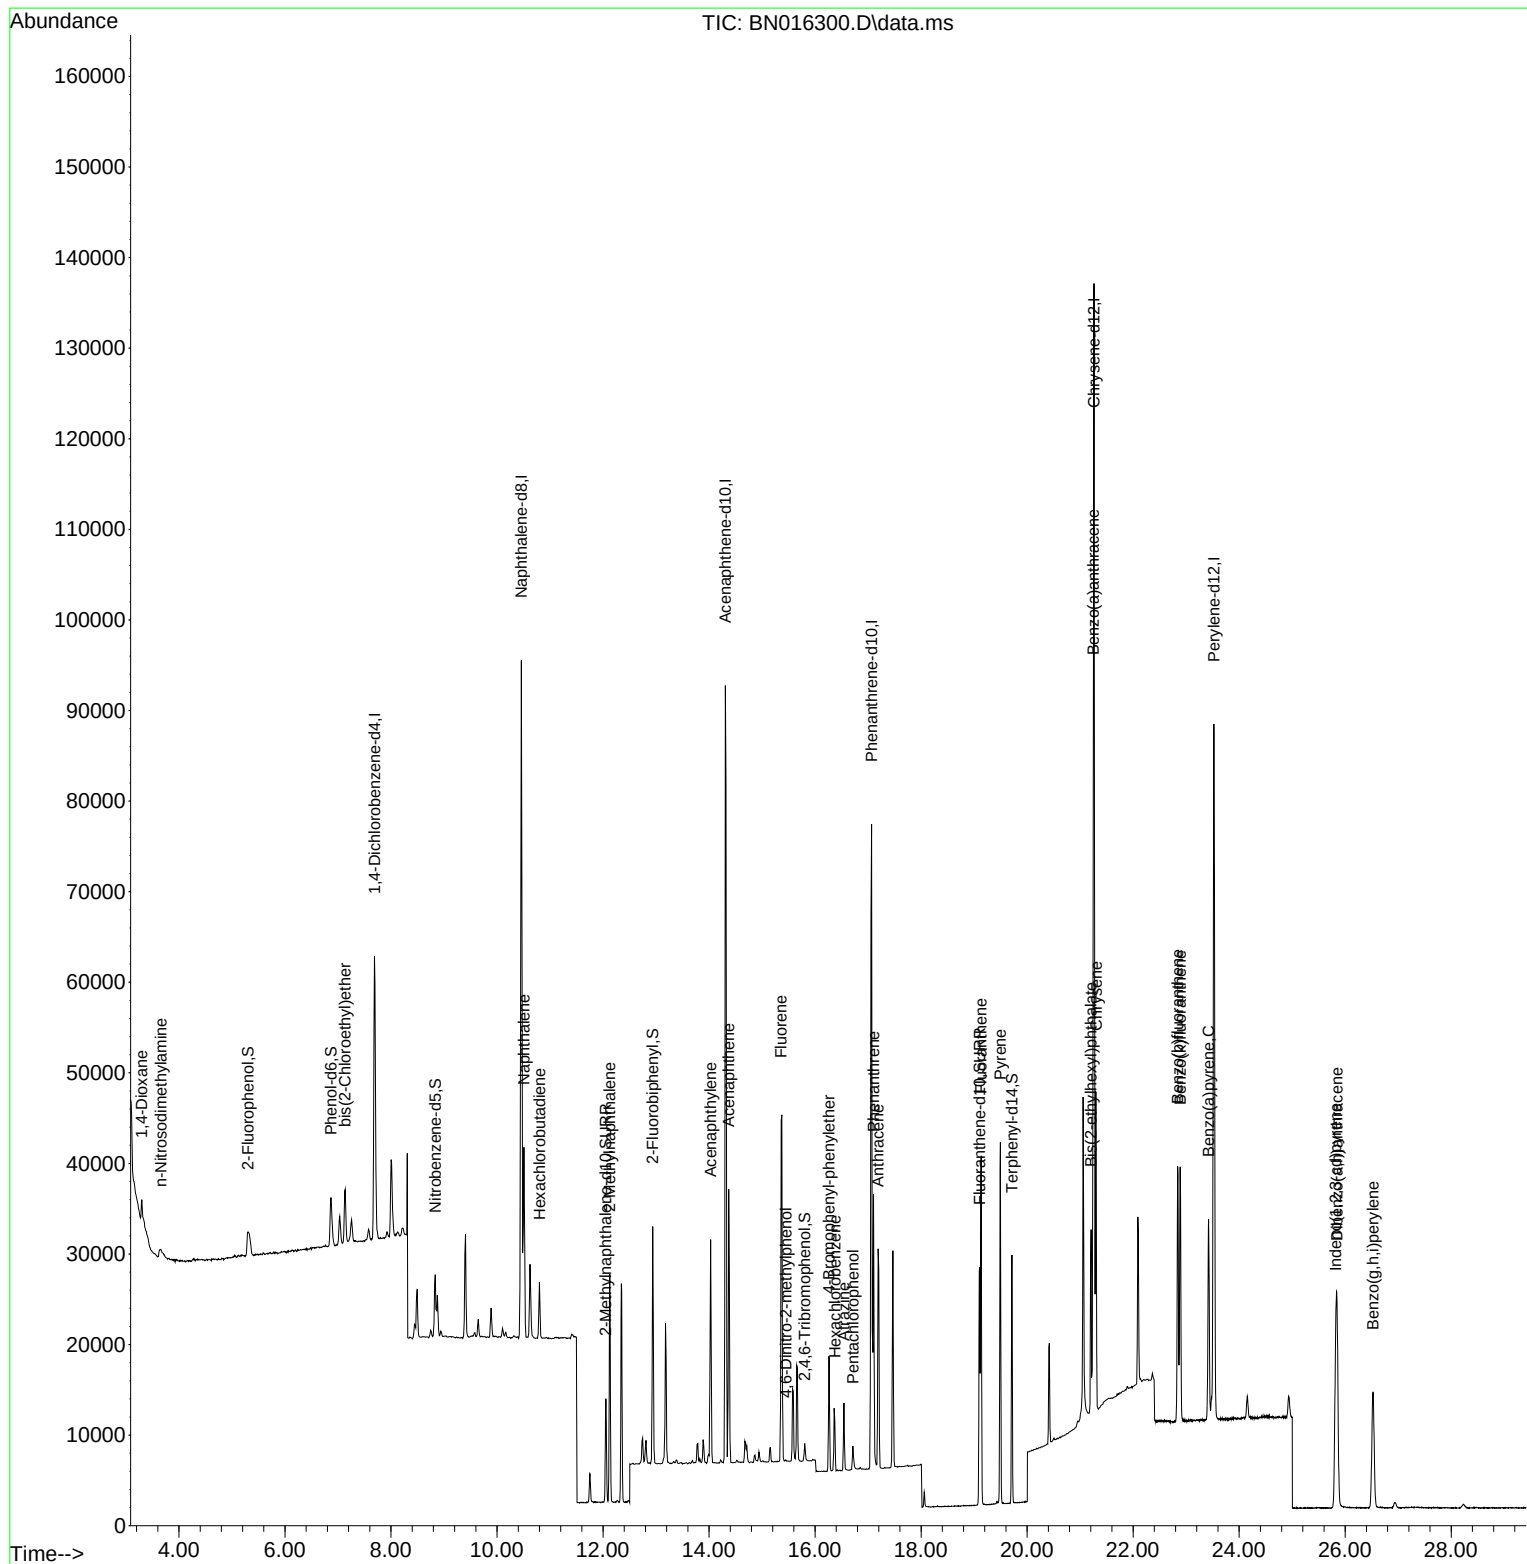




#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.688 min Scan# 500
 Delta R.T. 0.000 min
 Lab File: BN016300.D
 Acq: 17 Sep 2021 16:12




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:152 Resp: 20676
 Ion Ratio Lower Upper
 152 100
 150 151.5 125.6 188.4
 115 60.8 50.2 75.2

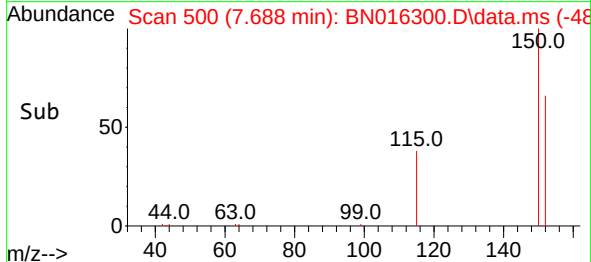

#2
 1,4-Dioxane
 Concen: 0.100 ng
 RT: 3.299 min Scan# 24
 Delta R.T. -0.009 min
 Lab File: BN016300.D
 Acq: 17 Sep 2021 16:12

Tgt Ion: 88 Resp: 733
 Ion Ratio Lower Upper
 88 100
 43 320.2 20.3 30.5#
 58 90.9 69.9 104.9


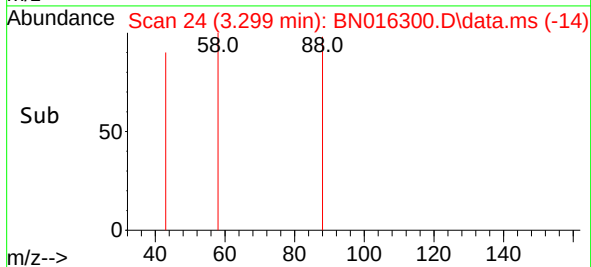

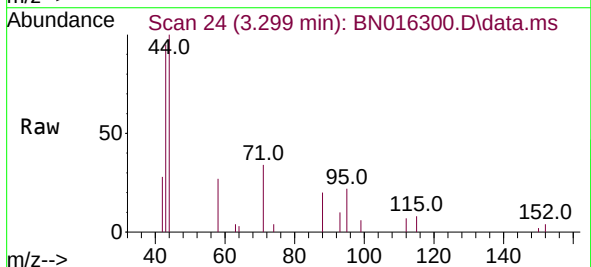




#3
n-Nitrosodimethylamine
Concen: 0.097 ng
RT: 3.659 min Scan# 63
Delta R.T. 0.037 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion: 42 Resp: 1476
Ion Ratio Lower Upper
42 100
74 123.3 113.6 170.4
44 19.0 0.0 0.0#

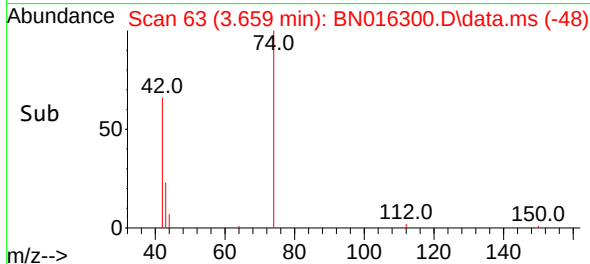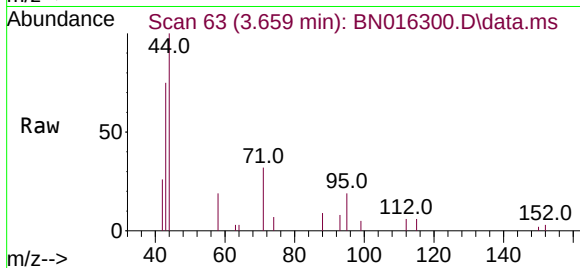

#4
2-Fluorophenol
Concen: 0.103 ng
RT: 5.300 min Scan# 241
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion: 112 Resp: 5447
Ion Ratio Lower Upper
112 100
64 62.2 47.3 70.9
63 32.0 23.4 35.0


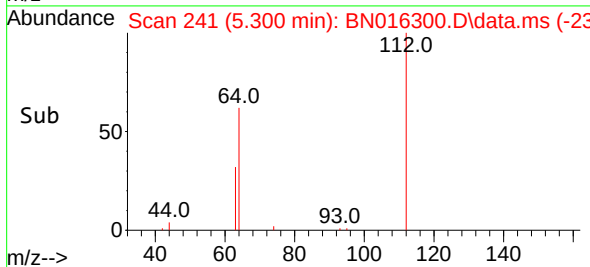

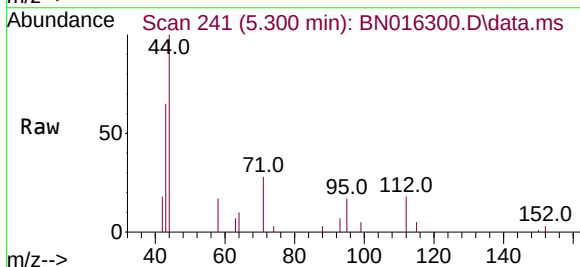




#5
Phenol-d6
Concen: 0.100 ng
RT: 6.868 min Scan# 411
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion: 99 Resp: 6629
Ion Ratio Lower Upper
99 100
42 24.8 14.0 21.0#
71 31.8 23.8 35.6

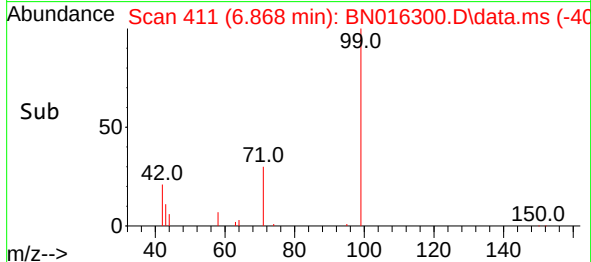

#6
bis(2-Chloroethyl)ether
Concen: 0.106 ng
RT: 7.135 min Scan# 440
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion: 93 Resp: 5751
Ion Ratio Lower Upper
93 100
63 86.6 63.4 95.0
95 34.3 26.8 40.2


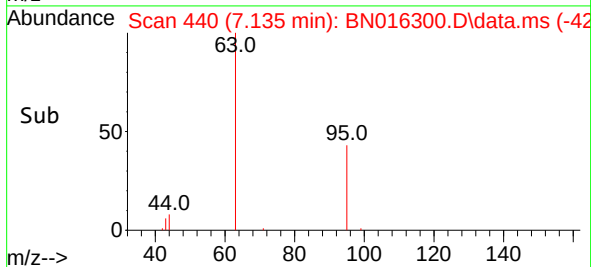

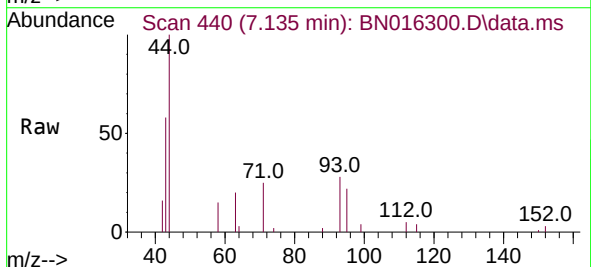




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.457 min Scan# 737
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:	136	Resp:	96588
Ion Ratio	Lower	Upper	
136	100		
137	11.7	8.8	13.2
54	11.5	5.3	7.9#
68	8.8	3.9	5.9#

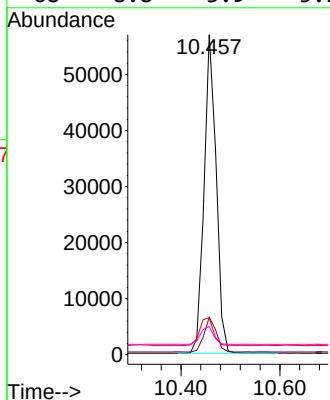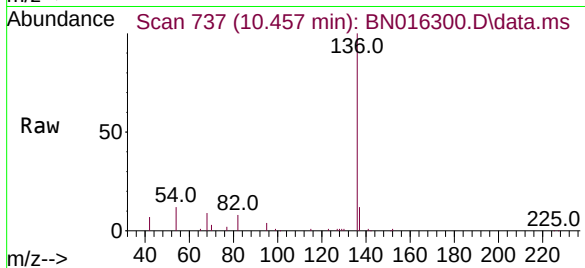

#8
Nitrobenzene-d5
Concen: 0.075 ng
RT: 8.835 min Scan# 609
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:	82	Resp:	5797
Ion Ratio	Lower	Upper	
82	100		
128	32.9	31.7	47.5
54	60.2	46.4	69.6

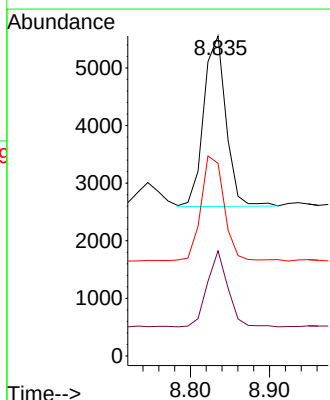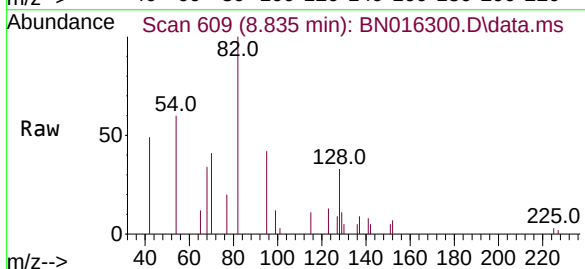



#9

Naphthalene

Concen: 0.104 ng

RT: 10.508 min Scan# 741

Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12





Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1

Tgt Ion:	128	Resp:	26925
Ion	Ratio	Lower	Upper
128	100		
129	13.6	8.9	13.3#
127	15.2	10.1	15.1#

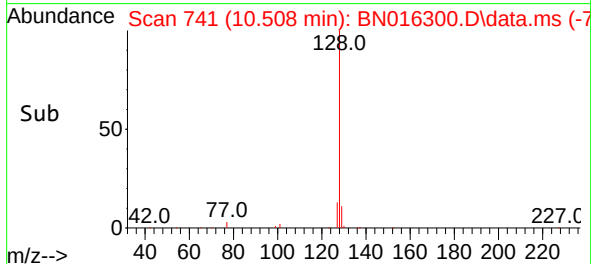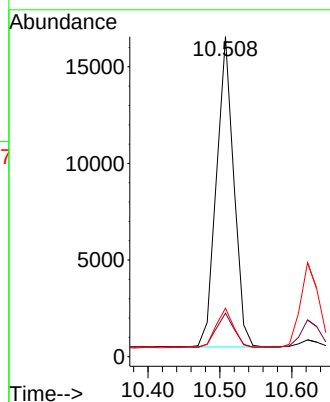

#10

Hexachlorobutadiene

Concen: 0.093 ng




RT: 10.799 min Scan# 764


Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12

Tgt Ion:	225	Resp:	4880
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	63.7	51.5	77.3



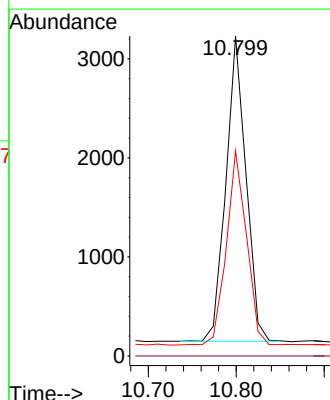





#11
2-Methylnaphthalene-d10
Concen: 0.101 ng
RT: 12.051 min Scan# 942
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:152 Resp: 15189
Ion Ratio Lower Upper
152 100
151 20.2 16.1 24.1

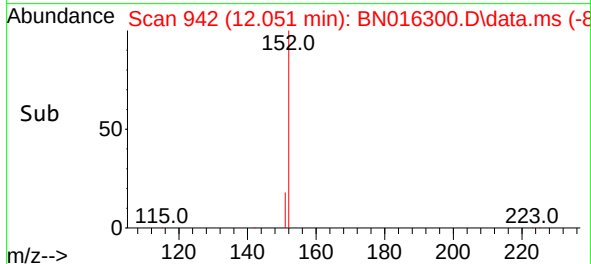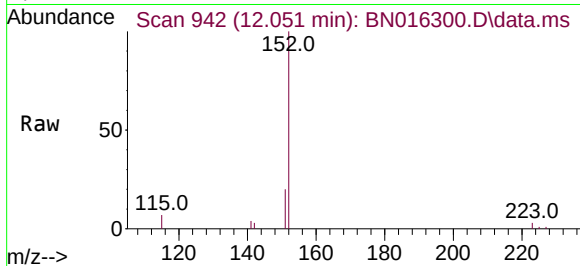

#12
2-Methylnaphthalene
Concen: 0.102 ng
RT: 12.127 min Scan# 959
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:142 Resp: 17756
Ion Ratio Lower Upper
142 100
141 88.7 69.8 104.8
115 36.8 24.4 36.6#


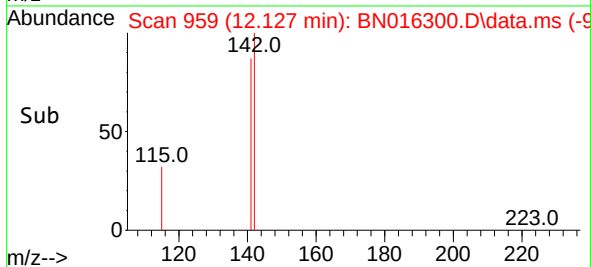

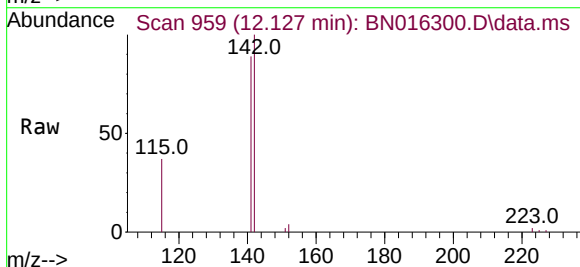


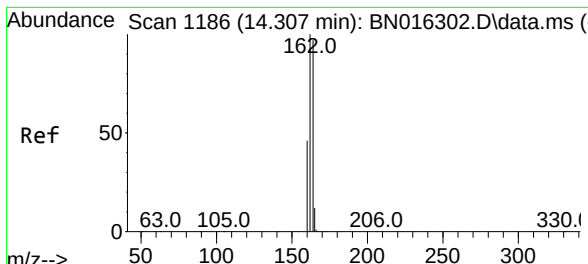

#13
 Acenaphthene-d10
 Concen: 0.400 ng
 RT: 14.307 min Scan# 1186
 Delta R.T. -0.000 min
 Lab File: BN016300.D
 Acq: 17 Sep 2021 16:12




Instrument :
 BNA_N
 ClientSampleId :
 SSTDICC0.1


Tgt Ion:	164	Resp:	55322
Ion Ratio	Lower	Upper	
164	100		
162	103.9	79.0	118.4
160	47.5	34.1	51.1

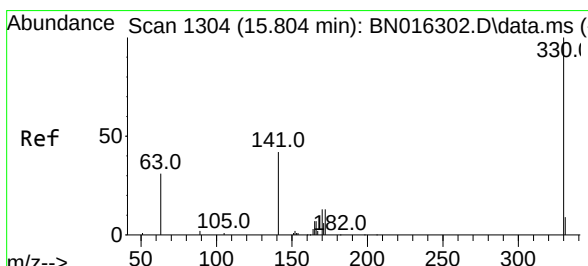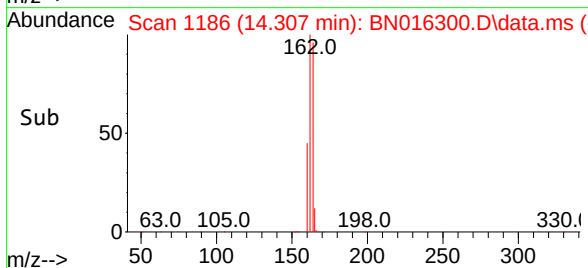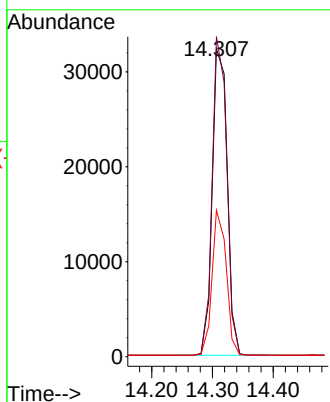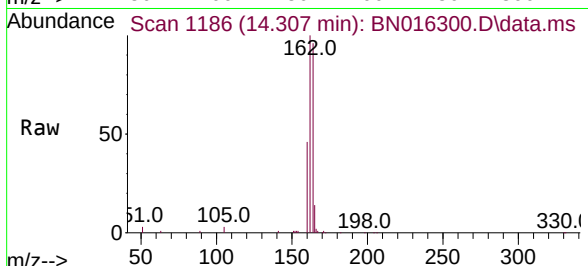

#14
 2,4,6-Tribromophenol
 Concen: 0.062 ng
 RT: 15.804 min Scan# 1304
 Delta R.T. -0.000 min
 Lab File: BN016300.D
 Acq: 17 Sep 2021 16:12

Tgt Ion:	330	Resp:	1399
Ion Ratio	Lower	Upper	
330	100		
332	0.0	0.0	0.0
141	50.2	25.0	37.4


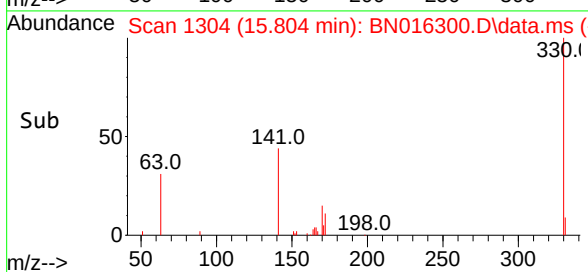
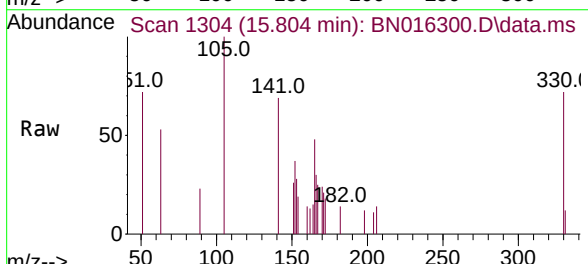
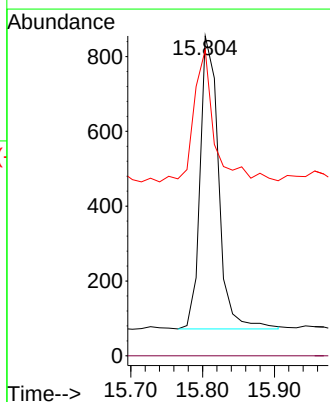




#15
2-Fluorobiphenyl
Concen: 0.103 ng
RT: 12.936 min Scan# 1078
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:172 Resp: 22289
Ion Ratio Lower Upper
172 100
171 35.8 27.8 41.6
170 24.3 18.2 27.2

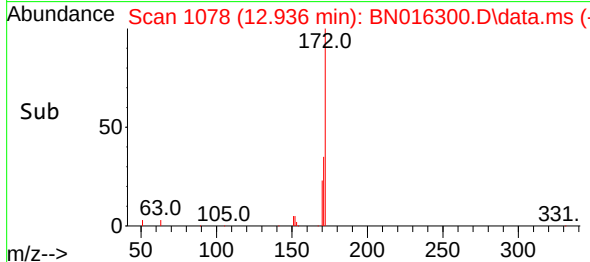

#16
Acenaphthylene
Concen: 0.102 ng
RT: 14.027 min Scan# 1164
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:152 Resp: 25187
Ion Ratio Lower Upper
152 100
151 19.6 15.2 22.8
153 13.1 10.5 15.7


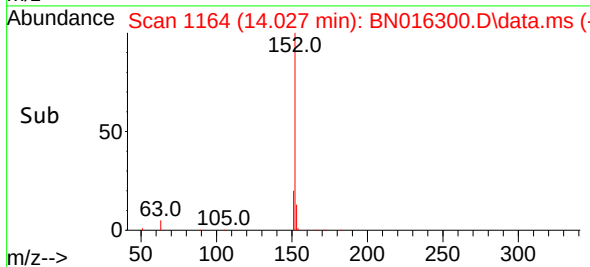

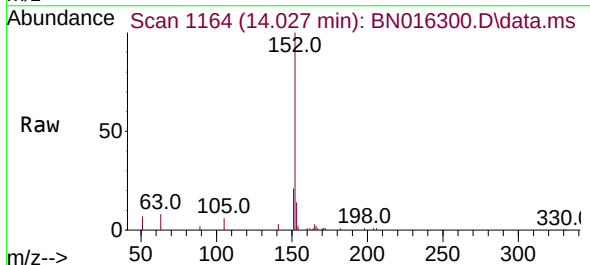




#17
Acenaphthene
Concen: 0.097 ng
RT: 14.370 min Scan# 1191
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:154 Resp: 15653
Ion Ratio Lower Upper
154 100
153 112.0 89.3 133.9
152 53.0 42.2 63.4



#18
Fluorene
Concen: 0.098 ng
RT: 15.360 min Scan# 1269
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:166 Resp: 19464
Ion Ratio Lower Upper
166 100
165 97.0 76.7 115.1
167 13.7 10.9 16.3


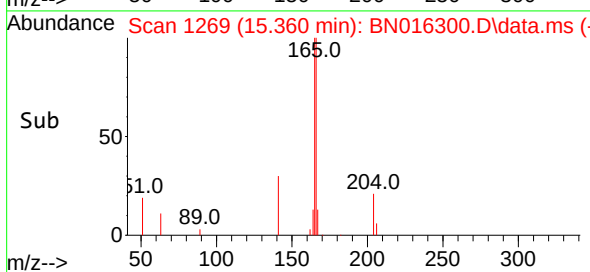




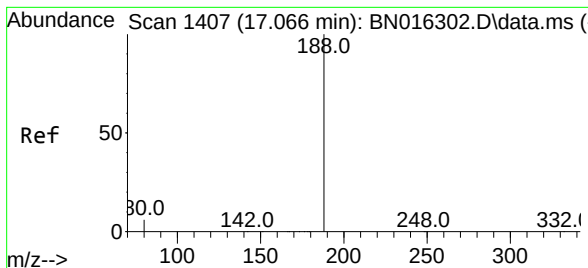

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.066 min Scan# 1407
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:188 Resp: 103794
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 7.0 7.0 10.6#

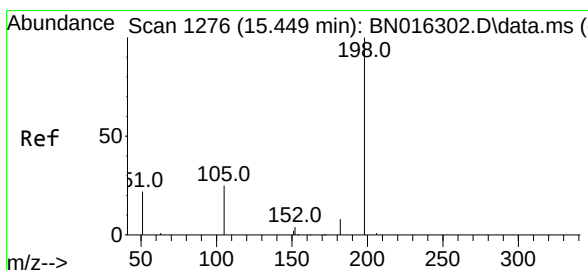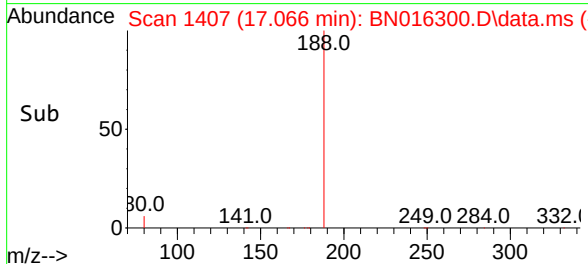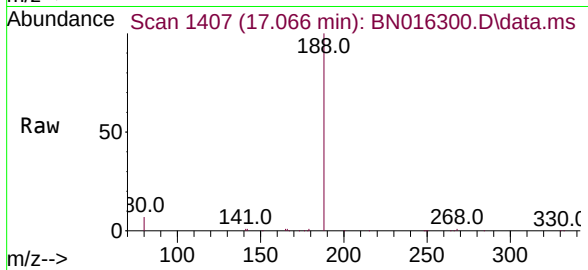

#20
4,6-Dinitro-2-methylphenol
Concen: 0.030 ng
RT: 15.448 min Scan# 1276
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:198 Resp: 174
Ion Ratio Lower Upper
198 100
182 84.4 26.6 39.8#
77 0.0 0.0 0.0


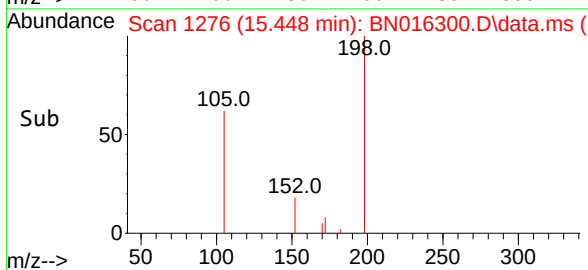

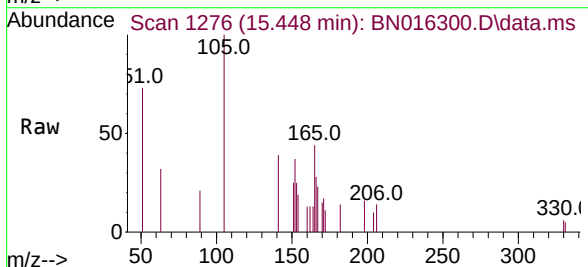


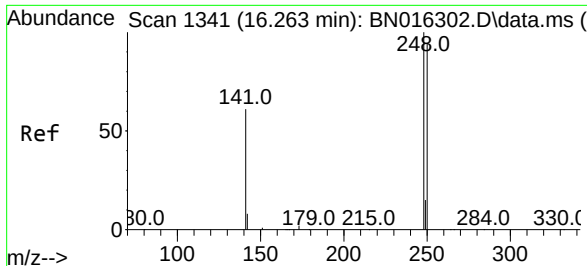

#21
4-Bromophenyl-phenylether
Concen: 0.108 ng
RT: 16.263 min Scan# 1341
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:248 Resp: 6007
Ion Ratio Lower Upper
248 100
250 95.1 80.5 120.7
141 69.1 34.8 52.2#

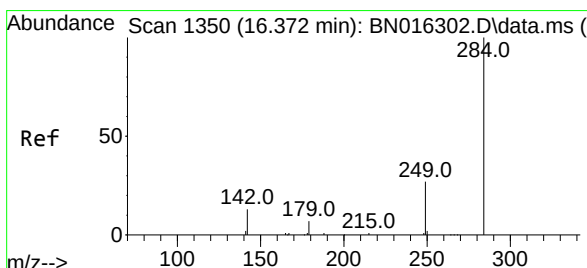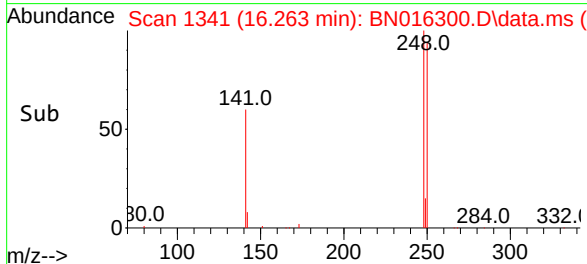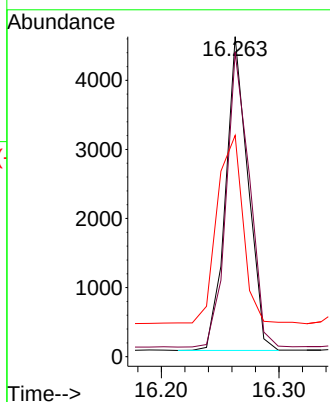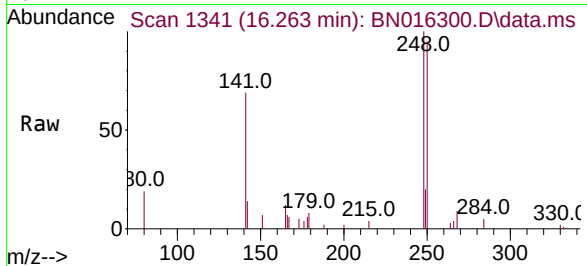

#22
Hexachlorobenzene
Concen: 0.086 ng
RT: 16.372 min Scan# 1350
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:284 Resp: 5694
Ion Ratio Lower Upper
284 100
142 36.9 22.6 34.0#
249 31.9 24.4 36.6

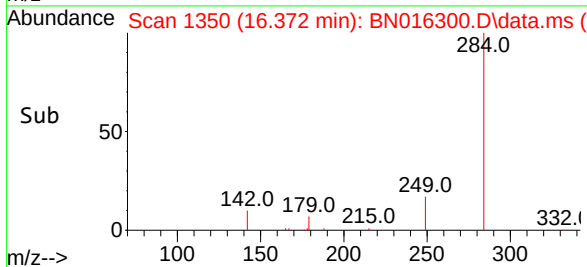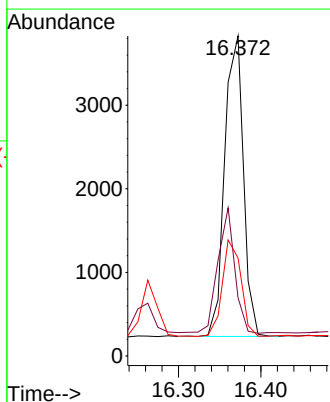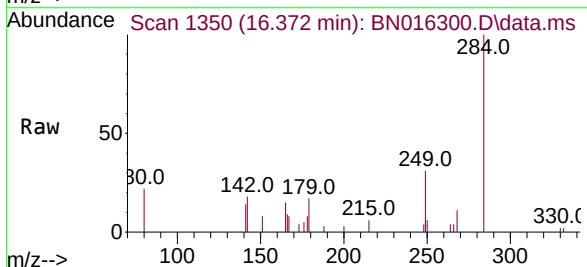



#23

Atrazine

Concen: 0.109 ng

RT: 16.543 min Scan# 1364

Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12





Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1

Tgt Ion:	200	Resp:	5574
Ion Ratio	Lower	Upper	
200	100		
173	28.6	18.7	28.1#
215	51.8	41.6	62.4

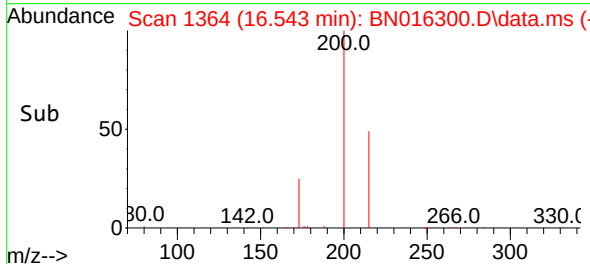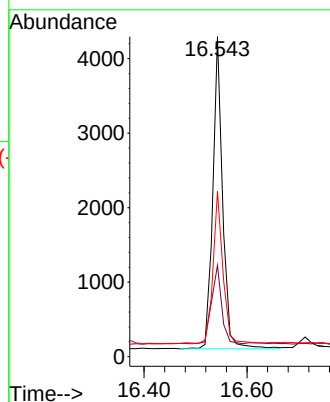

#24

Pentachlorophenol

Concen: 0.129 ng




RT: 16.713 min Scan# 1378


Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12

Tgt Ion:	266	Resp:	1518
Ion Ratio	Lower	Upper	
266	100		
264	61.0	50.6	75.8
268	67.3	52.6	79.0


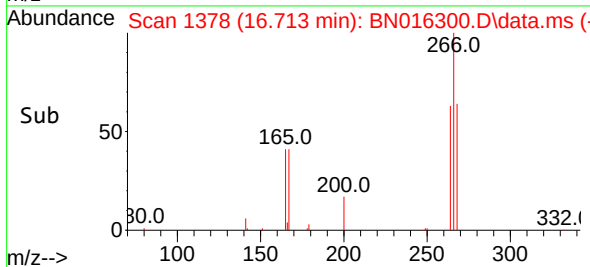
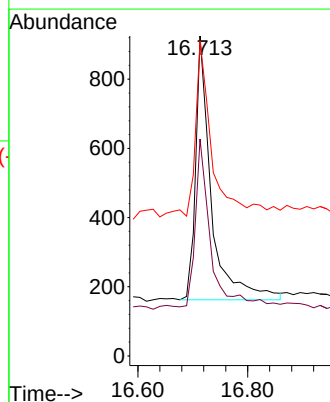
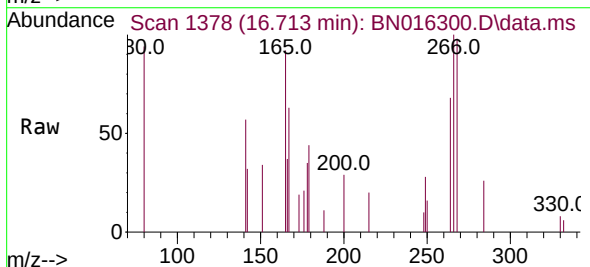




#25
Phenanthrene
Concen: 0.097 ng
RT: 17.102 min Scan# 1410
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:178 Resp: 29235
Ion Ratio Lower Upper
178 100
176 18.7 14.4 21.6
179 16.9 12.2 18.4

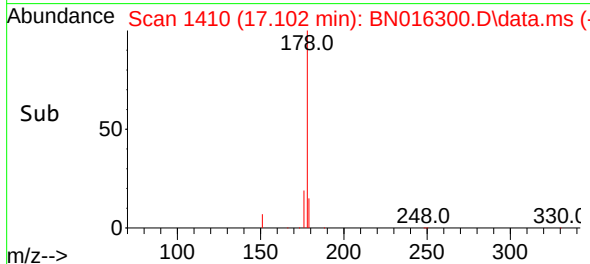

#26
Anthracene
Concen: 0.102 ng
RT: 17.188 min Scan# 1417
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:178 Resp: 28261
Ion Ratio Lower Upper
178 100
176 18.3 13.9 20.9
179 15.2 12.2 18.4


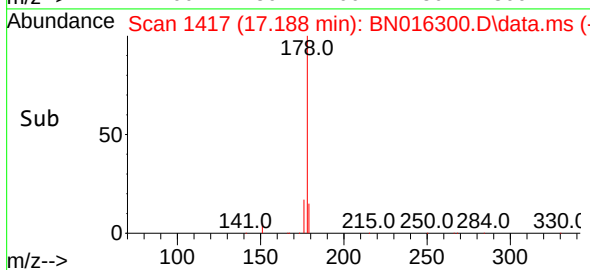

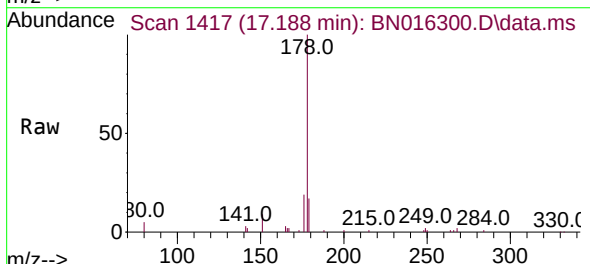




#27
Fluoranthene-d10
Concen: 0.098 ng
RT: 19.102 min Scan# 1704
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:212 Resp: 29886
Ion Ratio Lower Upper
212 100
106 11.8 9.8 14.6
104 6.6 5.4 8.2

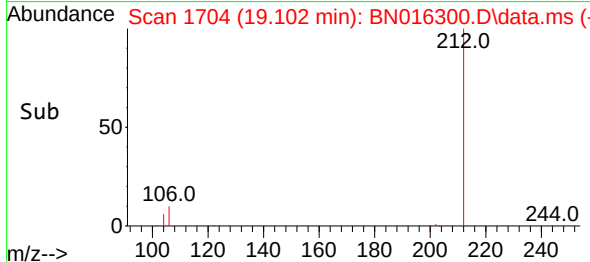

#28
Fluoranthene
Concen: 0.096 ng
RT: 19.132 min Scan# 1710
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:202 Resp: 34032
Ion Ratio Lower Upper
202 100
101 10.0 8.5 12.7
203 17.4 13.8 20.8

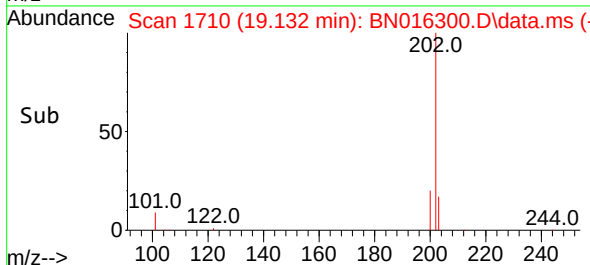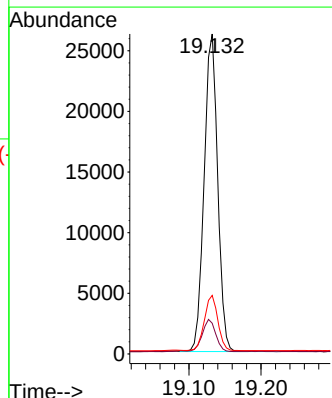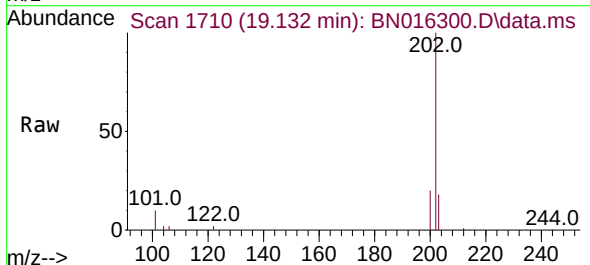

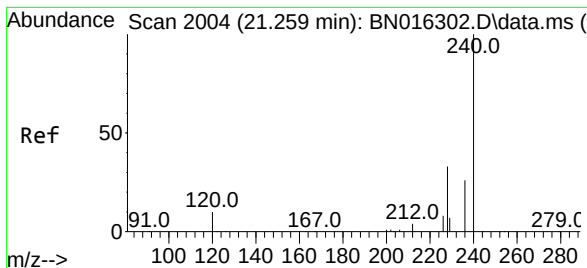

#29

Chrysene-d12

Concen: 0.400 ng

RT: 21.259 min Scan# 2004

Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12

Tgt Ion:240 Resp: 102667

Ion Ratio Lower Upper

240 100

120 10.0 5.3 7.9#





236 26.4 19.8 29.8

Instrument :

BNA_N

ClientSampleId :

SSTDIC0.1

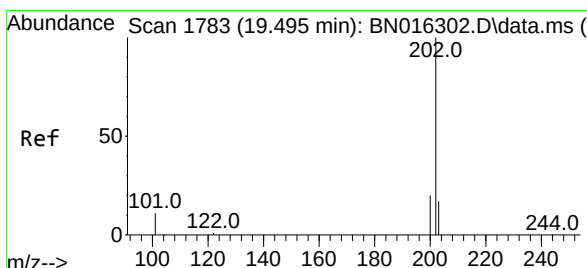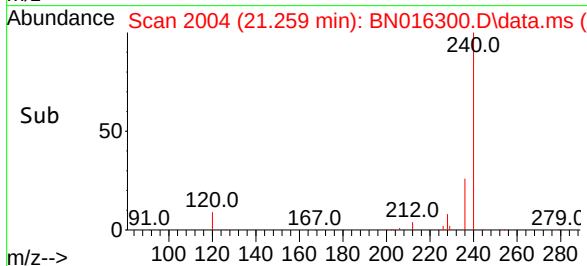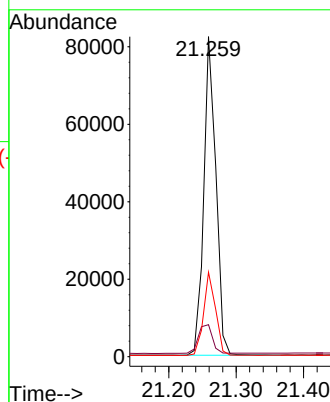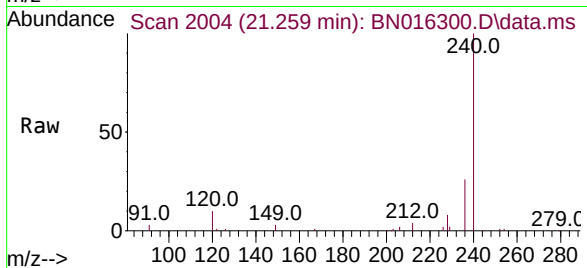

#30

Pyrene

Concen: 0.101 ng

RT: 19.495 min Scan# 1783

Delta R.T. -0.000 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12




Tgt Ion:202 Resp: 35169


Ion Ratio Lower Upper

202 100

200 20.5 15.8 23.6

203 17.7 13.9 20.9


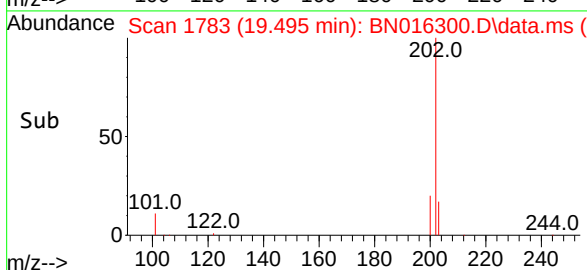
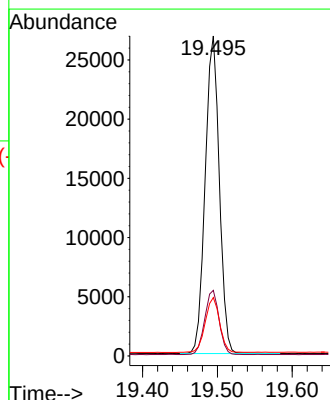
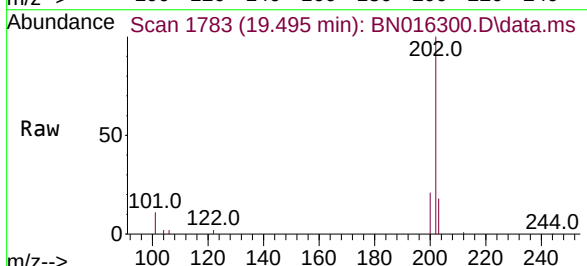




#31
Terphenyl-d14
Concen: 0.105 ng
RT: 19.713 min Scan# 1827
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:244 Resp: 27166
Ion Ratio Lower Upper
244 100
212 7.7 5.5 8.3
122 11.4 9.0 13.4

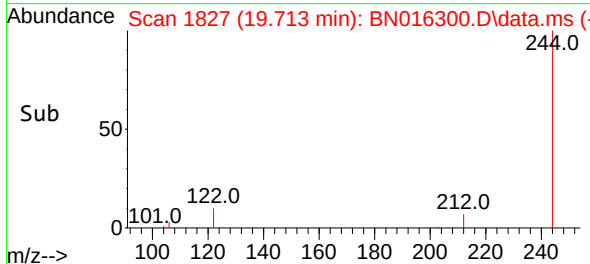

#32
Benzo(a)anthracene
Concen: 0.108 ng
RT: 21.248 min Scan# 2003
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:228 Resp: 34431
Ion Ratio Lower Upper
228 100
226 26.1 20.8 31.2
229 20.2 15.8 23.6




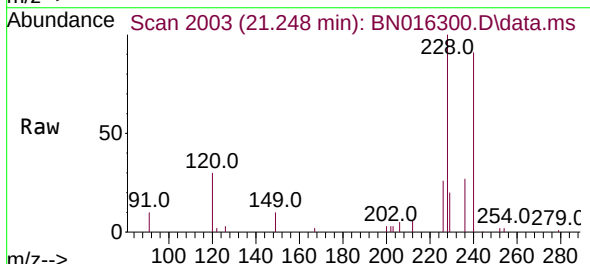




#33
Chrysene
Concen: 0.106 ng
RT: 21.302 min Scan# 2008
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:228	Resp:	33513
Ion Ratio	Lower	Upper
228	100	
226	28.8	23.0 34.4
229	20.4	15.6 23.4

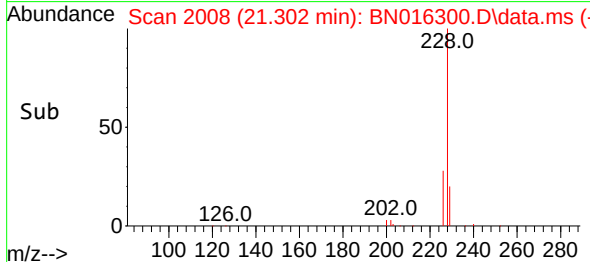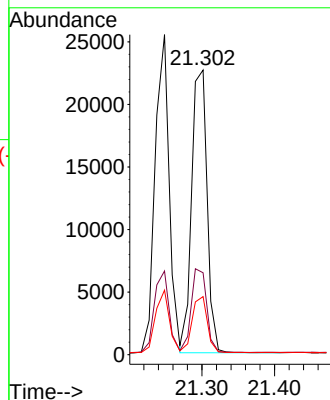

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.097 ng
RT: 21.206 min Scan# 1999
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:149	Resp:	19060
Ion Ratio	Lower	Upper
149	100	
167	29.0	23.4 35.0
279	5.4	3.9 5.9

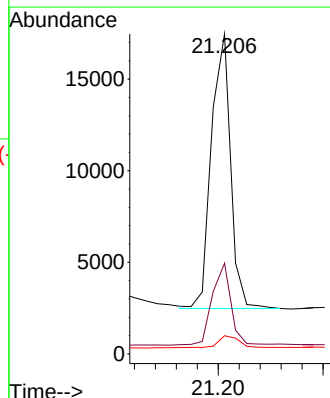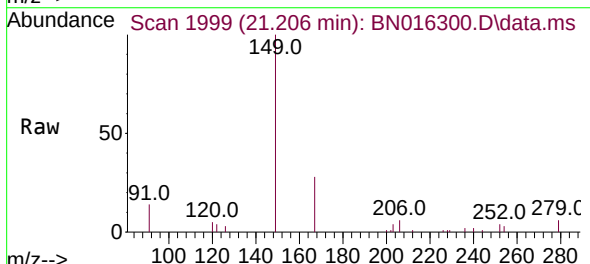



#35

Perylene-d12

Concen: 0.400 ng

RT: 23.522 min Scan# 2438

Delta R.T. -0.004 min

Lab File: BN016300.D

Acq: 17 Sep 2021 16:12

Instrument :





BNA_N

ClientSampleId :

SSTDIC0.1

Tgt Ion:264 Resp: 101998

Ion	Ratio	Lower	Upper
264	100		
260	24.4	18.9	28.3
265	34.1	23.7	35.5

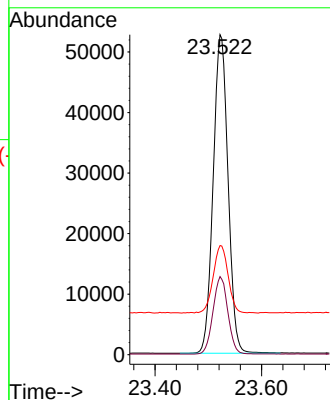

#36

Indeno(1,2,3-cd)pyrene

Concen: 0.191 ng

RT: 25.819 min Scan# 3109




Delta R.T. -0.004 min


Lab File: BN016300.D

Acq: 17 Sep 2021 16:12

Tgt Ion:276 Resp: 32376

Ion	Ratio	Lower	Upper
276	100		
138	24.8	19.3	28.9
277	25.2	20.2	30.2


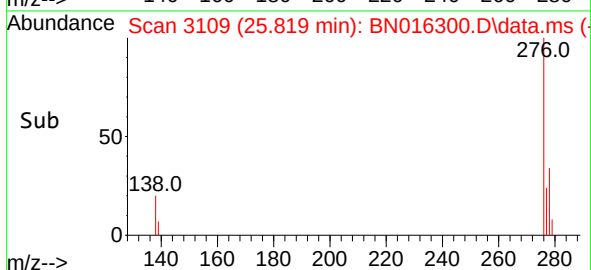
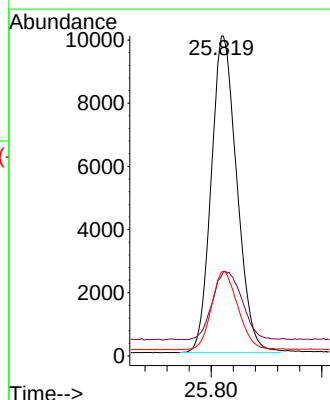





#37
Benzo(b)fluoranthene
Concen: 0.089 ng
RT: 22.841 min Scan# 2239
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1


Tgt Ion:252 Resp: 34910
Ion Ratio Lower Upper
252 100
253 27.5 18.2 27.2#
125 16.3 8.4 12.6#

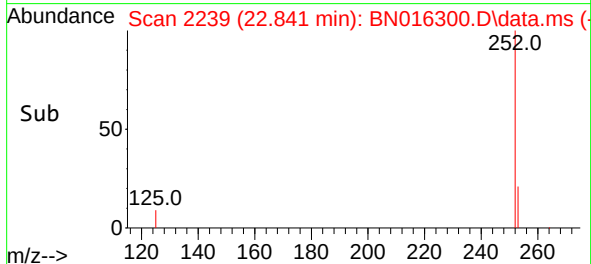

#38
Benzo(k)fluoranthene
Concen: 0.094 ng
RT: 22.889 min Scan# 2253
Delta R.T. 0.003 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:252 Resp: 32853
Ion Ratio Lower Upper
252 100
253 28.8 18.2 27.2#
125 21.2 8.2 12.4#


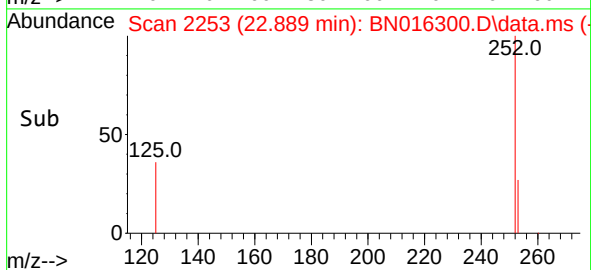

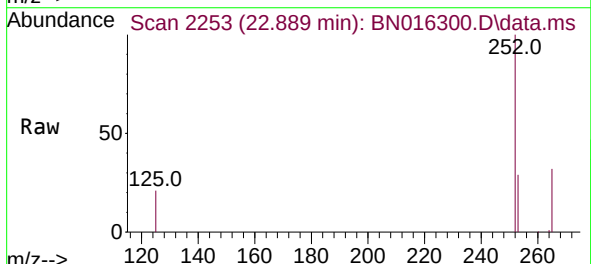




#39
Benzo(a)pyrene
Concen: 0.105 ng
RT: 23.423 min Scan# 2409
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12




Instrument :
BNA_N
ClientSampleId :
SSTDICC0.1


Tgt Ion:252 Resp: 30839
Ion Ratio Lower Upper
252 100
253 29.6 18.7 28.1#
125 19.0 9.9 14.9#

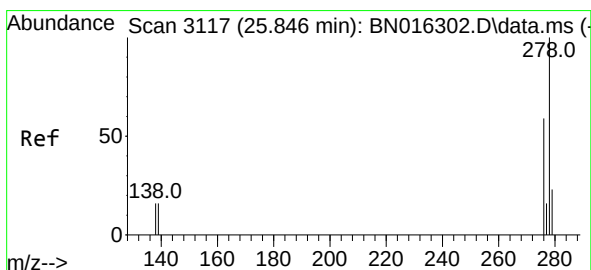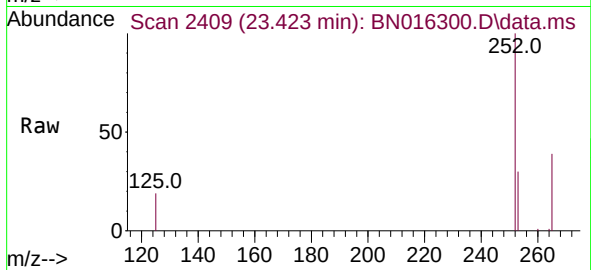

#40
Dibenzo(a,h)anthracene
Concen: 0.213 ng
RT: 25.846 min Scan# 3117
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Tgt Ion:278 Resp: 27614
Ion Ratio Lower Upper
278 100
139 23.6 14.2 21.2#
279 29.0 21.3 31.9

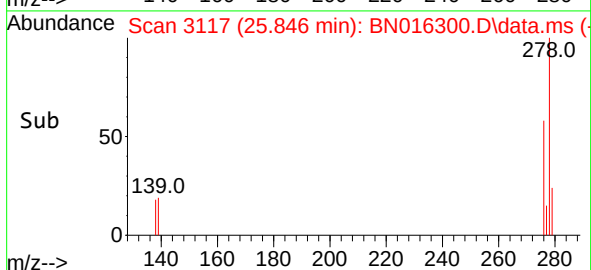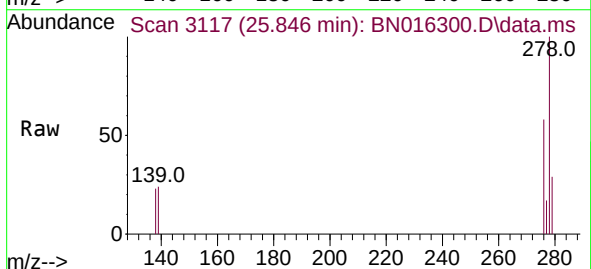

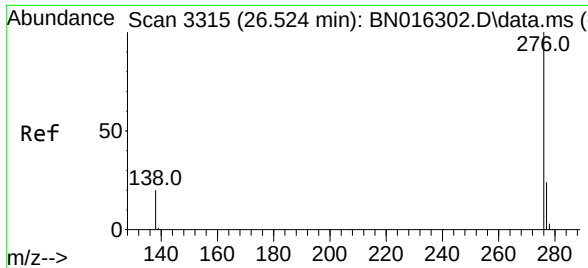

#41
Benzo(g,h,i)perylene
Concen: 0.193 ng
RT: 26.524 min Scan# 3315
Delta R.T. -0.000 min
Lab File: BN016300.D
Acq: 17 Sep 2021 16:12

Instrument :
BNA_N
ClientSampleId :
SSTDIC0.1

Tgt Ion:	276	Resp:	27158
Ion Ratio	Lower	Upper	
276	100		
277	25.7	20.5	30.7
138	25.6	18.2	27.4

