
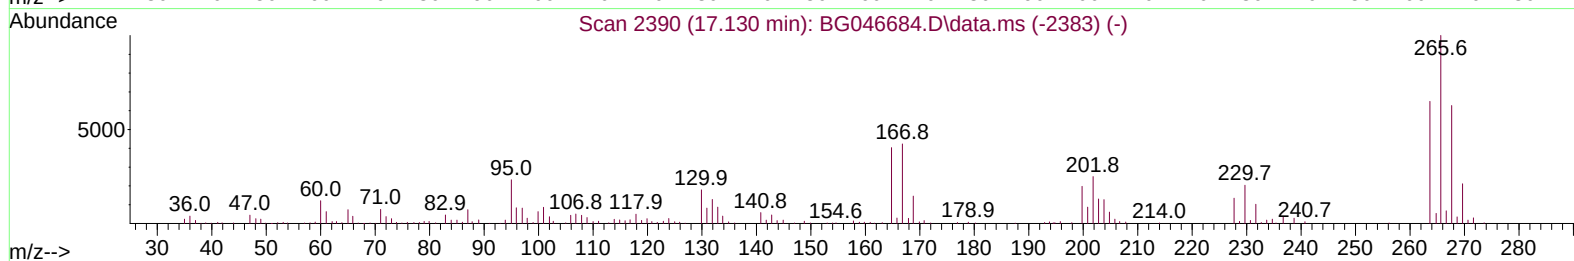
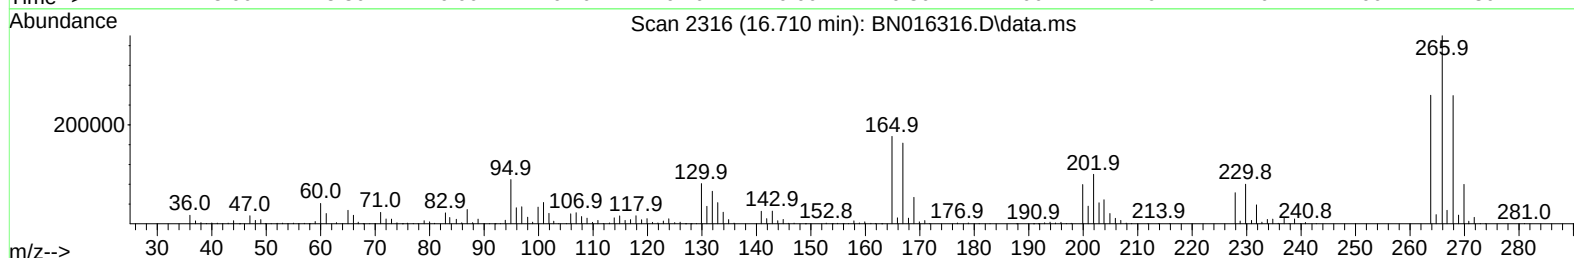


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016316.D
Acq On : 18 Sep 2021 03:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 05:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 18 04:59:53 2021
Response via : Initial Calibration

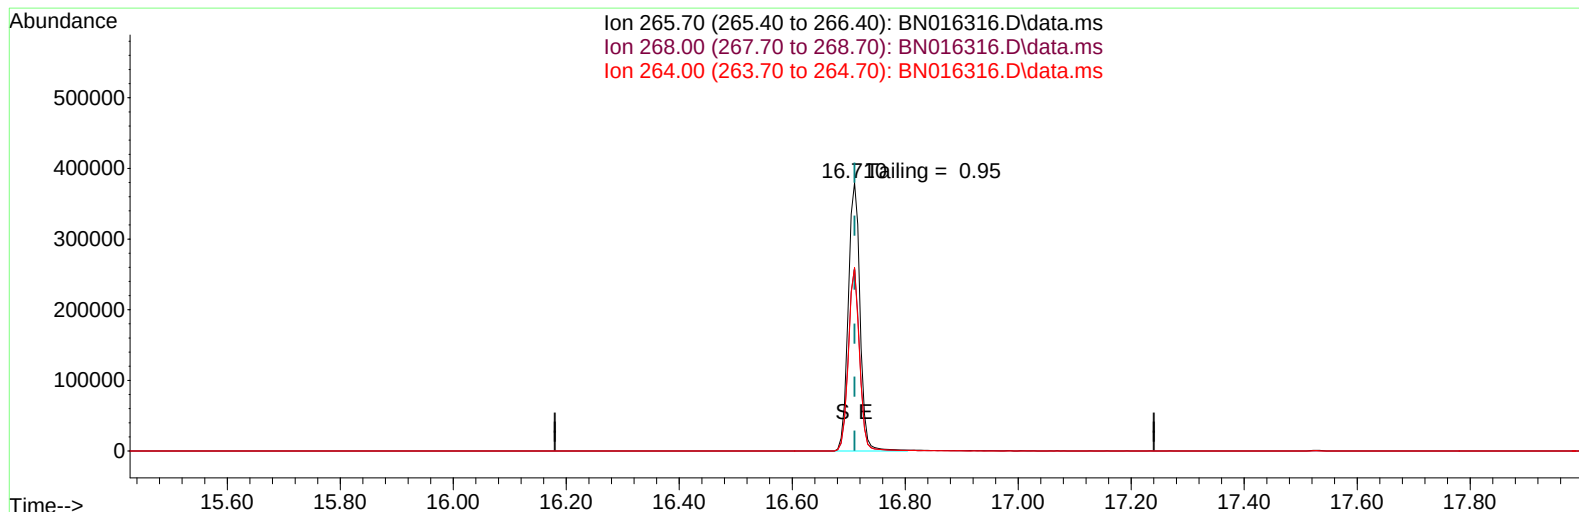

TIC: BN016316.D\data.ms

(70) Pentachlorophenol (C)




16.710min (0.000) 23503.18 ng

response 554079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.21
264.00	61.60	68.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016316.D
Acq On : 18 Sep 2021 03:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 05:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 18 04:59:53 2021
Response via : Initial Calibration

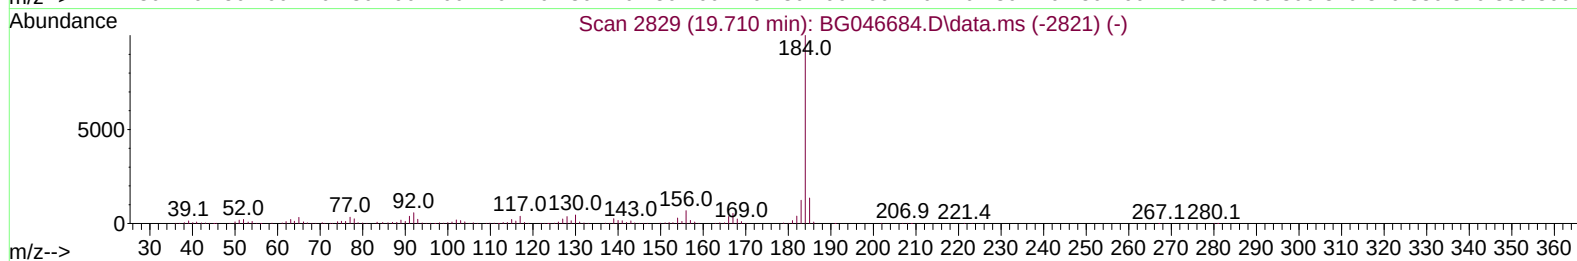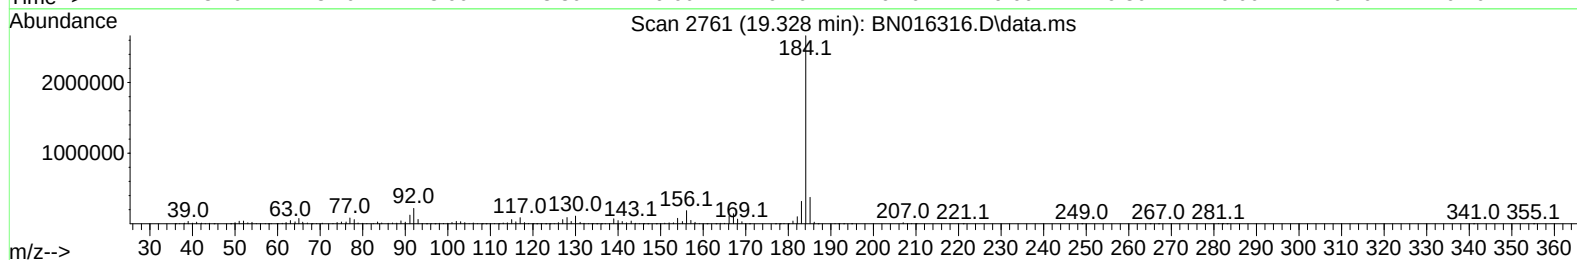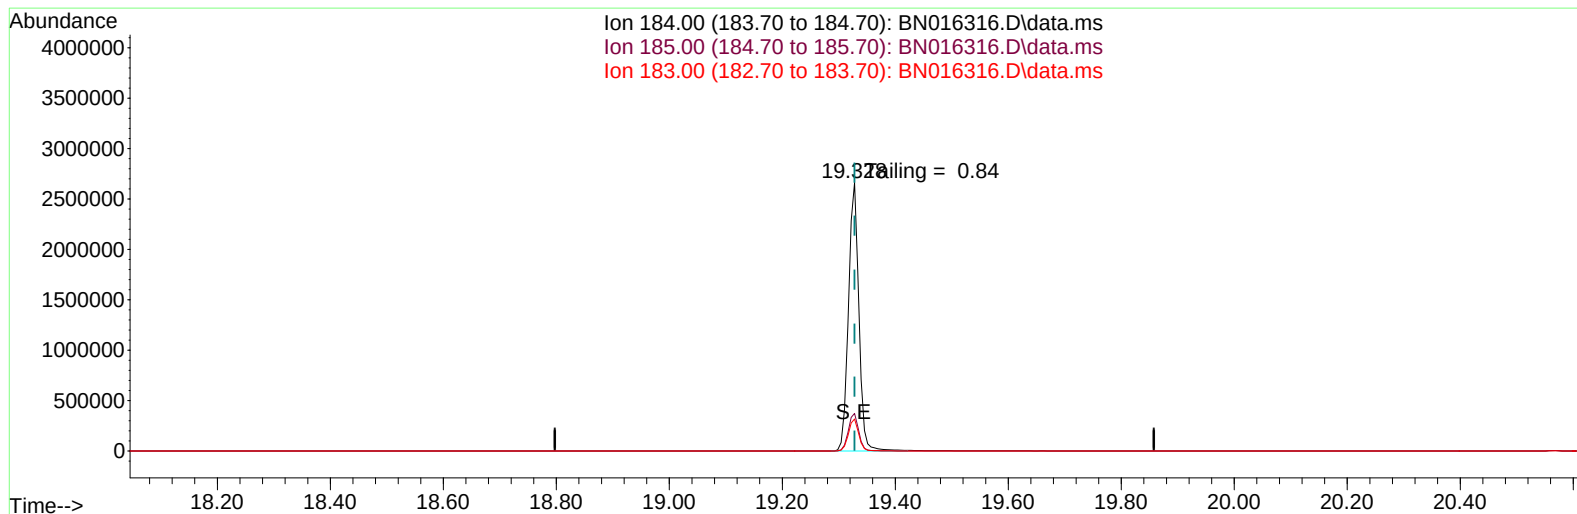

TIC: BN016316.D\data.ms

(77) Benzidine

19.328min (0.000) 0.00 ng

response 3426150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.95
0.00	0.00	0.00