

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016331.D
 Acq On : 18 Sep 2021 12:44
 Operator : CG/JU
 Sample : M3750-05
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 NAPL-AREA-03-(10-12)-END-POINT

Quant Time: Sep 20 00:56:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 17 23:59:14 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.688	152	28532	0.400	ng	0.00
7) Naphthalene-d8	10.457	136	131671	0.400	ng	0.00
13) Acenaphthene-d10	14.307	164	72779	0.400	ng	0.00
19) Phenanthrene-d10	17.054	188	139596	0.400	ng	-0.01
29) Chrysene-d12	21.259	240	145729	0.400	ng	# 0.00
35) Perylene-d12	23.525	264	152317	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.319	112	18519	0.259	ng	0.02
5) Phenol-d6	6.868	99	21252	0.245	ng	0.00
8) Nitrobenzene-d5	8.822	82	19300	0.247	ng	-0.01
11) 2-Methylnaphthalene-d10	12.047	152	46322	0.223	ng	0.00
14) 2,4,6-Tribromophenol	15.804	330	6692	0.313	ng	0.00
15) 2-Fluorobiphenyl	12.936	172	60696	0.213	ng	0.00
27) Fluoranthene-d10	19.098	212	126543	0.313	ng	0.00
31) Terphenyl-d14	19.708	244	101185	0.300	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	21.195	149	23820	0.094	ng	Qvalue 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016331.D
Acq On : 18 Sep 2021 12:44
Operator : CG/JU
Sample : M3750-05
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT

Quant Time: Sep 20 00:56:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 17 23:59:14 2021
Response via : Initial Calibration




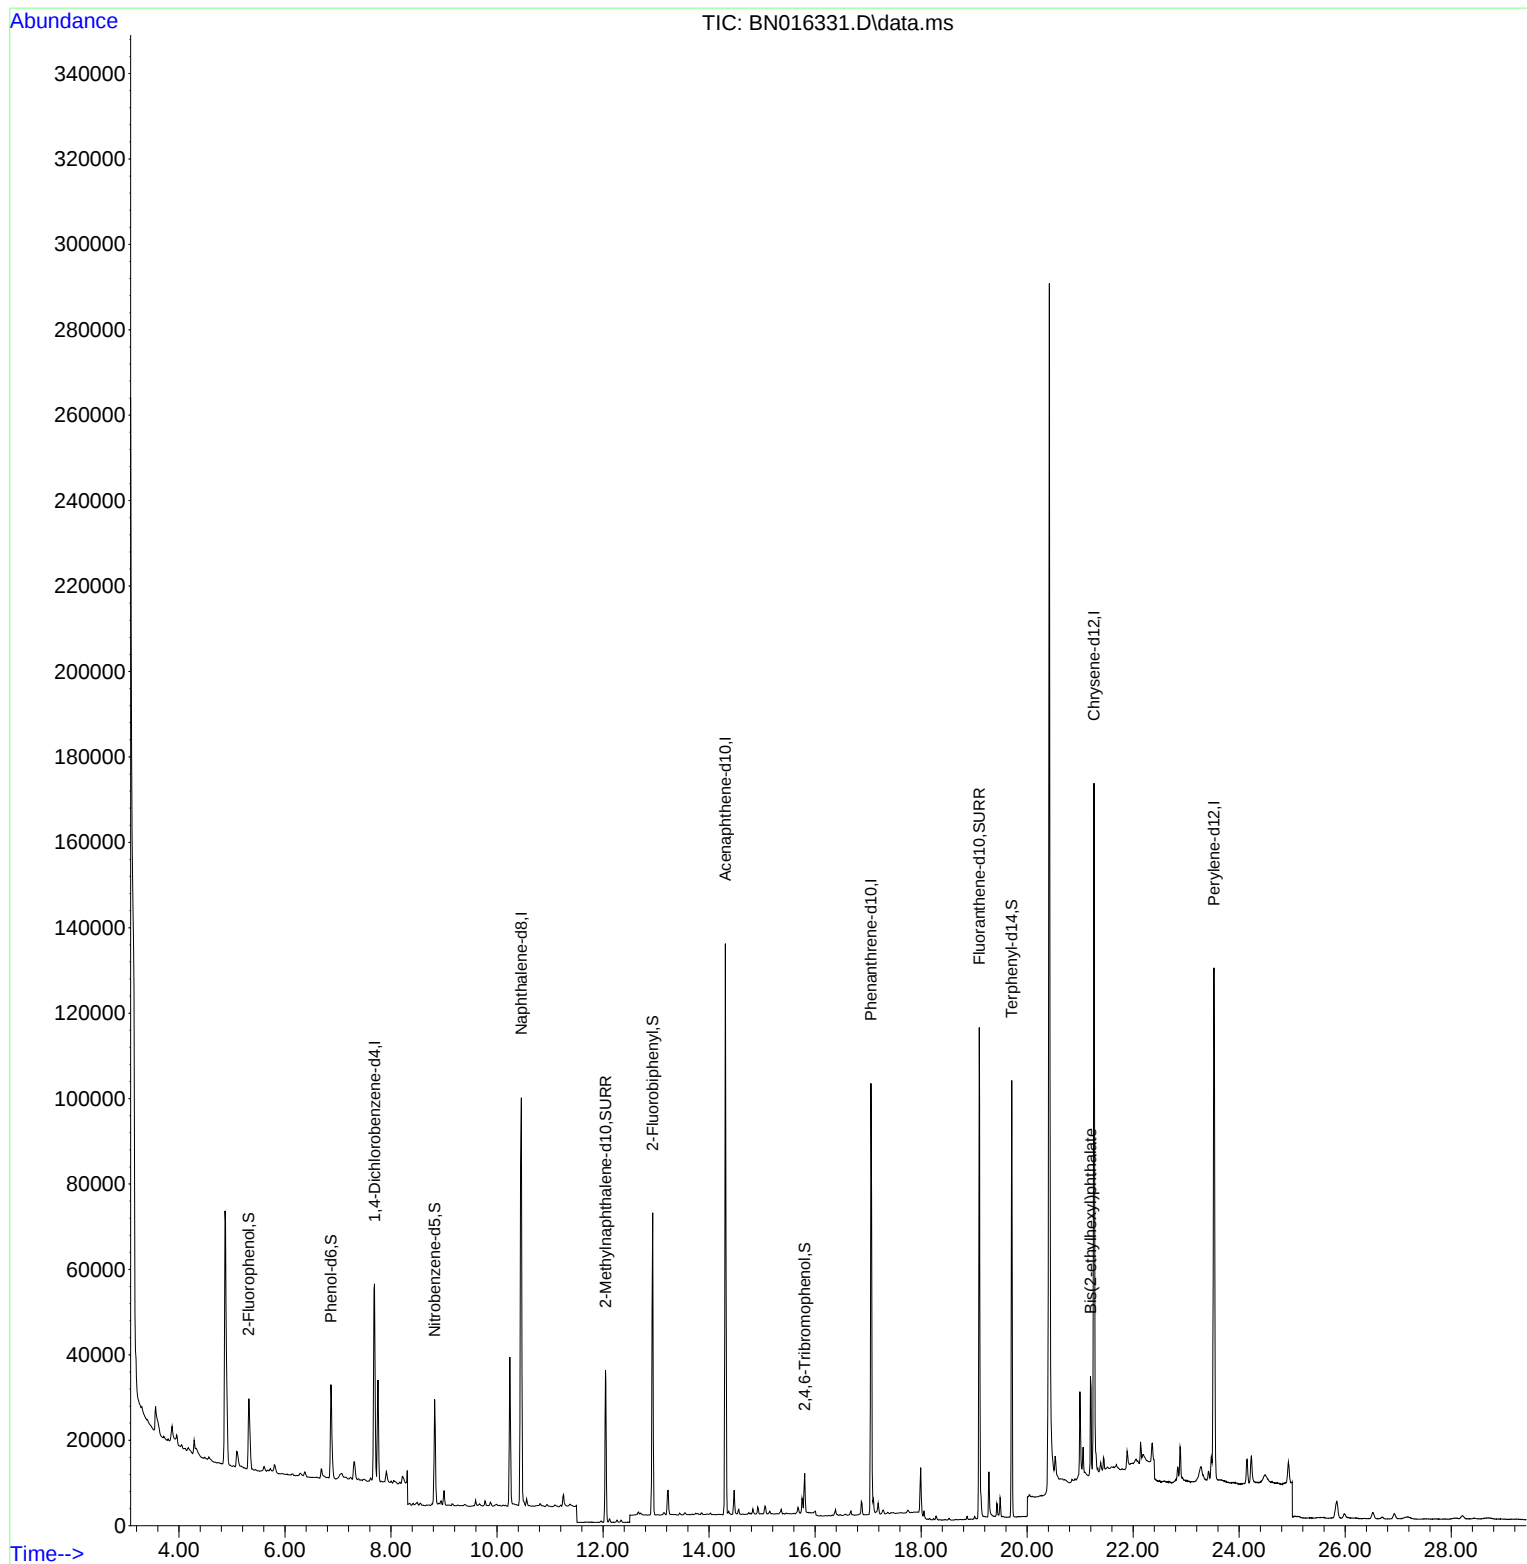




#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.688 min Scan# 500
Delta R.T. 0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion:152 Resp: 28532
Ion Ratio Lower Upper
152 100
150 154.6 125.6 188.4
115 57.2 50.2 75.2

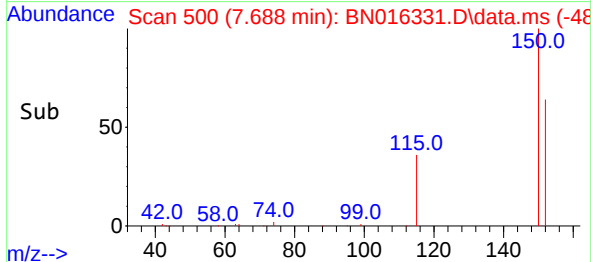

#4
2-Fluorophenol
Concen: 0.259 ng
RT: 5.319 min Scan# 243
Delta R.T. 0.018 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:112 Resp: 18519
Ion Ratio Lower Upper
112 100
64 60.7 47.3 70.9
63 31.5 23.4 35.0


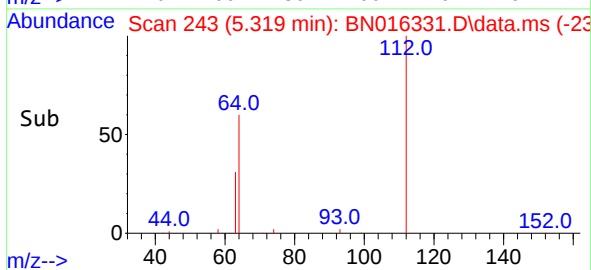

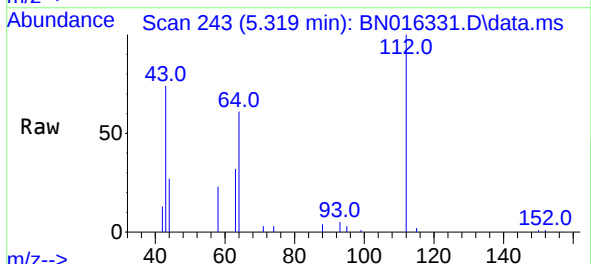




#5
Phenol-d6
Concen: 0.245 ng
RT: 6.868 min Scan# 411
Delta R.T. 0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion: 99 Resp: 21252
Ion Ratio Lower Upper
99 100
42 22.7 14.0 21.0#
71 31.9 23.8 35.6

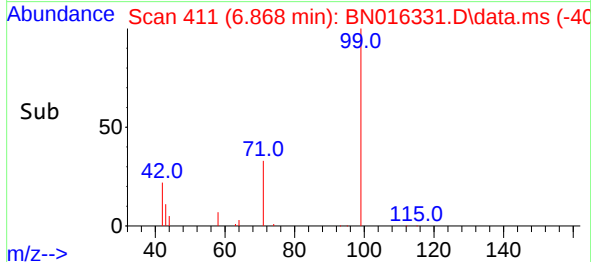

#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.457 min Scan# 737
Delta R.T. 0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:136 Resp: 131671
Ion Ratio Lower Upper
136 100
137 11.1 8.8 13.2
54 6.3 5.3 7.9
68 4.3 3.9 5.9



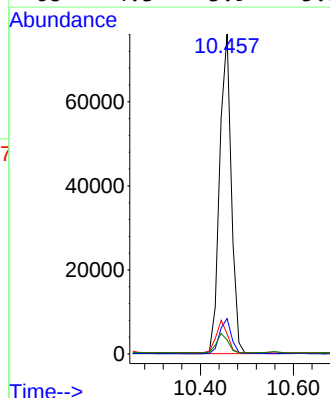
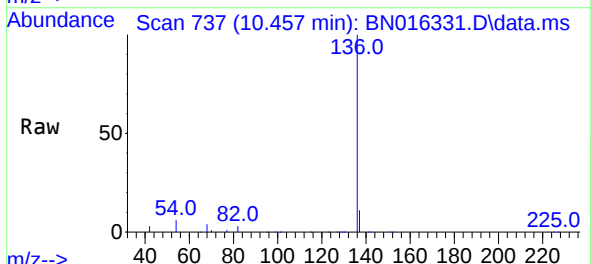


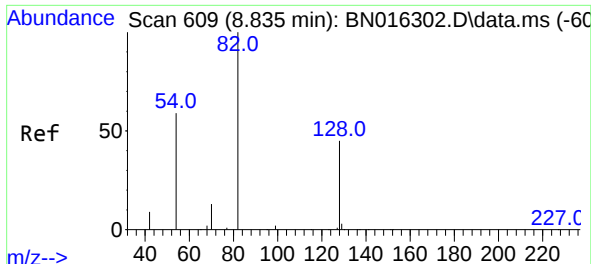

#8
Nitrobenzene-d5
Concen: 0.247 ng
RT: 8.822 min Scan# 608
Delta R.T. -0.013 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion: 82 Resp: 19300
Ion Ratio Lower Upper
82 100
128 38.8 31.7 47.5
54 67.0 46.4 69.6



#11
2-Methylnaphthalene-d10
Concen: 0.223 ng
RT: 12.047 min Scan# 941
Delta R.T. -0.004 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion: 152 Resp: 46322
Ion Ratio Lower Upper
152 100
151 20.4 16.1 24.1




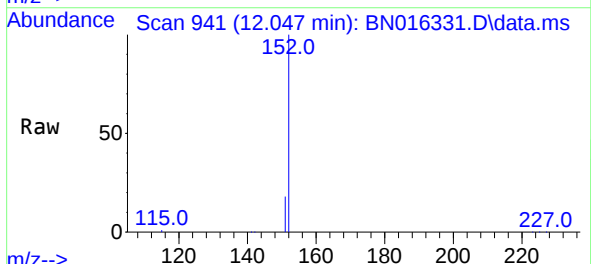




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.307 min Scan# 1186
Delta R.T. -0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion:164 Resp: 72779
Ion Ratio Lower Upper
164 100
162 101.5 79.0 118.4
160 45.3 34.1 51.1

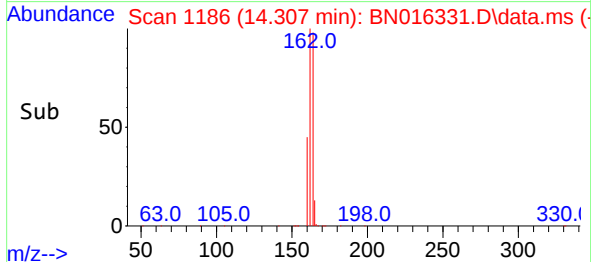

#14
2,4,6-Tribromophenol
Concen: 0.313 ng
RT: 15.804 min Scan# 1304
Delta R.T. -0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:330 Resp: 6692
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 39.1 25.0 37.4#


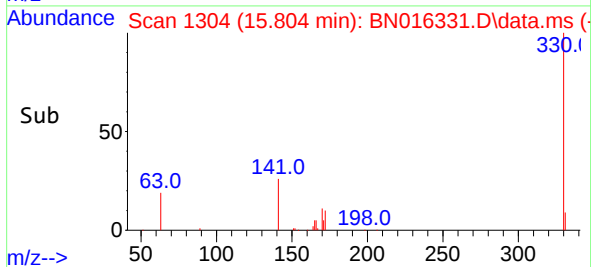

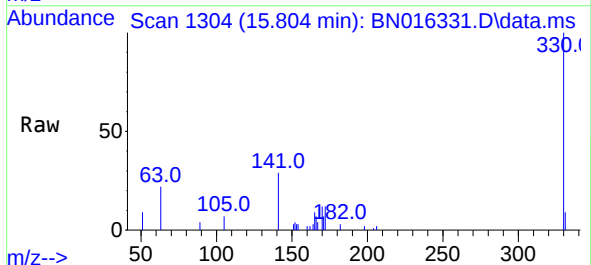




#15
2-Fluorobiphenyl
Concen: 0.213 ng
RT: 12.936 min Scan# 1078
Delta R.T. 0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion:	172	Resp:	60696
Ion	Ratio	Lower	Upper
172	100		
171	34.0	27.8	41.6
170	22.2	18.2	27.2

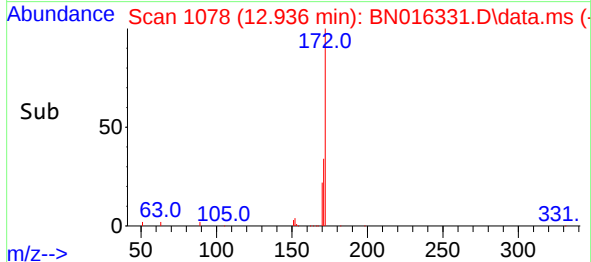

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.054 min Scan# 1406
Delta R.T. -0.012 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:	188	Resp:	139596
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	10.3	7.0	10.6


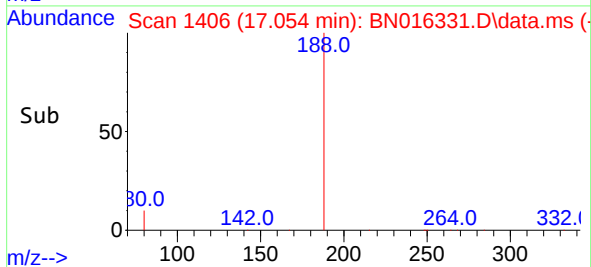

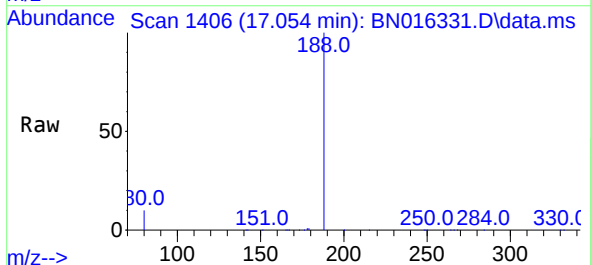




#27
Fluoranthene-d10
Concen: 0.313 ng
RT: 19.098 min Scan# 1703
Delta R.T. -0.005 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion:212 Resp: 126543
Ion Ratio Lower Upper
212 100
106 11.4 9.8 14.6
104 6.2 5.4 8.2

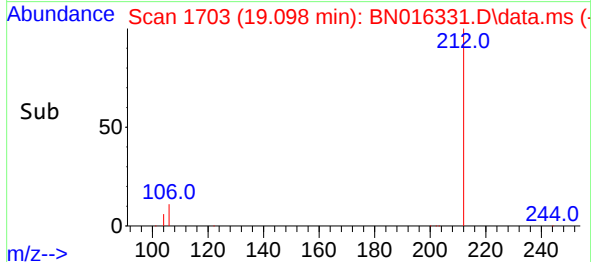

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.259 min Scan# 2004
Delta R.T. -0.000 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:240 Resp: 145729
Ion Ratio Lower Upper
240 100
120 10.1 5.3 7.9#
236 26.4 19.8 29.8



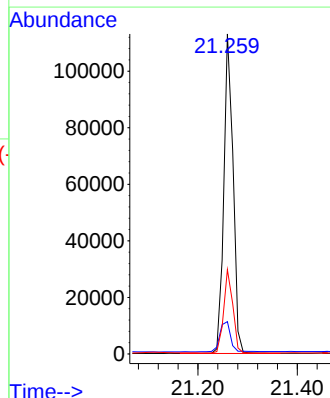
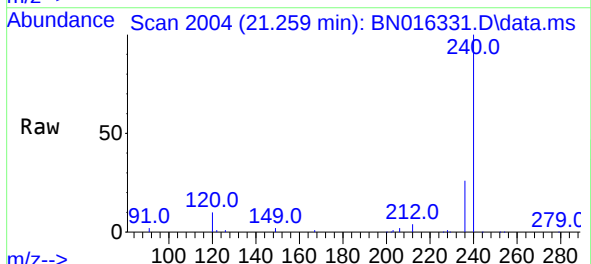




#31
Terphenyl-d14
Concen: 0.300 ng
RT: 19.708 min Scan# 1826
Delta R.T. -0.005 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44




Instrument :
BNA_N
ClientSampleId :
NAPL-AREA-03-(10-12)-END-POINT


Tgt Ion:244 Resp: 101185
Ion Ratio Lower Upper
244 100
212 7.2 5.5 8.3
122 11.0 9.0 13.4

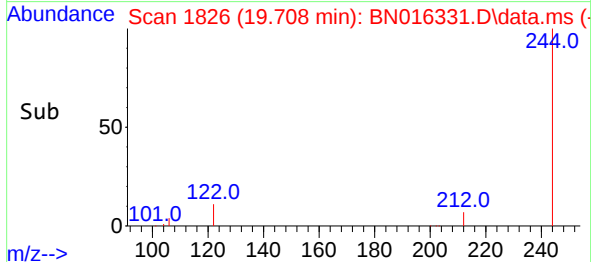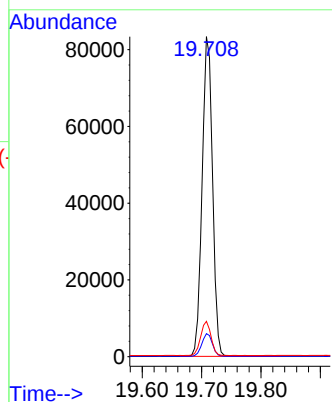

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.094 ng
RT: 21.195 min Scan# 1998
Delta R.T. -0.011 min
Lab File: BN016331.D
Acq: 18 Sep 2021 12:44

Tgt Ion:149 Resp: 23820
Ion Ratio Lower Upper
149 100
167 28.1 23.4 35.0
279 4.6 3.9 5.9

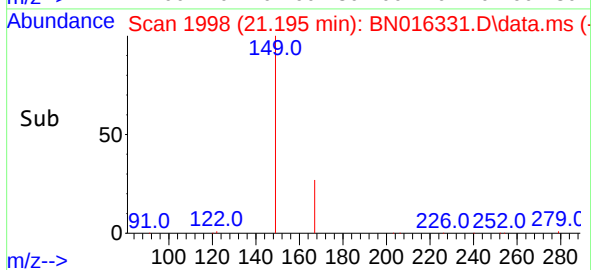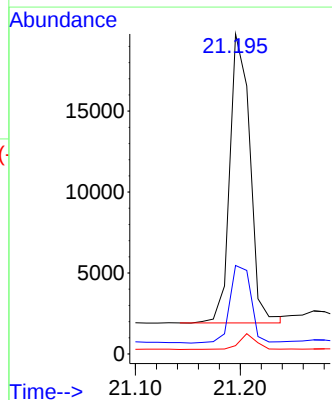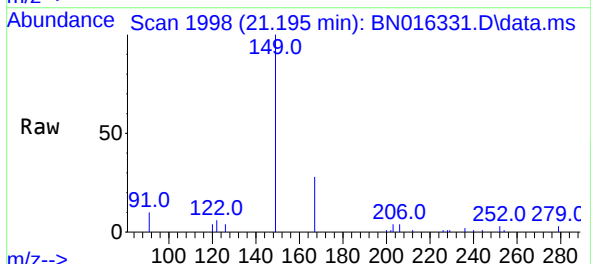

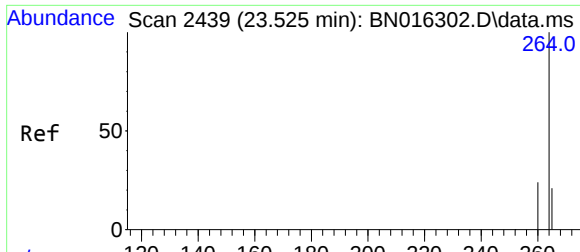

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.525 min Scan# 2439
 Delta R.T. 0.000 min
 Lab File: BN016331.D
 Acq: 18 Sep 2021 12:44

Instrument :
 BNA_N
 ClientSampleId :
 NAPL-AREA-03-(10-12)-END-POINT

Tgt Ion:264 Resp: 152317

Ion	Ratio	Lower	Upper
264	100		
260	24.3	18.9	28.3
265	27.8	23.7	35.5

