
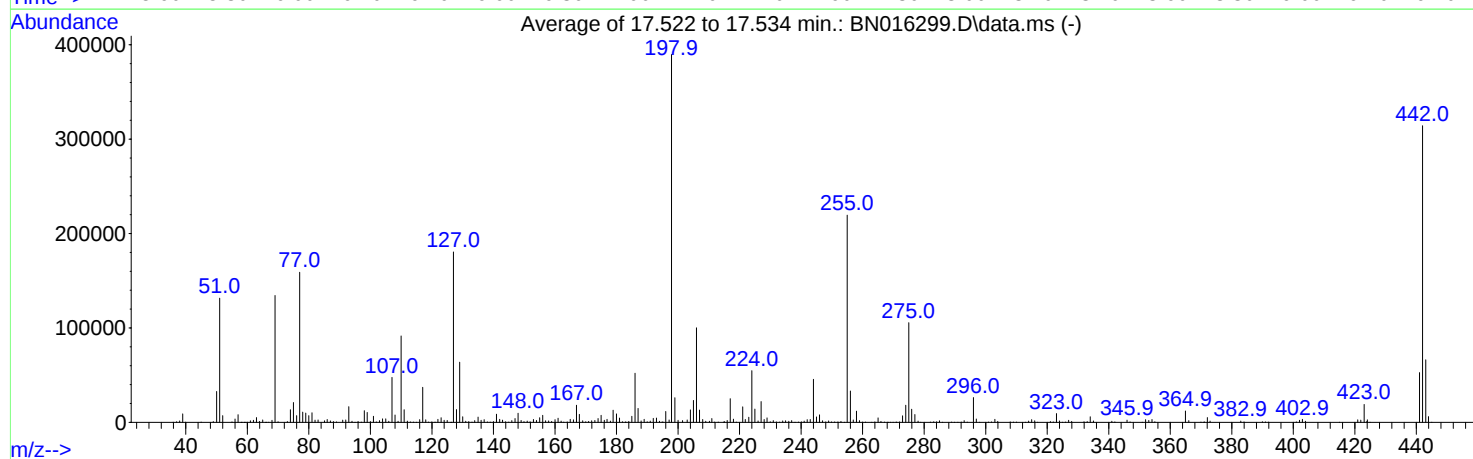


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016299.D
 Acq On : 17 Sep 2021 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 20 11:09:23 2021

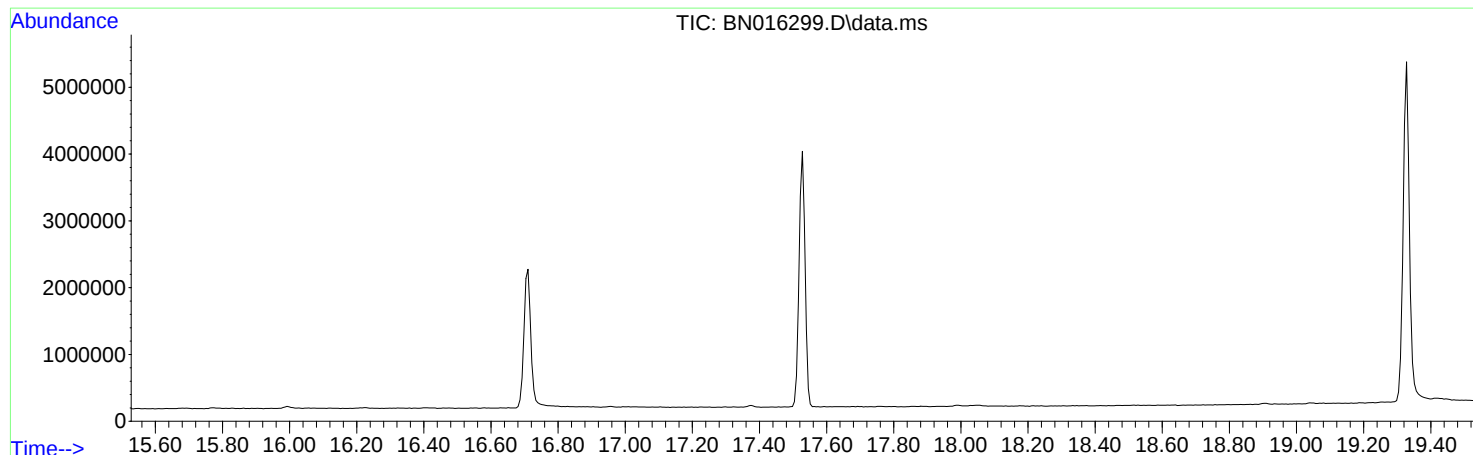




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	131597	PASS
68	69	0.00	2	1.6	2214	PASS
69	198	0.00	100	34.5	134373	PASS
70	69	0.00	2	0.5	734	PASS
127	198	10	80	46.3	180603	PASS
197	198	0.00	2	0.7	2624	PASS
198	198	100	100	100.0	389675	PASS
199	198	5	9	6.7	26080	PASS
275	198	10	60	27.1	105645	PASS
365	198	1	100	3.1	12124	PASS
441	198	0.01	100	13.5	52661	PASS
442	442	50	100	100.0	314219	PASS
443	442	15	24	21.1	66221	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016299.D
 Acq On : 17 Sep 2021 15:35
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 18 00:08:12 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 18 00:08:04 2021
 Response via : Initial Calibration

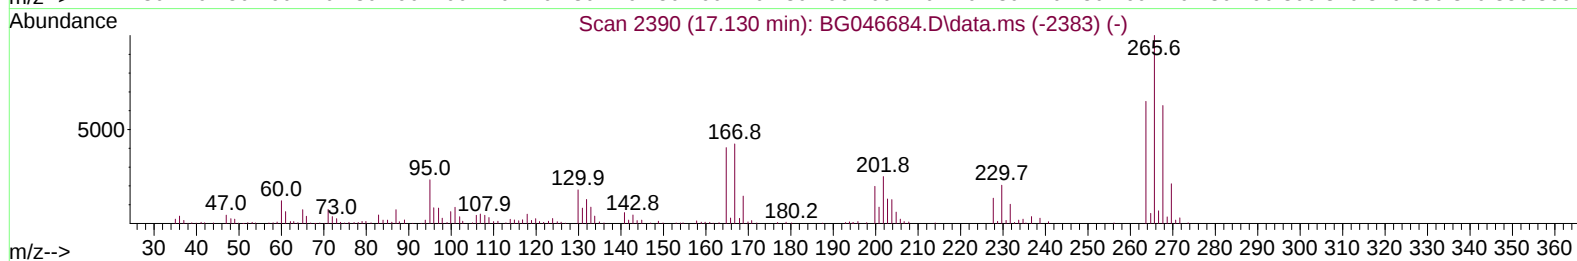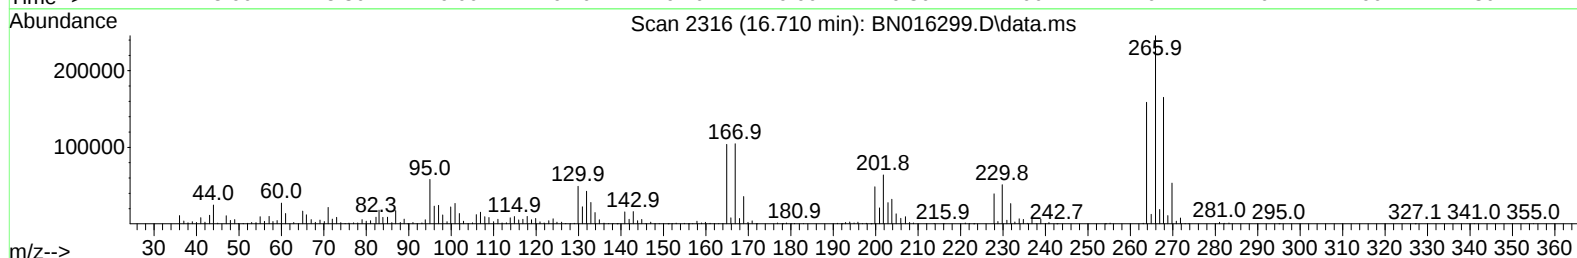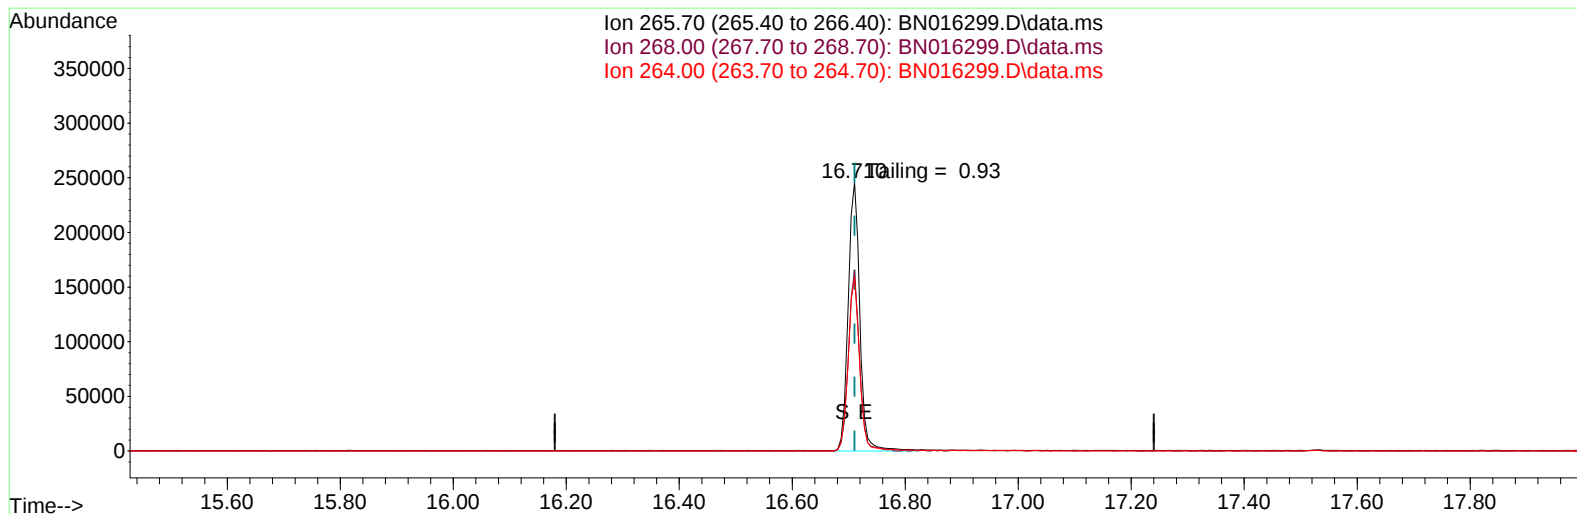

TIC: BN016299.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 19262.92 ng




response 353588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	67.27
264.00	61.60	64.69
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016299.D
Acq On : 17 Sep 2021 15:35
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 00:08:12 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 18 00:08:04 2021
Response via : Initial Calibration

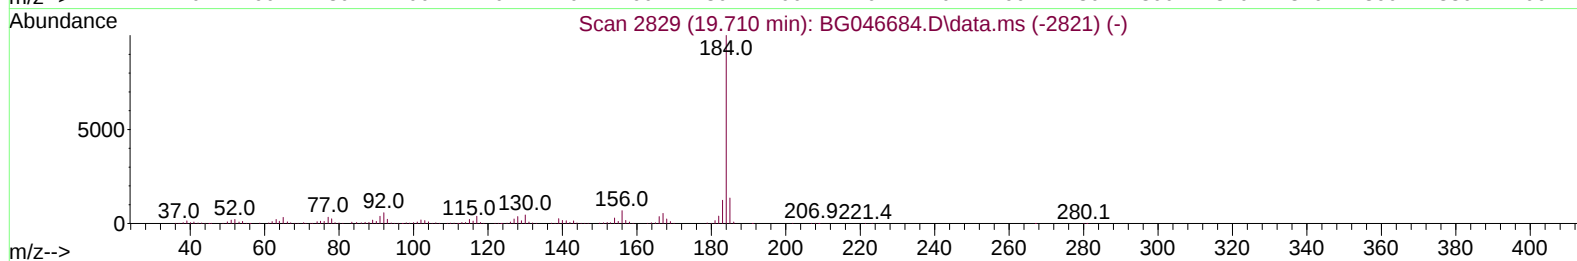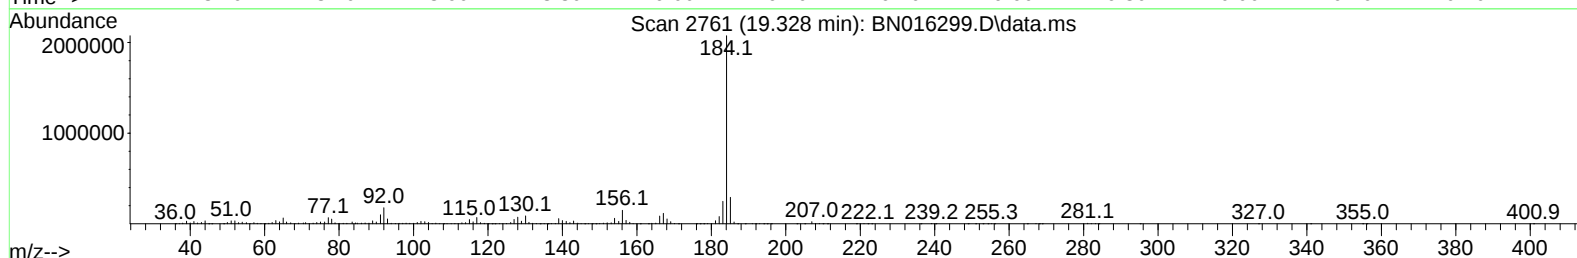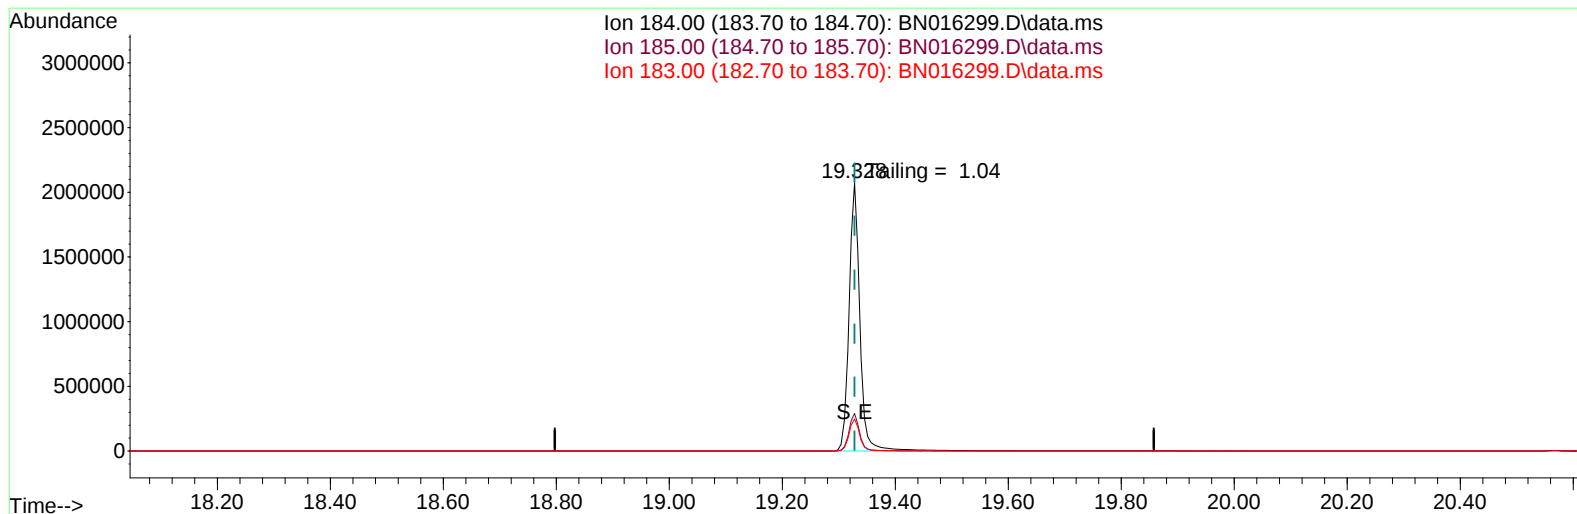

TIC: BN016299.D\data.ms

(77) Benzidine

19.328min (0.000) 173851.30 ng

response 2770619

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.03
183.00	13.20	11.91
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2021	BNA_N	<u>BN016299.D</u>
Compound Name	Response	Retention Time
DDT	1145207	20.56
DDD	2400	20.12
DDE	1721	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4121	1149328	0.36

Instrument :
BNA_N
ClientSampleId :
DFTPP