


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016316.D
 Acq On : 18 Sep 2021 03:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 20 11:09:23 2021

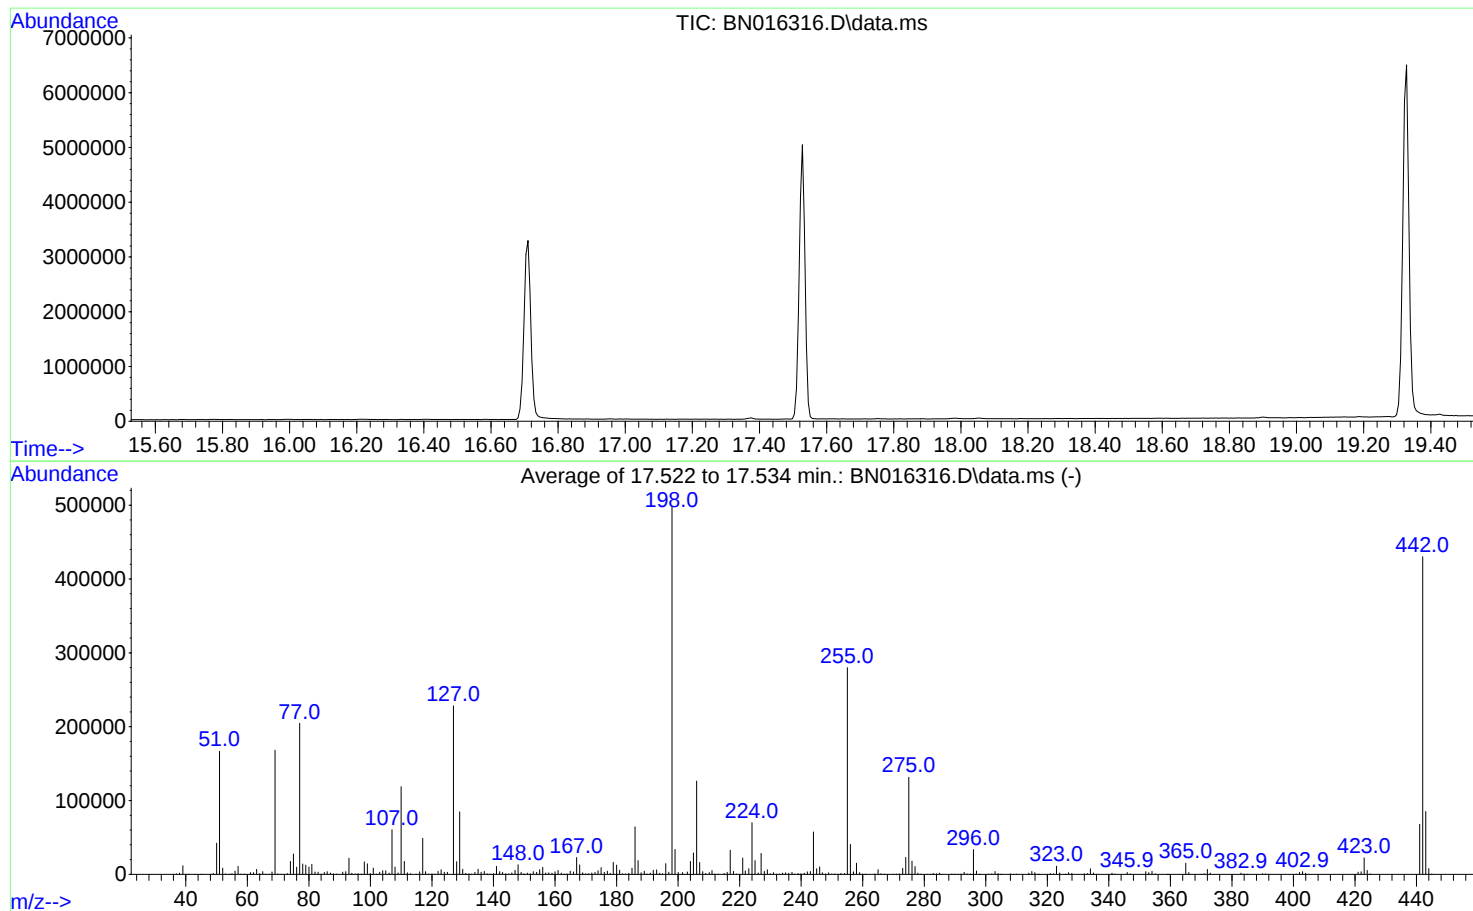




AutoFind: Scans 2454, 2455, 2456; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	166722	PASS
68	69	0.00	2	1.9	3261	PASS
69	198	0.00	100	33.8	168205	PASS
70	69	0.00	2	0.4	685	PASS
127	198	10	80	45.8	228245	PASS
197	198	0.00	2	0.6	3036	PASS
198	198	100	100	100.0	498176	PASS
199	198	5	9	6.8	33752	PASS
275	198	10	60	26.4	131573	PASS
365	198	1	100	3.0	15171	PASS
441	198	0.01	100	13.6	67768	PASS
442	442	50	100	100.0	430208	PASS
443	442	15	24	19.8	85275	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
Data File : BN016316.D
Acq On : 18 Sep 2021 03:43
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 18 05:00:03 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 18 04:59:53 2021
Response via : Initial Calibration

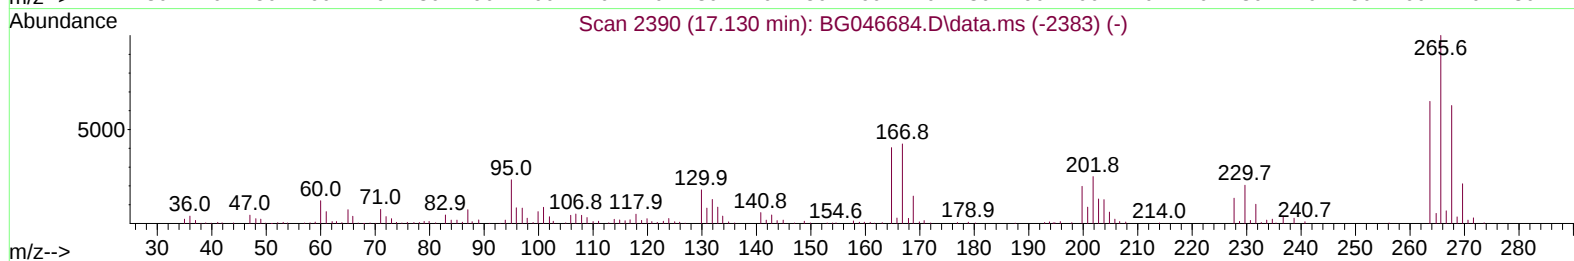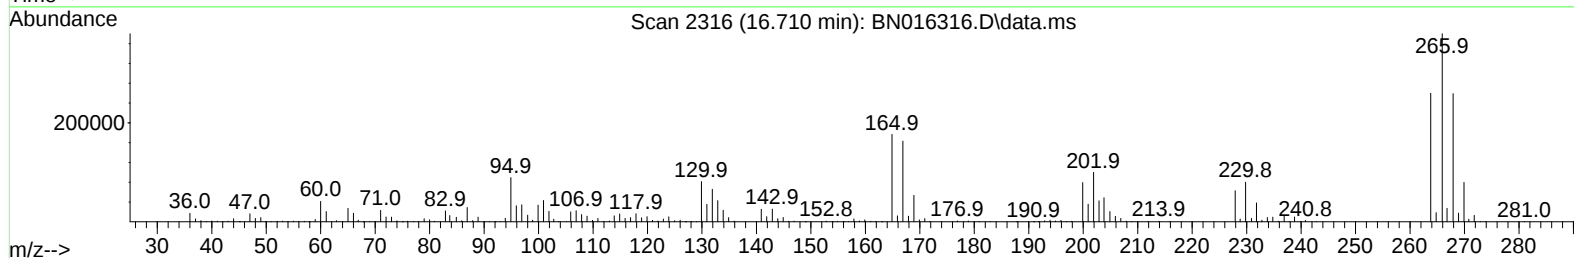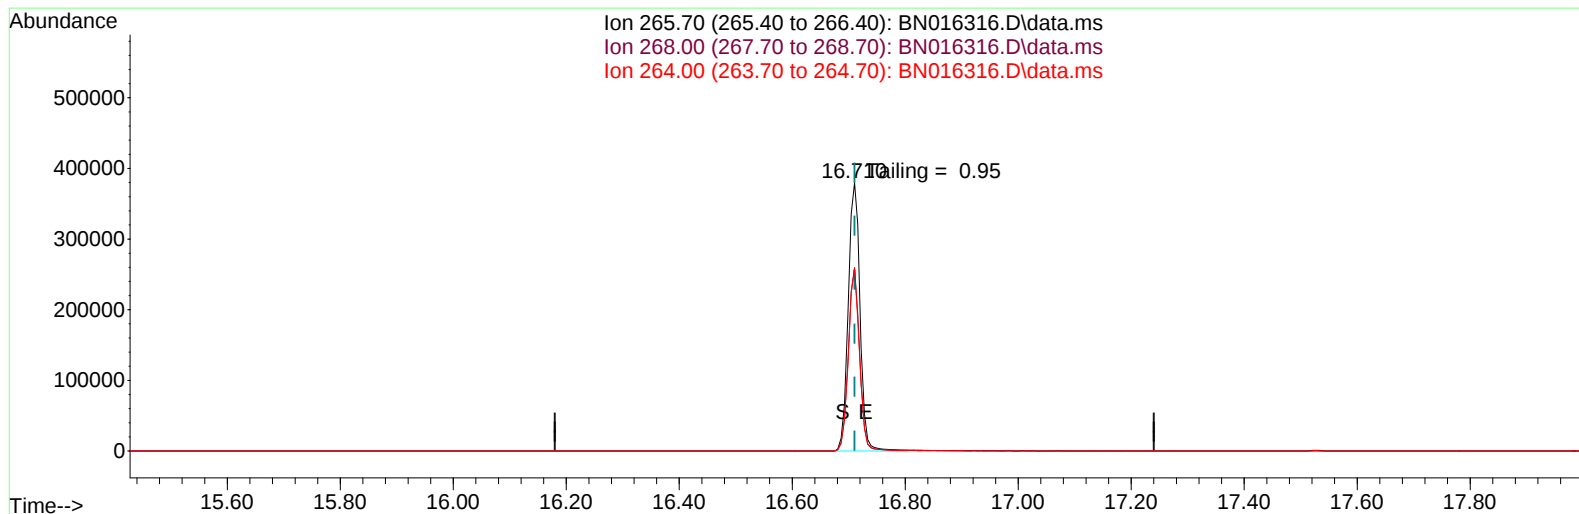

TIC: BN016316.D\data.ms

(70) Pentachlorophenol (C)

16.710min (0.000) 23503.18 ng




response 554079

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	68.21
264.00	61.60	68.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091721\
 Data File : BN016316.D
 Acq On : 18 Sep 2021 03:43
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Sep 18 05:00:03 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 18 04:59:53 2021
 Response via : Initial Calibration

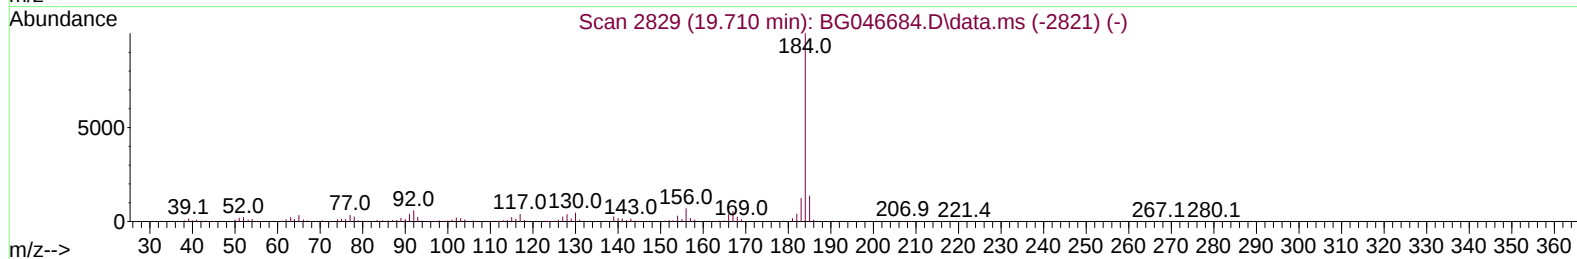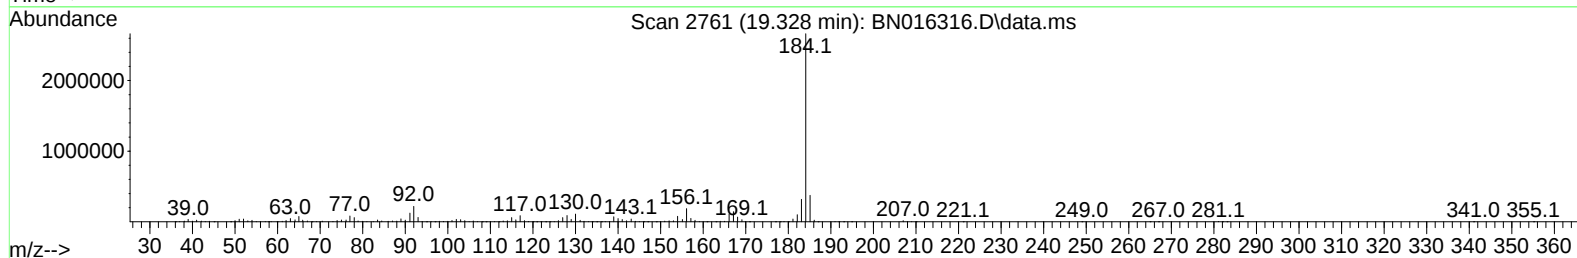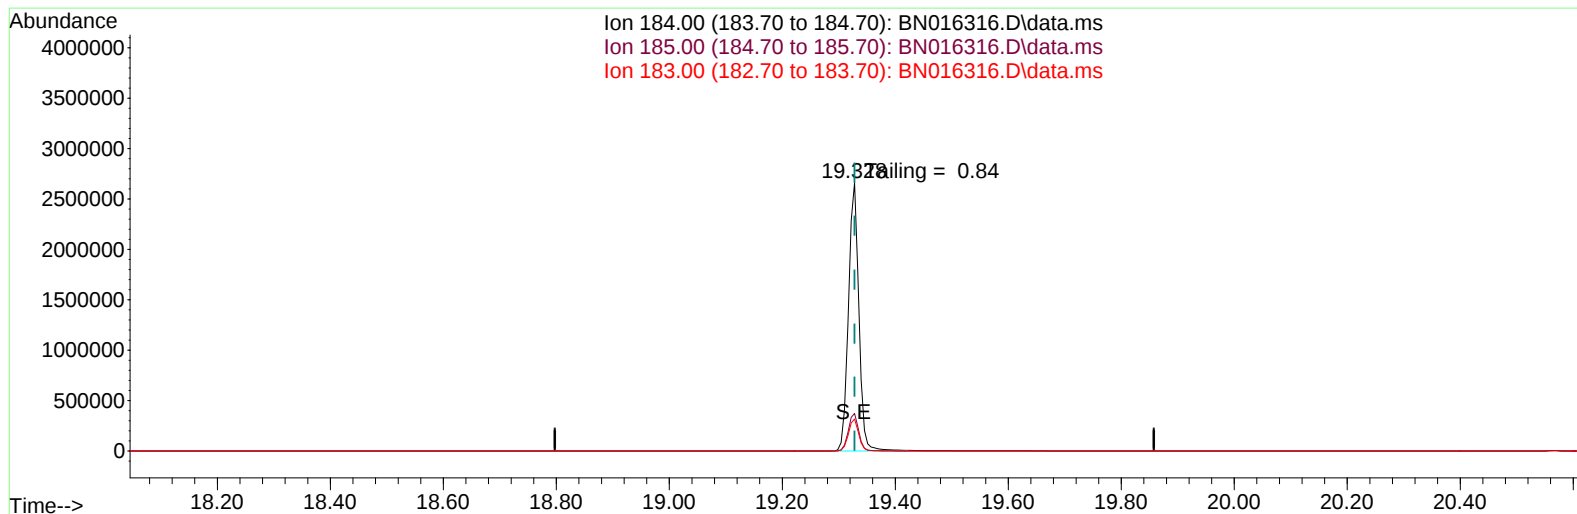

TIC: BN016316.D\data.ms

(77) Benzidine

19.328min (0.000) 0.00 ng

response 3426150

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.04
183.00	13.20	11.95
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/17/2021	BNA_N	<u>BN016316.D</u>
Compound Name	Response	Retention Time
DDT	1579453	20.569
DDD	23688	20.122
DDE	2597	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26285	1605738	1.64

Instrument :
BNA_N
ClientSampleId :
DFTPP