

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
 Data File : BN037750.D
 Acq On : 17 Sep 2025 17:36
 Operator : RC/JU
 Sample : Q3095-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW179D1-20250908

Quant Time: Sep 17 18:05:06 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	6641	0.400	ng	0.00
7) Naphthalene-d8	10.637	136	17861	0.400	ng	-0.01
13) Acenaphthene-d10	14.495	164	7906	0.400	ng	0.00
19) Phenanthrene-d10	17.235	188	13742	0.400	ng	0.00
29) Chrysene-d12	21.411	240	11462	0.400	ng	# 0.00
35) Perylene-d12	23.747	264	11339	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.399	112	2038	0.134	ng	0.00
5) Phenol-d6	6.988	99	1521	0.077	ng	0.00
8) Nitrobenzene-d5	8.982	82	4613	0.353	ng	-0.01
11) 2-Methylnaphthalene-d10	12.238	152	7496	0.317	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	834	0.404	ng	0.00
15) 2-Fluorobiphenyl	13.115	172	11872	0.359	ng	0.00
27) Fluoranthene-d10	19.267	212	13070	0.379	ng	0.00
31) Terphenyl-d14	19.866	244	9983	0.429	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.304	88	1507	0.218	ng	# 84
34) Bis(2-ethylhexyl)phtha...	21.340	149	2119	0.179	ng	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037750.D
Acq On : 17 Sep 2025 17:36
Operator : RC/JU
Sample : Q3095-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908


Quant Time: Sep 17 18:05:06 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration

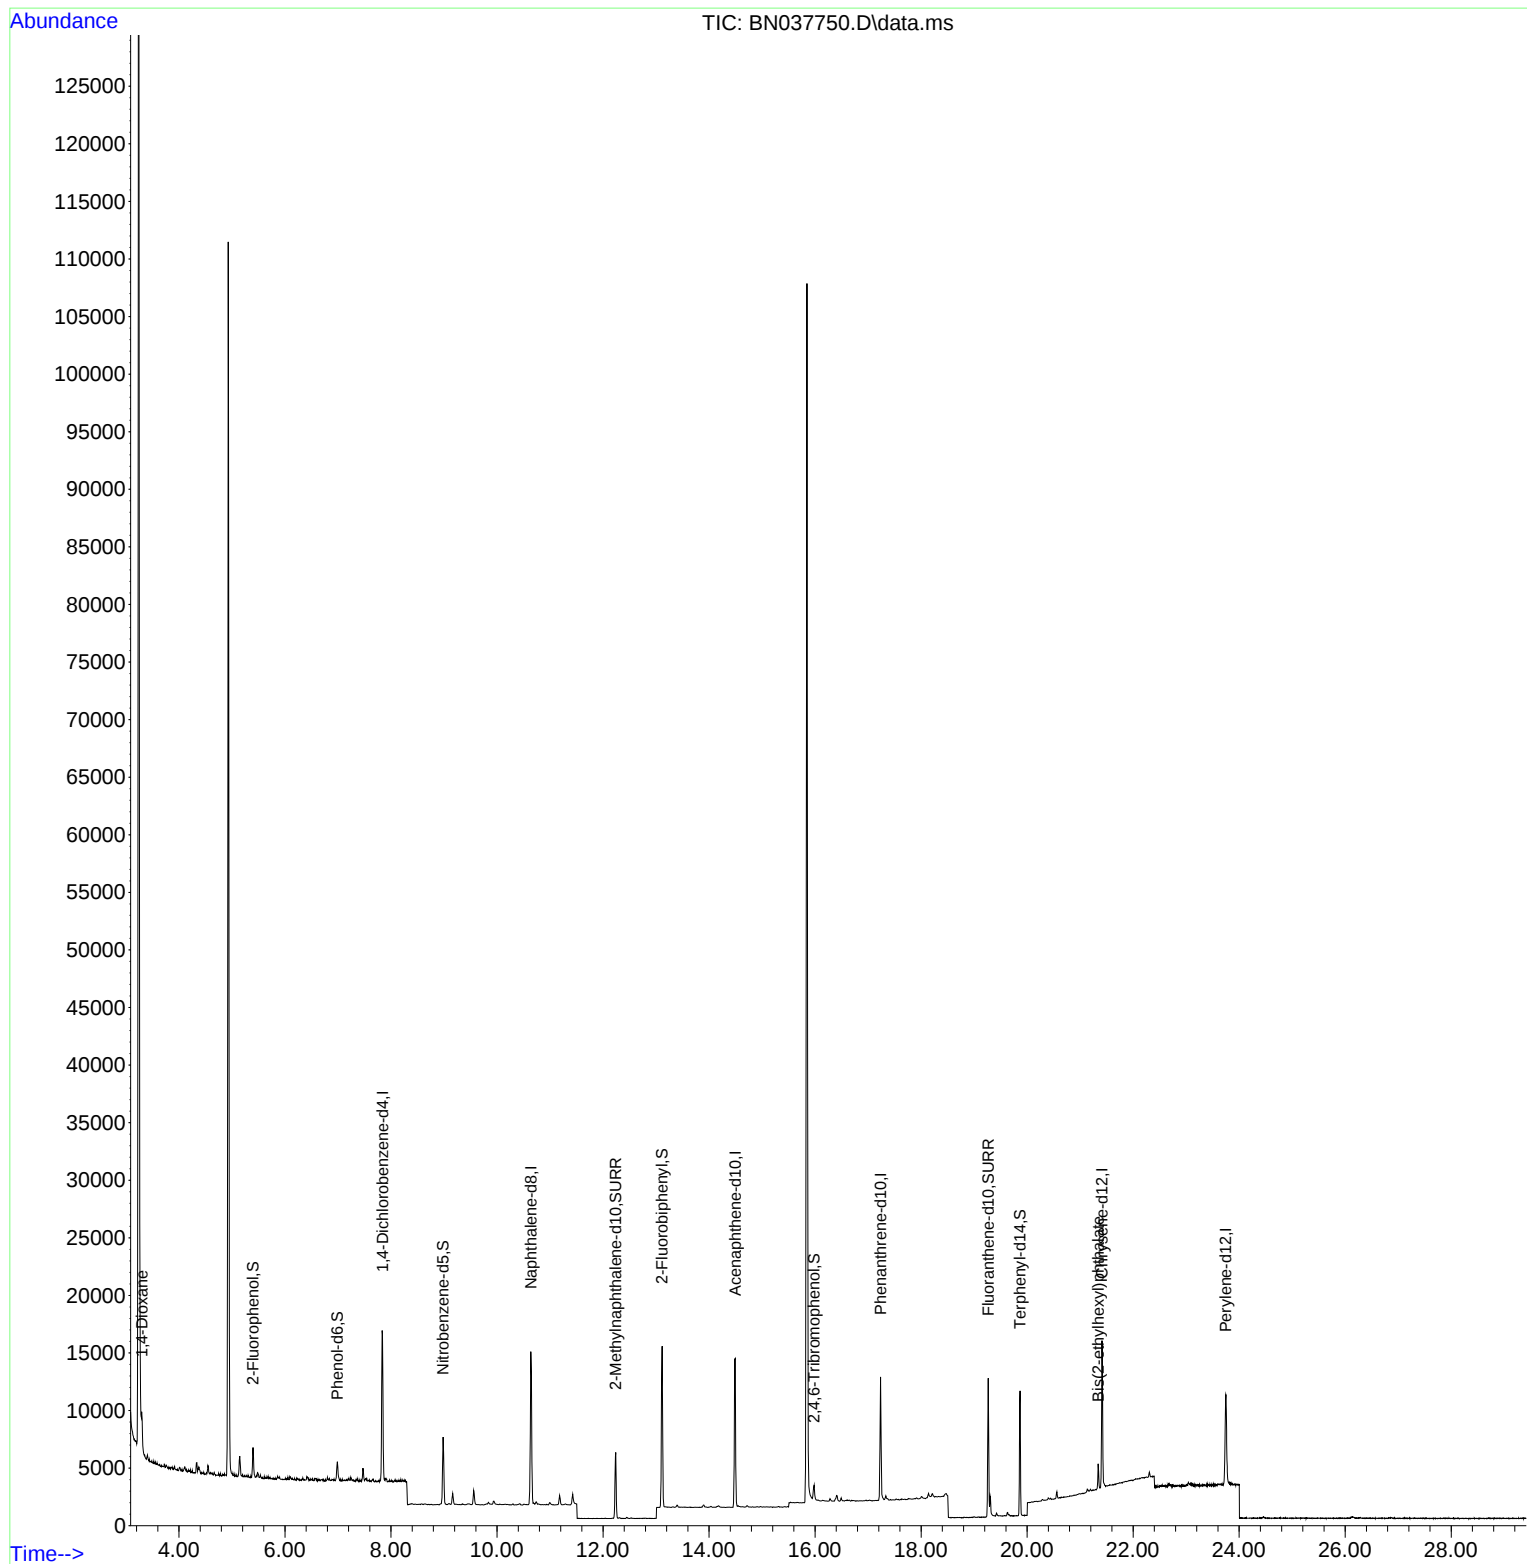


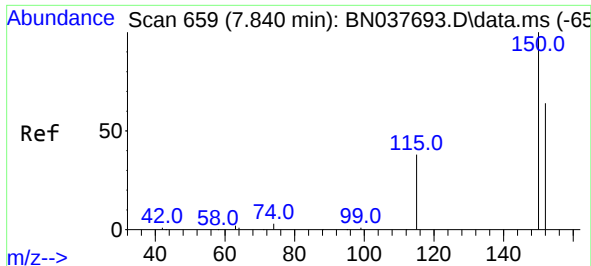


#1
1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.840 min Scan# 61
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908



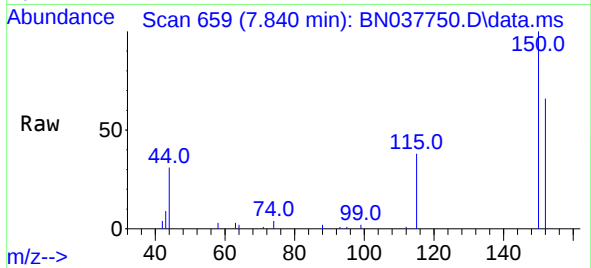


Tgt Ion:152 Resp: 6641
Ion Ratio Lower Upper
152 100
150 152.2 124.5 186.7
115 57.4 49.2 73.8

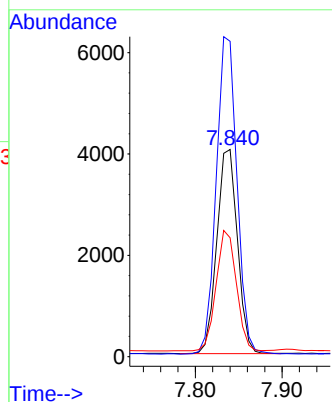

#2
1,4-Dioxane
Concen: 0.218 ng
RT: 3.304 min Scan# 31
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion: 88 Resp: 1507
Ion Ratio Lower Upper
88 100
43 61.9 26.8 40.2#
58 79.1 61.9 92.9

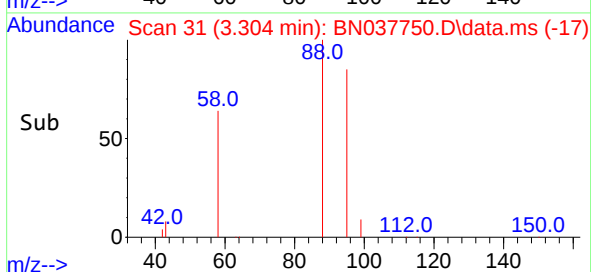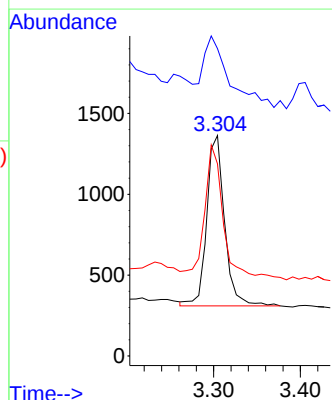



#4

2-Fluorophenol

Concen: 0.134 ng

RT: 5.399 min Scan# 321

Delta R.T. -0.000 min

Lab File: BN037750.D

Acq: 17 Sep 2025 17:36

Instrument :

BNA_N

ClientSampleId :

MW179D1-20250908





Tgt Ion:112 Resp: 2038

Ion Ratio Lower Upper

112 100

64 54.4 44.9 67.3

63 30.1 24.7 37.1

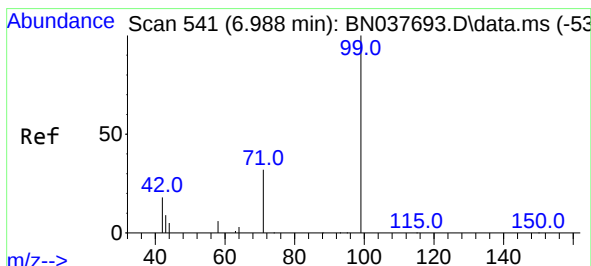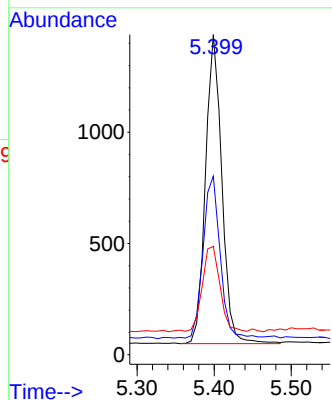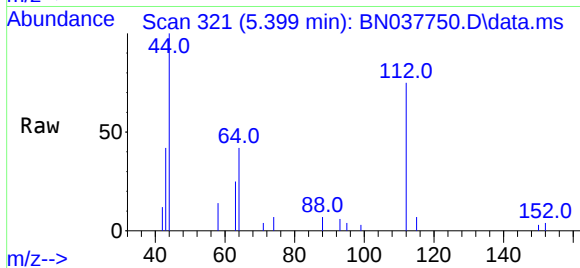

#5

Phenol-d6

Concen: 0.077 ng

RT: 6.988 min Scan# 541

Delta R.T. -0.000 min

Lab File: BN037750.D

Acq: 17 Sep 2025 17:36




Tgt Ion: 99 Resp: 1521


Ion Ratio Lower Upper

99 100

42 24.6 16.6 24.8

71 36.8 26.7 40.1

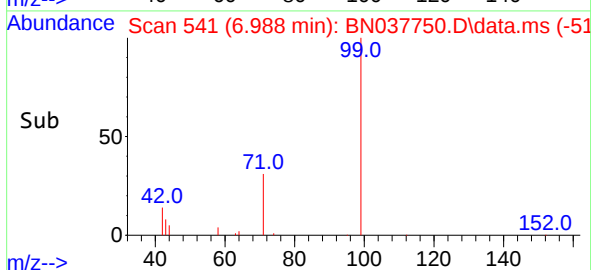
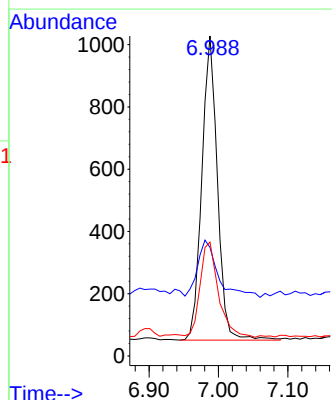
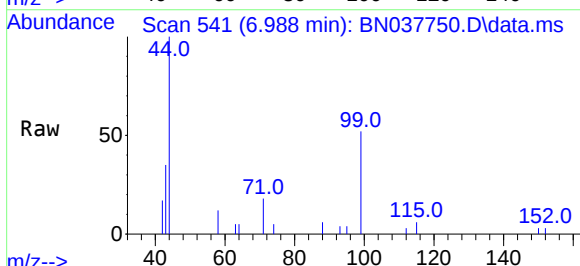




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.637 min Scan# 94
Delta R.T. -0.011 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36




Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908

Tgt Ion:	136	Resp:	17861
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.1	13.7
54	8.8	6.3	9.5
68	7.1	5.0	7.4

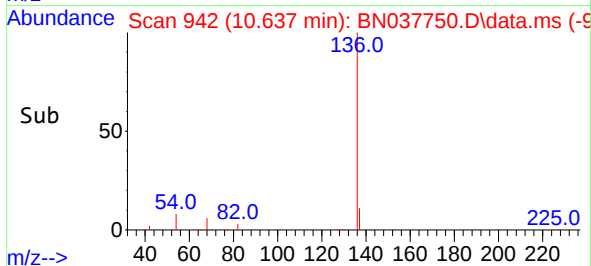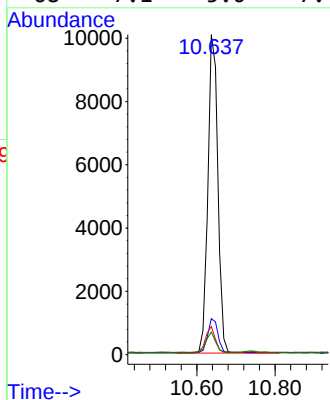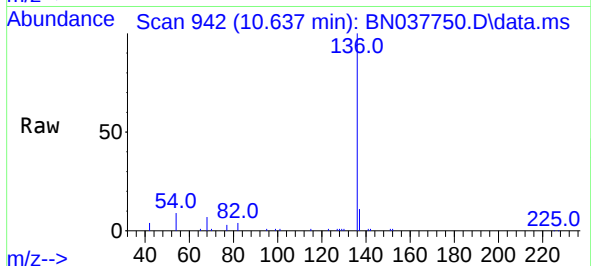

#8
Nitrobenzene-d5
Concen: 0.353 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:	82	Resp:	4613
Ion	Ratio	Lower	Upper
82	100		
128	40.9	38.3	57.5
54	54.1	41.4	62.2


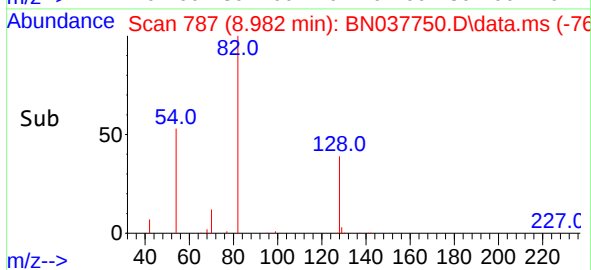
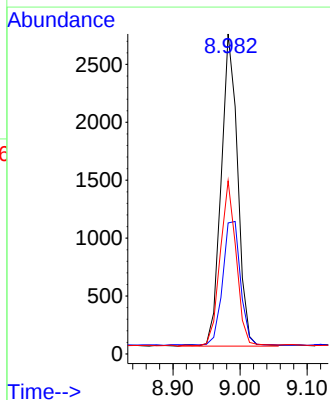





#11
2-Methylnaphthalene-d10
Concen: 0.317 ng
RT: 12.238 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36




Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908


Tgt Ion:152 Resp: 7496
Ion Ratio Lower Upper
152 100
151 20.8 17.0 25.6

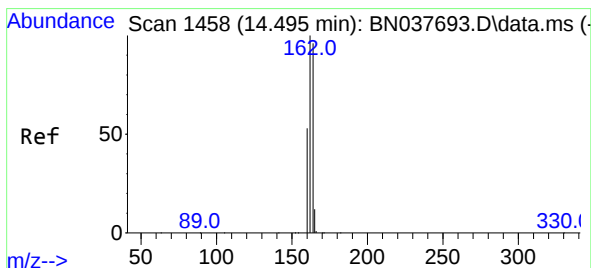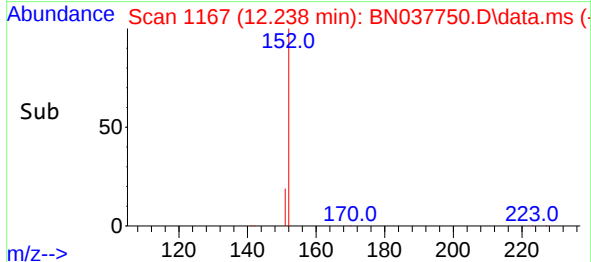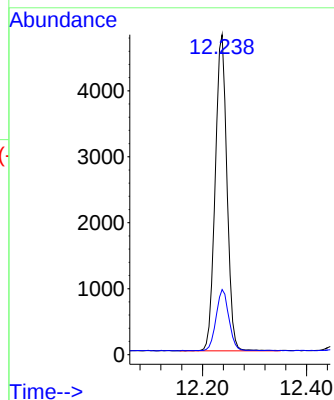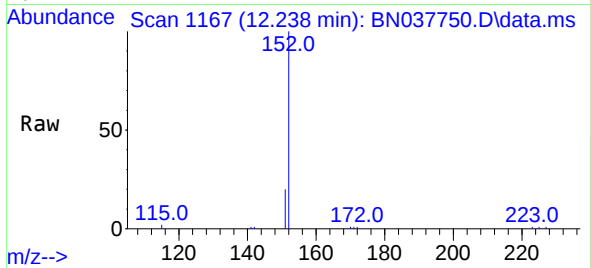

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.495 min Scan# 1458
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:164 Resp: 7906
Ion Ratio Lower Upper
164 100
162 102.2 83.1 124.7
160 53.2 44.3 66.5


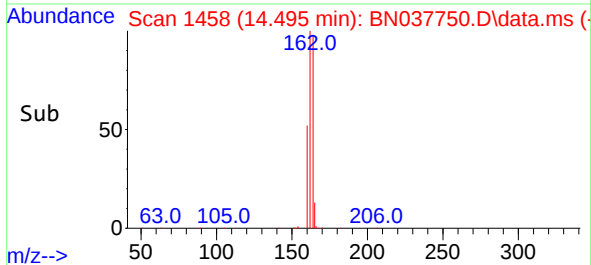
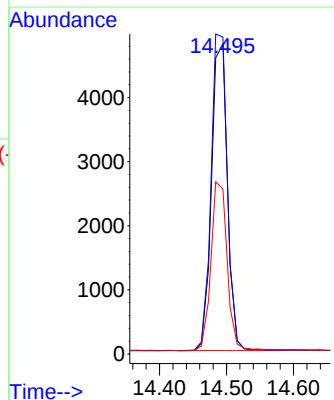
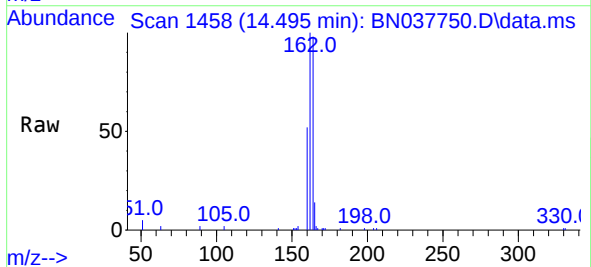




#14
2,4,6-Tribromophenol
Concen: 0.404 ng
RT: 15.982 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36




Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908


Tgt Ion:	330	Resp:	834
Ion	Ratio	Lower	Upper
330	100		
332	93.4	75.3	112.9
141	43.5	35.0	52.4

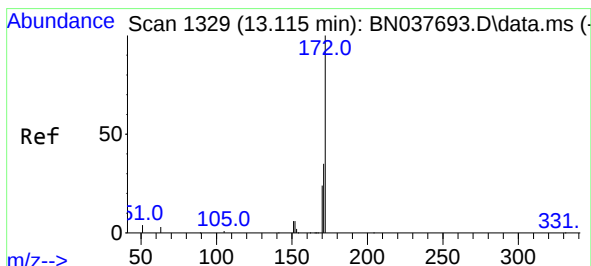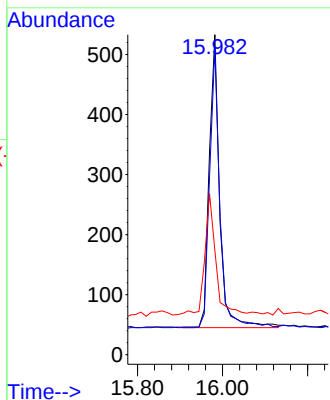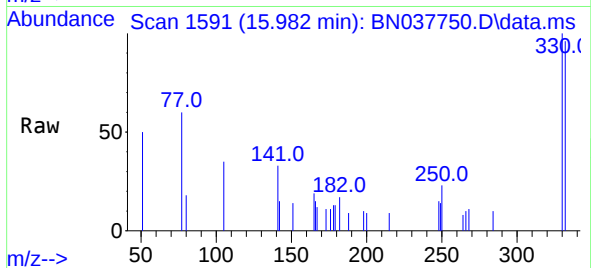

#15
2-Fluorobiphenyl
Concen: 0.359 ng
RT: 13.115 min Scan# 1329
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:	172	Resp:	11872
Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.6	43.0
170	23.7	19.8	29.8


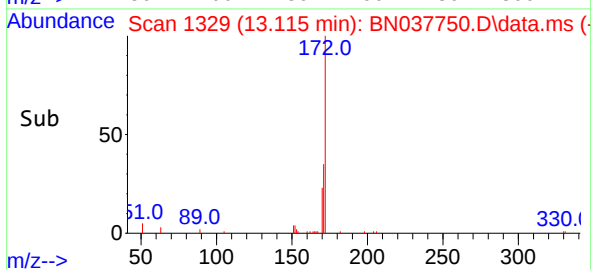
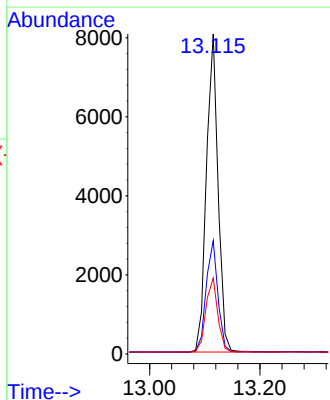



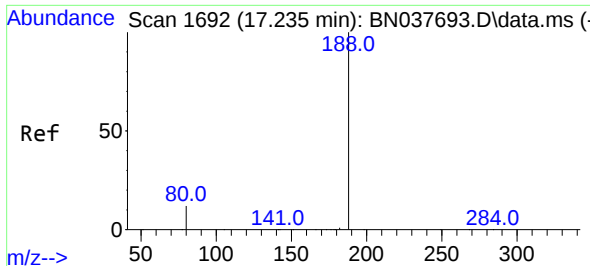

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.235 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36




Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908

Tgt Ion:188 Resp: 13742
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.6 10.6 15.8

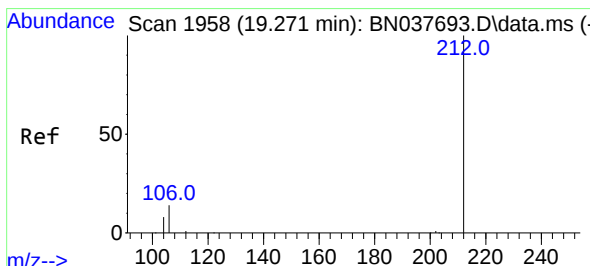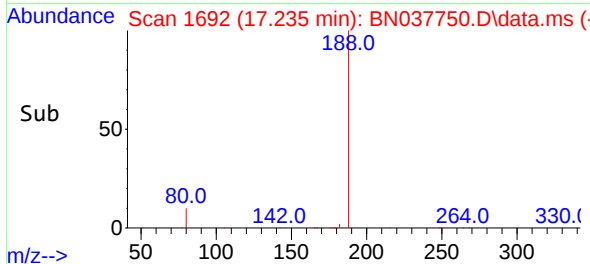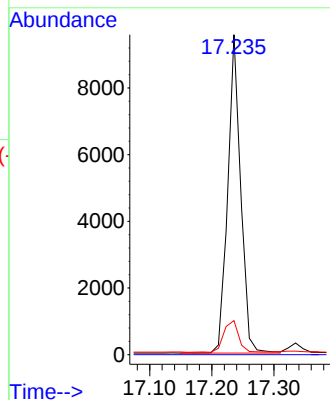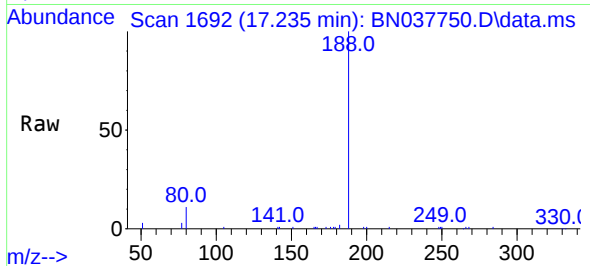

#27
Fluoranthene-d10
Concen: 0.379 ng
RT: 19.267 min Scan# 1957
Delta R.T. -0.005 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:212 Resp: 13070
Ion Ratio Lower Upper
212 100
106 15.4 12.2 18.2
104 8.4 6.9 10.3

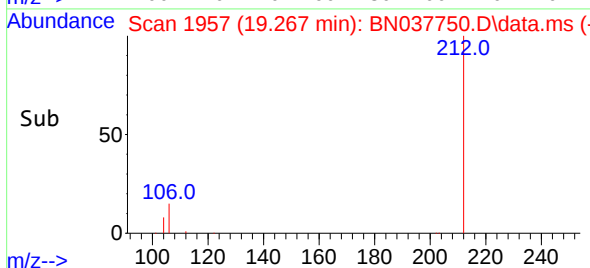
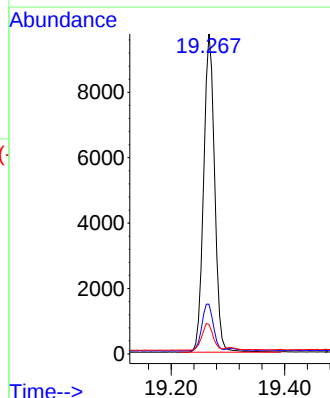
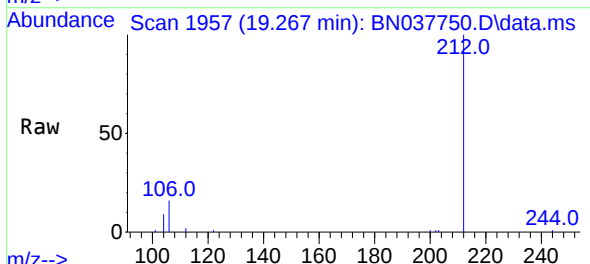




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.411 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36




Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908


Tgt Ion:240 Resp: 11462
Ion Ratio Lower Upper
240 100
120 17.7 9.2 13.8#
236 29.4 22.6 33.8

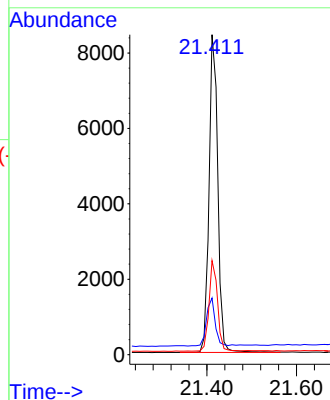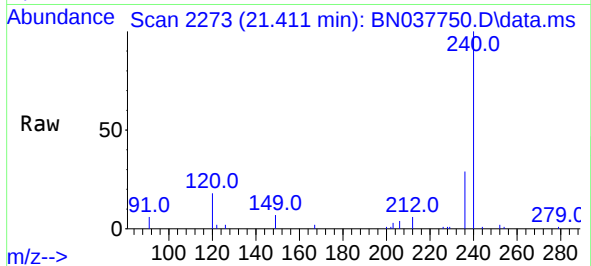

#31
Terphenyl-d14
Concen: 0.429 ng
RT: 19.866 min Scan# 2086
Delta R.T. -0.005 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:244 Resp: 9983
Ion Ratio Lower Upper
244 100
212 8.9 7.5 11.3
122 16.4 13.2 19.8


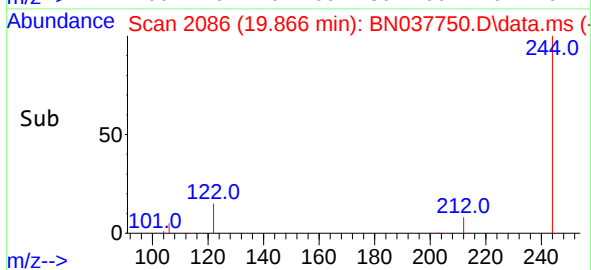
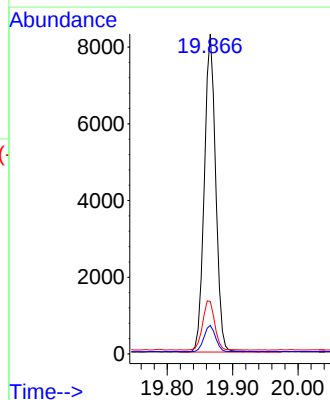



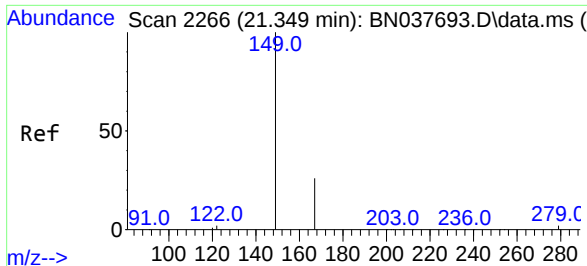

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.179 ng
RT: 21.340 min Scan# 2119
Delta R.T. -0.009 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Instrument :
BNA_N
ClientSampleId :
MW179D1-20250908

Tgt Ion:149 Resp: 2119
Ion Ratio Lower Upper
149 100
167 26.0 20.8 31.2
279 4.6 3.3 4.9

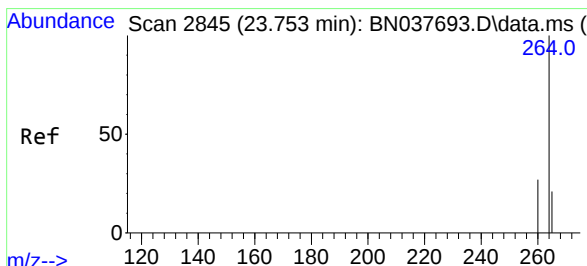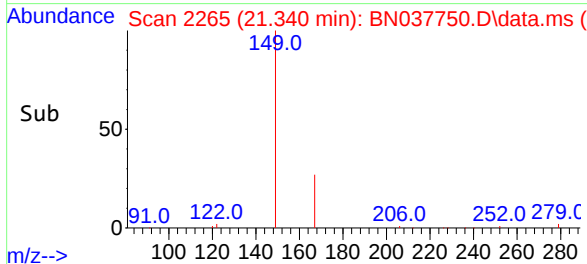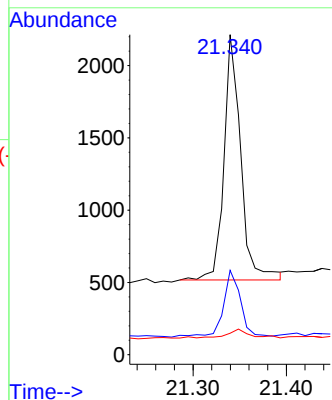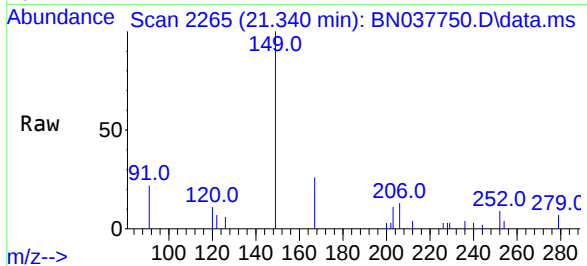

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.747 min Scan# 2843
Delta R.T. -0.006 min
Lab File: BN037750.D
Acq: 17 Sep 2025 17:36

Tgt Ion:264 Resp: 11339
Ion Ratio Lower Upper
264 100
260 26.6 21.8 32.8
265 61.8 39.4 59.2#

