
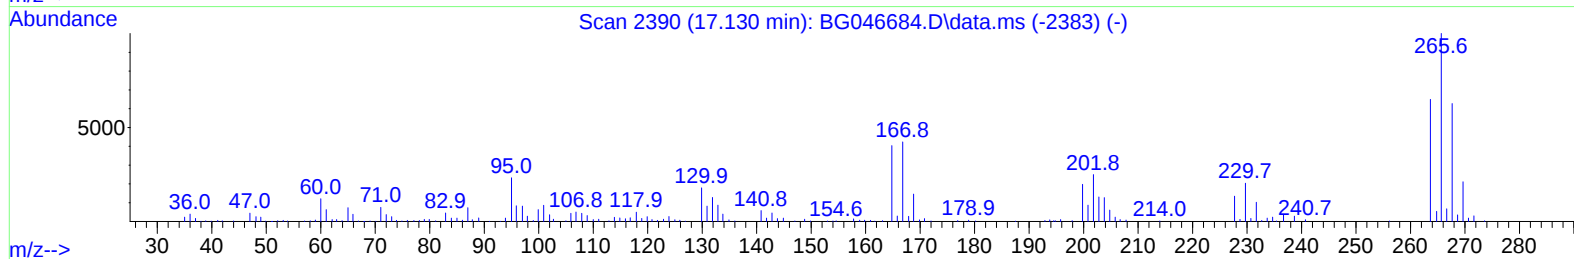
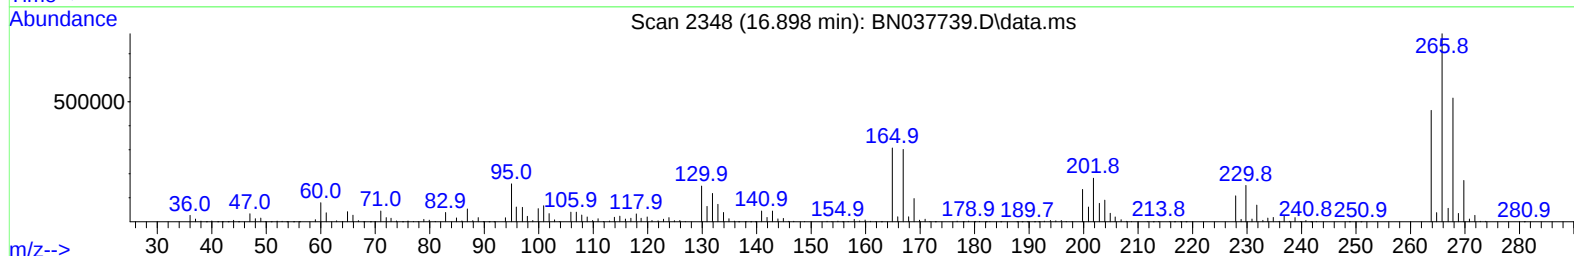


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037739.D
Acq On : 17 Sep 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 12:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 17 12:55:52 2025
Response via : Initial Calibration

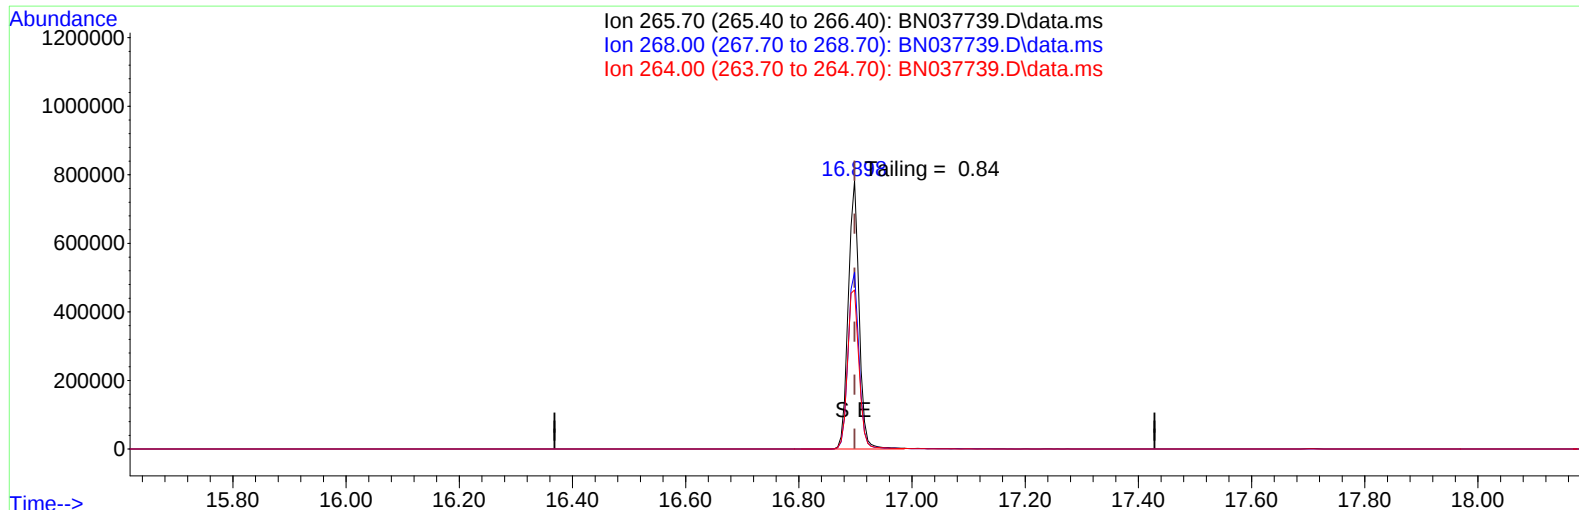

TIC: BN037739.D\data.ms

(70) Pentachlorophenol (C)




16.898min (0.000) 620.62 ng

response 1035710

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.84
264.00	61.60	59.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037739.D
Acq On : 17 Sep 2025 10:46
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 17 12:56:01 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 17 12:55:52 2025
Response via : Initial Calibration

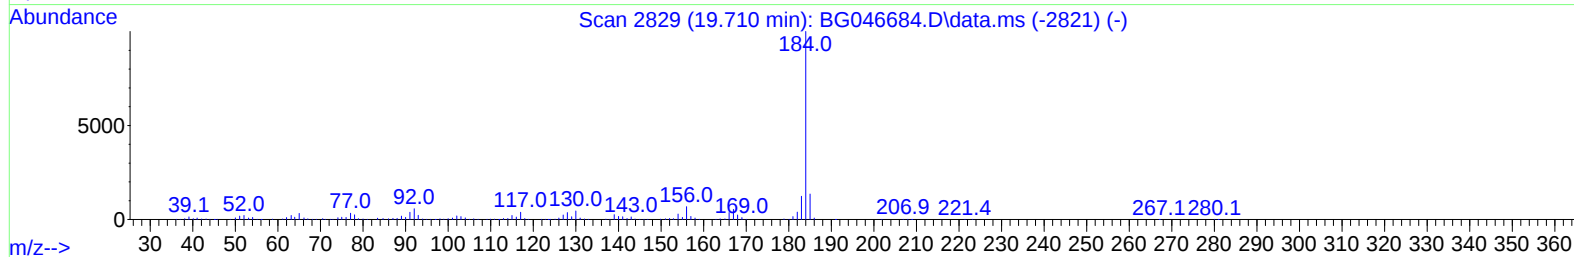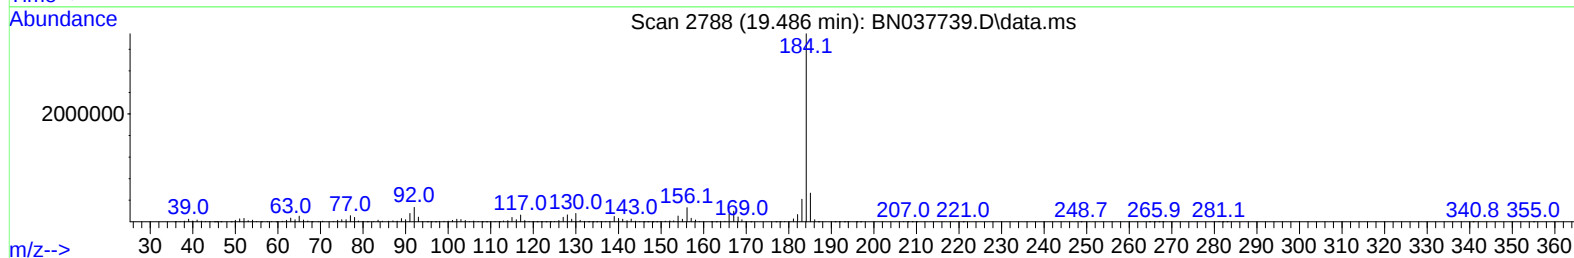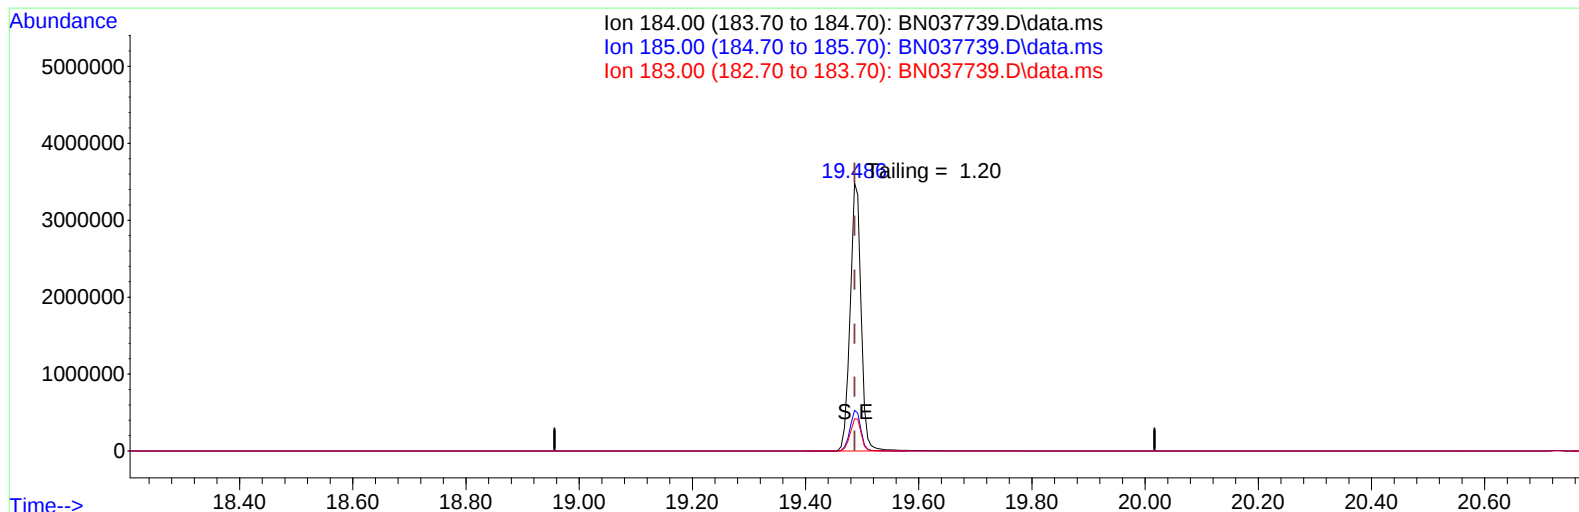

TIC: BN037739.D\data.ms

(77) Benzidine**19.486min (0.000) 3519.75 ng****response 4617215**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.21
183.00	13.20	12.01
0.00	0.00	0.00