
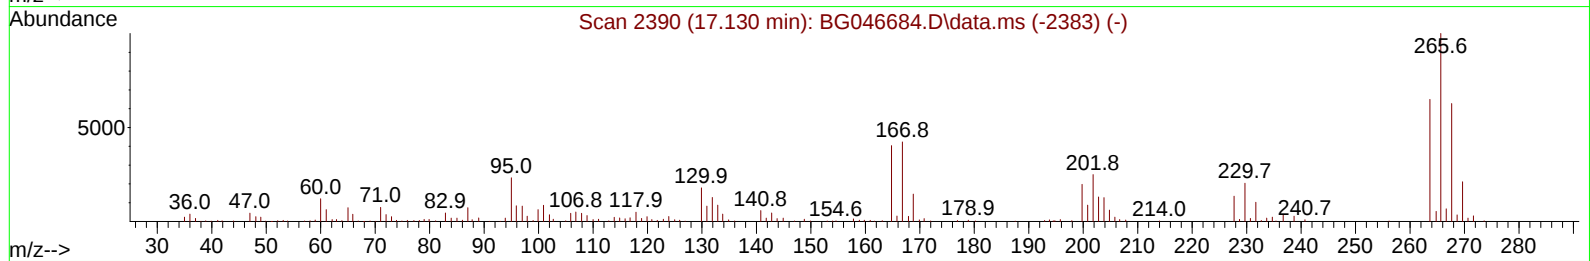
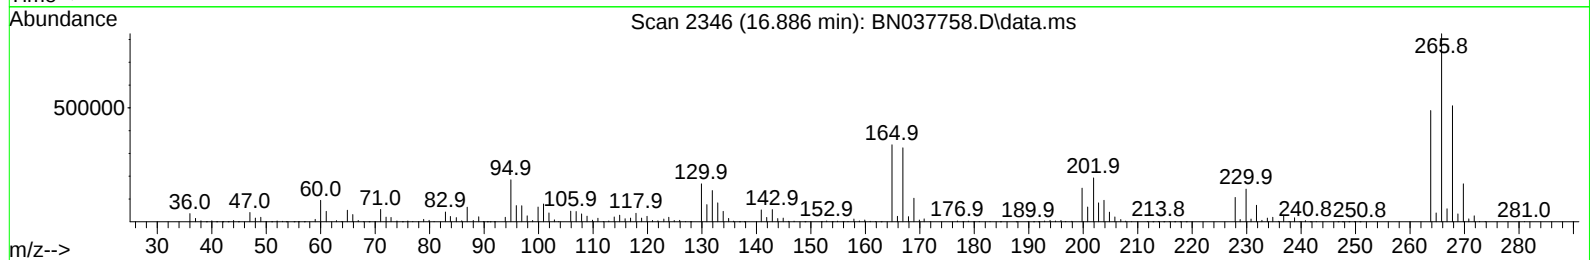


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037758.D
Acq On : 18 Sep 2025 02:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 08:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 08:37:03 2025
Response via : Initial Calibration

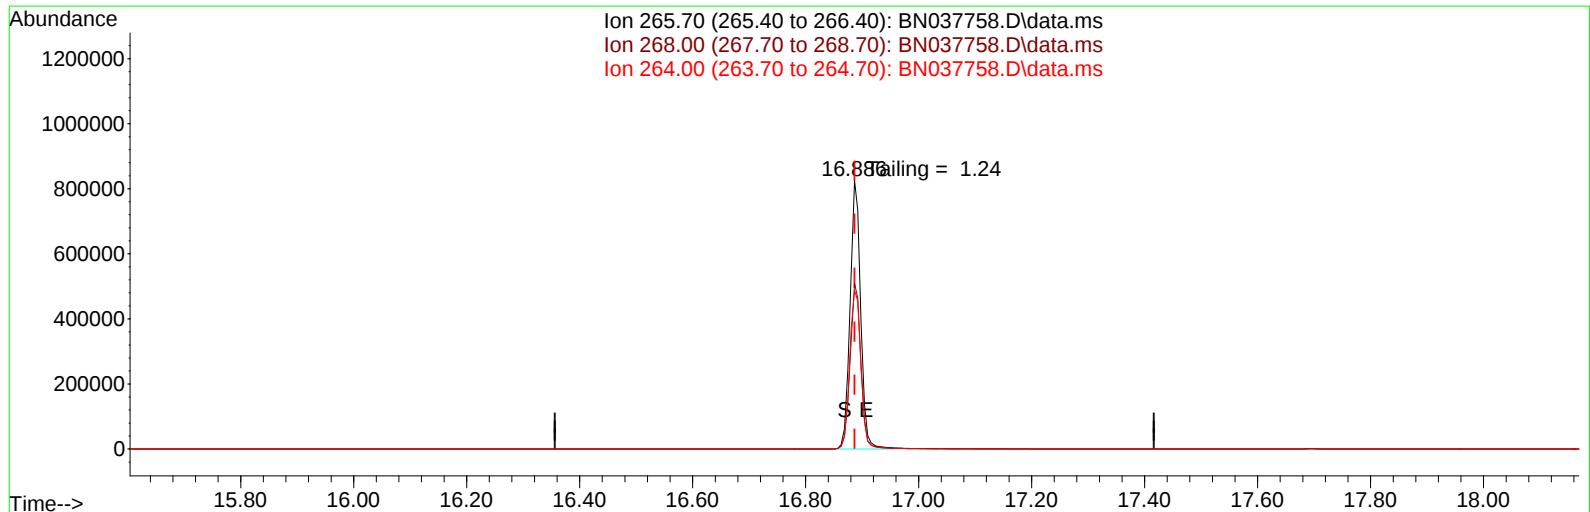

TIC: BN037758.D\data.ms

(70) Pentachlorophenol (C)




16.886min (0.000) 150096.94 ng

response 1070732

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.72
264.00	61.60	59.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037758.D
Acq On : 18 Sep 2025 02:06
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 08:37:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 18 08:37:03 2025
Response via : Initial Calibration

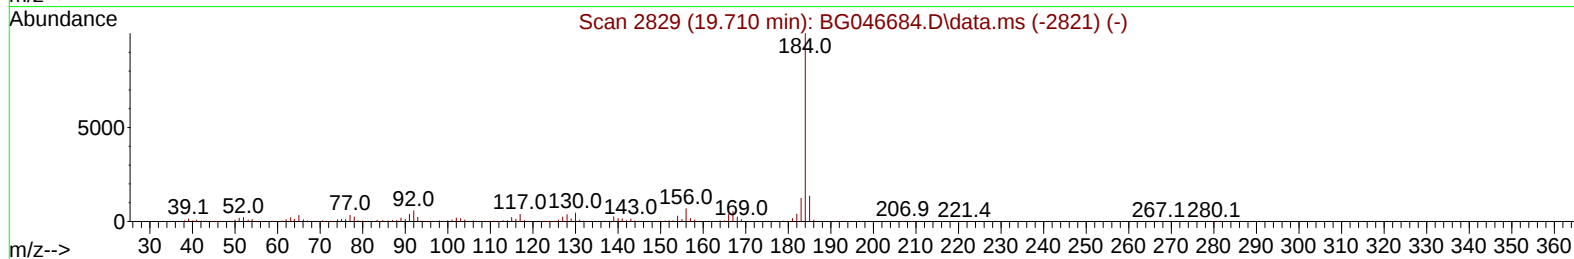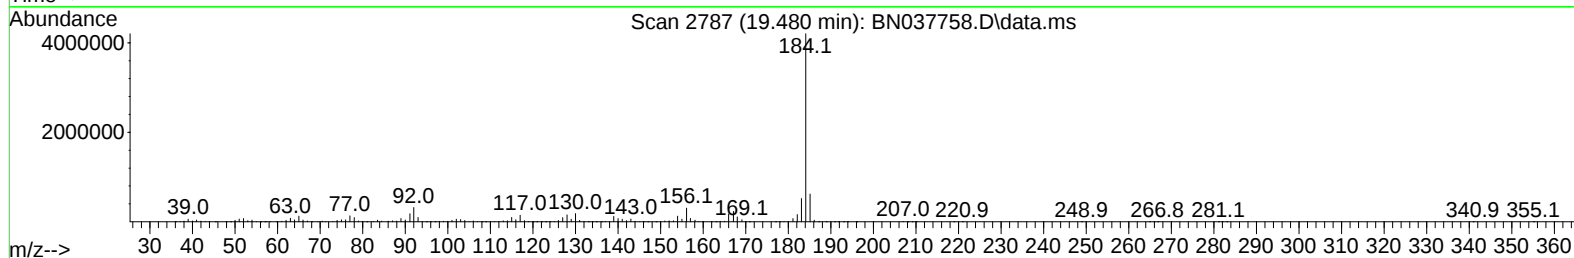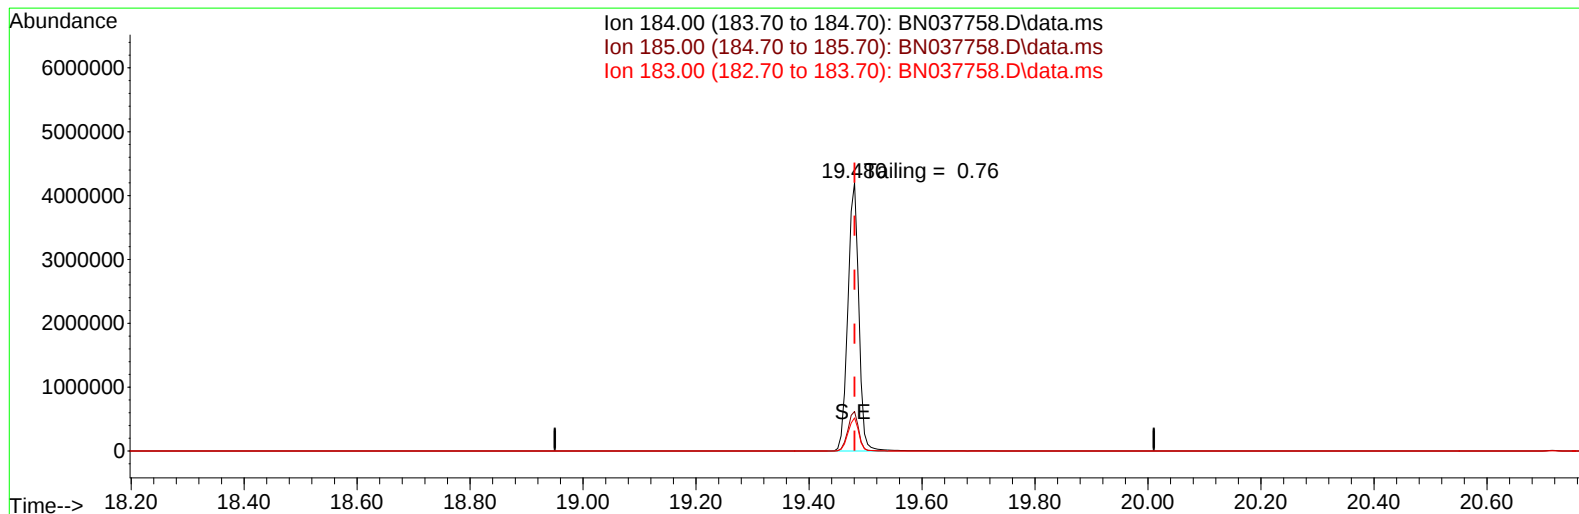

TIC: BN037758.D\data.ms

(77) Benizidine**19.480min (0.000) 95951.94 ng****response 5587198**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.72
183.00	13.20	12.39
0.00	0.00	0.00