

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
 Data File : BN037752.D
 Acq On : 17 Sep 2025 18:49
 Operator : RC/JU
 Sample : Q3095-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW179D2-20250909

Quant Time: Sep 17 19:13:55 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.840	152	6450	0.400	ng	0.00
7) Naphthalene-d8	10.637	136	17530	0.400	ng	-0.01
13) Acenaphthene-d10	14.494	164	7934	0.400	ng	0.00
19) Phenanthrene-d10	17.235	188	13430	0.400	ng	# 0.00
29) Chrysene-d12	21.411	240	10479	0.400	ng	# 0.00
35) Perylene-d12	23.747	264	10489	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.399	112	1456	0.098	ng	0.00
5) Phenol-d6	6.988	99	1014	0.053	ng	0.00
8) Nitrobenzene-d5	8.982	82	4086	0.319	ng	-0.01
11) 2-Methylnaphthalene-d10	12.238	152	6853	0.295	ng	0.00
14) 2,4,6-Tribromophenol	15.982	330	686	0.332	ng	0.00
15) 2-Fluorobiphenyl	13.115	172	10696	0.322	ng	0.00
27) Fluoranthene-d10	19.266	212	11725	0.348	ng	0.00
31) Terphenyl-d14	19.866	244	8402	0.395	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.297	88	4057	0.604	ng	# 94
34) Bis(2-ethylhexyl)phtha...	21.339	149	1006	0.093	ng	# 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091725\
Data File : BN037752.D
Acq On : 17 Sep 2025 18:49
Operator : RC/JU
Sample : Q3095-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Quant Time: Sep 17 19:13:55 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration

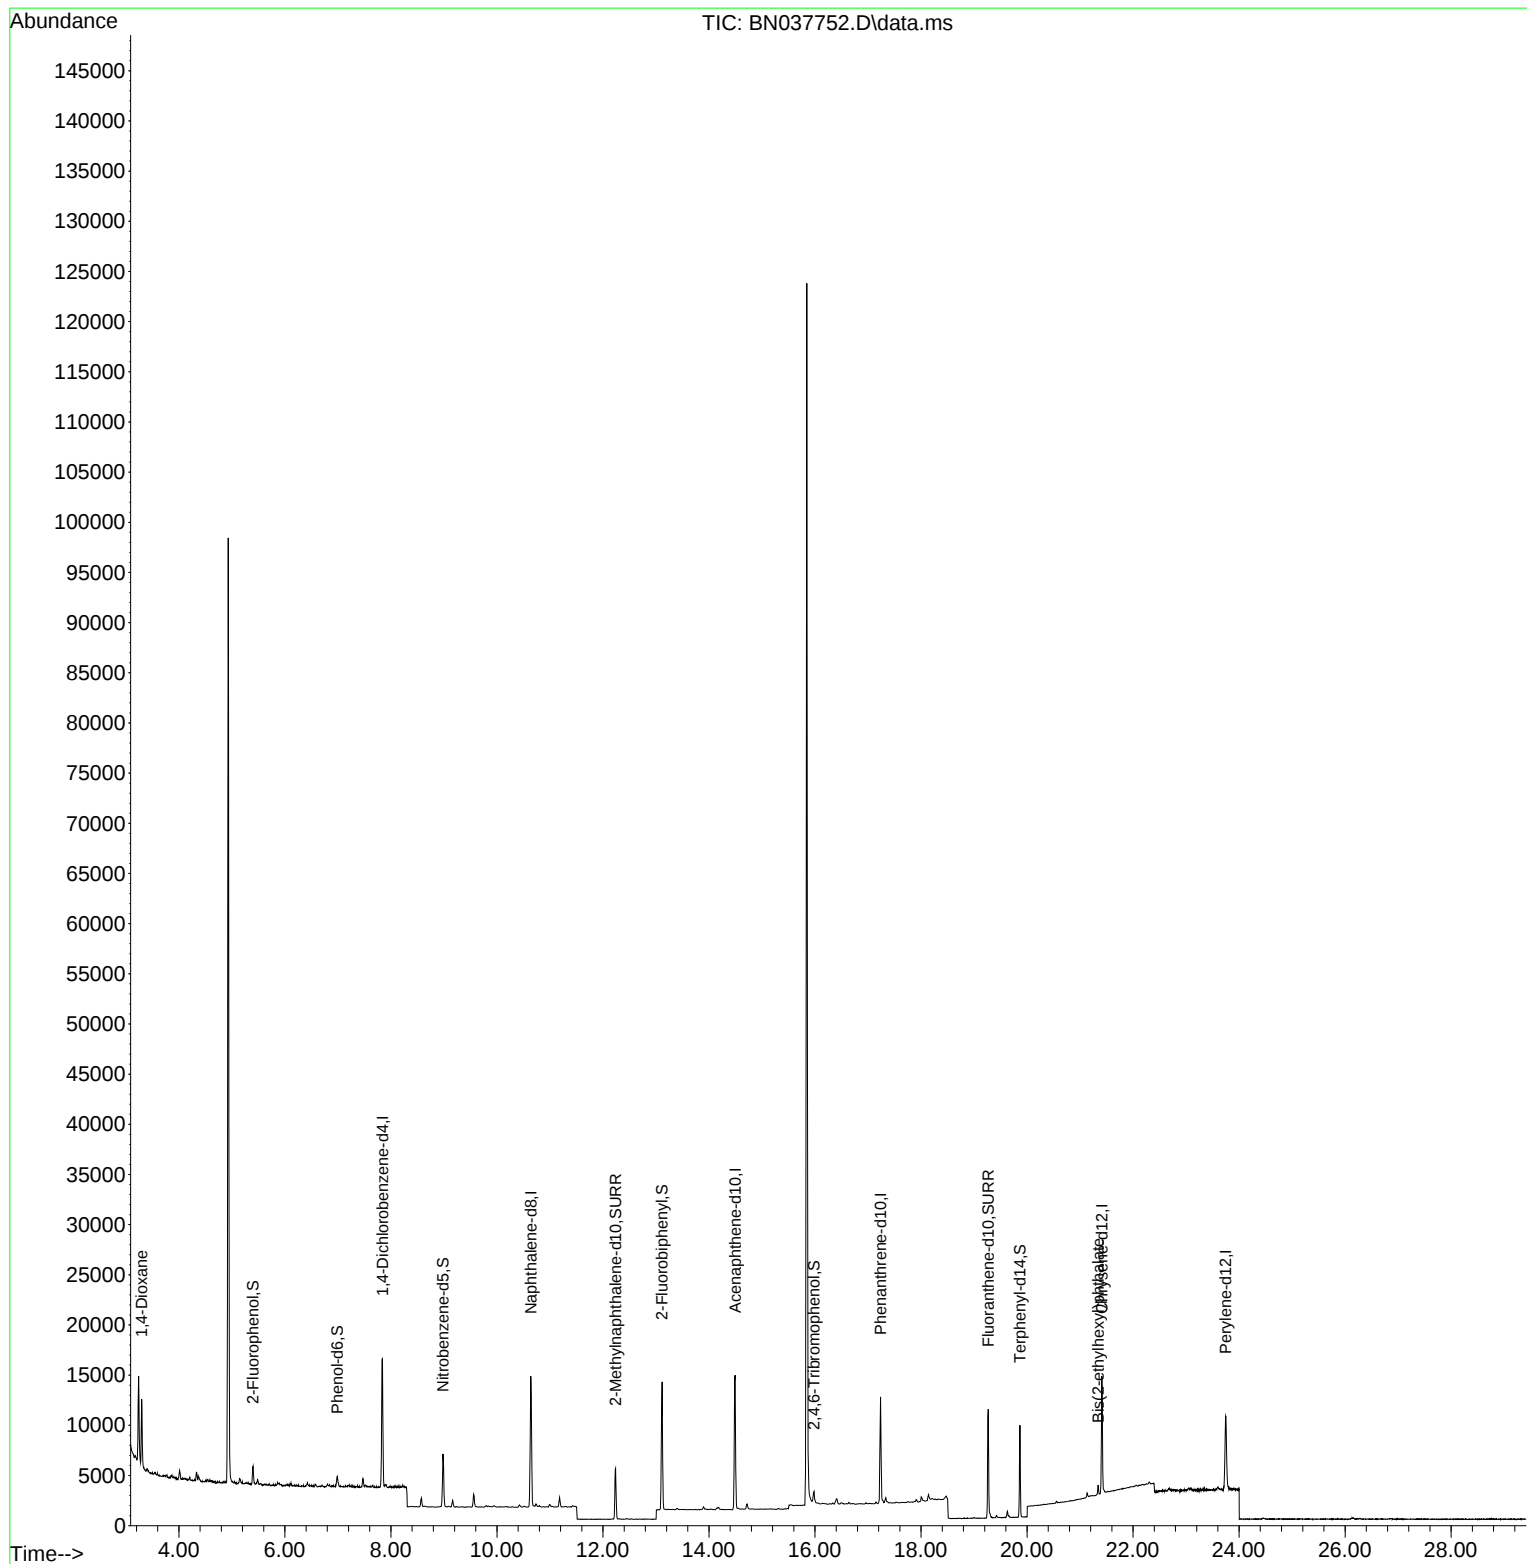






#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.840 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: BN037752.D
 Acq: 17 Sep 2025 18:49

Instrument :
 BNA_N
 ClientSampleId :
 MW179D2-20250909







Tgt Ion:152 Resp: 6450
 Ion Ratio Lower Upper
 152 100
 150 150.0 124.5 186.7
 115 58.2 49.2 73.8

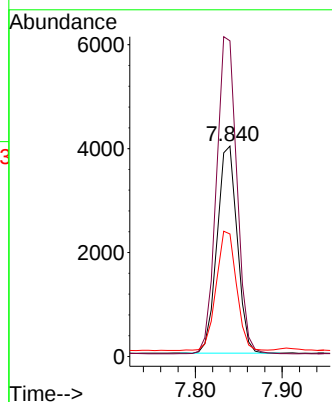

#2
 1,4-Dioxane
 Concen: 0.604 ng
 RT: 3.297 min Scan# 30
 Delta R.T. -0.007 min
 Lab File: BN037752.D
 Acq: 17 Sep 2025 18:49

Tgt Ion: 88 Resp: 4057
 Ion Ratio Lower Upper
 88 100
 43 42.4 26.8 40.2#
 58 76.2 61.9 92.9


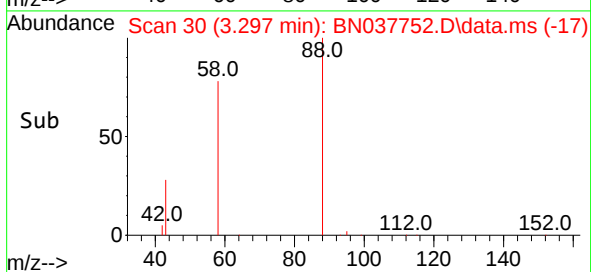
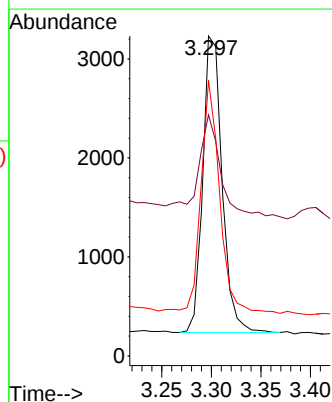





#4
2-Fluorophenol
Concen: 0.098 ng
RT: 5.399 min Scan# 321
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion: 112 Resp: 1456
Ion Ratio Lower Upper
112 100
64 52.8 44.9 67.3
63 29.1 24.7 37.1

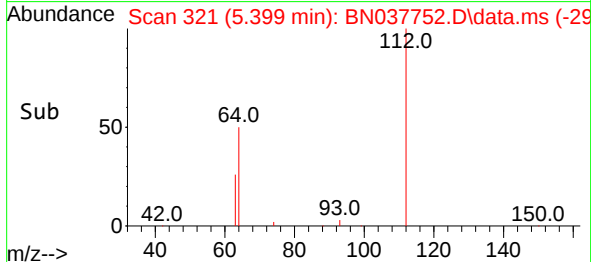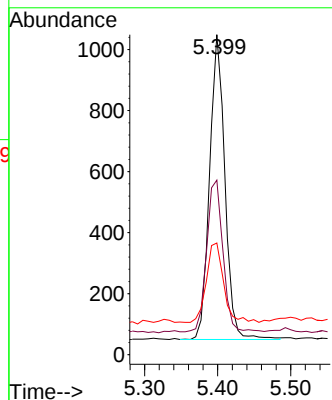

#5
Phenol-d6
Concen: 0.053 ng
RT: 6.988 min Scan# 541
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion: 99 Resp: 1014
Ion Ratio Lower Upper
99 100
42 23.3 16.6 24.8
71 37.9 26.7 40.1


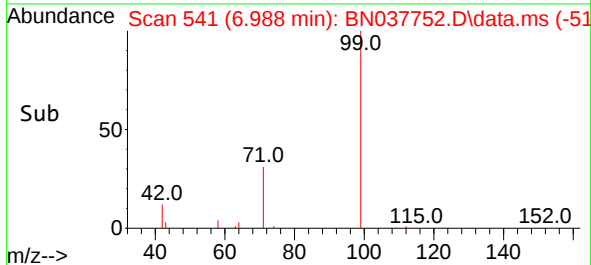
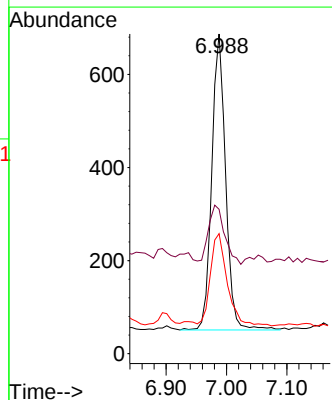
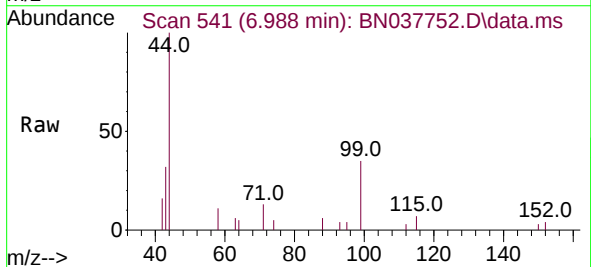




#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.637 min Scan# 94
Delta R.T. -0.011 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion:	136	Resp:	17530
Ion	Ratio	Lower	Upper
136	100		
137	11.6	9.1	13.7
54	8.9	6.3	9.5
68	6.8	5.0	7.4

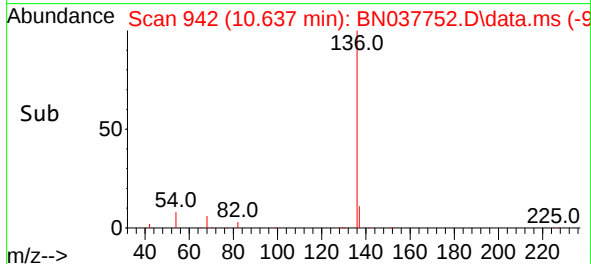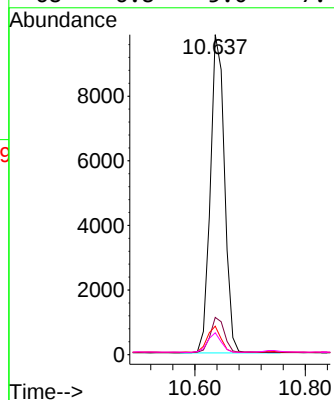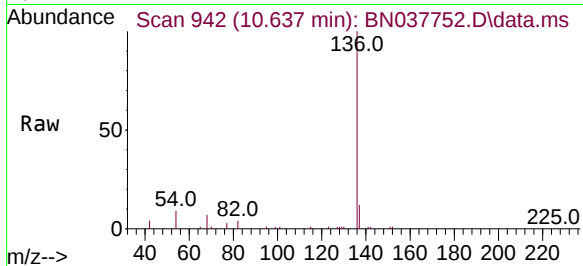

#8
Nitrobenzene-d5
Concen: 0.319 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion:	82	Resp:	4086
Ion	Ratio	Lower	Upper
82	100		
128	41.1	38.3	57.5
54	53.1	41.4	62.2


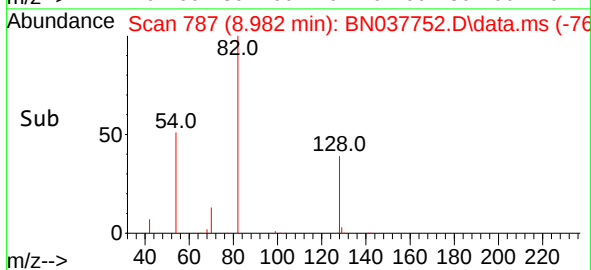
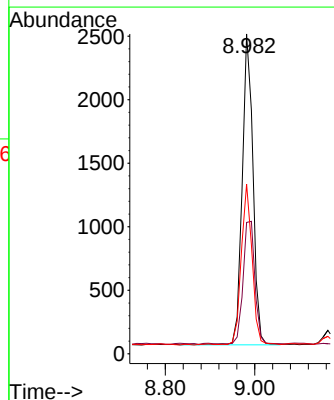
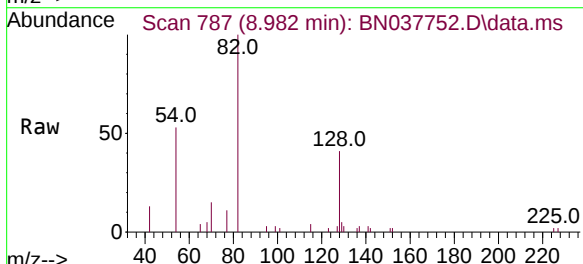




#11
2-Methylnaphthalene-d10
Concen: 0.295 ng
RT: 12.238 min Scan# 1167
Delta R.T. -0.005 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion:152 Resp: 6853
Ion Ratio Lower Upper
152 100
151 21.2 17.0 25.6

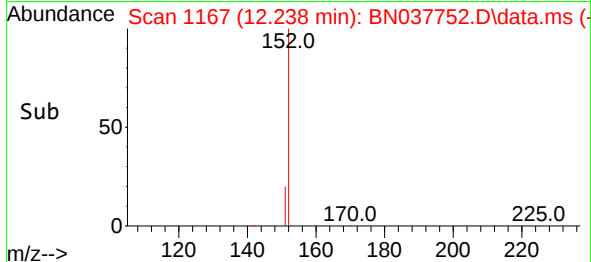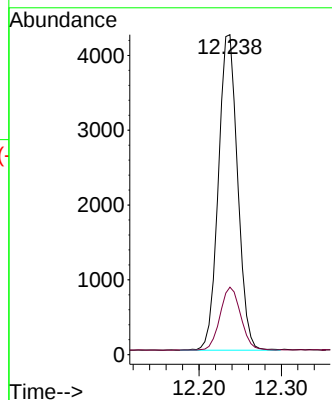

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.494 min Scan# 1458
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion:164 Resp: 7934
Ion Ratio Lower Upper
164 100
162 103.2 83.1 124.7
160 52.8 44.3 66.5


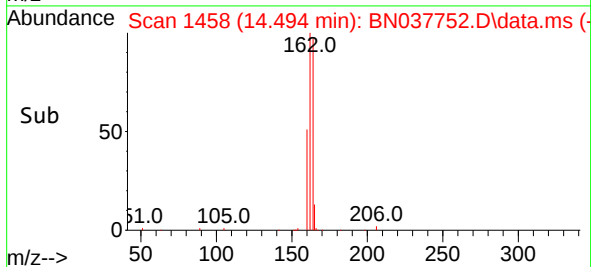
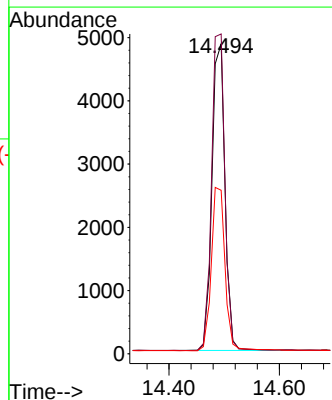
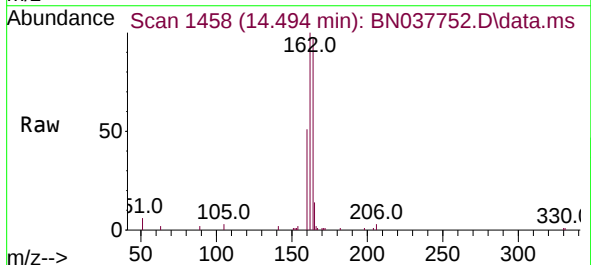




#14
2,4,6-Tribromophenol
Concen: 0.332 ng
RT: 15.982 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion:	330	Resp:	686
Ion Ratio	Lower	Upper	
330	100		
332	100.1	75.3	112.9
141	46.5	35.0	52.4

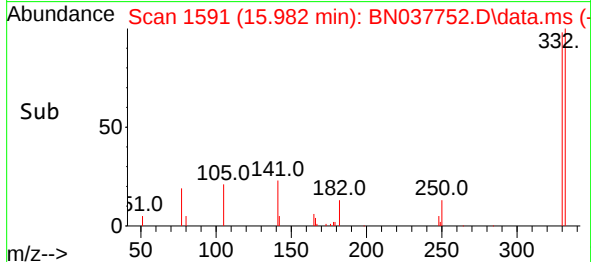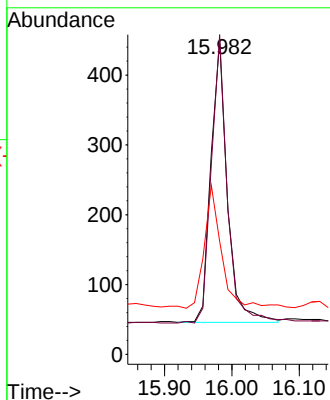

#15
2-Fluorobiphenyl
Concen: 0.322 ng
RT: 13.115 min Scan# 1329
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion:	172	Resp:	10696
Ion Ratio	Lower	Upper	
172	100		
171	35.0	28.6	43.0
170	24.0	19.8	29.8


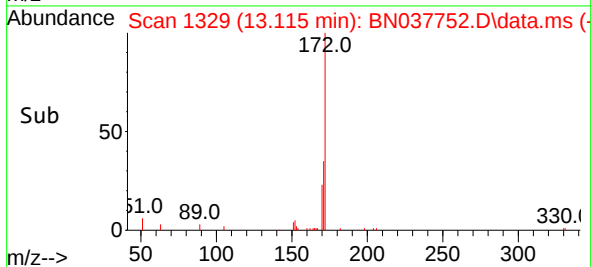
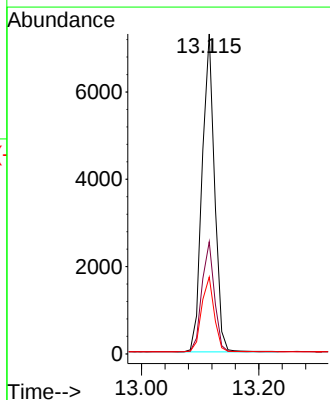
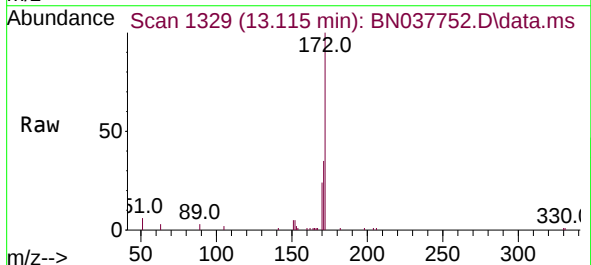




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.235 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion:188 Resp: 13430
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.3 10.6 15.8#

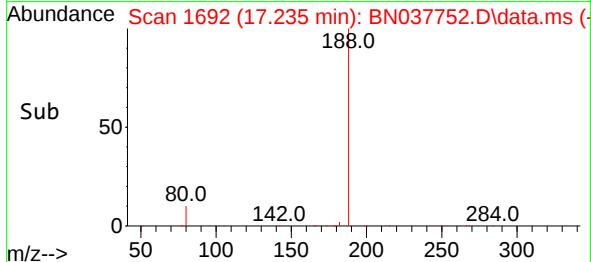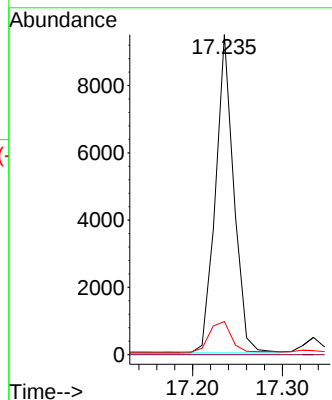

#27
Fluoranthene-d10
Concen: 0.348 ng
RT: 19.266 min Scan# 1957
Delta R.T. -0.005 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion:212 Resp: 11725
Ion Ratio Lower Upper
212 100
106 15.4 12.2 18.2
104 8.8 6.9 10.3


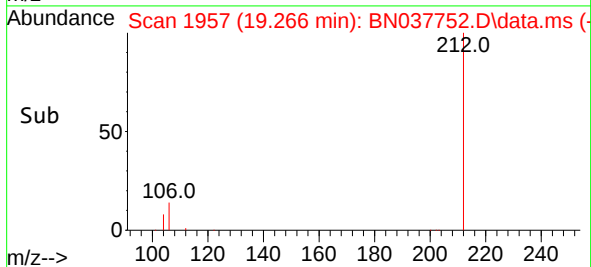
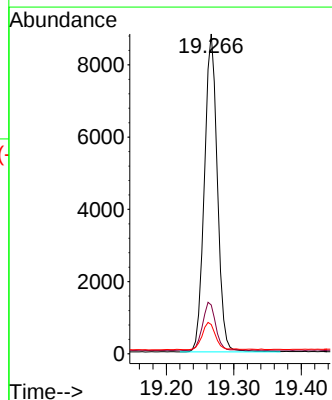
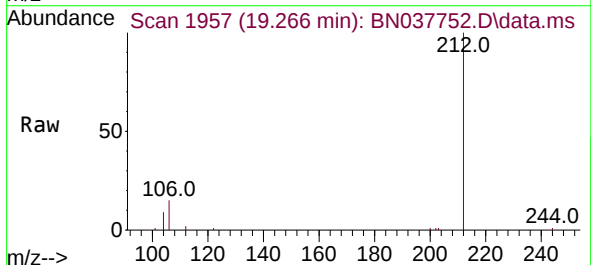




#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.411 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49




Instrument :
BNA_N
ClientSampleId :
MW179D2-20250909


Tgt Ion:240 Resp: 10479
Ion Ratio Lower Upper
240 100
120 16.9 9.2 13.8#
236 29.2 22.6 33.8

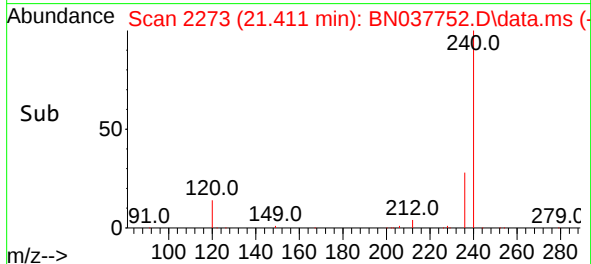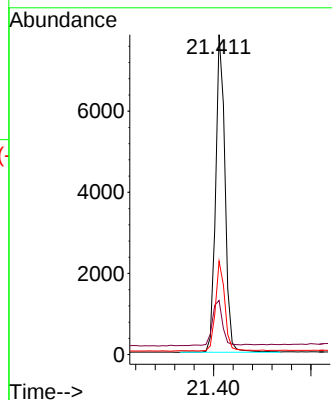

#31
Terphenyl-d14
Concen: 0.395 ng
RT: 19.866 min Scan# 2086
Delta R.T. -0.005 min
Lab File: BN037752.D
Acq: 17 Sep 2025 18:49

Tgt Ion:244 Resp: 8402
Ion Ratio Lower Upper
244 100
212 9.4 7.5 11.3
122 16.2 13.2 19.8


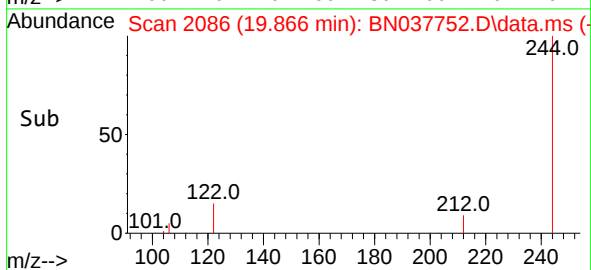
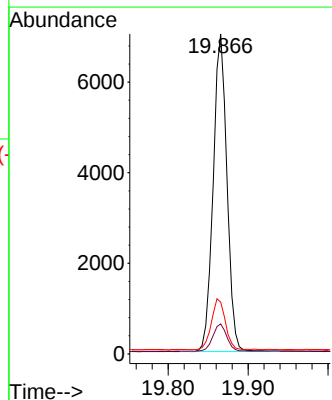
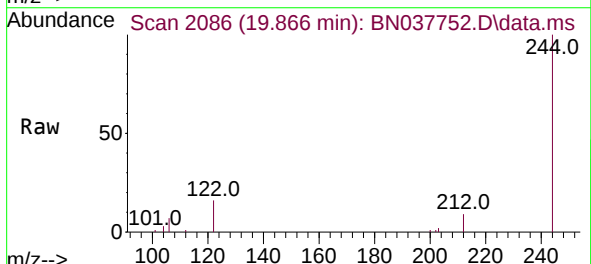


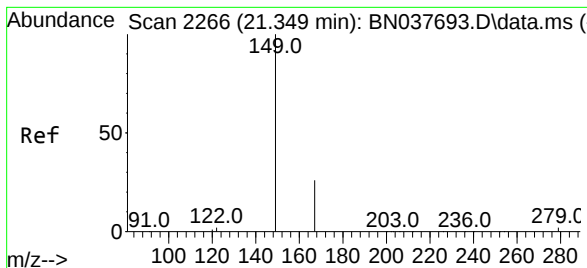

#34
 Bis(2-ethylhexyl)phthalate
 Concen: 0.093 ng
 RT: 21.339 min Scan# 21
 Delta R.T. -0.009 min
 Lab File: BN037752.D
 Acq: 17 Sep 2025 18:49

Instrument :
 BNA_N
 ClientSampleId :
 MW179D2-20250909

Tgt Ion:149 Resp: 1006
 Ion Ratio Lower Upper
 149 100
 167 25.0 20.8 31.2
 279 6.3 3.3 4.9#

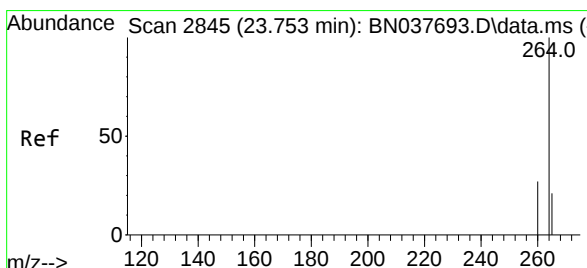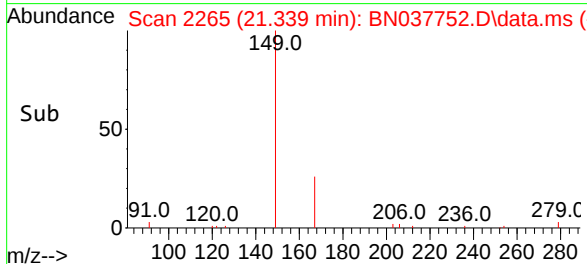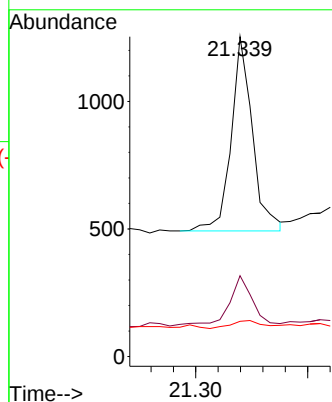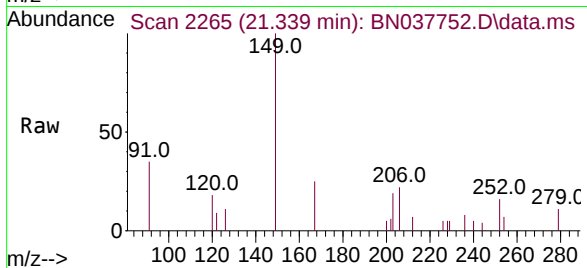

#35
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.747 min Scan# 2843
 Delta R.T. -0.006 min
 Lab File: BN037752.D
 Acq: 17 Sep 2025 18:49

Tgt Ion:264 Resp: 10489
 Ion Ratio Lower Upper
 264 100
 260 26.2 21.8 32.8
 265 65.3 39.4 59.2#

