

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091820\
 Data File : BN011838.D
 Acq On : 18 Sep 2020 16:45
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Quant Time: Sep 18 17:13:47 2020
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 18 10:47:35 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.715	152	2126	0.40	ng	0.00
7) Naphthalene-d8	10.504	136	7921	0.40	ng	0.01
13) Acenaphthene-d10	14.357	164	4886	0.40	ng	0.00
19) Phenanthrene-d10	17.102	188	11352	0.40	ng	0.00
29) Chrysene-d12	21.312	240	11976	0.40	ng	# 0.00
36) Perylene-d12	23.566	264	11759	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.307	112	2698	0.43	ng	0.00
5) Phenol-d6	6.877	99	3241	0.42	ng	0.00
8) Nitrobenzene-d5	8.856	82	3364	0.42	ng	0.00
11) 2-Methylnaphthalene-d10	12.091	152	5947	0.42	ng	0.00
14) 2,4,6-Tribromophenol	15.854	330	1127	0.45	ng	0.00
15) 2-Fluorobiphenyl	12.974	172	8779	0.42	ng	0.00
27) Fluoranthene-d10	19.147	212	14449	0.40	ng	0.00
31) Terphenyl-d14	19.752	244	12152	0.44	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.270	88	1149	0.36	ng	98
3) n-Nitrosodimethylamine	3.576	42	1854	0.44	ng	90
6) bis(2-Chloroethyl)ether	7.143	93	2739	0.40	ng	100
9) Naphthalene	10.542	128	9268	0.42	ng	99
10) Hexachlorobutadiene	10.846	225	2184	0.42	ng	# 99
12) 2-Methylnaphthalene	12.167	142	6491	0.42	ng	98
16) Acenaphthylene	14.078	152	9490	0.40	ng	99
17) Acenaphthene	14.420	154	6855	0.42	ng	97
18) Fluorene	15.410	166	8587	0.42	ng	99
20) 4,6-Dinitro-2-methylph...	15.486	198	784	0.40	ng	# 83
21) 4-Bromophenyl-phenylether	16.299	248	2669	0.39	ng	# 60
22) Hexachlorobenzene	16.420	284	3319	0.40	ng	98
23) Atrazine	16.579	200	2362	0.39	ng	99
24) Pentachlorophenol	16.761	266	1330	0.39	ng	99
25) Phenanthrene	17.151	178	14494	0.40	ng	99
26) Anthracene	17.236	178	12248	0.39	ng	100
28) Fluoranthene	19.176	202	17129	0.41	ng	99
30) Pyrene	19.539	202	16963	0.41	ng	100
32) Benzo(a)anthracene	21.290	228	15838	0.39	ng	97
33) Chrysene	21.343	228	17256	0.41	ng	98
34) Bis(2-ethylhexyl)phtha...	21.237	149	7426	0.36	ng	99
35) Indeno(1,2,3-cd)pyrene	25.825	276	21308	0.41	ng	98
37) Benzo(b)fluoranthene	22.888	252	18015	0.41	ng	# 96
38) Benzo(k)fluoranthene	22.933	252	18818	0.42	ng	# 97
39) Benzo(a)pyrene	23.467	252	15916	0.41	ng	# 92
40) Dibenzo(a,h)anthracene	25.842	278	17310	0.40	ng	96
41) Benzo(g,h,i)perylene	26.513	276	18361	0.40	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091820\
Data File : BN011838.D
Acq On : 18 Sep 2020 16:45
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Quant Time: Sep 18 17:13:47 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 10:47:35 2020
Response via : Initial Calibration

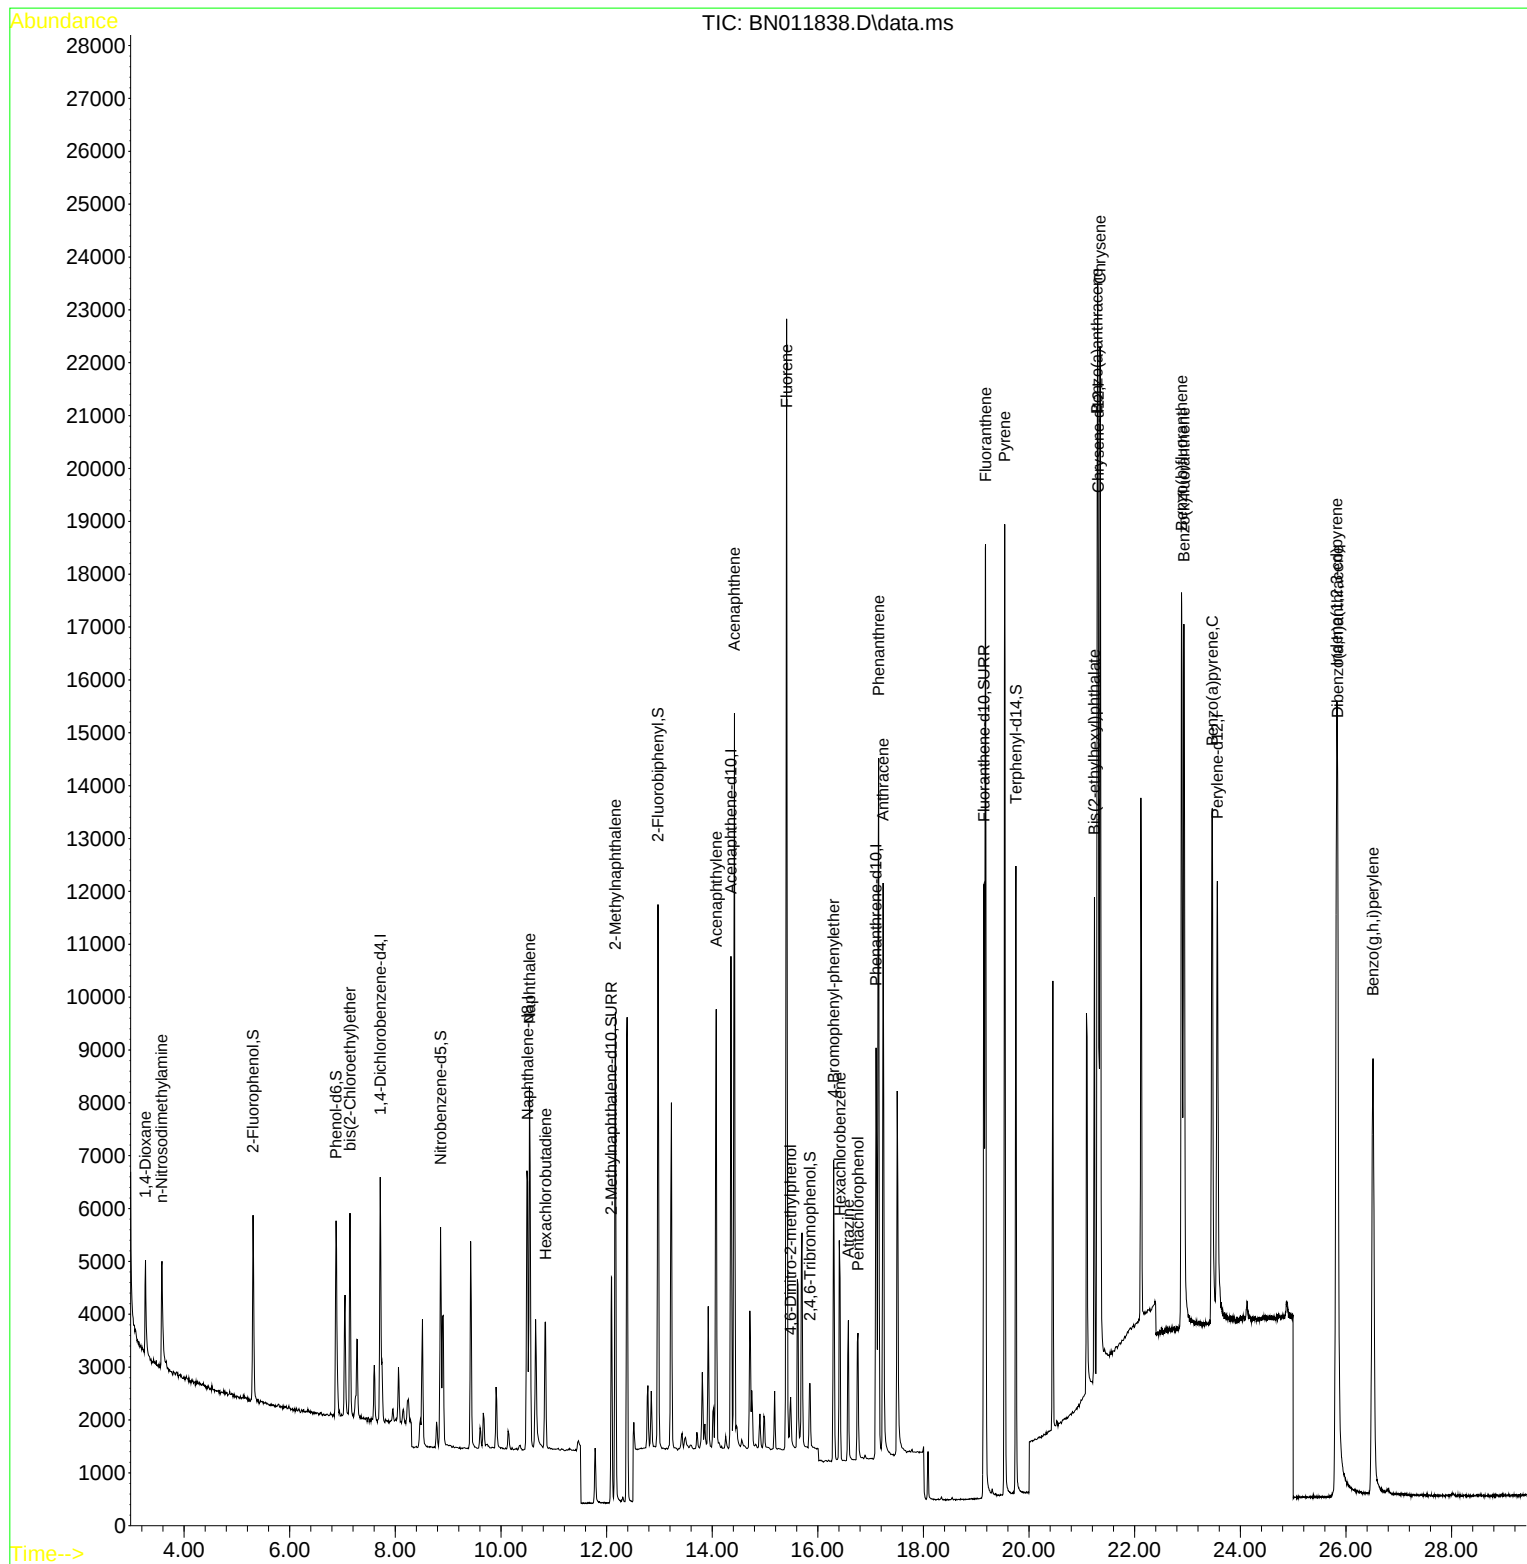






#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.715 min Scan# 588
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC

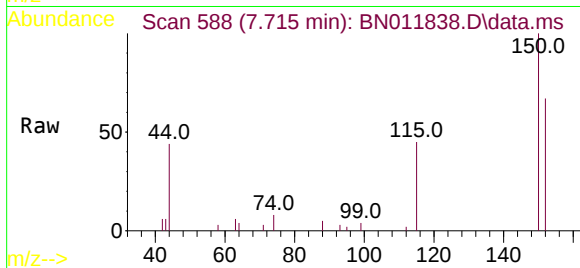



Tgt Ion:152 Resp: 2126
Ion Ratio Lower Upper
152 100
150 150.4 118.3 177.5
115 67.6 51.3 76.9

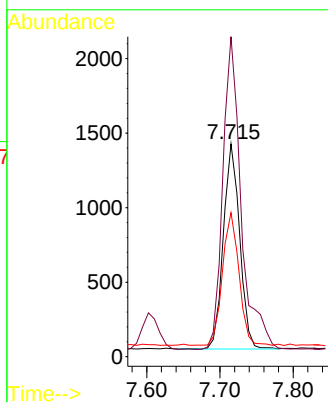


#2
1,4-Dioxane
Concen: 0.36 ng
RT: 3.270 min Scan# 36
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

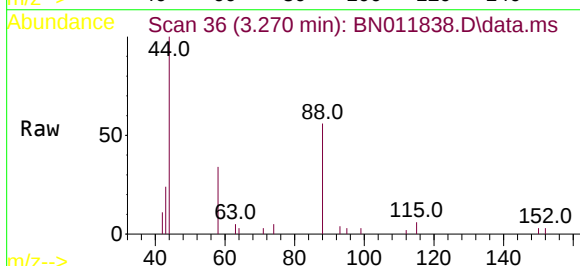

Tgt Ion: 88 Resp: 1149
Ion Ratio Lower Upper
88 100
58 78.9 63.3 94.9
43 37.2 33.0 49.4



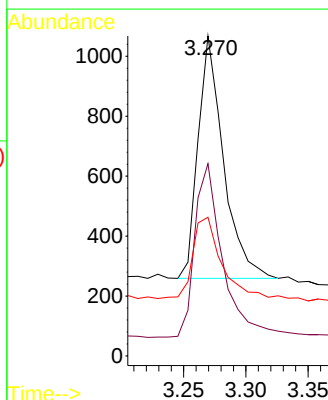



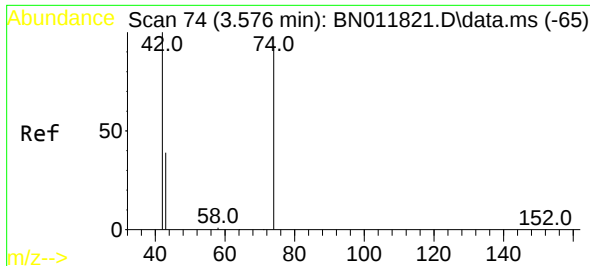

#3
n-Nitrosodimethylamine
Concen: 0.44 ng
RT: 3.576 min Scan# 74
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 42 Resp: 1854
Ion Ratio Lower Upper
42 100
74 89.9 64.4 96.6
44 7.2 6.7 10.1

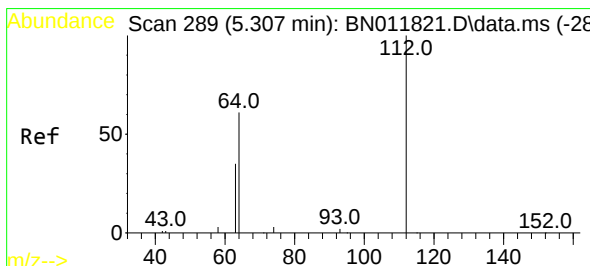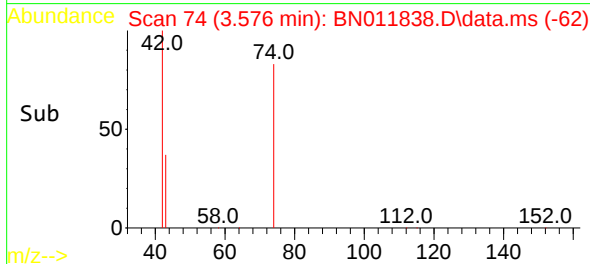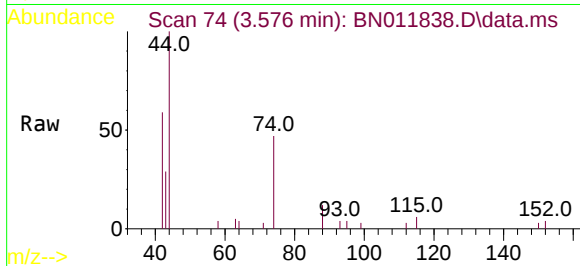

#4
2-Fluorophenol
Concen: 0.43 ng
RT: 5.307 min Scan# 289
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion: 112 Resp: 2698
Ion Ratio Lower Upper
112 100
64 62.9 49.0 73.6
63 36.7 31.8 47.6


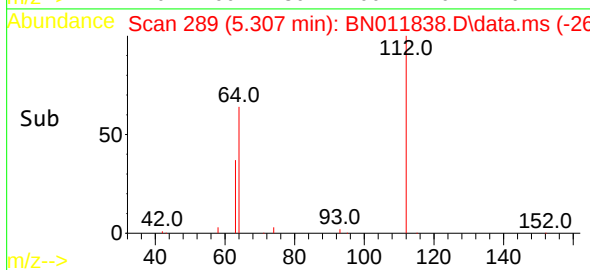

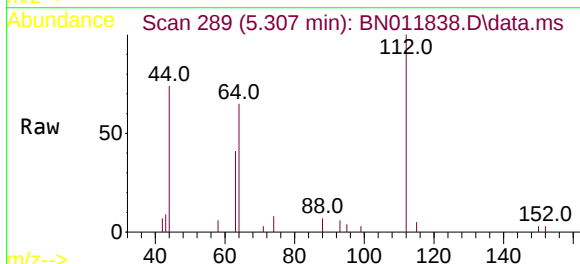




#5
Phenol-d6
Concen: 0.42 ng
RT: 6.877 min Scan# 484
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion: 99 Resp: 3241
Ion Ratio Lower Upper
99 100
42 26.8 23.4 35.0
71 44.5 38.1 57.1



#6
bis(2-Chloroethyl)ether
Concen: 0.40 ng
RT: 7.143 min Scan# 517
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion: 93 Resp: 2739
Ion Ratio Lower Upper
93 100
63 76.6 61.1 91.7
95 31.8 25.5 38.3


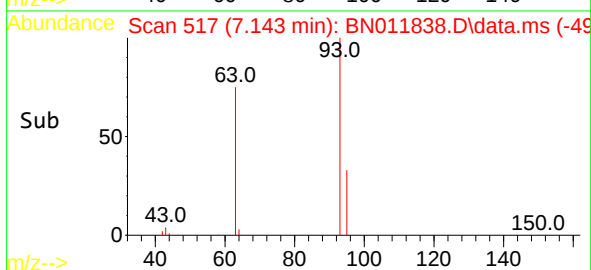
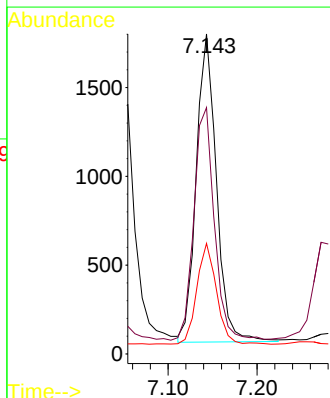





#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.504 min Scan# 835
Delta R.T. 0.013 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	136	Resp:	7921
Ion	Ratio	Lower	Upper
136	100		
137	11.9	9.5	14.3
54	5.6	5.6	8.4
68	4.0	3.2	4.8

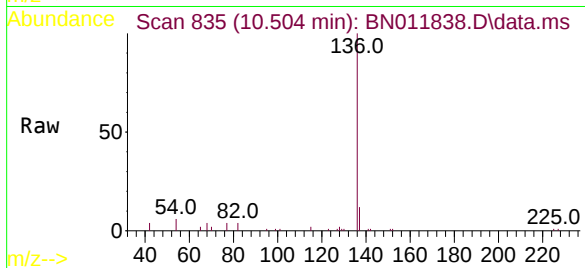

#8
Nitrobenzene-d5
Concen: 0.42 ng
RT: 8.856 min Scan# 705
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:	82	Resp:	3364
Ion	Ratio	Lower	Upper
82	100		
128	35.3	34.2	51.2
54	58.3	43.1	64.7


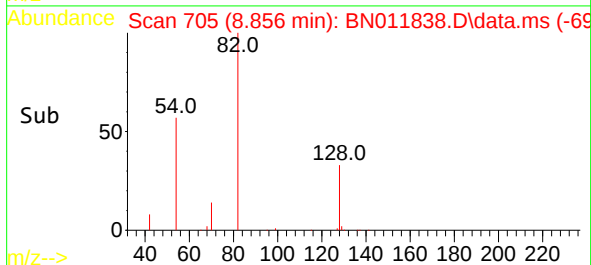
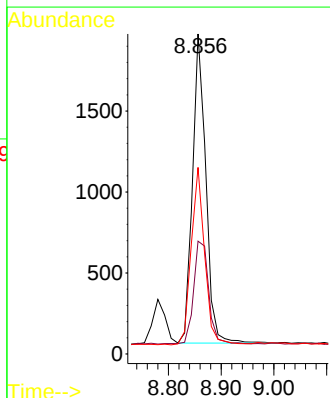
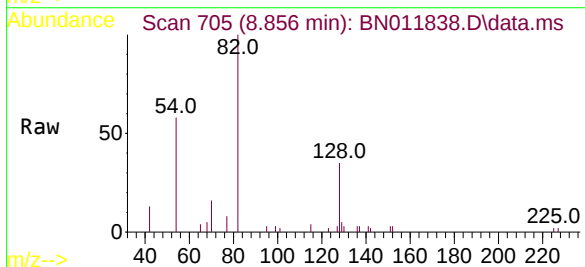




#9
Naphthalene
Concen: 0.42 ng
RT: 10.542 min Scan# 838
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:	128	Resp:	9268
Ion	Ratio	Lower	Upper
128	100		
129	11.5	9.7	14.5
127	14.2	11.0	16.4



#10
Hexachlorobutadiene
Concen: 0.42 ng
RT: 10.846 min Scan# 862
Delta R.T. 0.013 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:	225	Resp:	2184
Ion	Ratio	Lower	Upper
225	100		
223	0.0	0.0	0.0
227	64.1	51.9	77.9


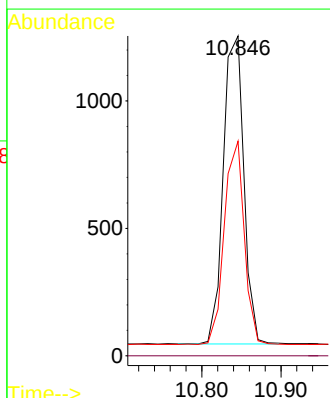






#11
2-Methylnaphthalene-d10
Concen: 0.42 ng
RT: 12.091 min Scan# 1044
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:152 Resp: 5947
Ion Ratio Lower Upper
152 100
151 20.4 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.42 ng
RT: 12.167 min Scan# 1061
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:142 Resp: 6491
Ion Ratio Lower Upper
142 100
141 89.4 70.0 105.0
115 43.7 35.8 53.6


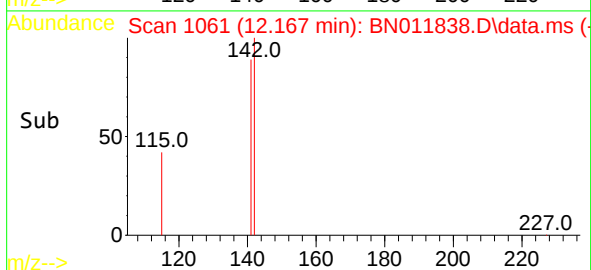




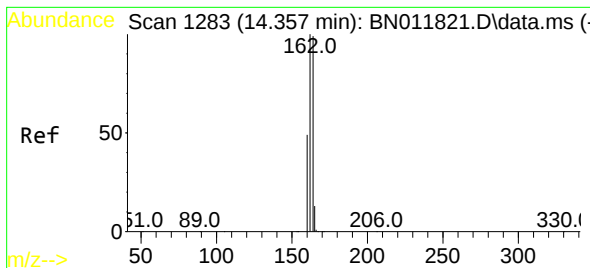

#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.357 min Scan# 1283
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:164 Resp: 4886
Ion Ratio Lower Upper
164 100
162 102.6 83.6 125.4
160 49.9 41.2 61.8

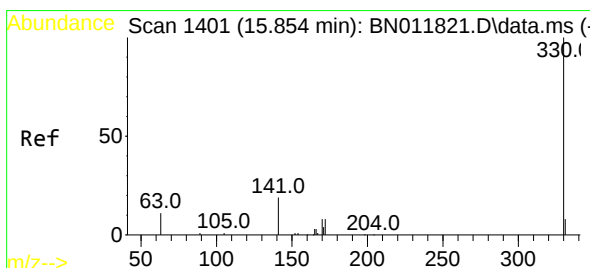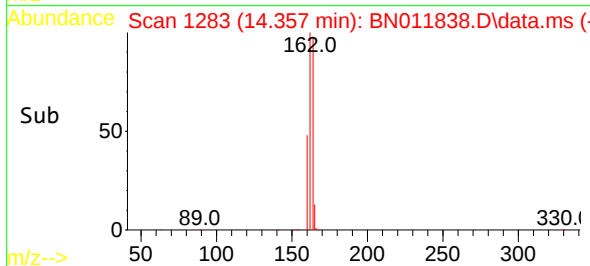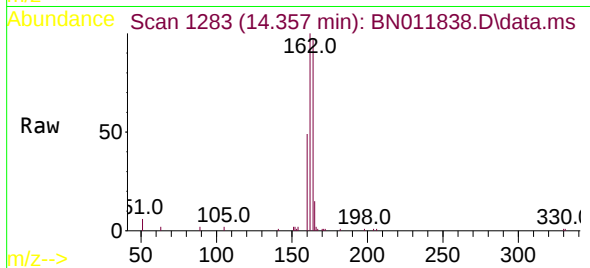

#14
2,4,6-Tribromophenol
Concen: 0.45 ng
RT: 15.854 min Scan# 1401
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:330 Resp: 1127
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 38.7 33.7 50.5


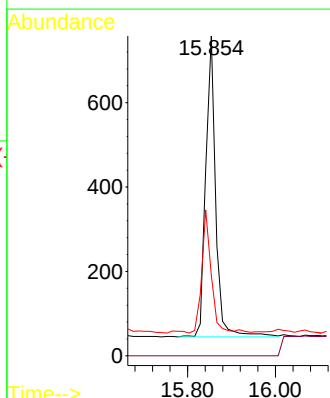
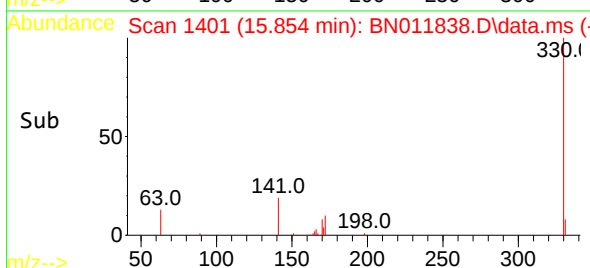
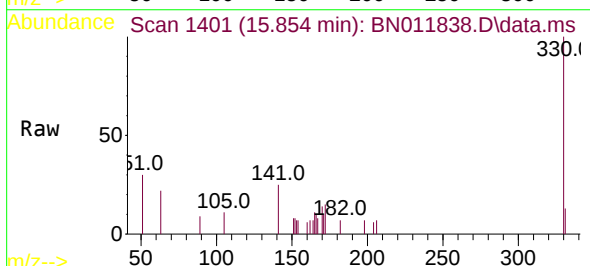




#15
2-Fluorobiphenyl
Concen: 0.42 ng
RT: 12.974 min Scan# 1174
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:172 Resp: 8779
Ion Ratio Lower Upper
172 100
171 35.8 27.4 41.2
170 24.2 17.8 26.6



#16
Acenaphthylene
Concen: 0.40 ng
RT: 14.078 min Scan# 1261
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:152 Resp: 9490
Ion Ratio Lower Upper
152 100
151 19.2 15.9 23.9
153 13.5 10.5 15.7


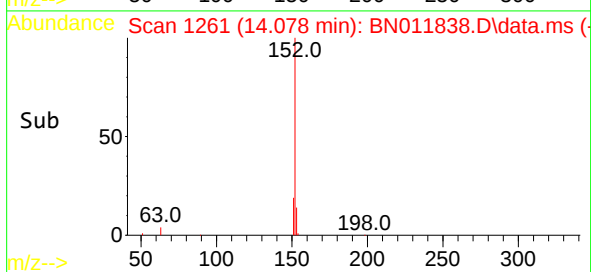






#17
Acenaphthene
Concen: 0.42 ng
RT: 14.420 min Scan# 1288
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:154 Resp: 6855
Ion Ratio Lower Upper
154 100
153 107.6 83.4 125.2
152 55.4 42.8 64.2

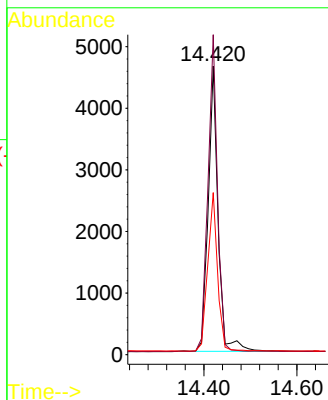

#18
Fluorene
Concen: 0.42 ng
RT: 15.410 min Scan# 1366
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:166 Resp: 8587
Ion Ratio Lower Upper
166 100
165 97.6 78.8 118.2
167 13.9 11.2 16.8



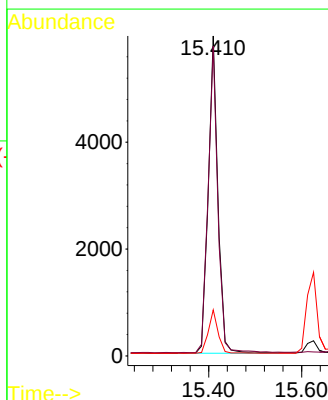
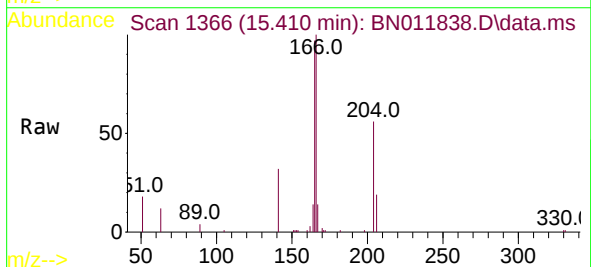




#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 17.102 min Scan# 1503
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:188 Resp: 11352
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.6 7.7 11.5



#20
4,6-Dinitro-2-methylphenol
Concen: 0.40 ng
RT: 15.486 min Scan# 1372
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:198 Resp: 784
Ion Ratio Lower Upper
198 100
51 72.4 45.0 67.4#
105 44.4 30.4 45.6


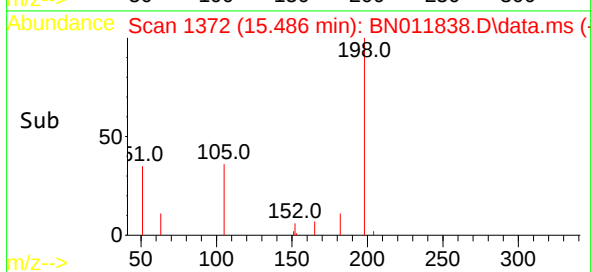




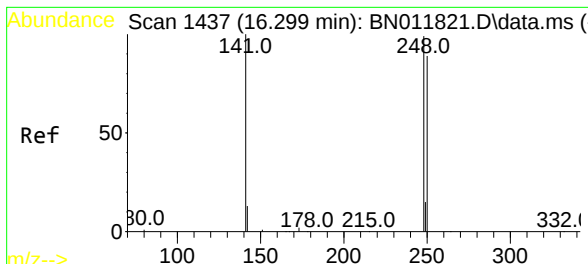

#21
4-Bromophenyl-phenylether
Concen: 0.39 ng
RT: 16.299 min Scan# 1437
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:248 Resp: 2669
Ion Ratio Lower Upper
248 100
250 89.1 82.7 124.1
141 107.8 33.7 50.5#

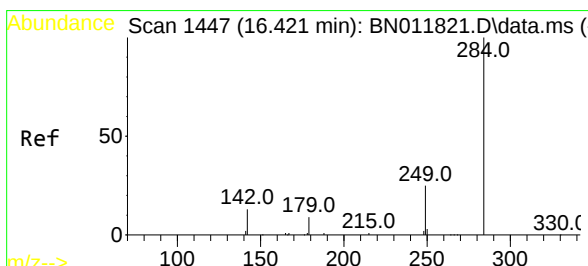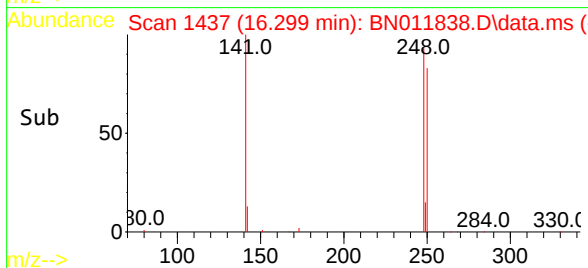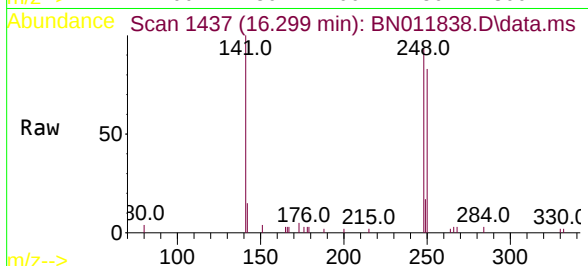

#22
Hexachlorobenzene
Concen: 0.40 ng
RT: 16.420 min Scan# 1447
Delta R.T. 0.012 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:284 Resp: 3319
Ion Ratio Lower Upper
284 100
142 39.0 32.4 48.6
249 32.3 26.8 40.2

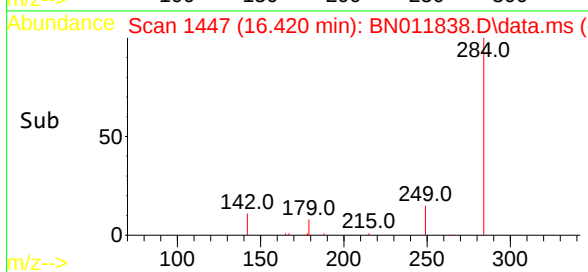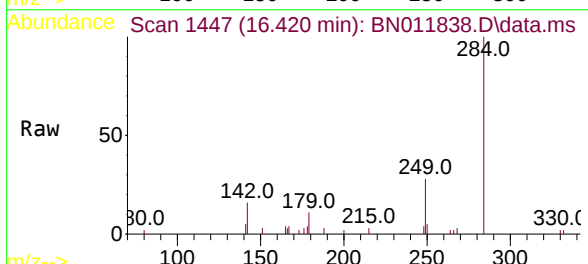



#23

Atrazine

Concen: 0.39 ng

RT: 16.579 min Scan# 1460

Delta R.T. 0.000 min

Lab File: BN011838.D

Acq: 18 Sep 2020 16:45





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4EC

Tgt Ion:	200	Resp:	2362
Ion	Ratio	Lower	Upper
200	100		
173	24.3	18.7	28.1
215	49.7	40.2	60.4

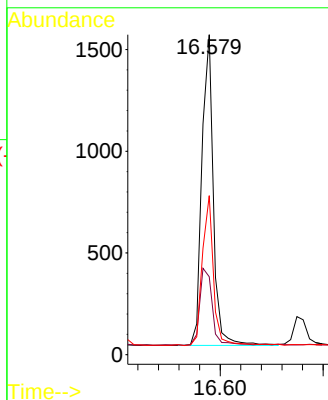

#24

Pentachlorophenol

Concen: 0.39 ng




RT: 16.761 min Scan# 1475


Delta R.T. 0.000 min

Lab File: BN011838.D

Acq: 18 Sep 2020 16:45

Tgt Ion:	266	Resp:	1330
Ion	Ratio	Lower	Upper
266	100		
264	63.4	51.2	76.8
268	66.3	52.4	78.6


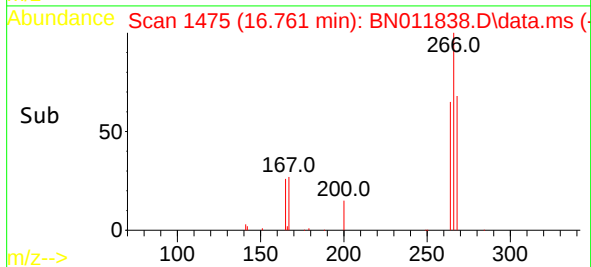
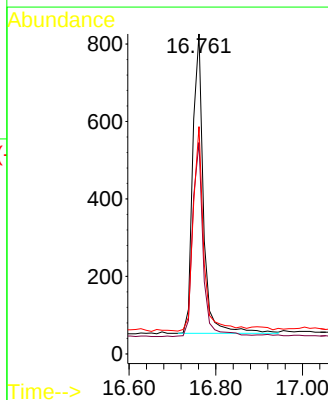
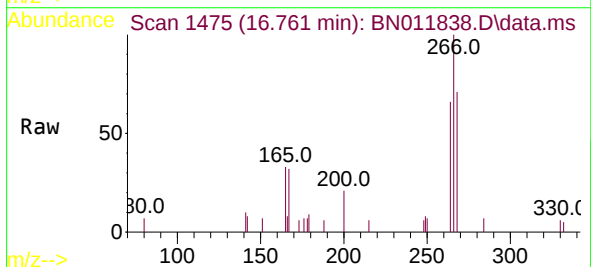




#25
Phenanthrene
Concen: 0.40 ng
RT: 17.151 min Scan# 1507
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:178 Resp: 14494
Ion Ratio Lower Upper
178 100
176 19.1 15.1 22.7
179 15.7 12.3 18.5



#26
Anthracene
Concen: 0.39 ng
RT: 17.236 min Scan# 1514
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:178 Resp: 12248
Ion Ratio Lower Upper
178 100
176 18.1 14.6 21.8
179 15.5 12.4 18.6


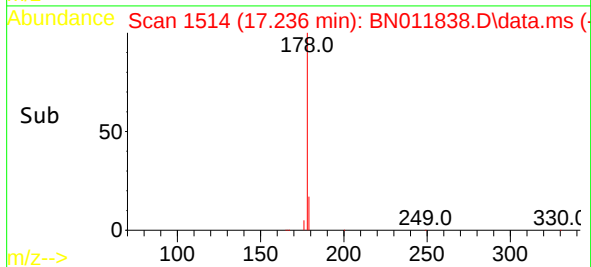

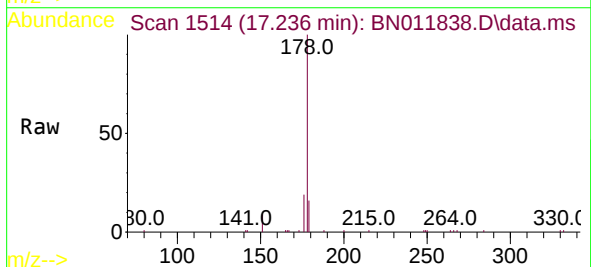




#27
Fluoranthene-d10
Concen: 0.40 ng
RT: 19.147 min Scan# 1806
Delta R.T. 0.005 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:212 Resp: 14449
Ion Ratio Lower Upper
212 100
106 9.0 6.4 9.6
104 5.2 3.9 5.9



#28
Fluoranthene
Concen: 0.41 ng
RT: 19.176 min Scan# 1812
Delta R.T. 0.005 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:202 Resp: 17129
Ion Ratio Lower Upper
202 100
101 7.7 5.4 8.2
203 17.0 13.8 20.6


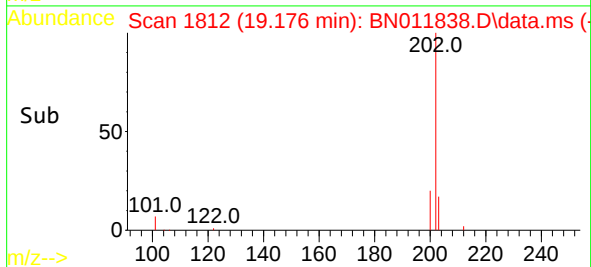

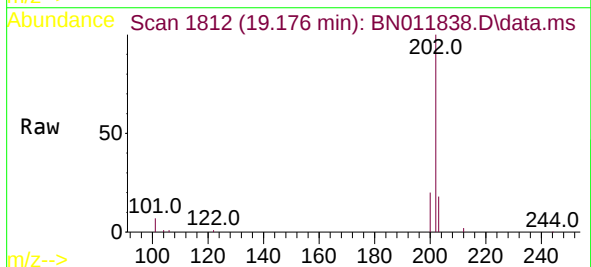


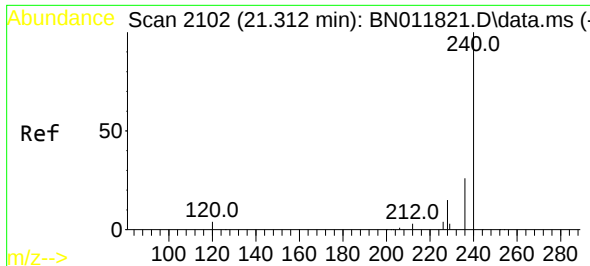

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.312 min Scan# 2102
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:240 Resp: 11976
Ion Ratio Lower Upper
240 100
120 7.1 3.5 5.3#
236 26.4 20.5 30.7

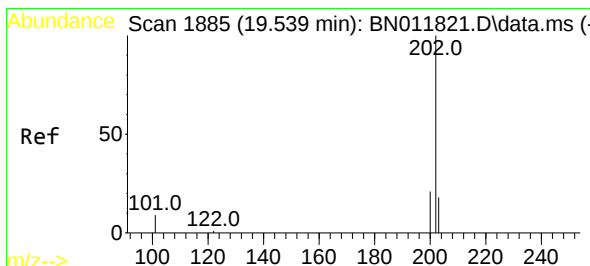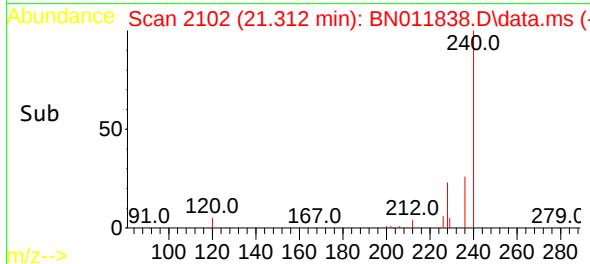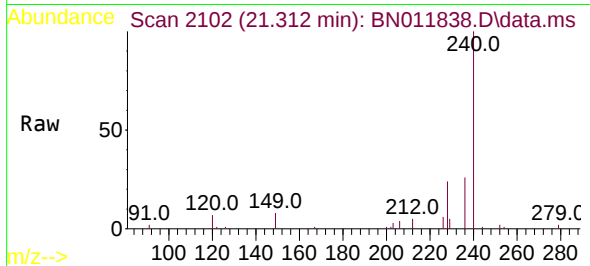

#30
Pyrene
Concen: 0.41 ng
RT: 19.539 min Scan# 1885
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:202 Resp: 16963
Ion Ratio Lower Upper
202 100
200 20.5 16.5 24.7
203 17.4 13.9 20.9


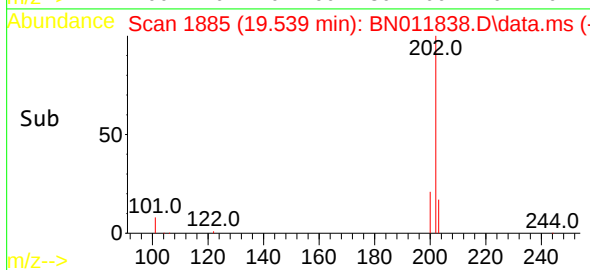

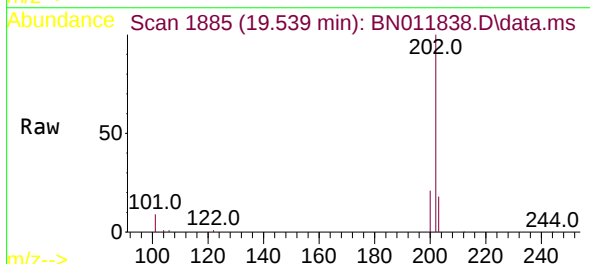




#31
Terphenyl-d14
Concen: 0.44 ng
RT: 19.752 min Scan# 1928
Delta R.T. 0.005 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:244 Resp: 12152
Ion Ratio Lower Upper
244 100
212 9.2 7.3 10.9
122 9.1 7.8 11.6



#32
Benzo(a)anthracene
Concen: 0.39 ng
RT: 21.290 min Scan# 2100
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:228 Resp: 15838
Ion Ratio Lower Upper
228 100
226 28.2 21.0 31.4
229 19.6 16.0 24.0


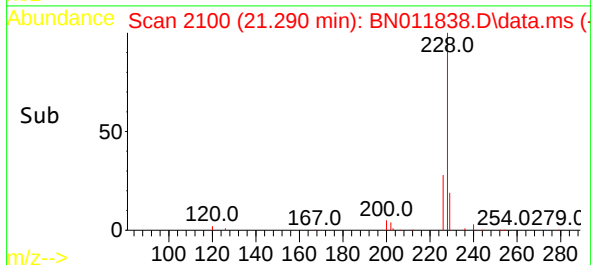

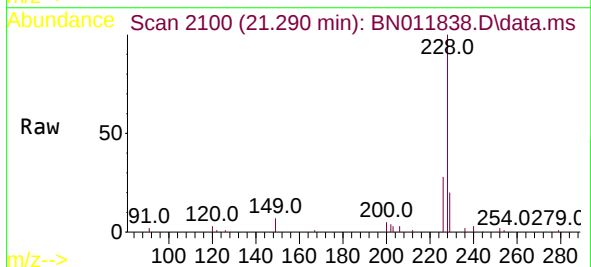


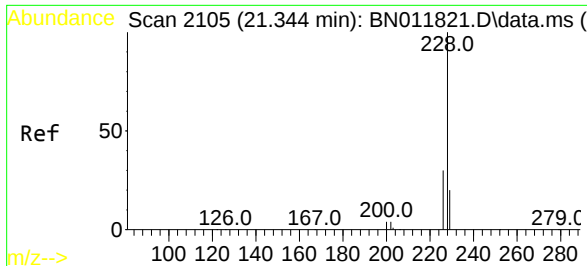

#33
Chrysene
Concen: 0.41 ng
RT: 21.343 min Scan# 2105
Delta R.T. 0.000 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:228 Resp: 17256
Ion Ratio Lower Upper
228 100
226 30.3 23.3 34.9
229 19.2 15.8 23.8

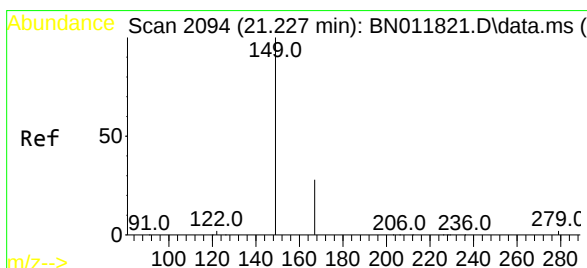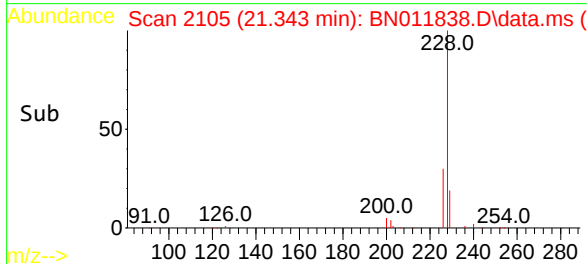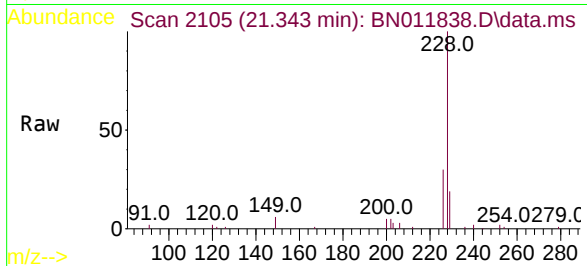

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.36 ng
RT: 21.237 min Scan# 2095
Delta R.T. 0.011 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:149 Resp: 7426
Ion Ratio Lower Upper
149 100
167 28.9 23.6 35.4
279 5.2 4.0 6.0


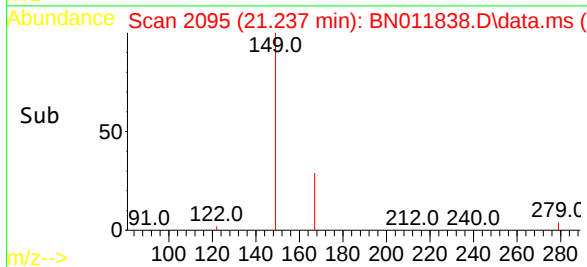

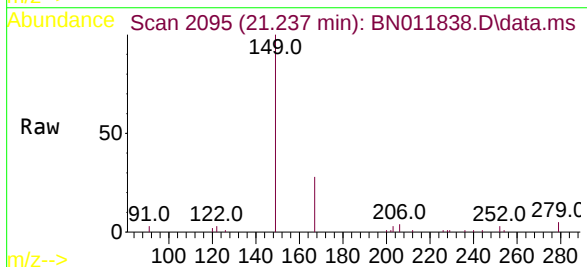




#35
Indeno(1,2,3-cd)pyrene
Concen: 0.41 ng
RT: 25.825 min Scan# 3204
Delta R.T. 0.010 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:276 Resp: 21308
Ion Ratio Lower Upper
276 100
138 17.5 13.0 19.4
277 24.8 20.0 30.0



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.566 min Scan# 2544
Delta R.T. 0.007 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45


Tgt Ion:264 Resp: 11759
Ion Ratio Lower Upper
264 100
260 24.8 19.6 29.4
265 64.3 38.6 58.0#

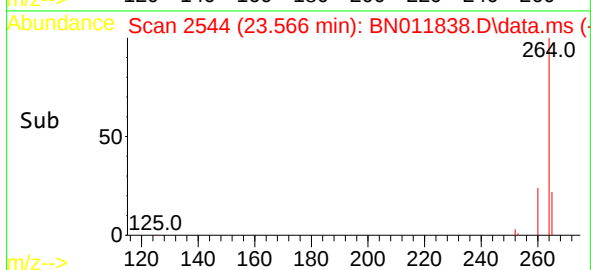






#37
Benzo(b)fluoranthene
Concen: 0.41 ng
RT: 22.888 min Scan# 2346
Delta R.T. 0.003 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45


Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC





Tgt Ion:252 Resp: 18015
Ion Ratio Lower Upper
252 100
253 25.1 19.1 28.7
125 10.2 6.2 9.2#




#38
Benzo(k)fluoranthene
Concen: 0.42 ng
RT: 22.933 min Scan# 2359
Delta R.T. 0.007 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45



Tgt Ion:252 Resp: 18818
Ion Ratio Lower Upper
252 100
253 25.4 19.3 28.9
125 9.6 6.0 9.0#



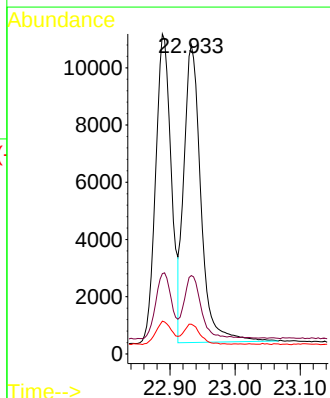





#39
Benzo(a)pyrene
Concen: 0.41 ng
RT: 23.467 min Scan# 2515
Delta R.T. 0.007 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4EC


Tgt Ion:252 Resp: 15916
Ion Ratio Lower Upper
252 100
253 27.9 19.8 29.6
125 13.7 7.3 10.9#



#40
Dibenzo(a,h)anthracene
Concen: 0.40 ng
RT: 25.842 min Scan# 3209
Delta R.T. 0.010 min
Lab File: BN011838.D
Acq: 18 Sep 2020 16:45

Tgt Ion:278 Resp: 17310
Ion Ratio Lower Upper
278 100
139 12.3 8.6 13.0
279 27.0 19.8 29.8

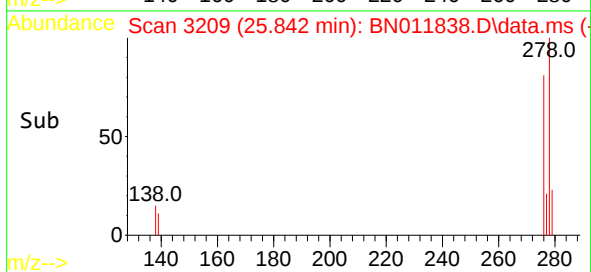

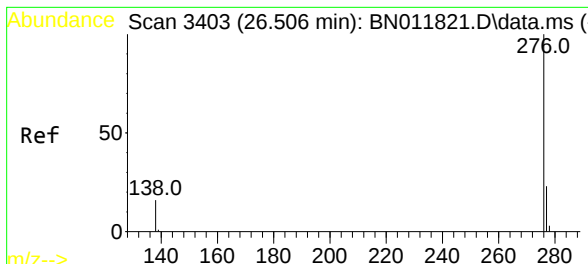

#41
 Benzo(g,h,i)perylene
 Concen: 0.40 ng
 RT: 26.513 min Scan# 3405
 Delta R.T. 0.007 min
 Lab File: BN011838.D
 Acq: 18 Sep 2020 16:45

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4EC

Tgt Ion:	276	Resp:	18361
Ion	Ratio	Lower	Upper
276	100		
277	25.2	19.4	29.0
138	16.3	11.3	16.9

