
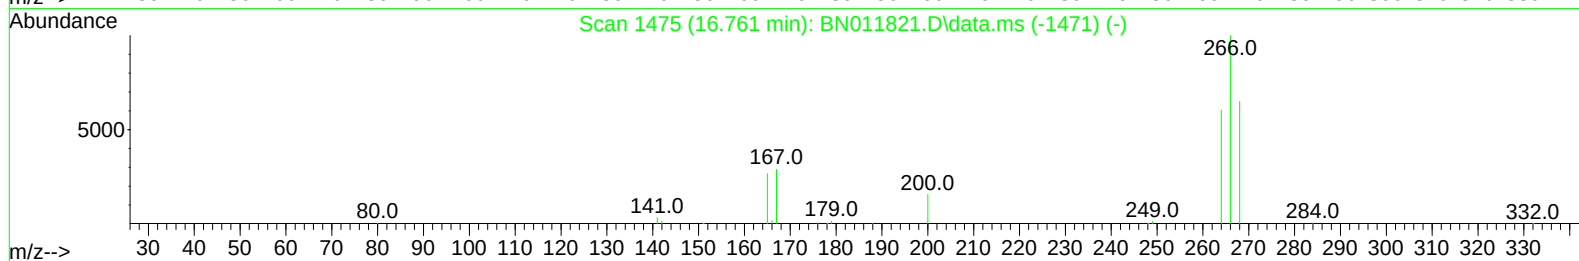
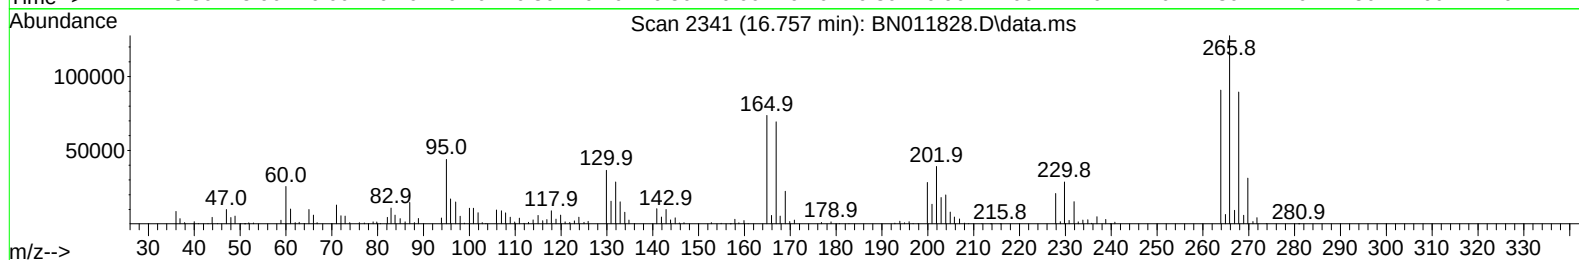


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091820\
Data File : BN011828.D
Acq On : 18 Sep 2020 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 21 01:06:00 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 18 10:47:35 2020
Response via : Initial Calibration

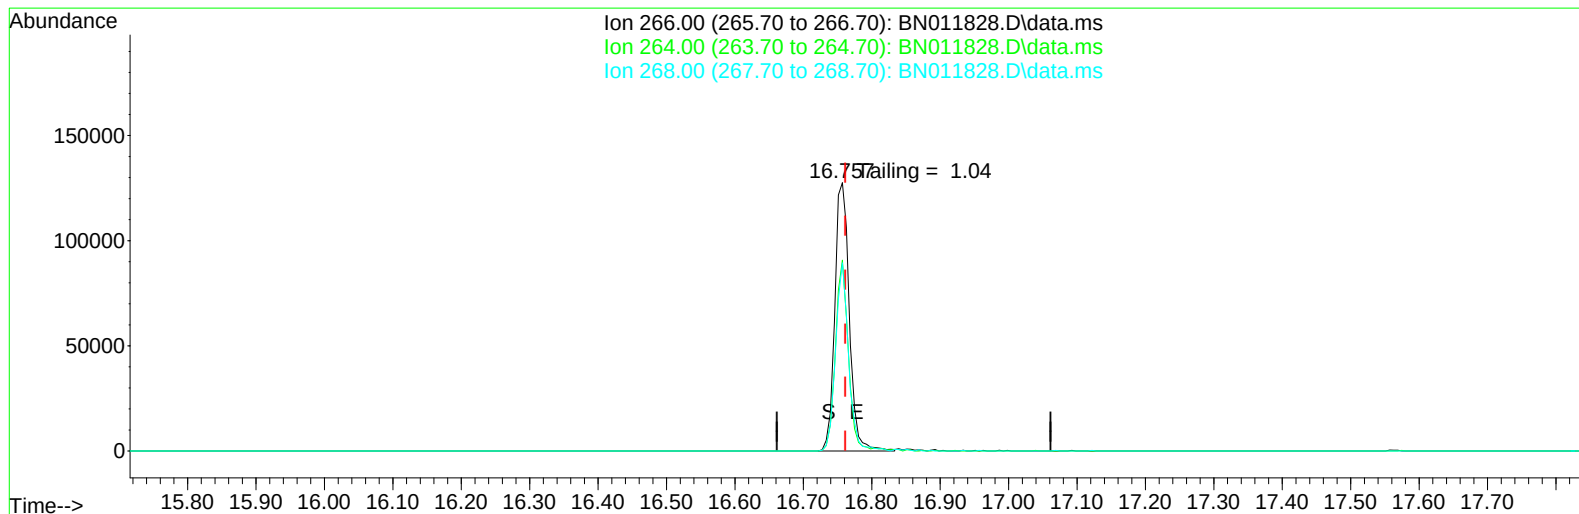

TIC: BN011828.D\data.ms

(24) Pentachlorophenol

16.757min (-0.004) 0.00 ng

response 188386

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	64.00	64.17
268.00	65.50	63.14
0.00	0.00	0.00