


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091820\
Data File : BN011828.D
Acq On : 18 Sep 2020 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091720.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Sep 18 10:47:35 2020

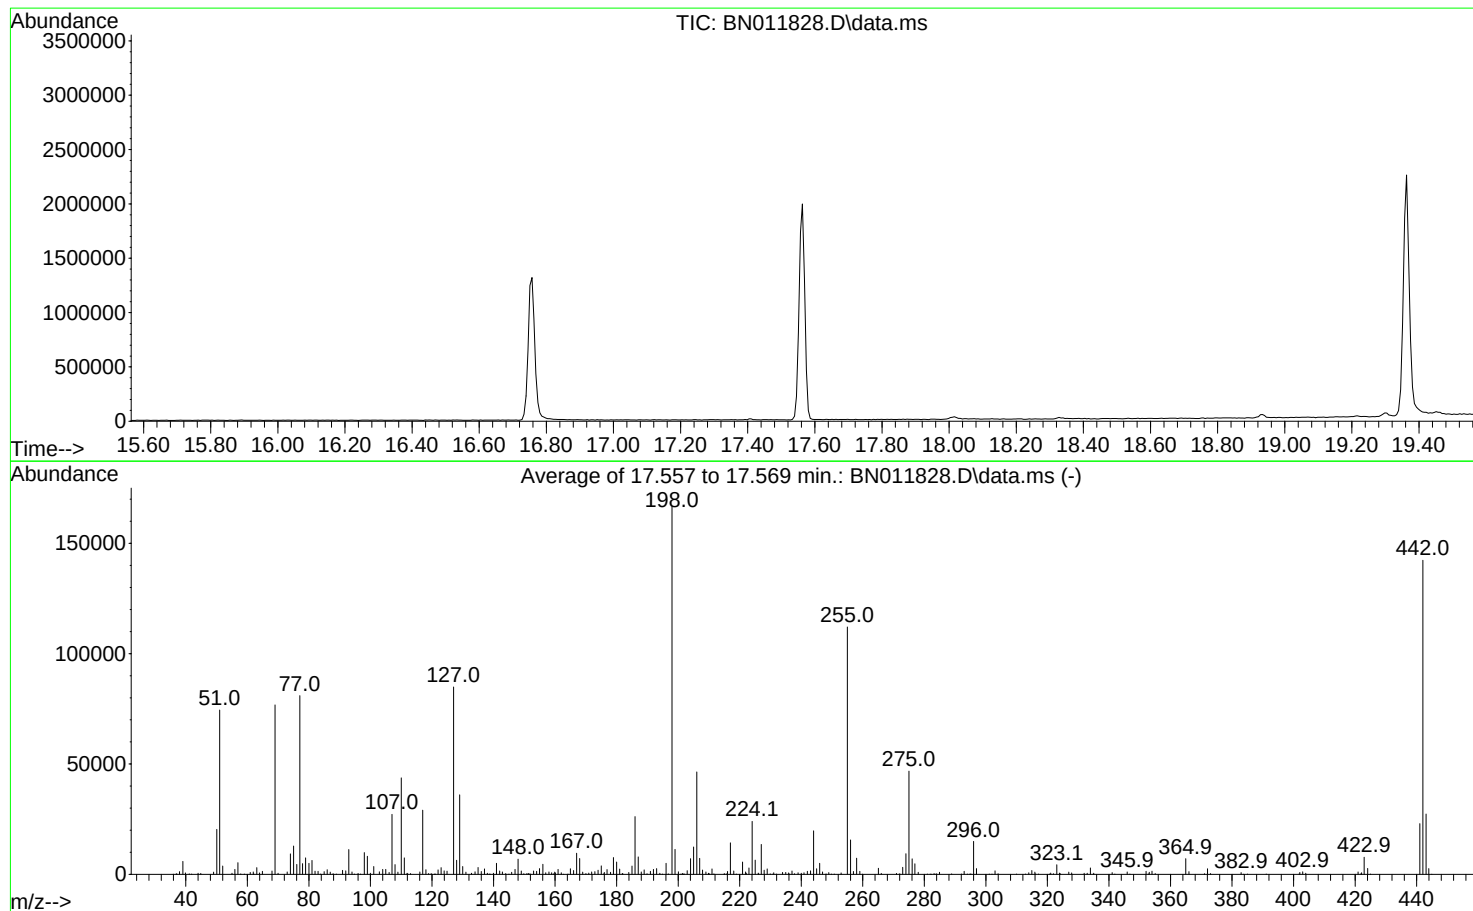

AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2470

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.7	74459	PASS
68	69	0.00	2	2.0	1547	PASS
69	198	0.00	100	46.1	76808	PASS
70	69	0.00	2	0.7	548	PASS
127	198	10	80	51.0	84933	PASS
197	198	0.00	2	0.2	255	PASS
198	198	100	100	100.0	166680	PASS
199	198	5	9	6.8	11302	PASS
275	198	10	60	28.0	46739	PASS
365	198	1	100	4.3	7100	PASS
441	198	0.01	100	13.8	22960	PASS
442	198	50	100	85.4	142349	PASS
443	442	15	24	19.2	27371	PASS