




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021817.D
 Acq On : 19 Sep 2022 23:50
 Operator : CG/JU
 Sample : N4595-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H4

Manual IntegrationsAPPROVED

Quant Time: Sep 20 00:28:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/20/2022
 Supervised By :mohammad ahmed 09/21/2022

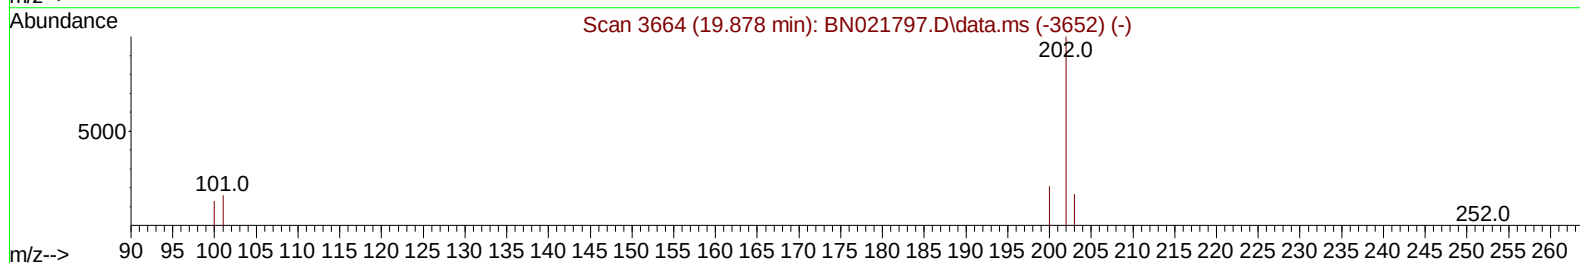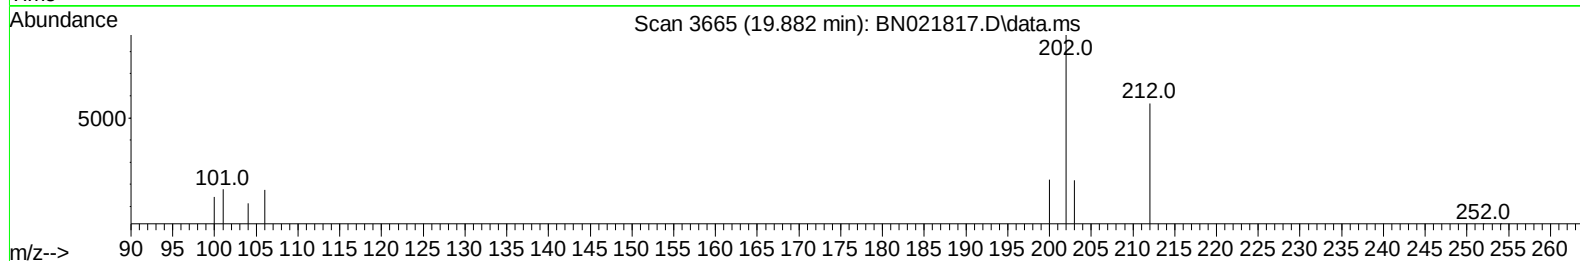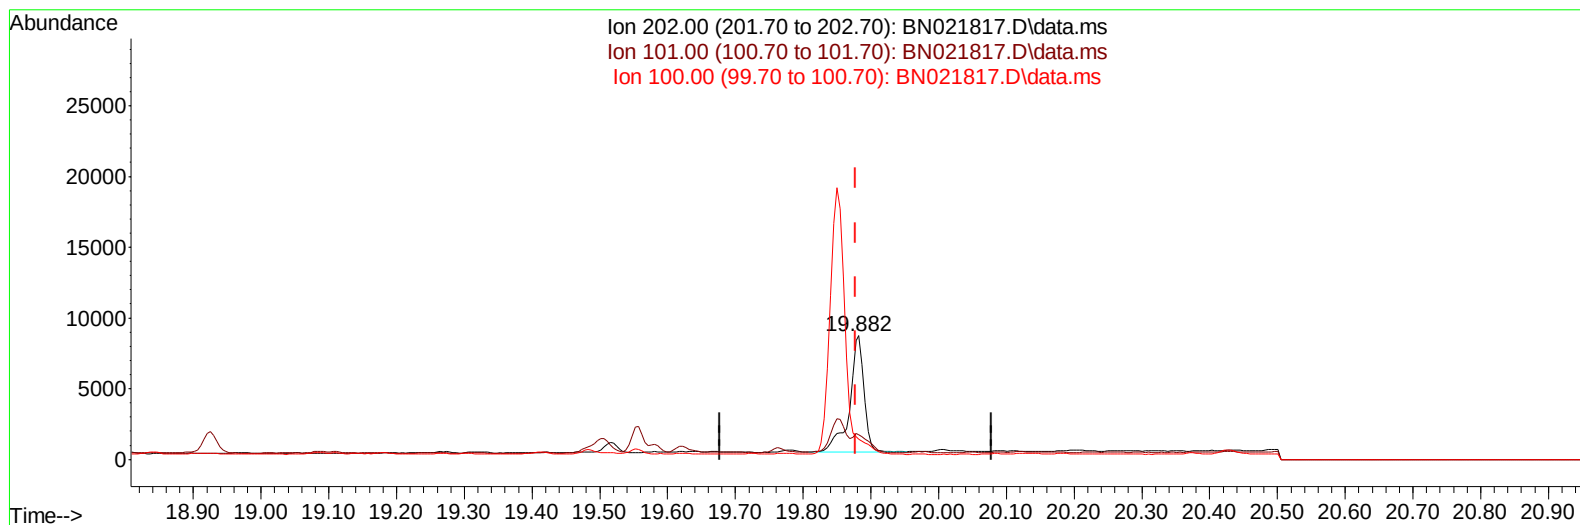

TIC: BN021817.D\data.ms

(20) Pyrene

19.882min (+ 0.005) 0.18 ng/u1

response 12529

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	20.19#
100.00	11.20	16.48#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021817.D
 Acq On : 19 Sep 2022 23:50
 Operator : CG/JU
 Sample : N4595-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H4

Manual IntegrationsAPPROVED

Quant Time: Sep 20 00:28:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/20/2022
 Supervised By :mohammad ahmed 09/21/2022

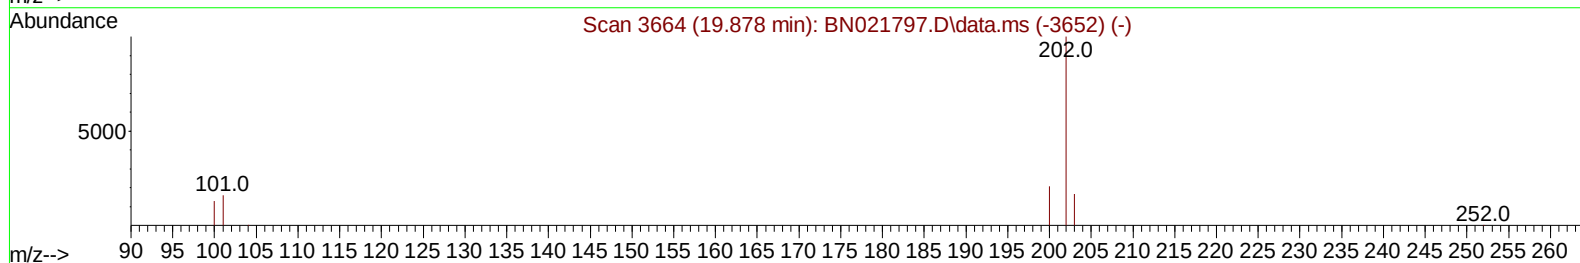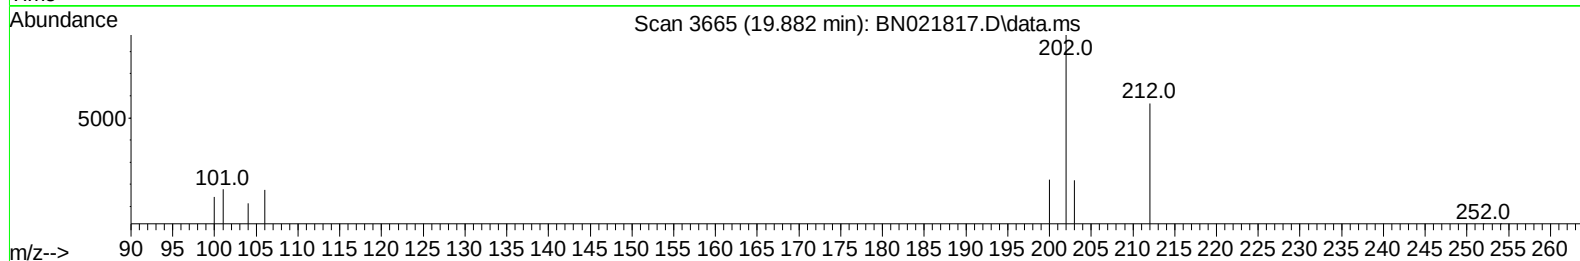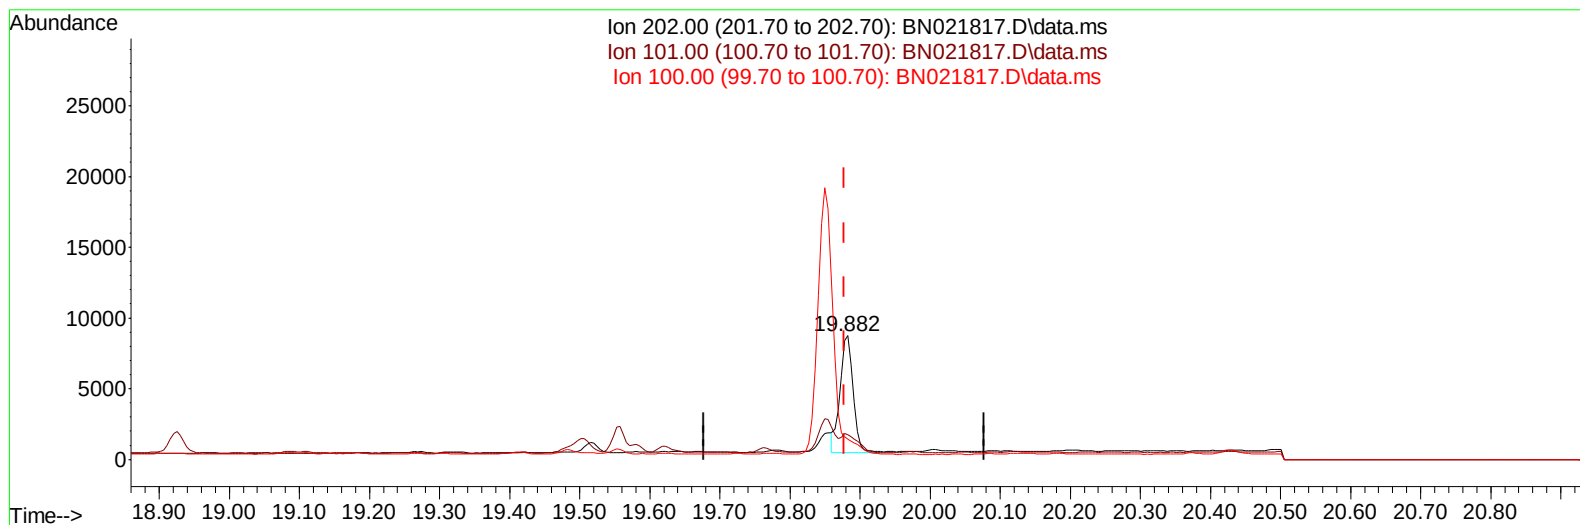

TIC: BN021817.D\data.ms

(20) Pyrene

19.882min (+ 0.005) 0.15 ng/ul m

response 10842

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	20.19#
100.00	11.20	16.48#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021817.D
 Acq On : 19 Sep 2022 23:50
 Operator : CG/JU
 Sample : N4595-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H4

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/20/2022
 Supervised By :mohammad ahmed 09/21/2022

Quant Time: Sep 20 00:28:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	6647	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	22079	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.708	164	13250	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	24848	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.644	240	15250	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	12408	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	31030	3.795	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	10998	0.315	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	21493	0.379	ng/ul	0.00
Target Compounds						Qvalue
16) Anthracene	17.595	178	8717	0.134	ng/ul#	82
20) Pyrene	19.882	202	10842m	0.154	ng/ul	
21) Benzo(a)anthracene	21.627	228	1738	0.034	ng/ul#	47

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021817.D
Acq On : 19 Sep 2022 23:50
Operator : CG/JU
Sample : N4595-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H4

Manual IntegrationsAPPROVED

Quant Time: Sep 20 00:28:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/20/2022
Supervised By :mohammad ahmed 09/21/2022

