




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021834.D
 Acq On : 20 Sep 2022 11:52
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:26:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

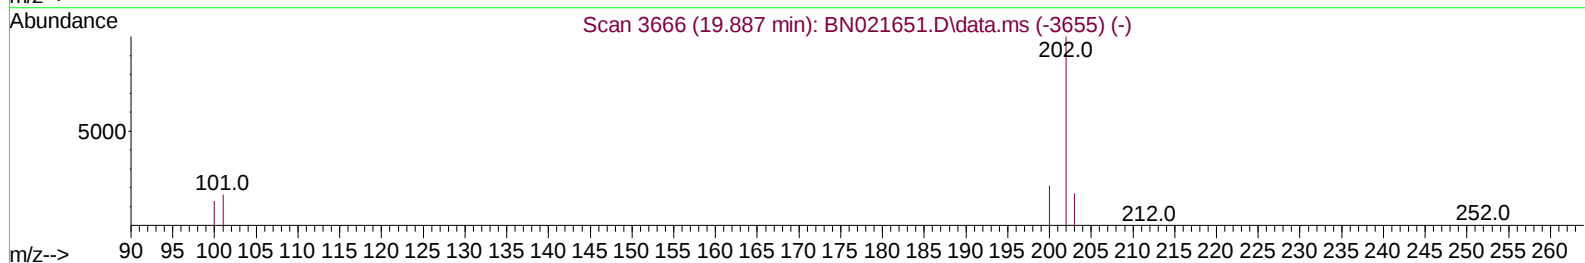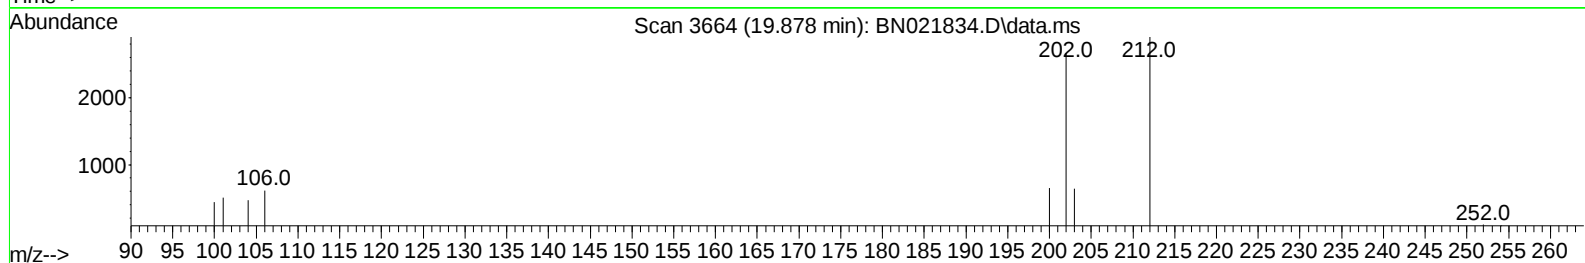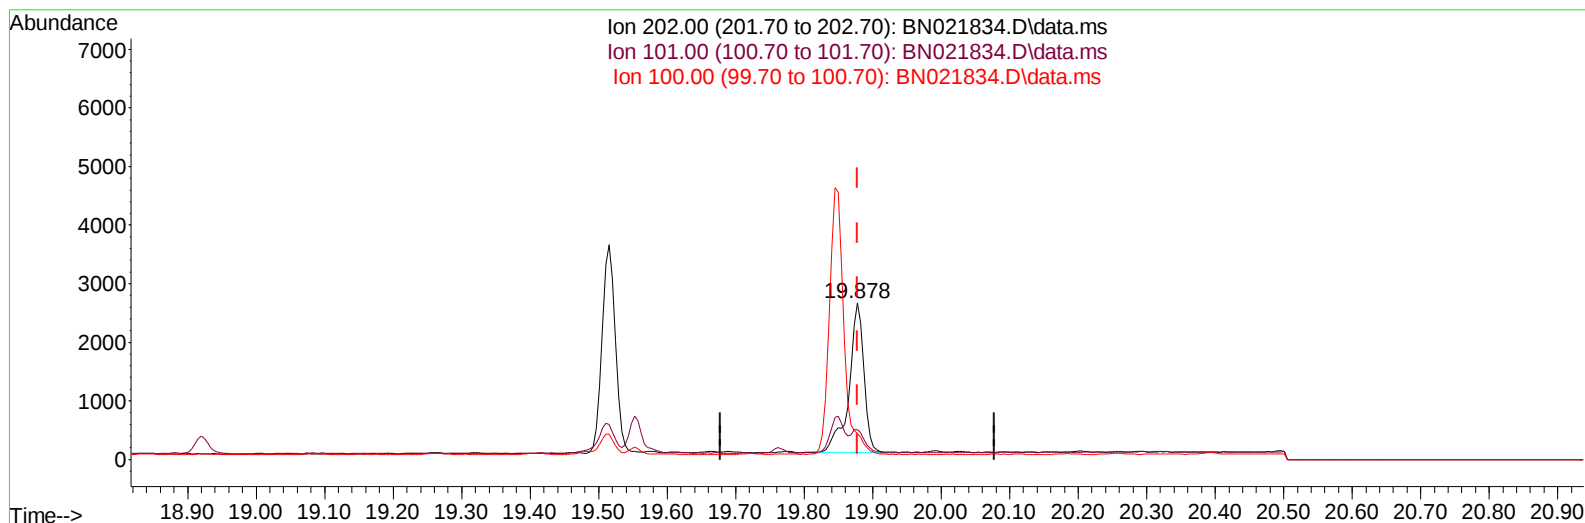

TIC: BN021834.D\data.ms

(20) Pyrene

19.878min (-0.000) 0.07 ng/u1

response 3853

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	19.04#
100.00	11.20	16.45#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021834.D
 Acq On : 20 Sep 2022 11:52
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:26:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

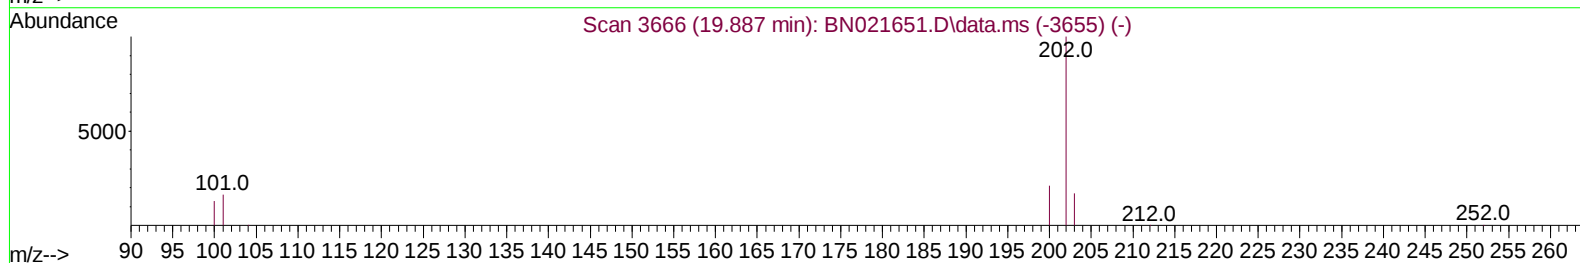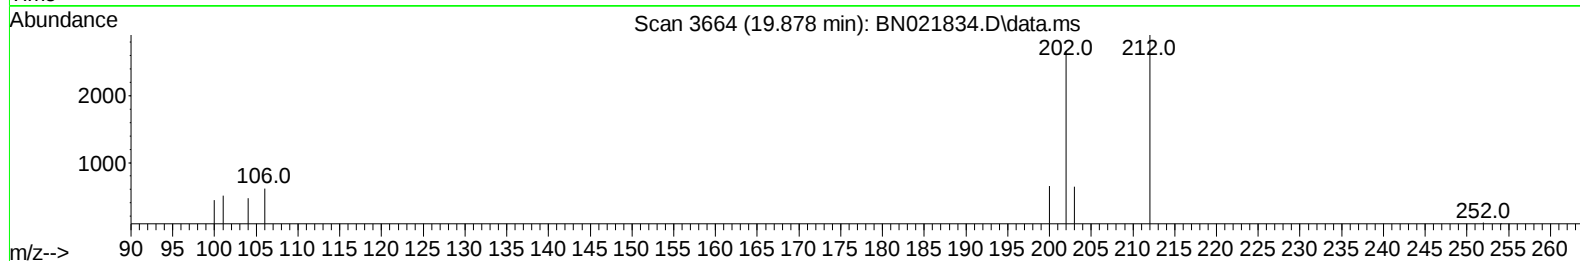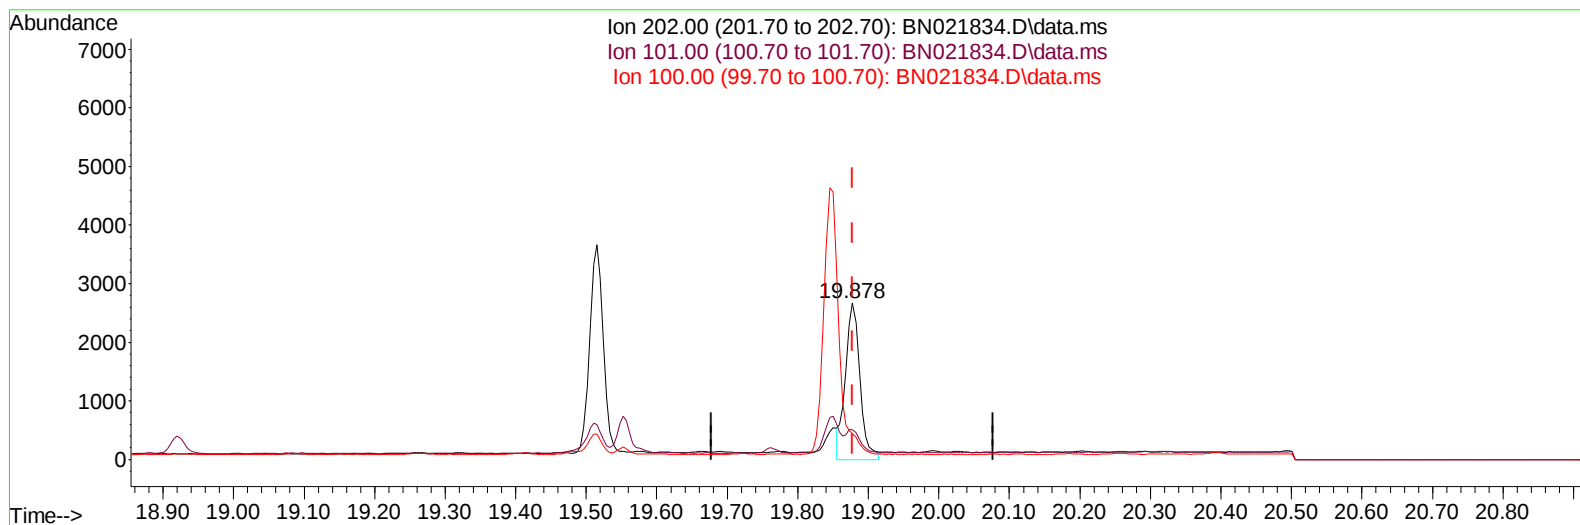

TIC: BN021834.D\data.ms

(20) Pyrene

19.878min (-0.000) 0.07 ng/ul m

response 3817

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	19.04#
100.00	11.20	16.45#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021834.D
 Acq On : 20 Sep 2022 11:52
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

Quant Time: Sep 21 04:26:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	8.051	152		5302	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136		17777	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164		10003	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188		19876	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240		11926	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264		9430	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.363	96		5000	0.767	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152		1899	0.067	ng/ul	0.00
18) Fluoranthene-d10	19.483	212		4024	0.091	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.401	88		3751	0.561	ng/ul	91
5) Naphthalene	10.927	128		4283	0.085	ng/ul	97
8) 1-Methylnaphthalene	12.758	142		2214	0.066	ng/ul	99
10) Acenaphthylene	14.425	152		1657	0.039	ng/ul#	72
11) Acenaphthene	14.768	153		159958	4.494	ng/ul	99
12) Fluorene	15.753	166		85547	2.143	ng/ul	99
15) Phenanthrene	17.498	178		63949	1.020	ng/ul	99
16) Anthracene	17.586	178		4692	0.090	ng/ul#	92
19) Fluoranthene	19.515	202		4805	0.086	ng/ul#	92
20) Pyrene	19.878	202		3817m	0.070	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021834.D
Acq On : 20 Sep 2022 11:52
Operator : CG/JU
Sample : N4595-08DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:26:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
Supervised By :mohammad ahmed 09/21/2022

