




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021836.D
 Acq On : 20 Sep 2022 13:07
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:49:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

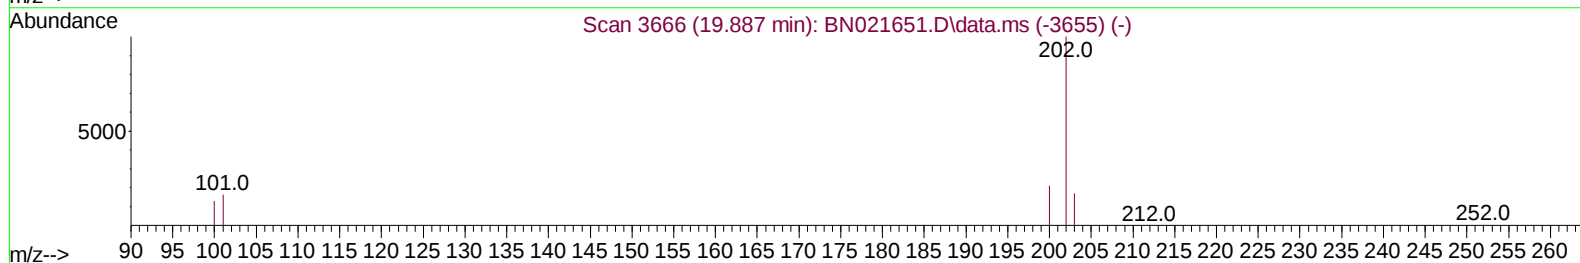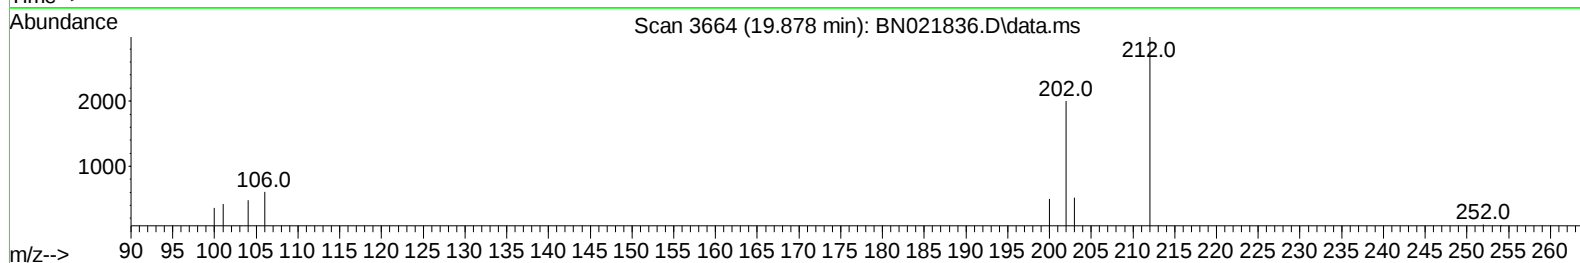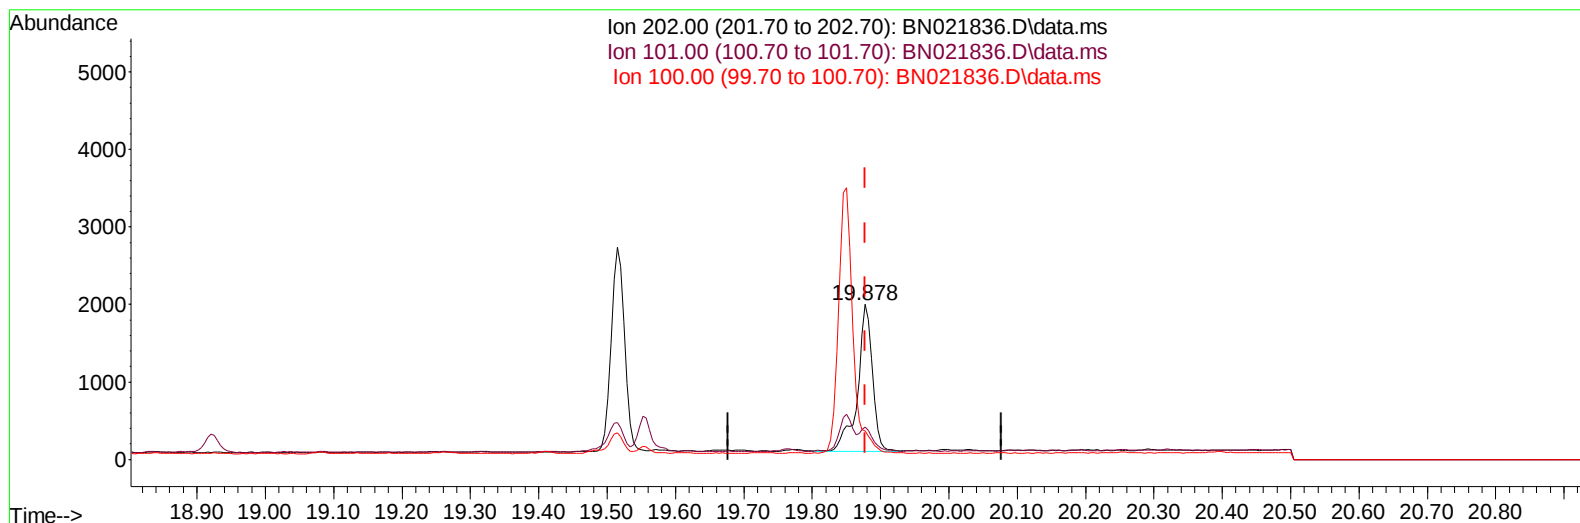

TIC: BN021836.D\data.ms

(20) Pyrene

19.878min (+ 0.000) 0.06 ng/u1

response 2919

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	20.87#
100.00	11.20	18.22#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021836.D
 Acq On : 20 Sep 2022 13:07
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:49:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

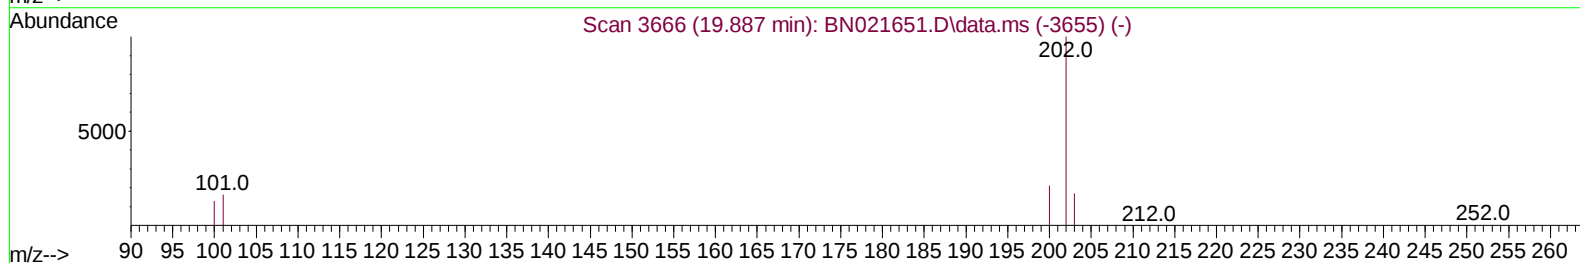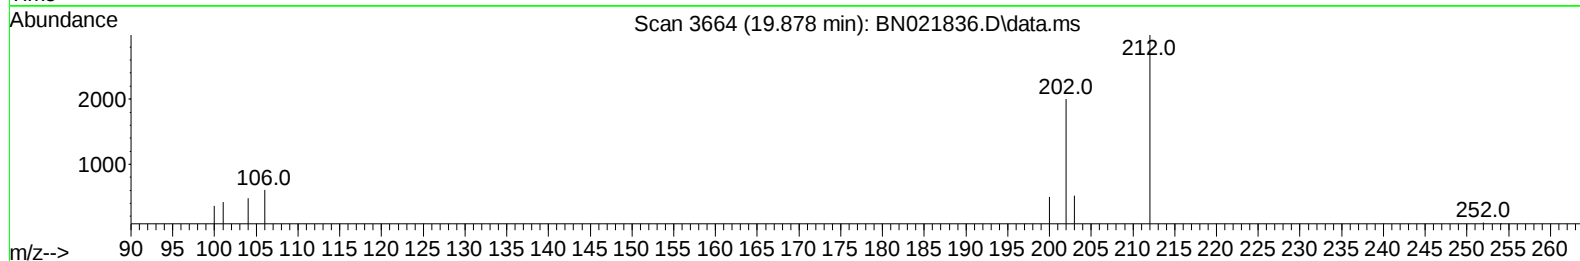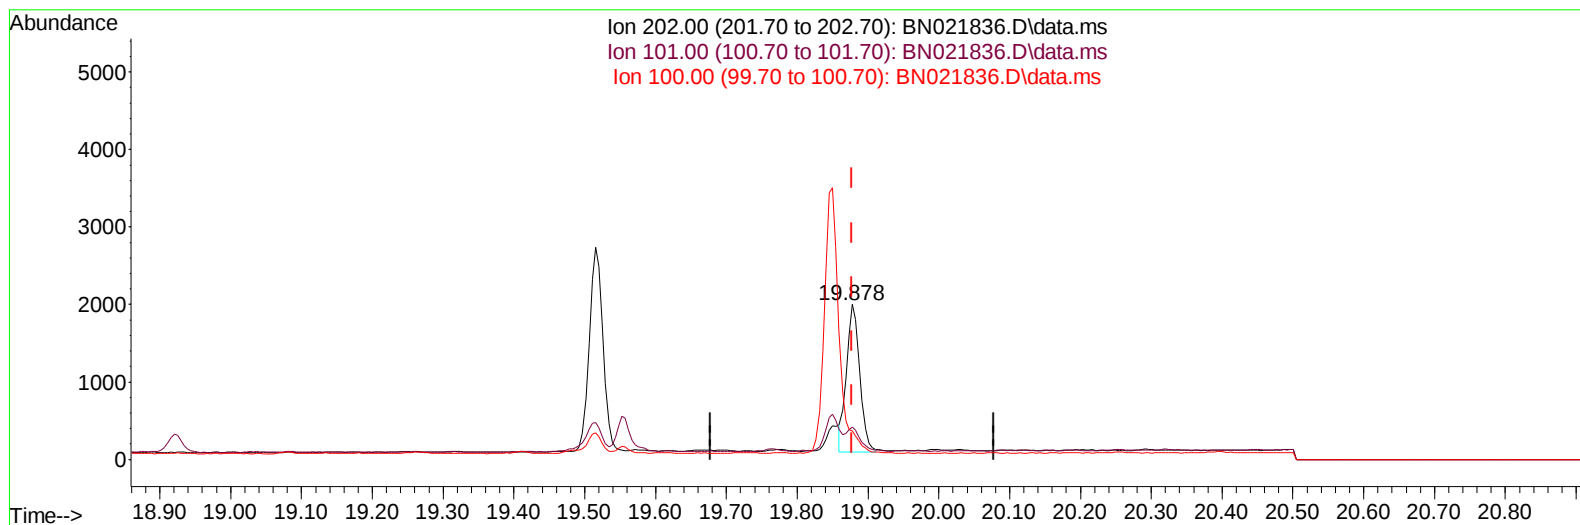

TIC: BN021836.D\data.ms

(20) Pyrene

19.878min (+ 0.000) 0.05 ng/ul m

response 2507

Ion	Exp%	Act%
202.00	100.00	100.00
101.00	14.10	20.87#
100.00	11.20	18.22#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021836.D
 Acq On : 20 Sep 2022 13:07
 Operator : CG/JU
 Sample : N4595-08DL 5X
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 09/21/2022
 Supervised By :mohammad ahmed 09/21/2022

Quant Time: Sep 21 04:49:23 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	4874	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	16281	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.708	164	9043	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.456	188	17185	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.650	240	10062	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	8193	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	2014	0.336	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	1561	0.061	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	3005	0.080	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.927	128	3560	0.078	ng/ul	97
8) 1-Methylnaphthalene	12.759	142	1811	0.059	ng/ul	97
10) Acenaphthylene	14.430	152	1326	0.035	ng/ul#	70
11) Acenaphthene	14.768	153	130901	4.068	ng/ul	99
12) Fluorene	15.753	166	68500	1.898	ng/ul	100
15) Phenanthrene	17.498	178	49528	0.914	ng/ul	99
16) Anthracene	17.591	178	3675	0.082	ng/ul#	92
19) Fluoranthene	19.515	202	3564	0.076	ng/ul#	90
20) Pyrene	19.878	202	2507m	0.054	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021836.D
Acq On : 20 Sep 2022 13:07
Operator : CG/JU
Sample : N4595-08DL 5X
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H9DL

Manual IntegrationsAPPROVED

Quant Time: Sep 21 04:49:23 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 09/21/2022
Supervised By :mohammad ahmed 09/21/2022

