

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021801.D
 Acq On : 19 Sep 2022 13:04
 Operator : CG/JU
 Sample : N4617-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8F7

Quant Time: Sep 20 00:24:12 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4642	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	15704	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	9572	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	18475	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	11939	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	9418	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	25015	4.380	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	6203	0.250	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	13781	0.310	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	107203	18.302	ng/ul#	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021801.D
Acq On : 19 Sep 2022 13:04
Operator : CG/JU
Sample : N4617-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8F7


Quant Time: Sep 20 00:24:12 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

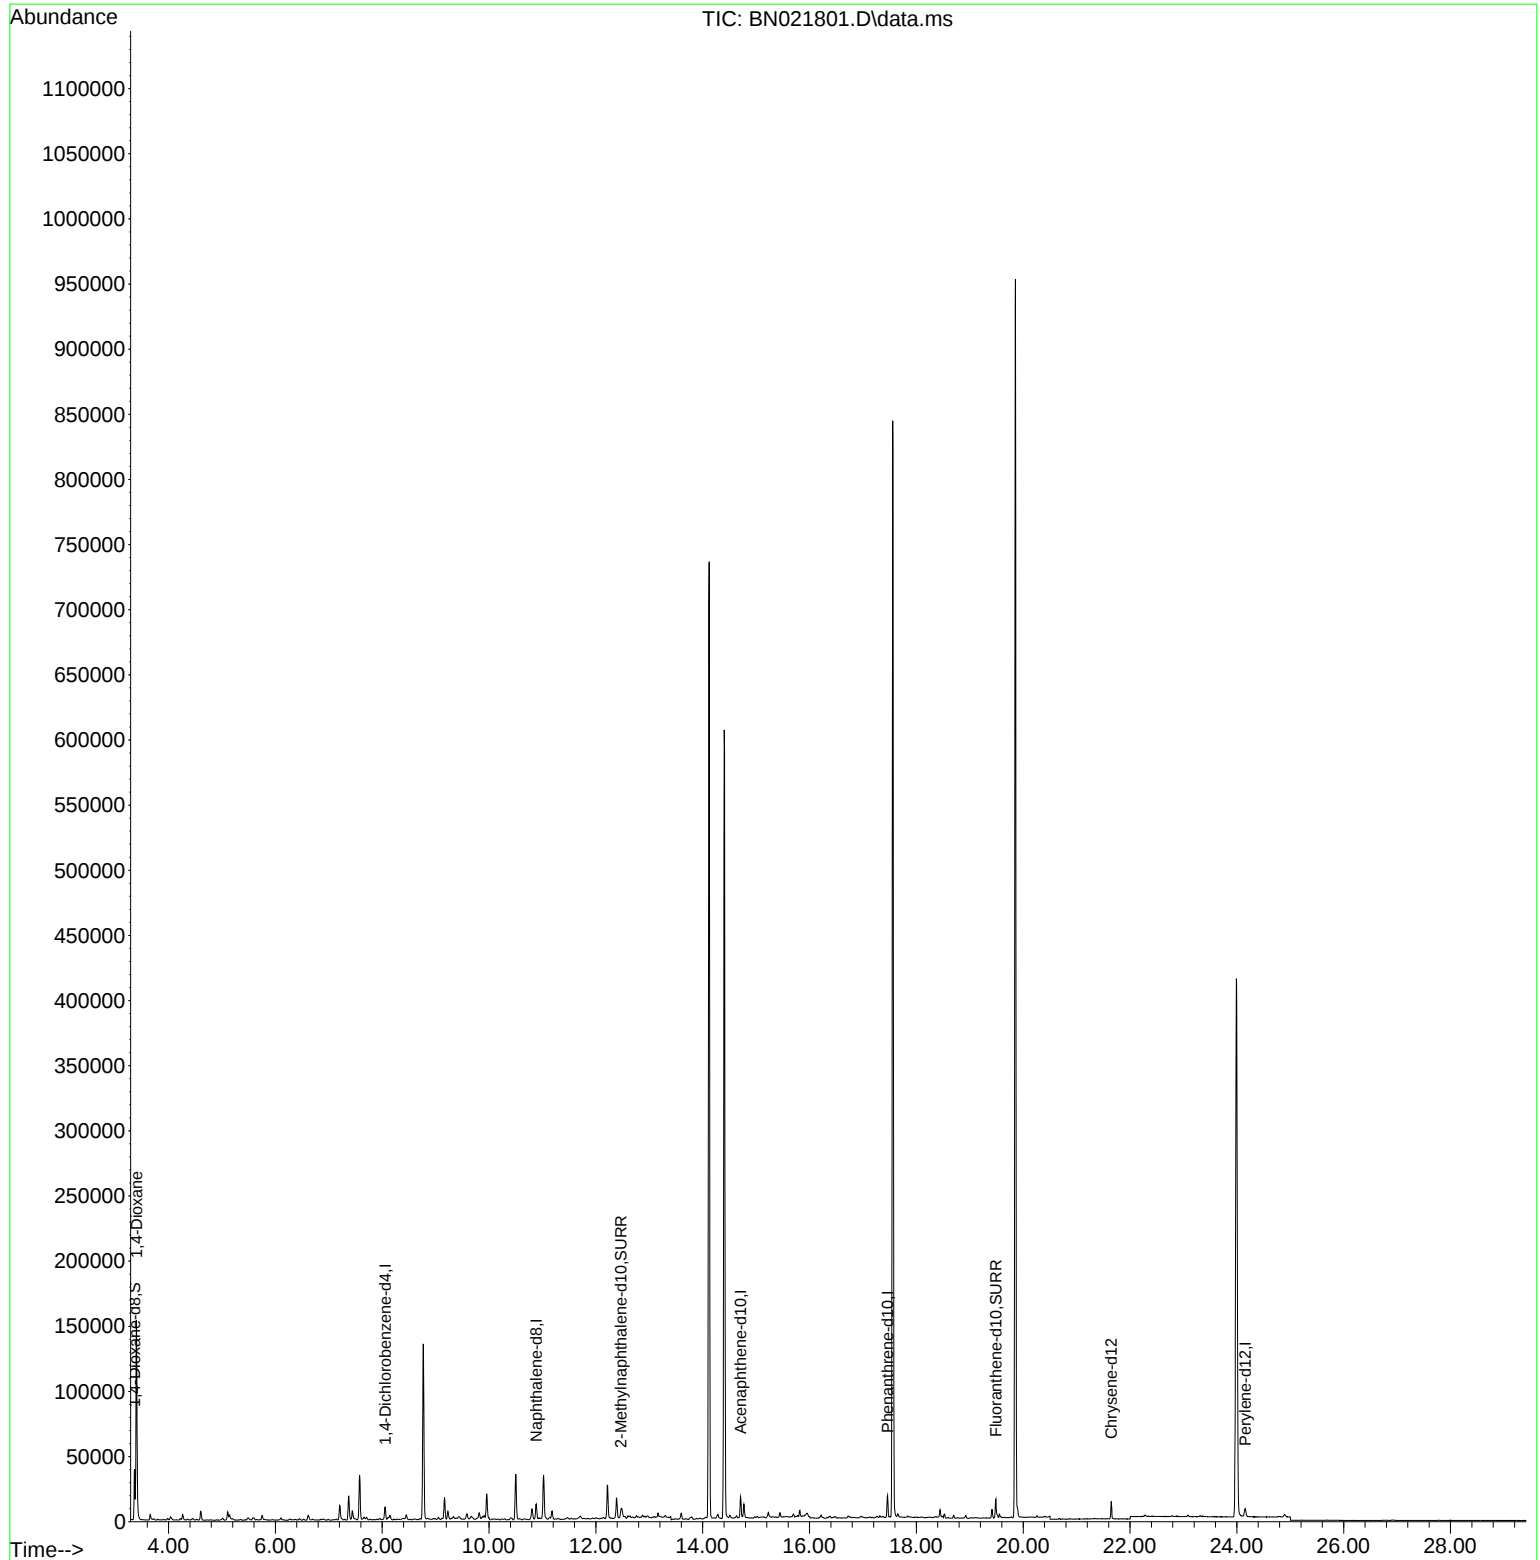

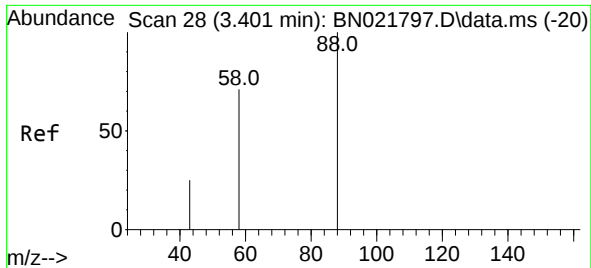

#2
 1,4-Dioxane
 Concen: 18.302 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021801.D
 Acq: 19 Sep 2022 13:04

Instrument :
 BNA_N
 ClientSampleId :
 CB8F7

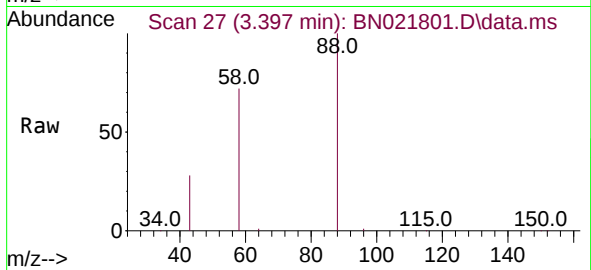

Tgt Ion: 88 Resp: 107203
 Ion Ratio Lower Upper
 88 100
 43 27.9 31.4 47.0#
 58 71.9 49.0 73.6

