

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021803.D
 Acq On : 19 Sep 2022 14:20
 Operator : CG/JU
 Sample : N4617-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8G5

Quant Time: Sep 20 00:24:36 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4369	0.400	ng/u1	0.00
4) Naphthalene-d8	10.883	136	14900	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.712	164	8633	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.460	188	17958	0.400	ng/u1	0.00
17) Chrysene-d12	21.650	240	11153	0.400	ng/u1	# 0.00
23) Perylene-d12	24.155	264	9036	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	24513	4.561	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.473	152	7553	0.320	ng/u1	0.00
18) Fluoranthene-d10	19.487	212	16382	0.395	ng/u1	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	1856	0.337	ng/u1	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021803.D
Acq On : 19 Sep 2022 14:20
Operator : CG/JU
Sample : N4617-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8G5

Quant Time: Sep 20 00:24:36 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

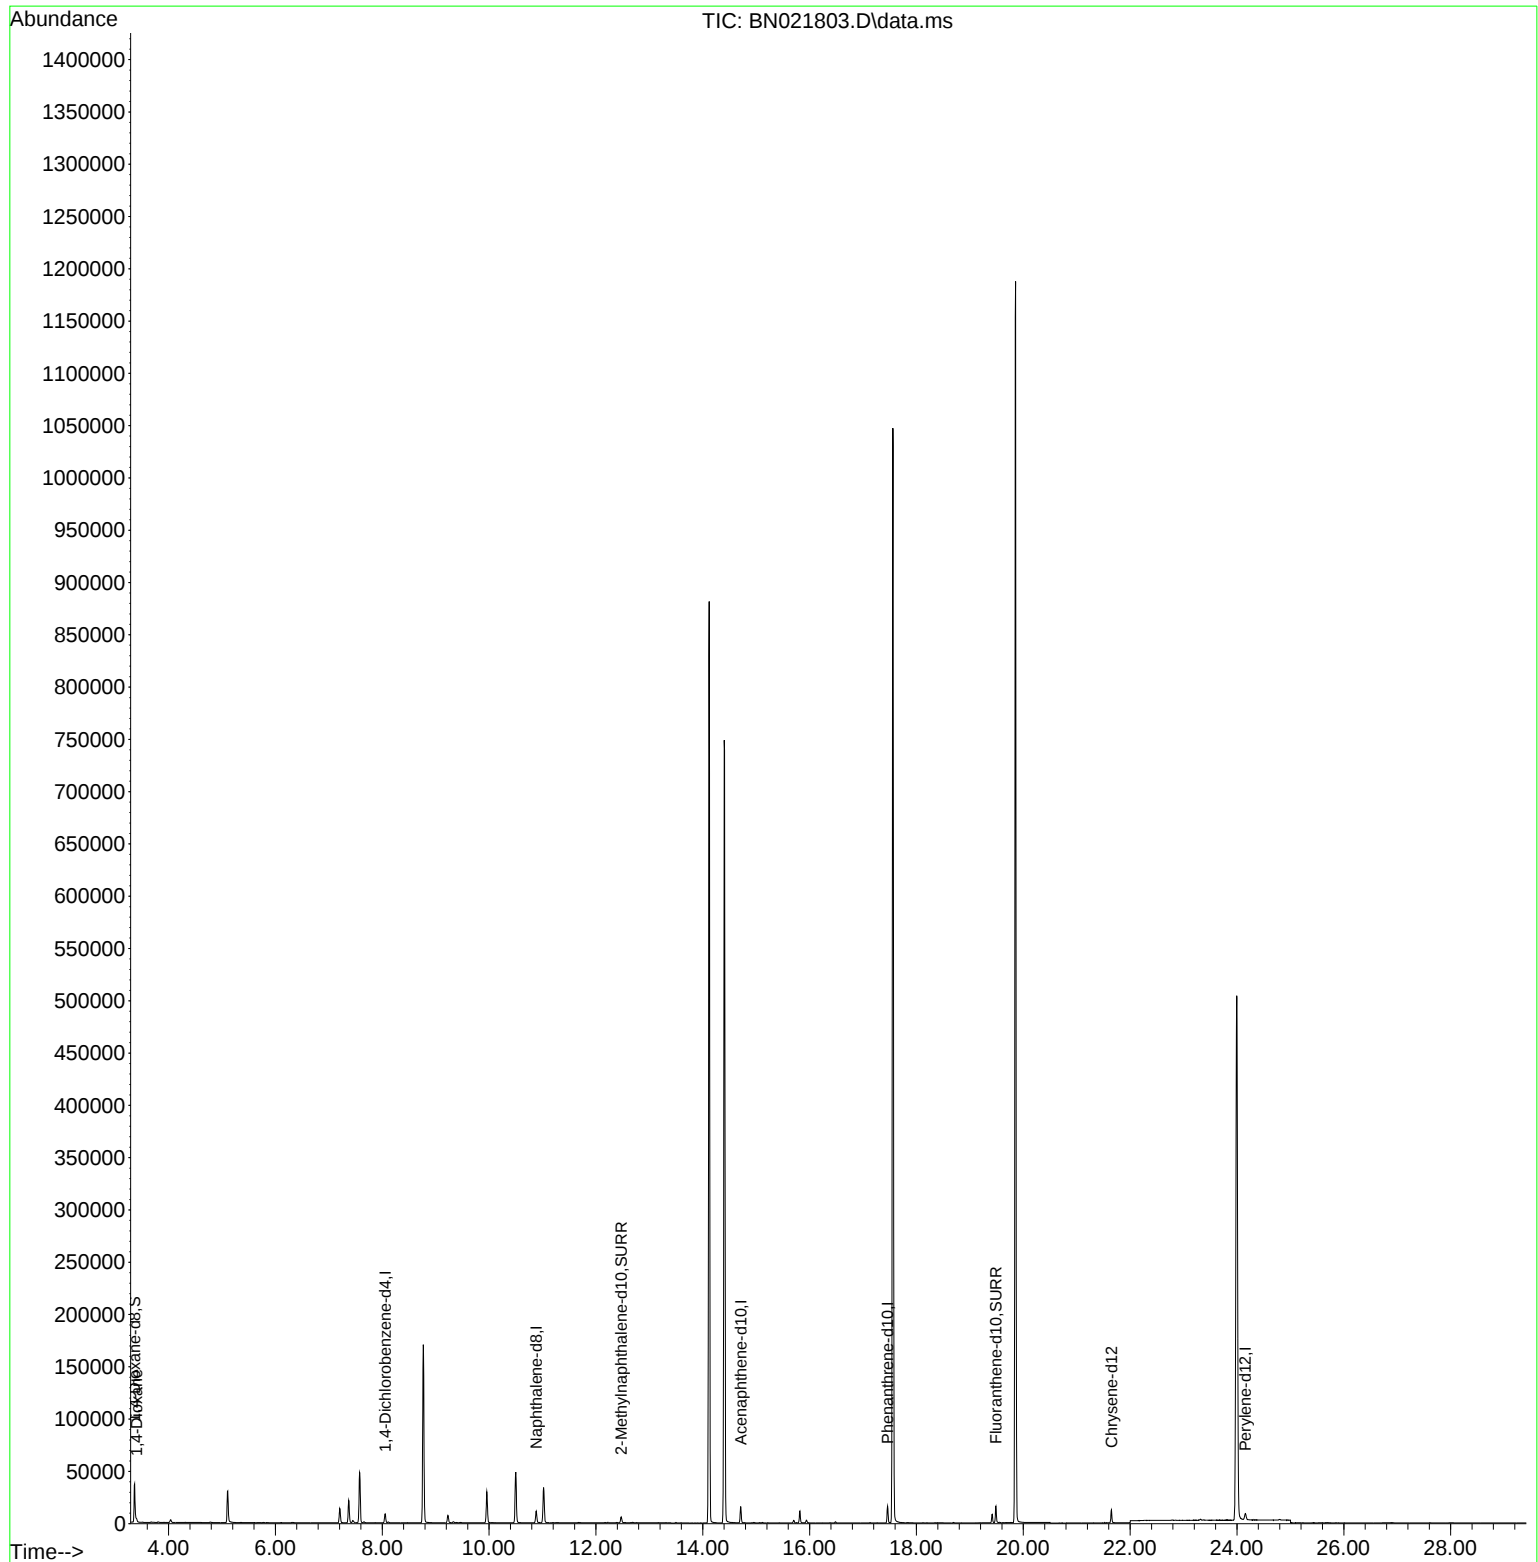

Abundance Scan 28 (3.401 min): BN021797.D\data.ms (-20)

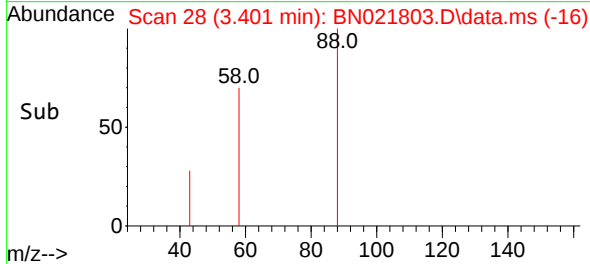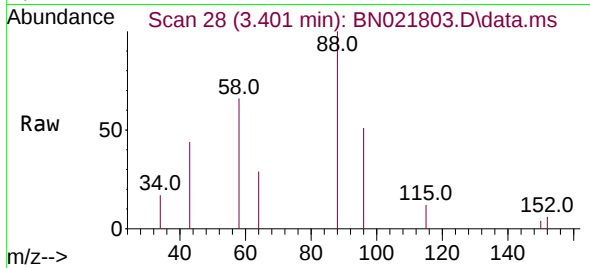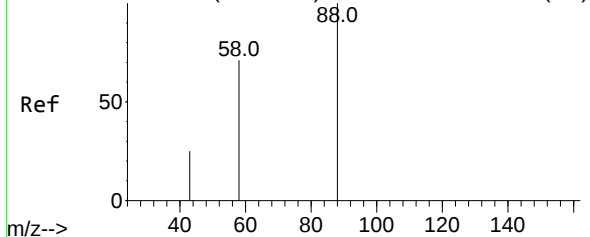

#2
1,4-Dioxane
Concen: 0.337 ng/ul
RT: 3.401 min Scan# 28
Delta R.T. -0.000 min
Lab File: BN021803.D
Acq: 19 Sep 2022 14:20

Instrument :
BNA_N
ClientSampleId :
CB8G5

Tgt Ion:	88	Resp:	1856
Ion	Ratio	Lower	Upper
88	100		
43	44.3	31.4	47.0
58	66.2	49.0	73.6

