

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021805.D
 Acq On : 19 Sep 2022 15:36
 Operator : CG/JU
 Sample : N4617-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8G7

Quant Time: Sep 20 00:24:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.054	152	4762	0.400	ng/u1	0.00
4) Naphthalene-d8	10.883	136	16242	0.400	ng/u1	# 0.00
9) Acenaphthene-d10	14.712	164	9640	0.400	ng/u1	0.00
13) Phenanthrene-d10	17.459	188	19442	0.400	ng/u1	# 0.00
17) Chrysene-d12	21.650	240	12727	0.400	ng/u1	# 0.00
23) Perylene-d12	24.158	264	9969	0.400	ng/u1	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	24014	4.099	ng/u1	0.00
6) 2-Methylnaphthalene-d10	12.472	152	6616	0.257	ng/u1	0.00
18) Fluoranthene-d10	19.487	212	15402	0.325	ng/u1	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.401	88	10096	1.680	ng/u1	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021805.D
Acq On : 19 Sep 2022 15:36
Operator : CG/JU
Sample : N4617-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8G7


Quant Time: Sep 20 00:24:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

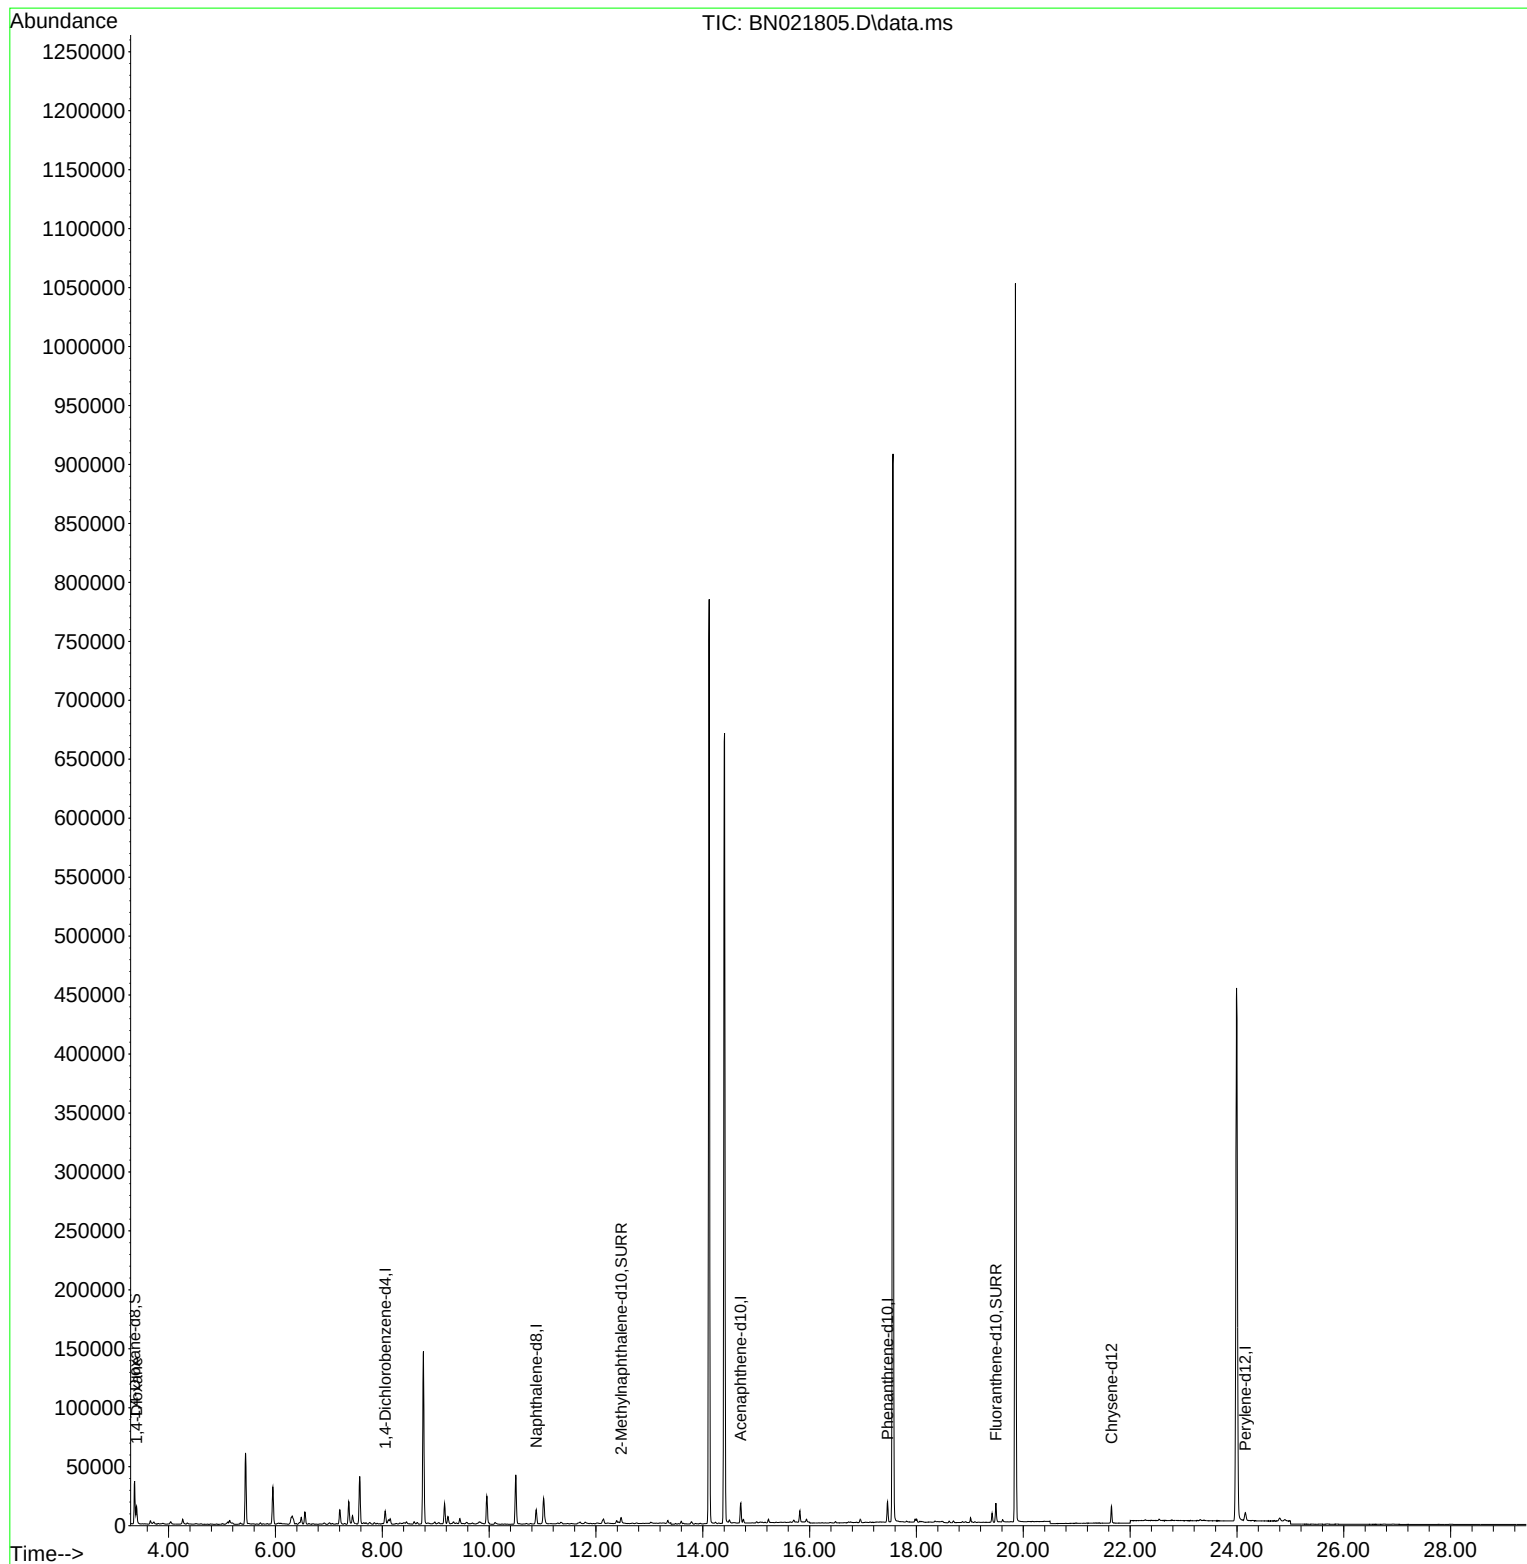

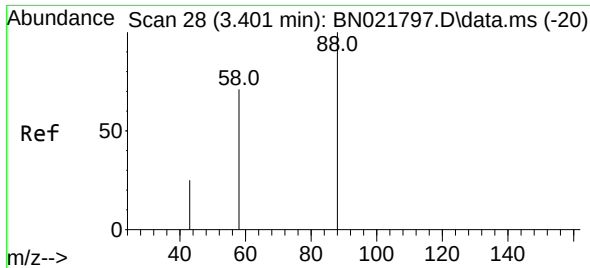

#2
 1,4-Dioxane
 Concen: 1.680 ng/ul
 RT: 3.401 min Scan# 28
 Delta R.T. -0.000 min
 Lab File: BN021805.D
 Acq: 19 Sep 2022 15:36

Instrument :
 BNA_N
 ClientSampleId :
 CB8G7

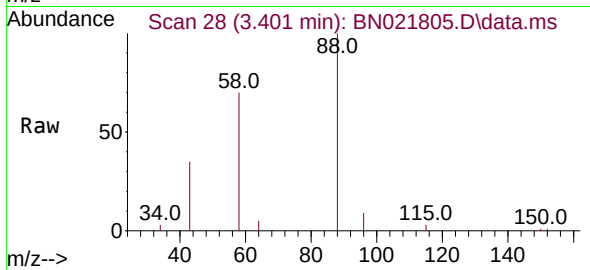

Tgt Ion:	88	Resp:	10096
Ion	Ratio	Lower	Upper
88	100		
43	35.1	31.4	47.0
58	69.6	49.0	73.6

