

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021809.D
 Acq On : 19 Sep 2022 18:08
 Operator : CG/JU
 Sample : N4617-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H2

Quant Time: Sep 20 00:25:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	4731	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	15886	0.400	ng/ul	0.00
9) Acenaphthene-d10	14.712	164	9106	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.464	188	18762	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.650	240	11989	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	9590	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	21525	3.698	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.473	152	7680	0.305	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	18572	0.416	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.405	88	262	0.044	ng/ul#	37


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021809.D
Acq On : 19 Sep 2022 18:08
Operator : CG/JU
Sample : N4617-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H2


Quant Time: Sep 20 00:25:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

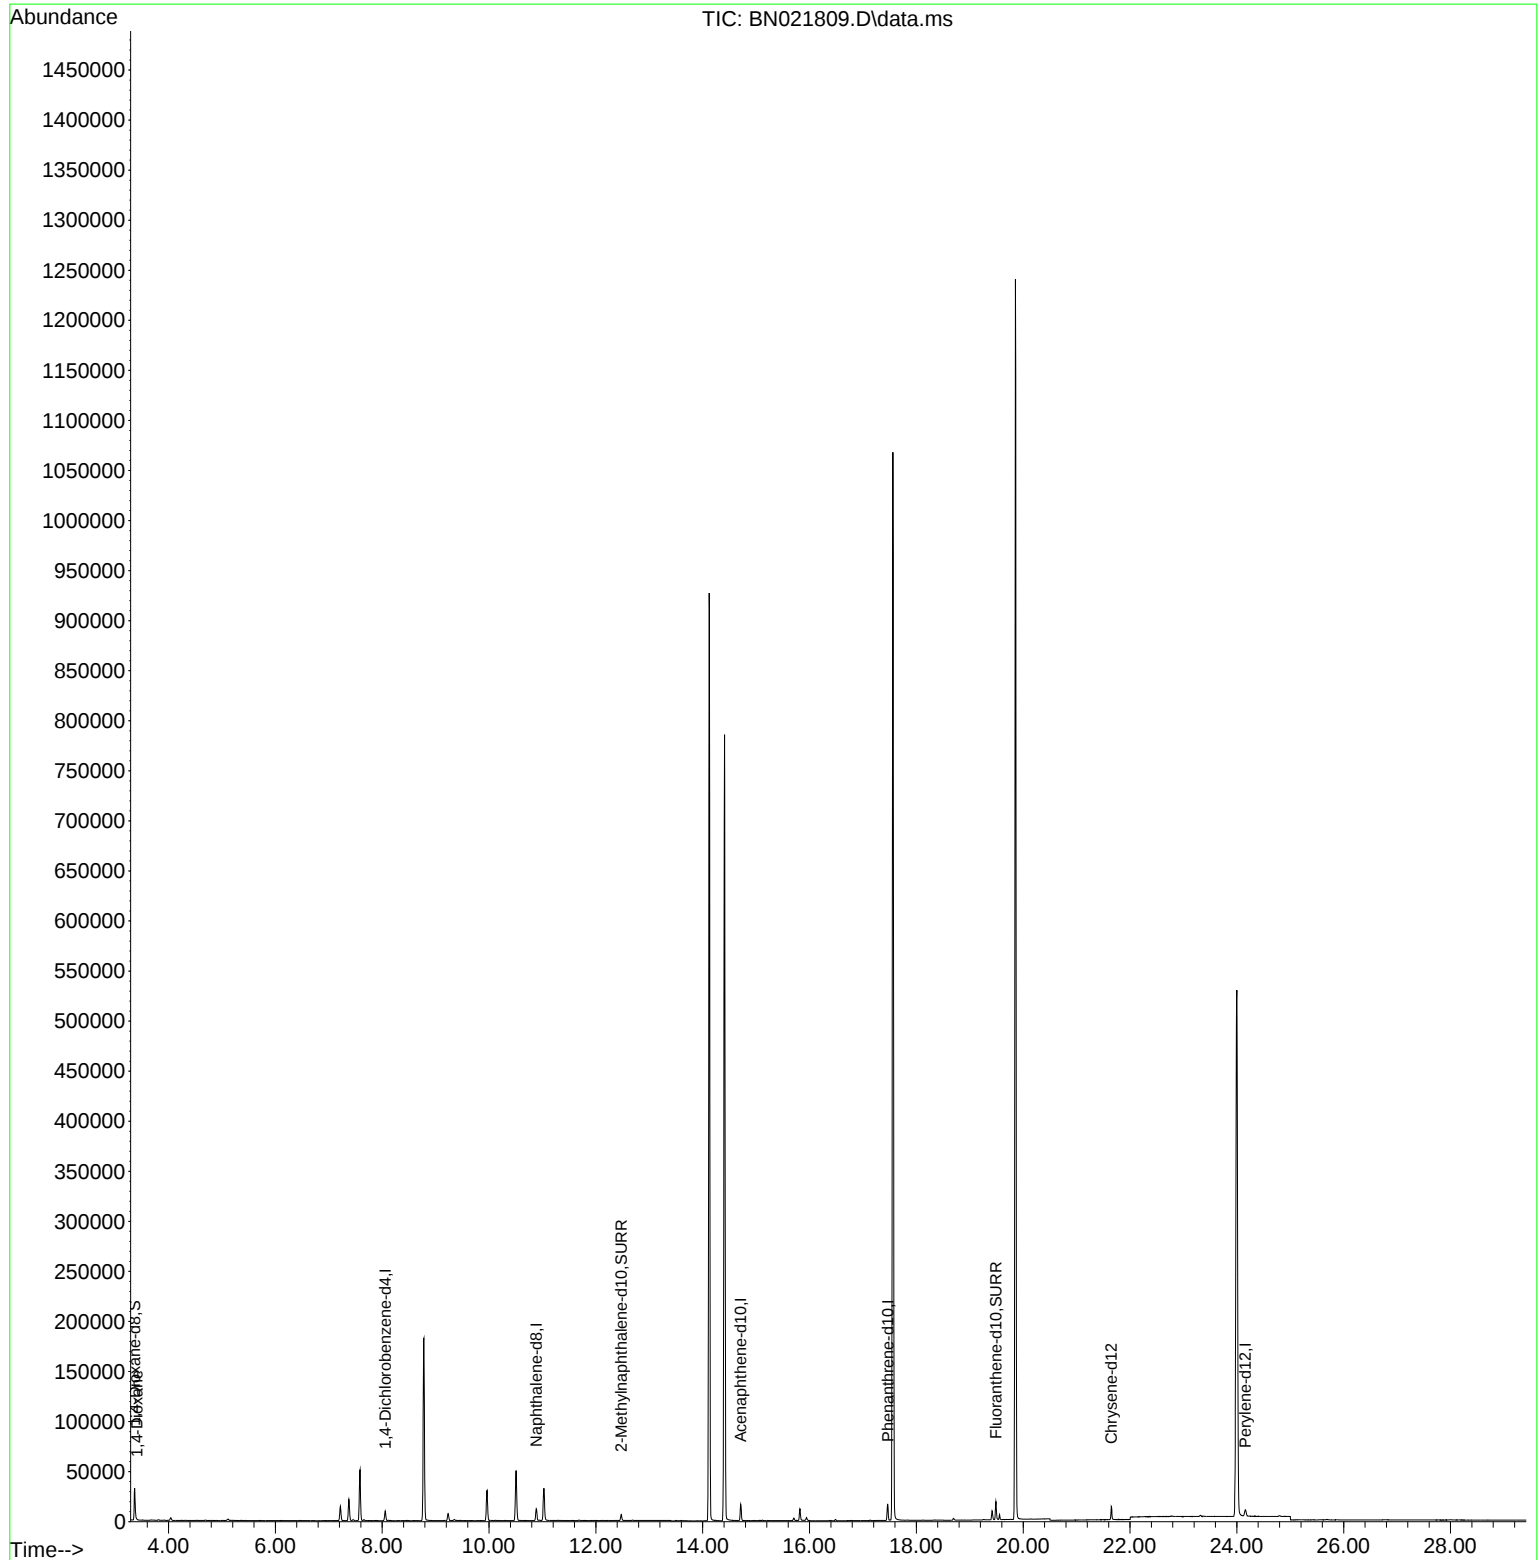

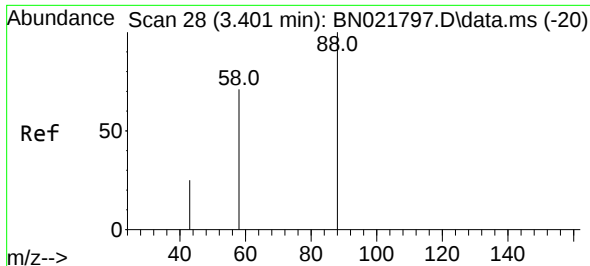

#2
 1,4-Dioxane
 Concen: 0.044 ng/ul
 RT: 3.405 min Scan# 29
 Delta R.T. 0.004 min
 Lab File: BN021809.D
 Acq: 19 Sep 2022 18:08

Instrument :
 BNA_N
 ClientSampleId :
 CB8H2

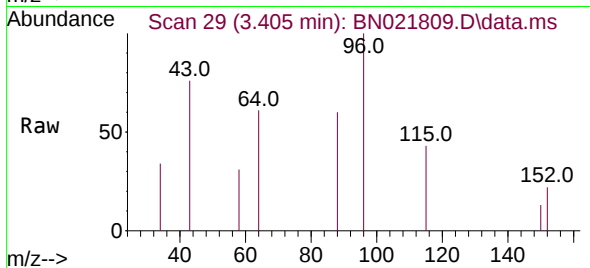

Tgt Ion: 88 Resp: 262

Ion	Ratio	Lower	Upper
88	100		
43	126.6	31.4	47.0#
58	51.8	49.0	73.6

