

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021819.D
 Acq On : 20 Sep 2022 01:06
 Operator : CG/JU
 Sample : N4595-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H8

Quant Time: Sep 20 01:55:28 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.055	152	6214	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	20726	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	12975	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	24471	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.650	240	15805	0.400	ng/ul	# 0.00
23) Perylene-d12	24.158	264	12427	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	26213	3.429	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8643	0.263	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	20861	0.355	ng/ul	0.00
Target Compounds						
16) Anthracene	17.595	178	3191	0.050	ng/ul#	Qvalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021819.D
Acq On : 20 Sep 2022 01:06
Operator : CG/JU
Sample : N4595-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H8


Quant Time: Sep 20 01:55:28 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

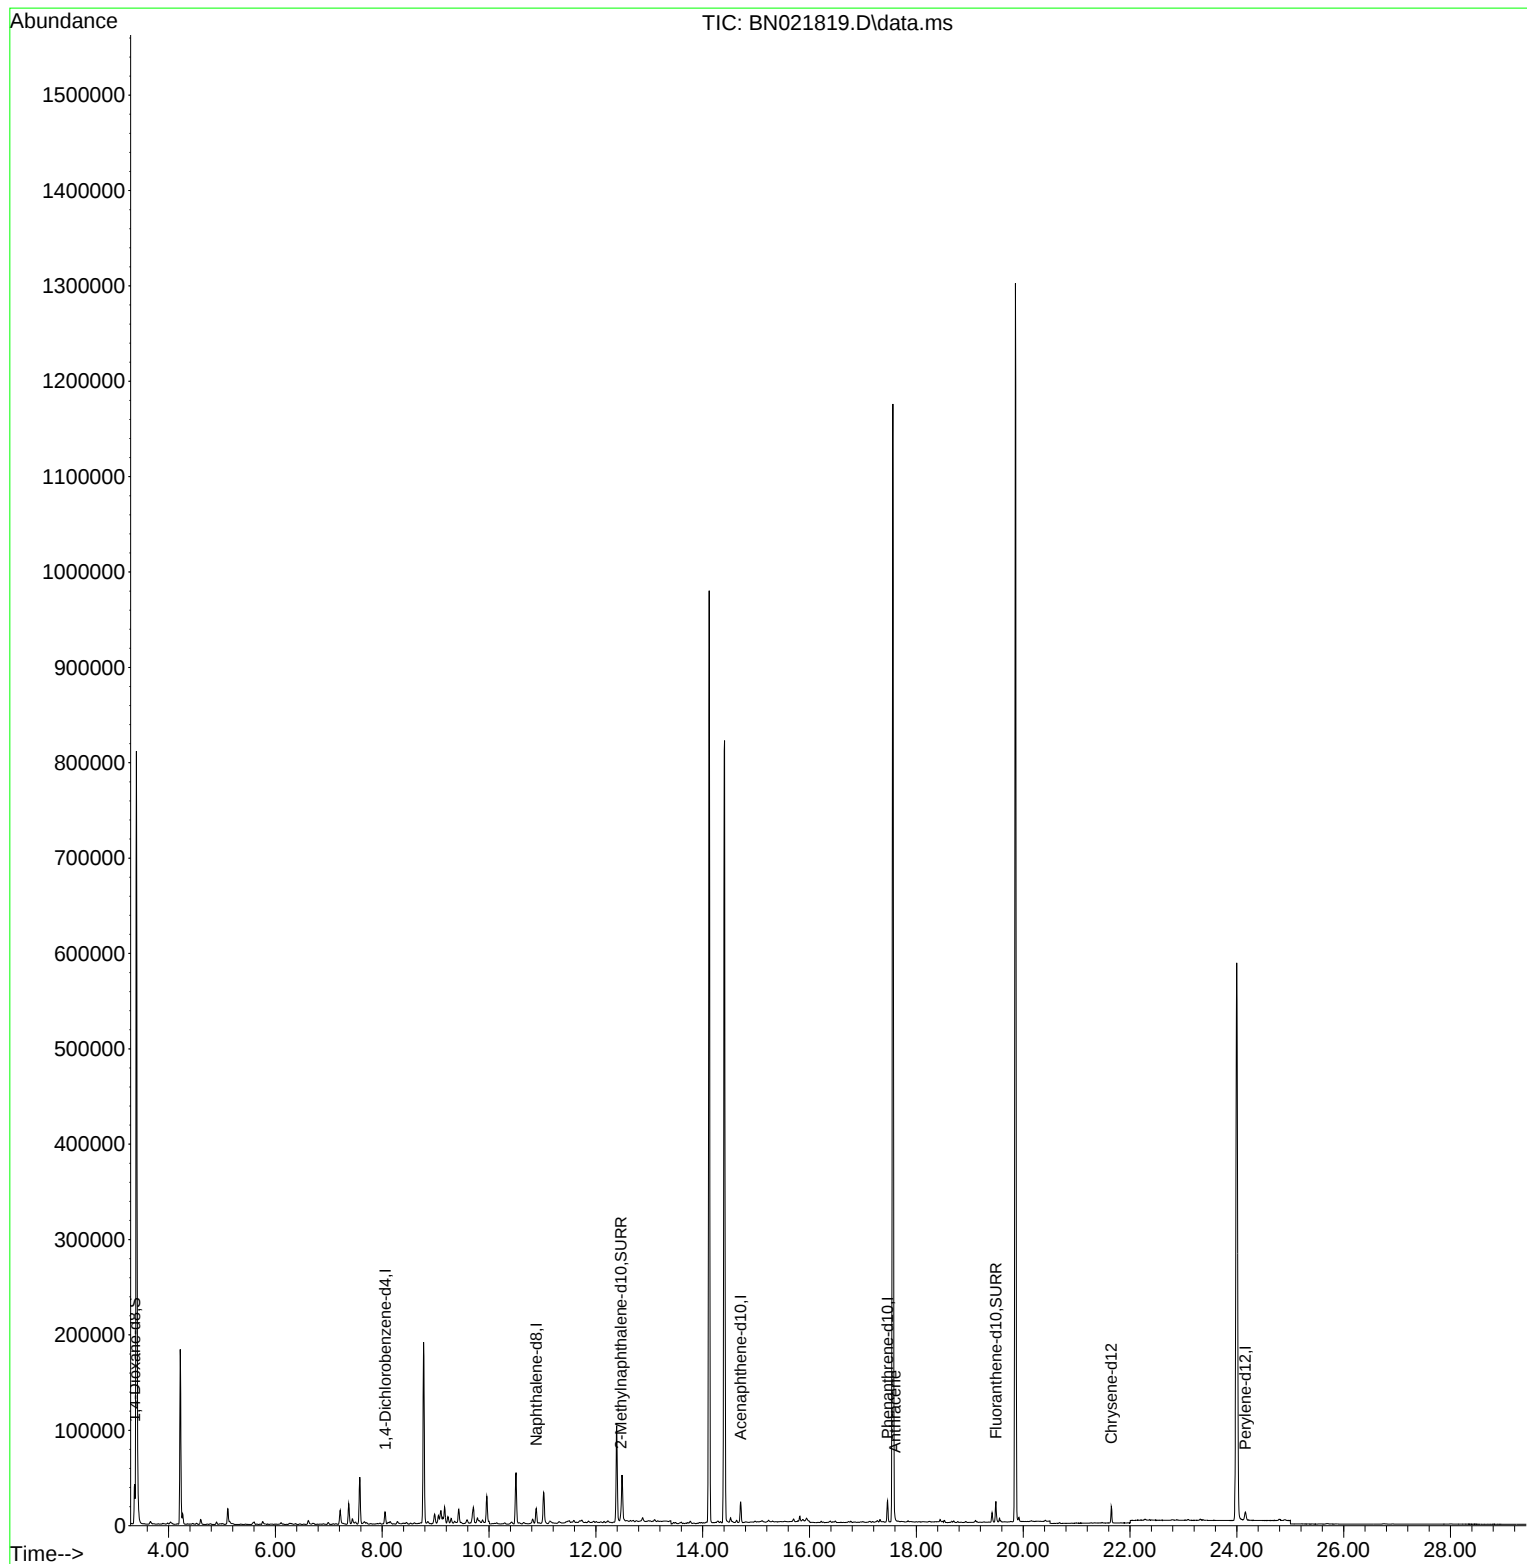

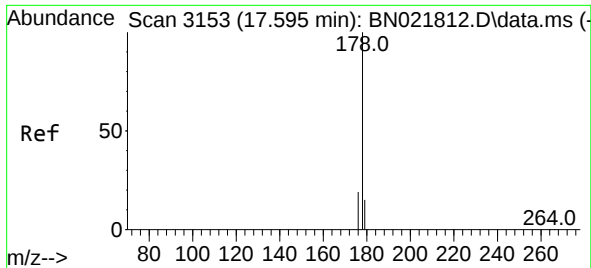

#16
 Anthracene
 Concen: 0.050 ng/ul
 RT: 17.595 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: BN021819.D
 Acq: 20 Sep 2022 01:06

Instrument :
 BNA_N
 ClientSampleId :
 CB8H8

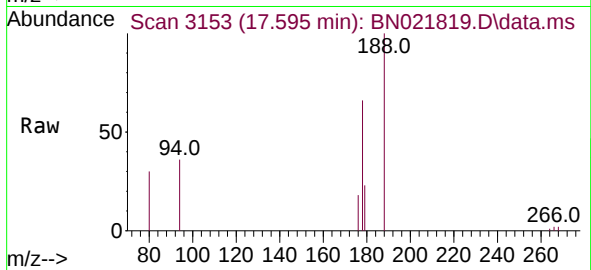

Tgt Ion:178 Resp: 3191
 Ion Ratio Lower Upper
 178 100
 179 34.3 12.9 19.3#
 176 27.5 15.9 23.9#

