

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021820.D
 Acq On : 20 Sep 2022 01:44
 Operator : CG/JU
 Sample : N4617-07
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H8

Quant Time: Sep 20 02:13:16 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5731	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	19145	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.712	164	11945	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	21825	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	13268	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	11148	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	21716	3.080	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8890	0.293	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	19981	0.405	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	600305	83.010	ng/ul#	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021820.D
Acq On : 20 Sep 2022 01:44
Operator : CG/JU
Sample : N4617-07
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H8


Quant Time: Sep 20 02:13:16 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

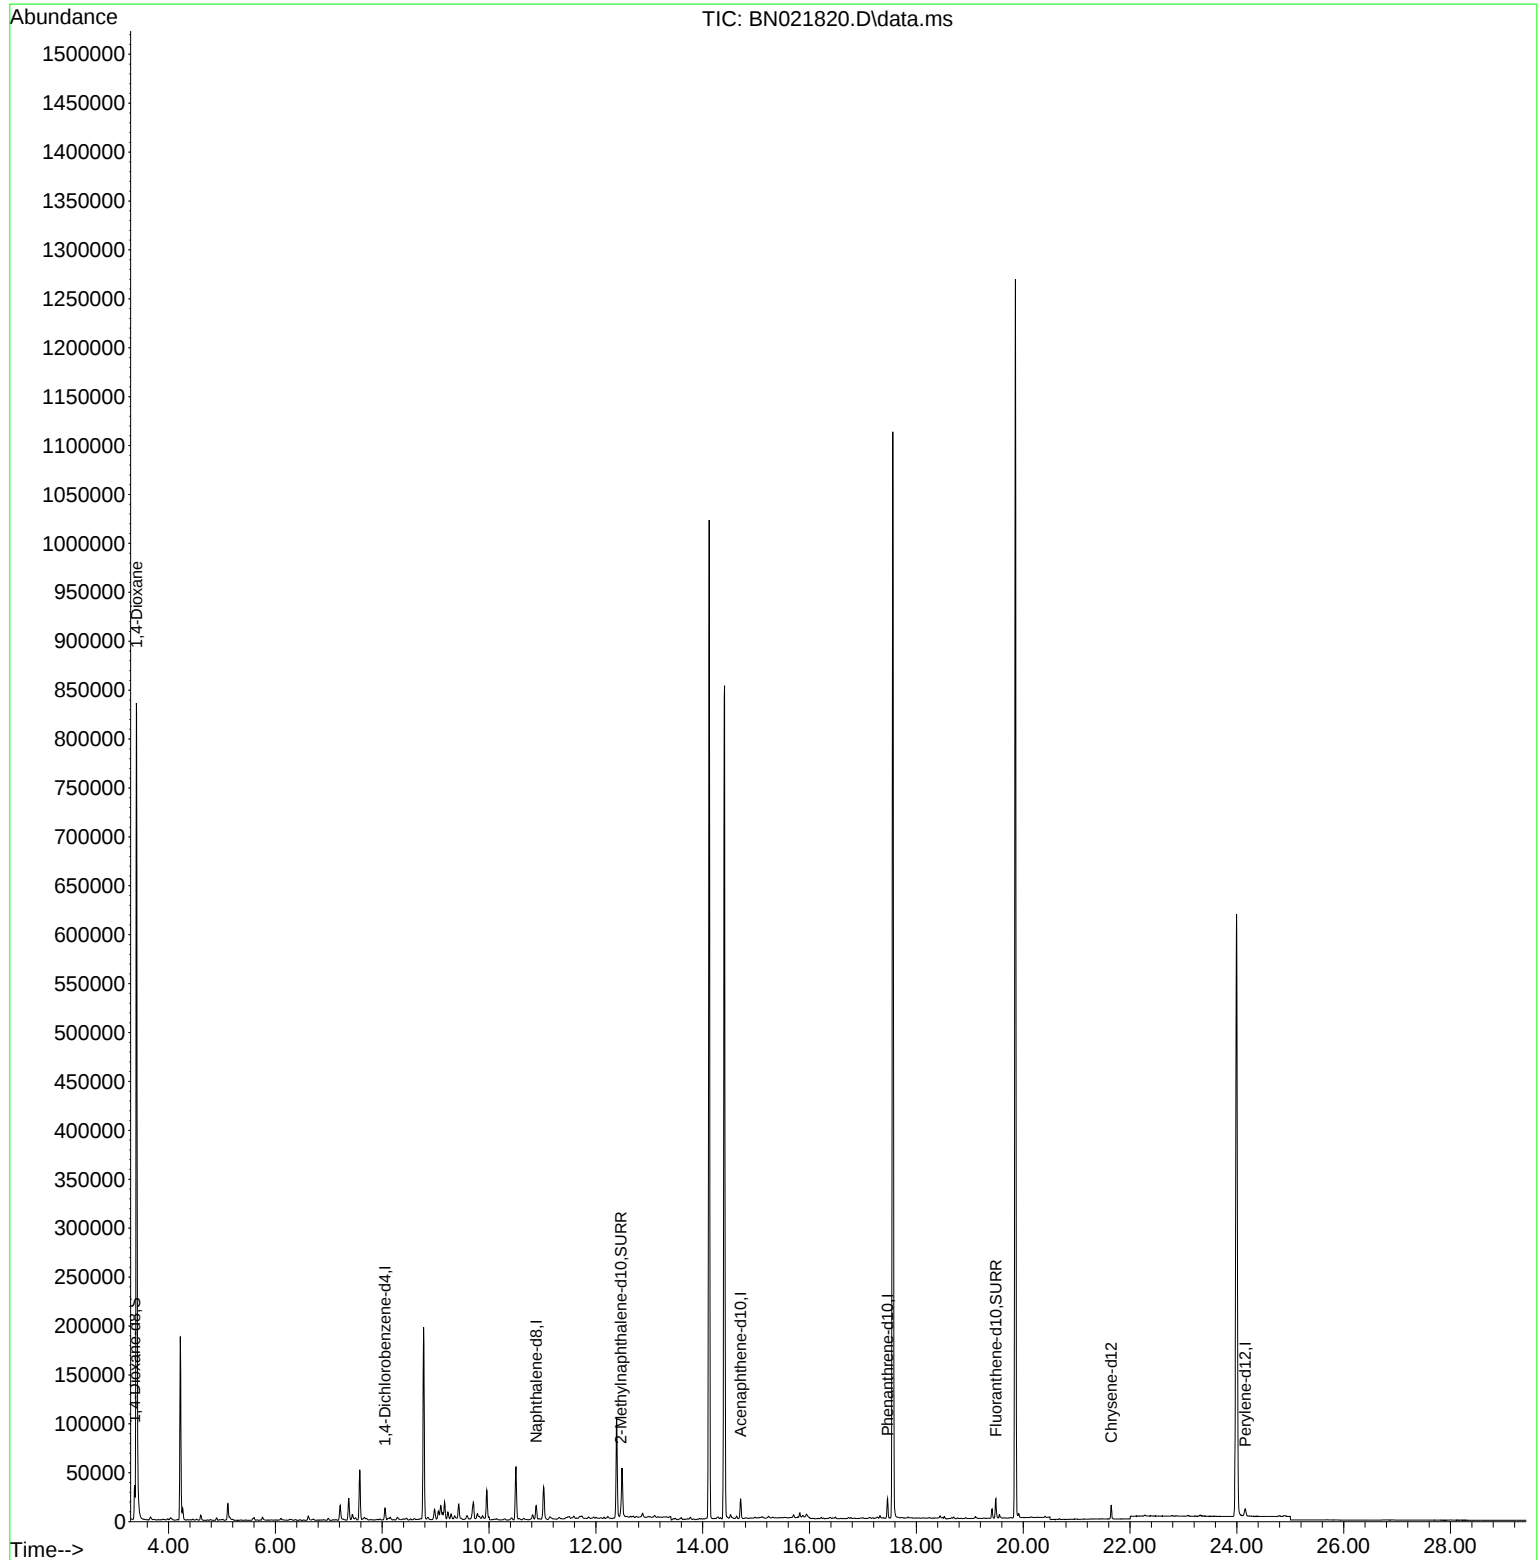

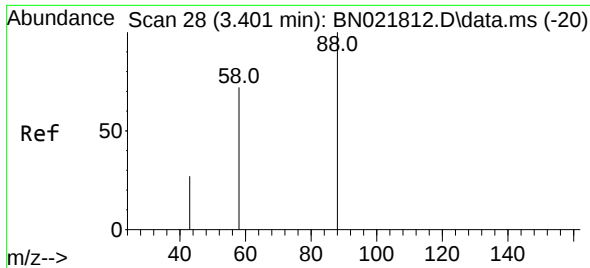

#2
 1,4-Dioxane
 Concen: 83.010 ng/ul
 RT: 3.401 min Scan# 28
 Delta R.T. 0.000 min
 Lab File: BN021820.D
 Acq: 20 Sep 2022 01:44

Instrument :
 BNA_N
 ClientSampleId :
 CB8H8

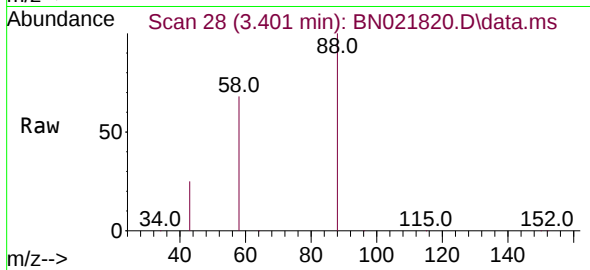

Tgt Ion: 88 Resp: 600305
 Ion Ratio Lower Upper
 88 100
 43 25.4 31.4 47.0#
 58 68.2 49.0 73.6

