

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021822.D
 Acq On : 20 Sep 2022 02:59
 Operator : CG/JU
 Sample : N4617-08
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9

Quant Time: Sep 20 03:30:53 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5143	0.400	ng/ul	0.00
4) Naphthalene-d8	10.883	136	17223	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.708	164	10395	0.400	ng/ul	# 0.00
13) Phenanthrene-d10	17.460	188	20660	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	13152	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	10499	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.364	96	22143	3.500	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	7673	0.281	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	17620	0.360	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	14878	2.293	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021822.D
Acq On : 20 Sep 2022 02:59
Operator : CG/JU
Sample : N4617-08
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
CB8H9


Quant Time: Sep 20 03:30:53 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

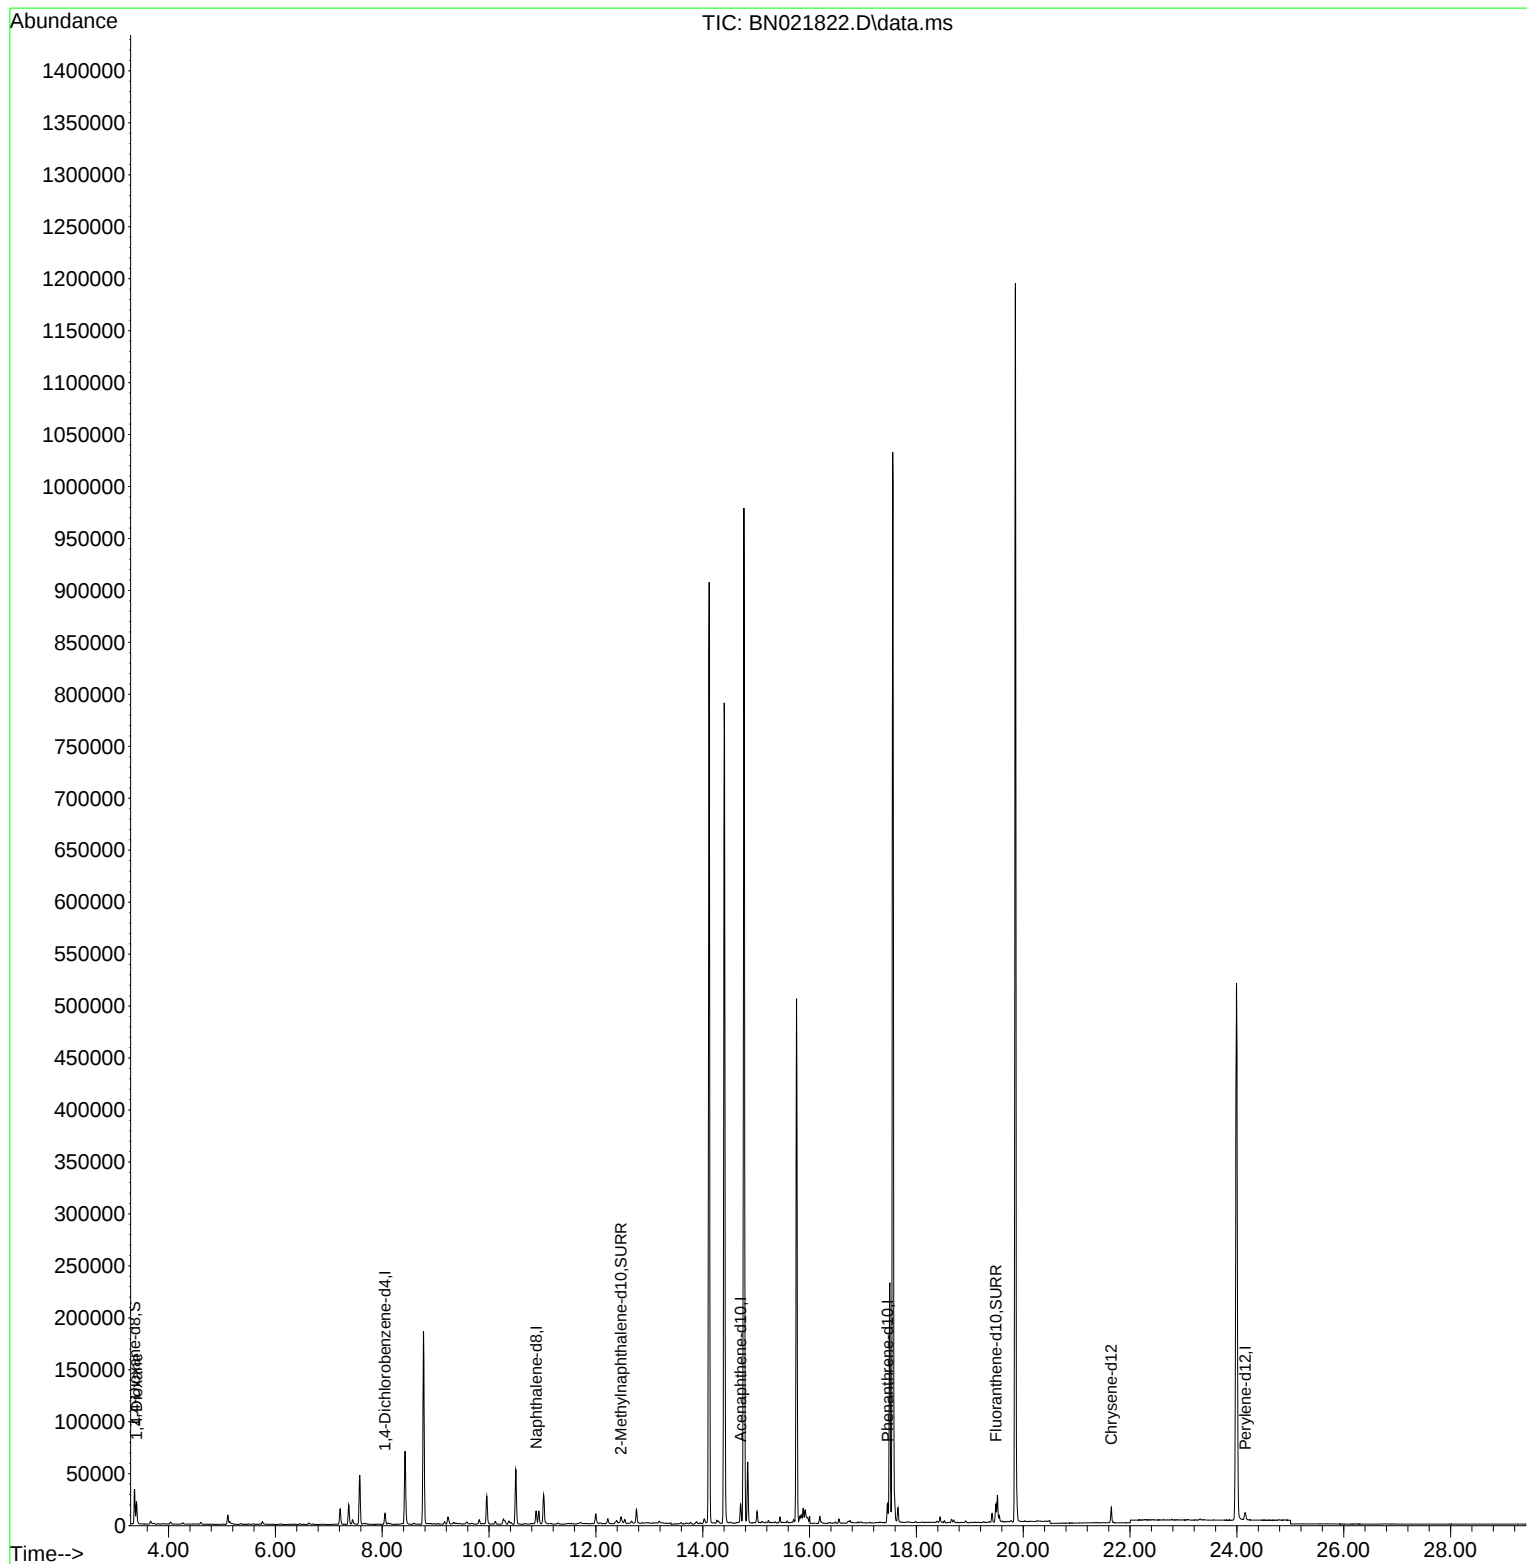

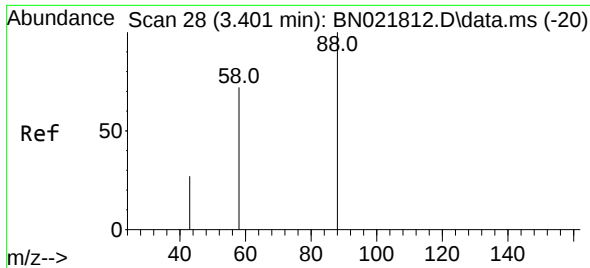

#2
 1,4-Dioxane
 Concen: 2.293 ng/ul
 RT: 3.401 min Scan# 28
 Delta R.T. 0.000 min
 Lab File: BN021822.D
 Acq: 20 Sep 2022 02:59

Instrument :
 BNA_N
 ClientSampleId :
 CB8H9

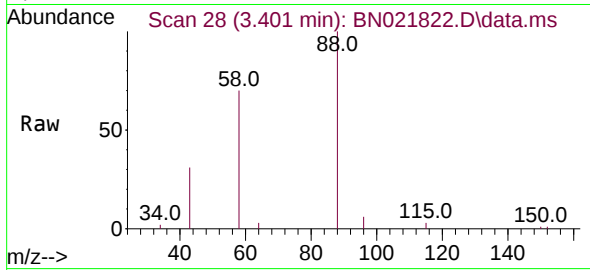

Tgt Ion: 88 Resp: 14878

Ion	Ratio	Lower	Upper
88	100		
43	30.6	31.4	47.0#
58	69.8	49.0	73.6

