

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021825.D
 Acq On : 20 Sep 2022 04:52
 Operator : CG/JU
 Sample : N4649-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ13

Quant Time: Sep 20 05:46:38 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	4607	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	15750	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	9808	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	19081	0.400	ng/ul	# 0.00
17) Chrysene-d12	21.647	240	11356	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	9452	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	27547	4.860	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8501	0.341	ng/ul	0.00
18) Fluoranthene-d10	19.487	212	20029	0.474	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	21332	3.669	ng/ul#	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021825.D
Acq On : 20 Sep 2022 04:52
Operator : CG/JU
Sample : N4649-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ13


Quant Time: Sep 20 05:46:38 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

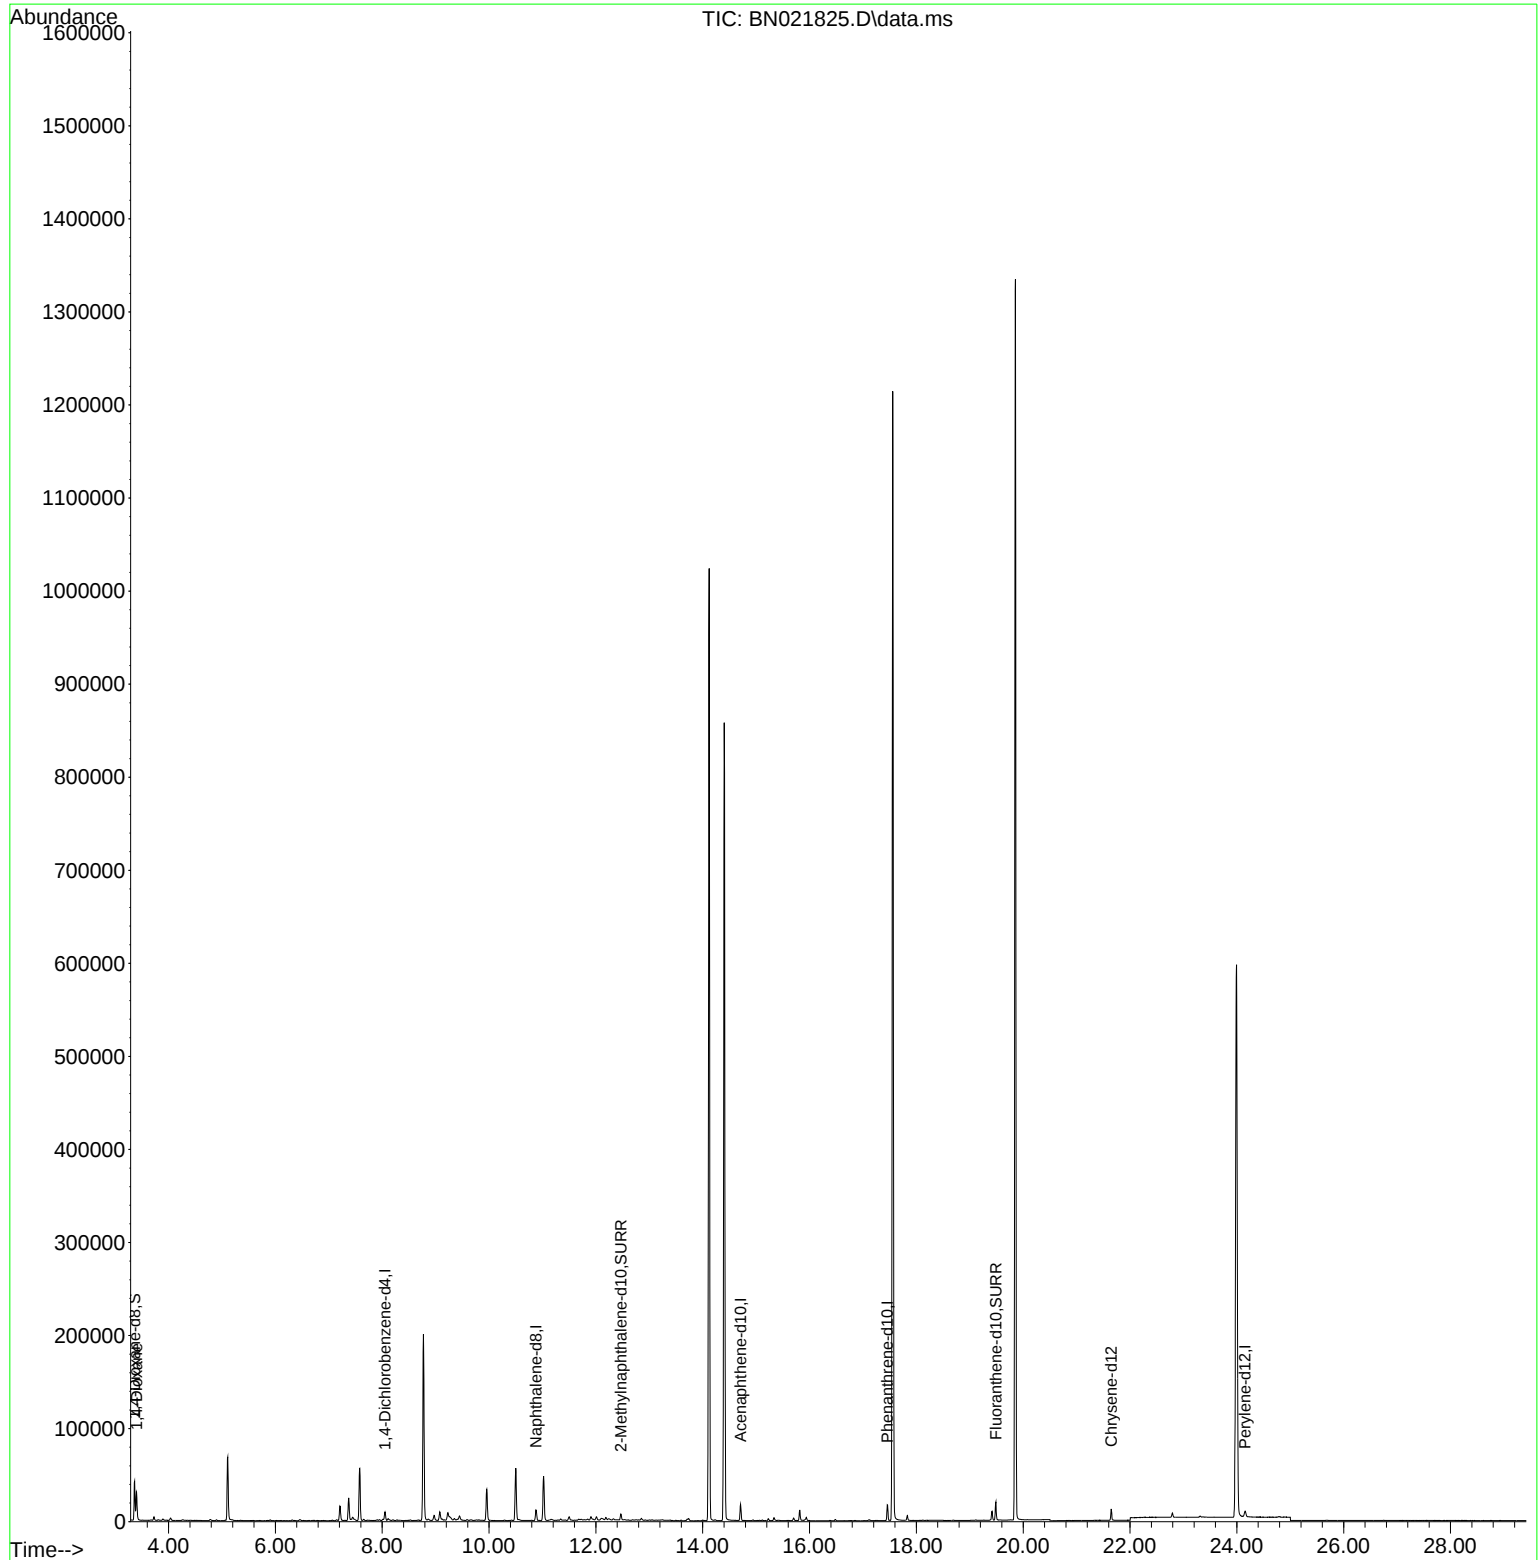

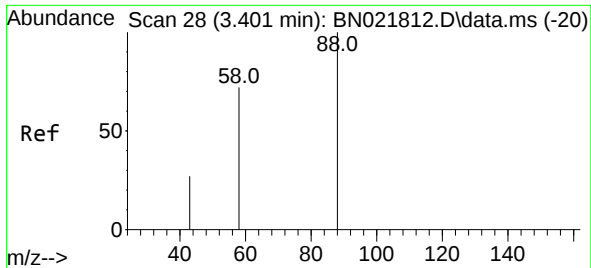

#2
 1,4-Dioxane
 Concen: 3.669 ng/ul
 RT: 3.401 min Scan# 28
 Delta R.T. -0.000 min
 Lab File: BN021825.D
 Acq: 20 Sep 2022 04:52

Instrument :
 BNA_N
 ClientSampleId :
 EXZ13

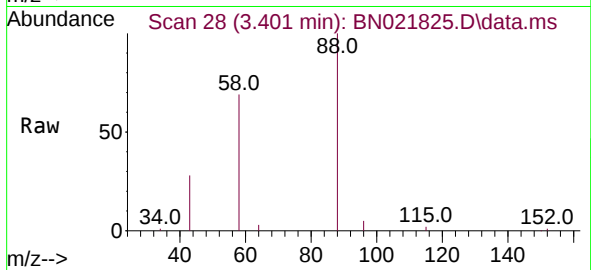

Tgt Ion: 88 Resp: 21332

Ion	Ratio	Lower	Upper
88	100		
43	28.1	31.4	47.0#
58	68.6	49.0	73.6

