

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021835.D
 Acq On : 20 Sep 2022 12:29
 Operator : CG/JU
 Sample : N4649-05
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ30

Quant Time: Sep 20 14:27:59 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.050	152	4516	0.400	ng/ul	0.00
4) Naphthalene-d8	10.877	136	15084	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	8668	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.455	188	17406	0.400	ng/ul	0.00
17) Chrysene-d12	21.650	240	10329	0.400	ng/ul	# 0.00
23) Perylene-d12	24.155	264	8411	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	27993	5.038	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.467	152	8943	0.374	ng/ul	0.00
18) Fluoranthene-d10	19.482	212	19160	0.499	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.401	88	201	0.035	ng/ul#	42


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021835.D
Acq On : 20 Sep 2022 12:29
Operator : CG/JU
Sample : N4649-05
Misc :
ALS Vial : 41 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ30


Quant Time: Sep 20 14:27:59 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

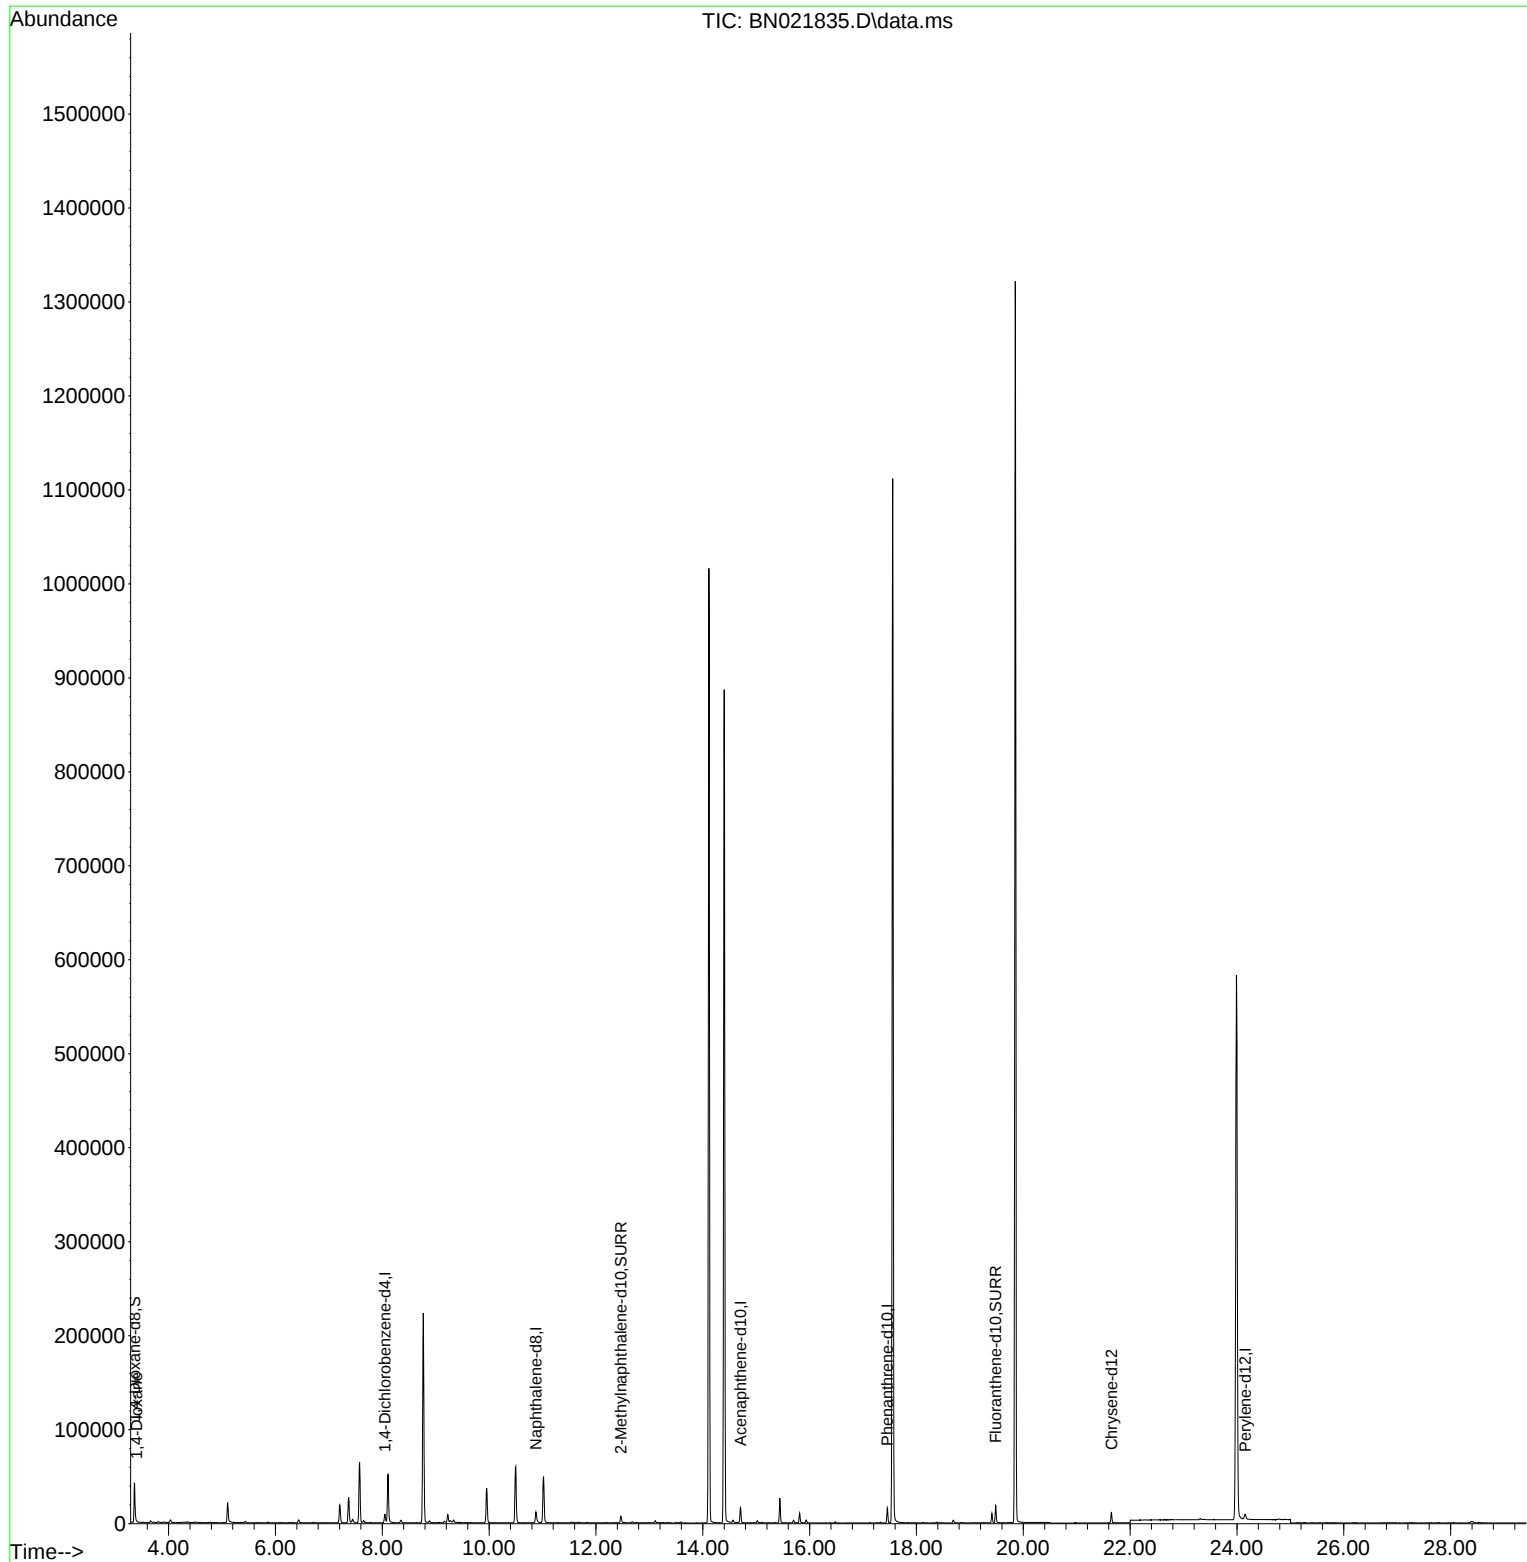

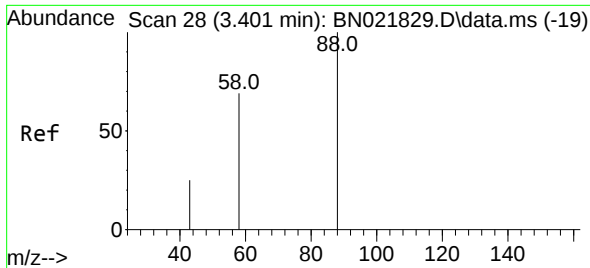

#2
 1,4-Dioxane
 Concen: 0.035 ng/ul
 RT: 3.401 min Scan# 28
 Delta R.T. -0.000 min
 Lab File: BN021835.D
 Acq: 20 Sep 2022 12:29

Instrument :
 BNA_N
 ClientSampleId :
 EXZ30

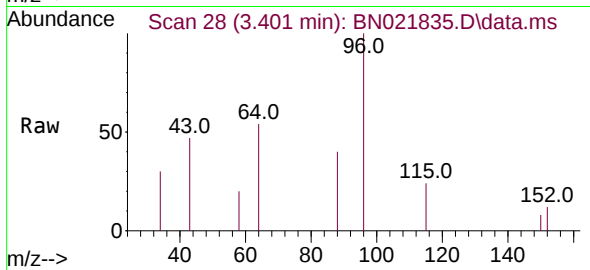

Tgt Ion: 88 Resp: 201
 Ion Ratio Lower Upper
 88 100
 43 117.8 31.4 47.0#
 58 51.3 49.0 73.6

