

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
 Data File : BN021841.D
 Acq On : 20 Sep 2022 16:17
 Operator : CG/JU
 Sample : N4649-10
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 EXZ38

Quant Time: Sep 20 16:46:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 20 00:20:21 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.051	152	5105	0.400	ng/ul	0.00
4) Naphthalene-d8	10.878	136	16966	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.707	164	9592	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.460	188	18618	0.400	ng/ul	0.00
17) Chrysene-d12	21.647	240	10705	0.400	ng/ul	# 0.00
23) Perylene-d12	24.152	264	9127	0.400	ng/ul	# 0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.363	96	25412	4.046	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.473	152	8645	0.322	ng/ul	0.00
18) Fluoranthene-d10	19.483	212	18300	0.460	ng/ul	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	3.397	88	19015	2.952	ng/ul#	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091922\
Data File : BN021841.D
Acq On : 20 Sep 2022 16:17
Operator : CG/JU
Sample : N4649-10
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
EXZ38


Quant Time: Sep 20 16:46:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SFAM-EPA-SIM-BN090822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 20 00:20:21 2022
Response via : Initial Calibration

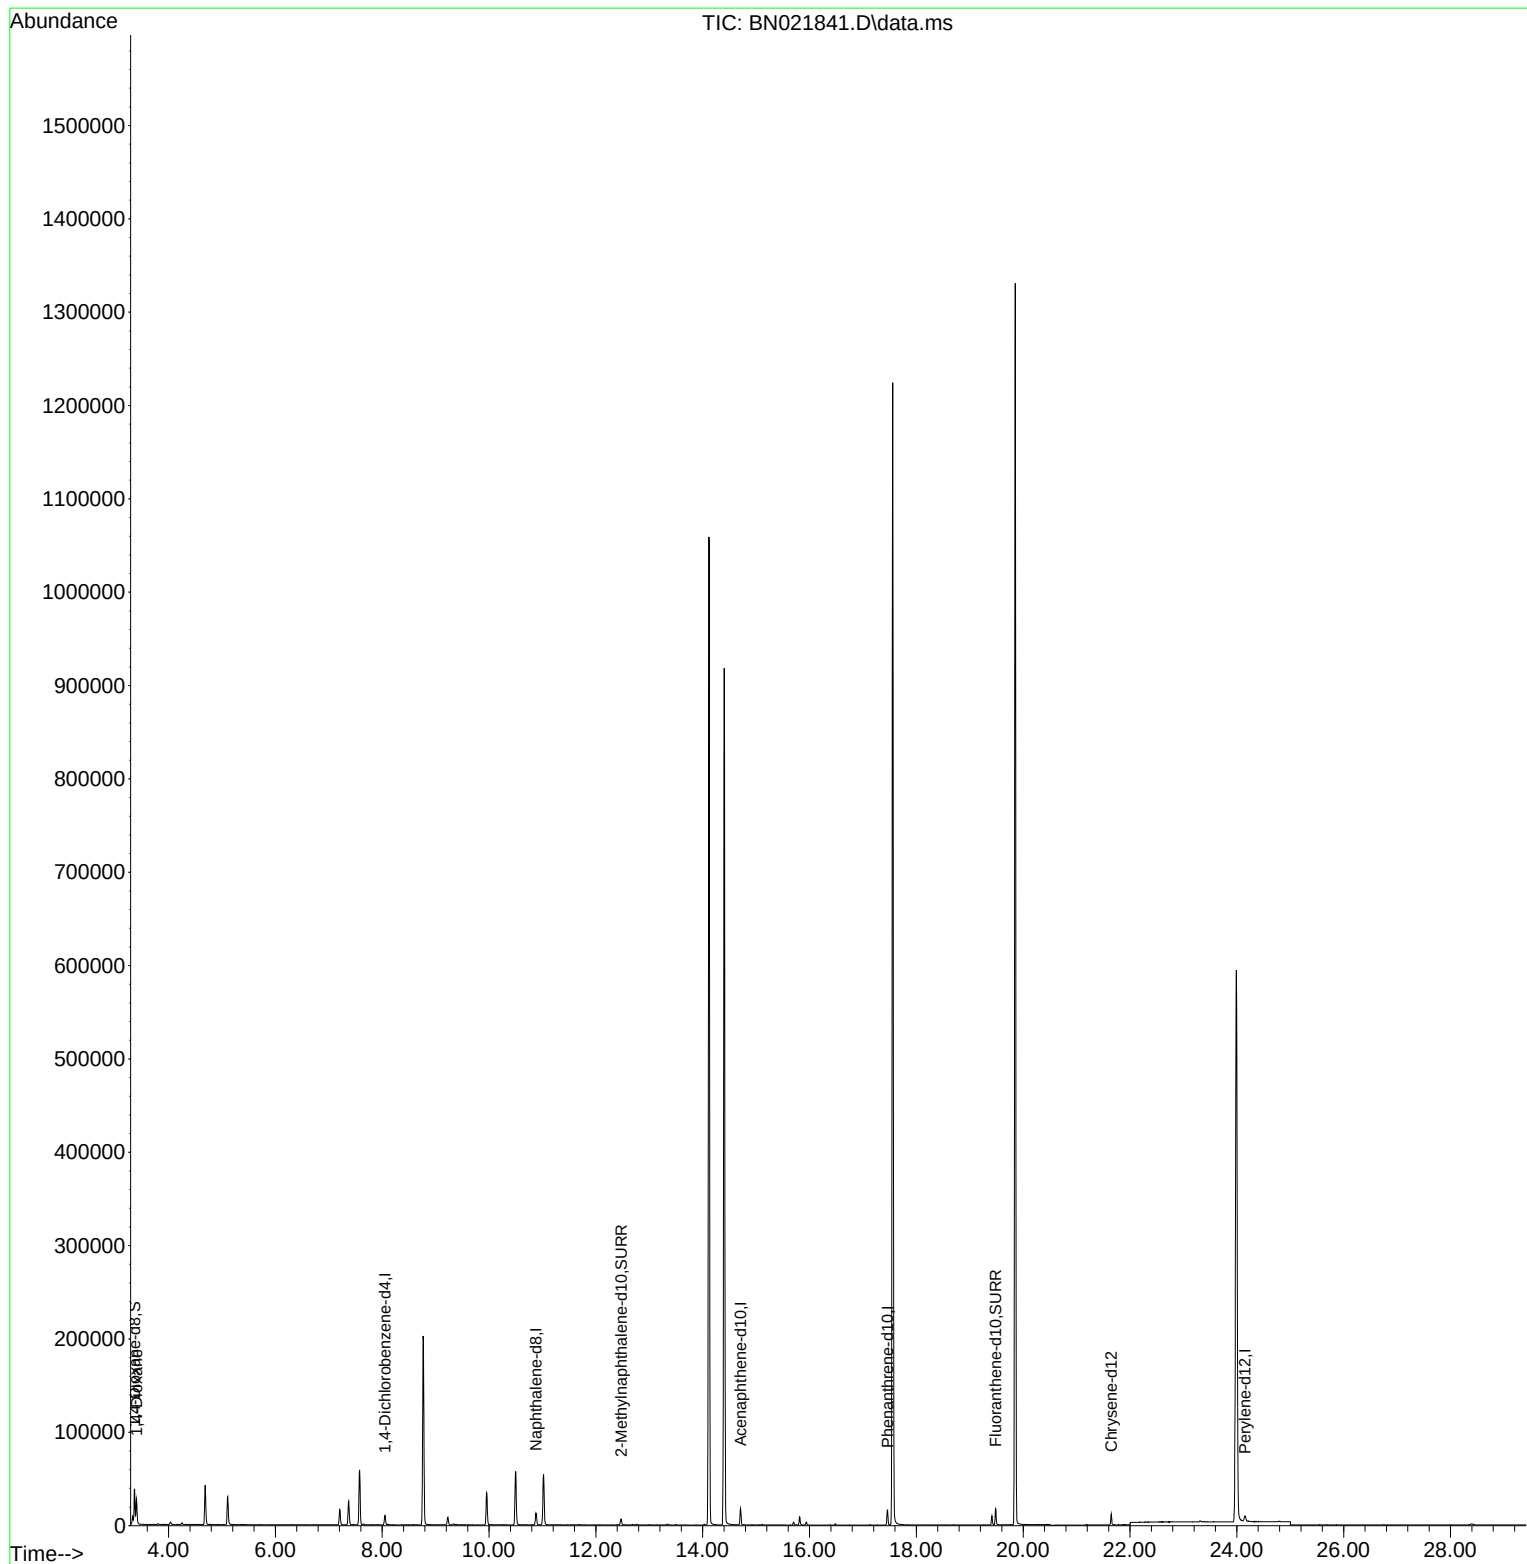

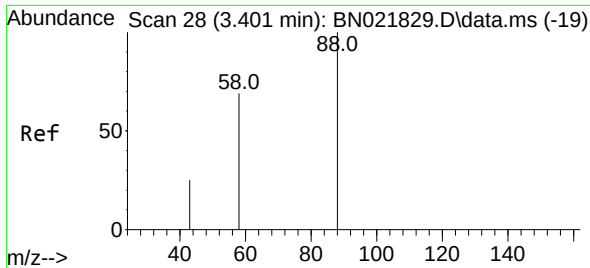

#2
 1,4-Dioxane
 Concen: 2.952 ng/ul
 RT: 3.397 min Scan# 21
 Delta R.T. -0.004 min
 Lab File: BN021841.D
 Acq: 20 Sep 2022 16:17

Instrument :
 BNA_N
 ClientSampleId :
 EXZ38

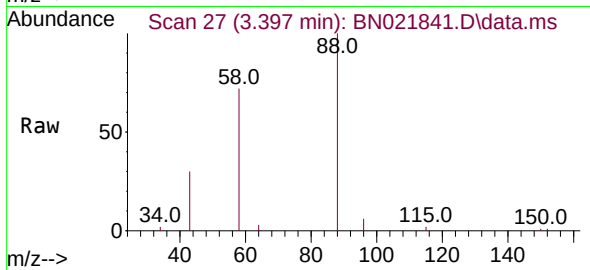

Tgt Ion: 88 Resp: 19015
 Ion Ratio Lower Upper
 88 100
 43 29.5 31.4 47.0#
 58 72.4 49.0 73.6

