
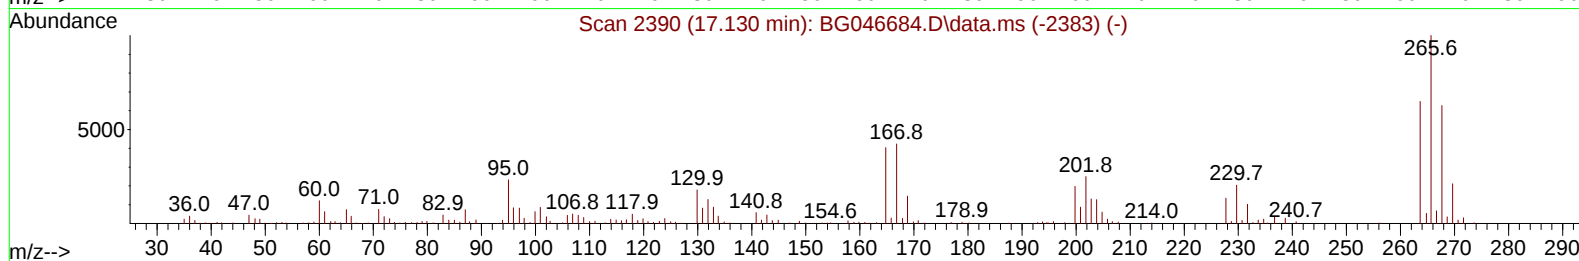
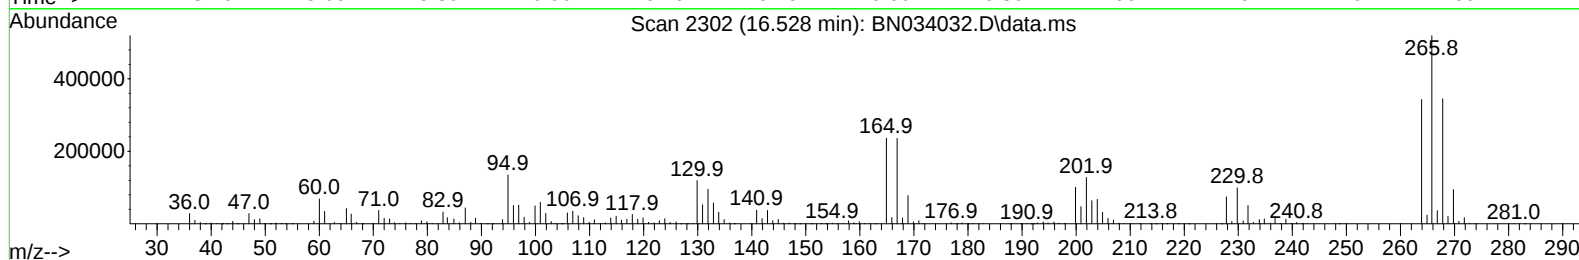


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034032.D
Acq On : 18 Sep 2024 08:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 17:07:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

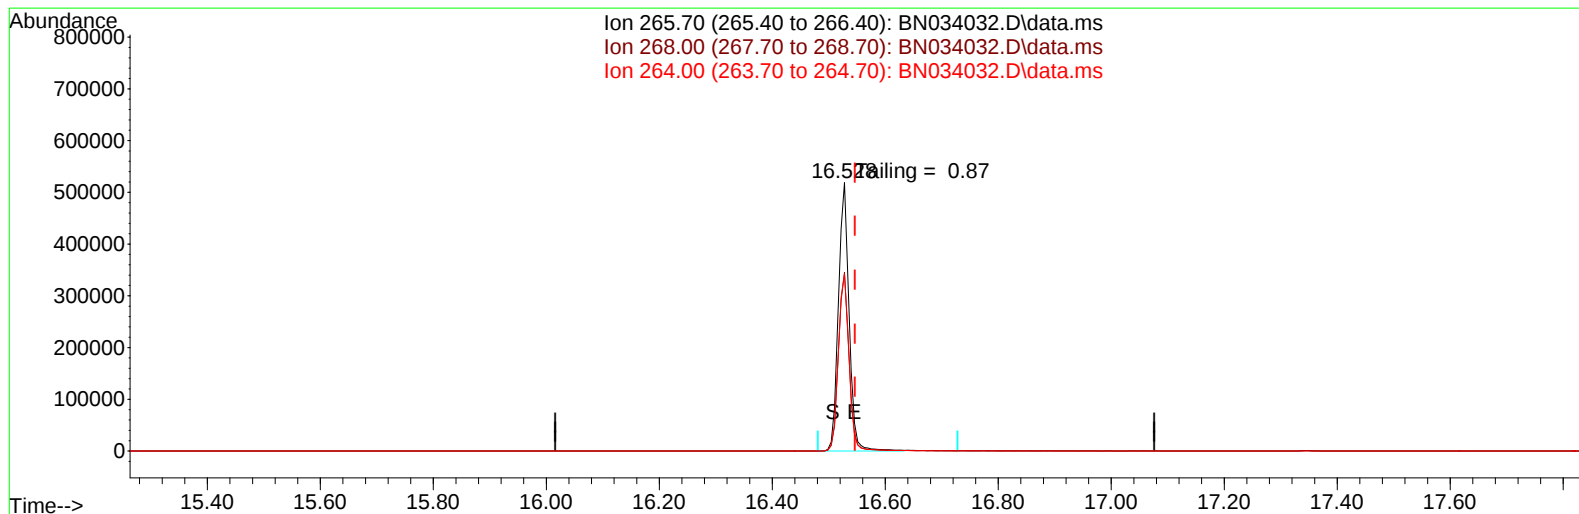

TIC: BN034032.D\data.ms

(70) Pentachlorophenol (C)




16.528min (-0.018) 32535.82 ng

response 682505

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	66.46
264.00	61.60	66.06
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034032.D
Acq On : 18 Sep 2024 08:34
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 18 17:07:36 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 10 04:22:28 2024
Response via : Initial Calibration

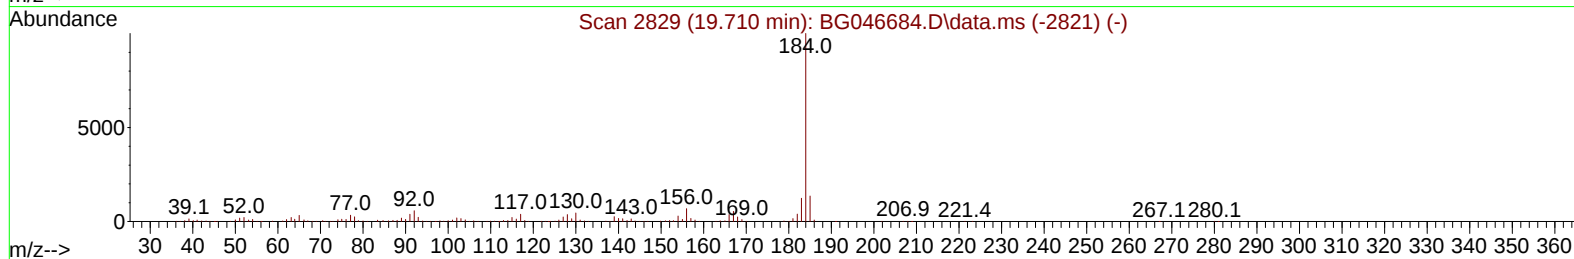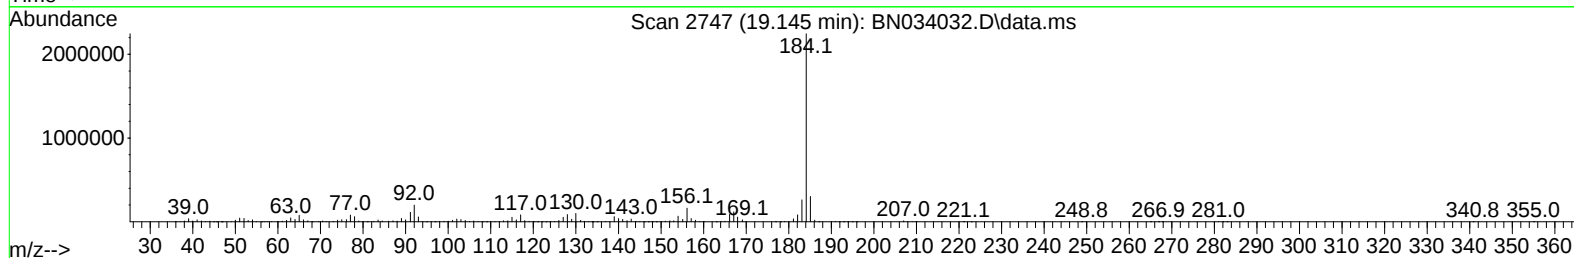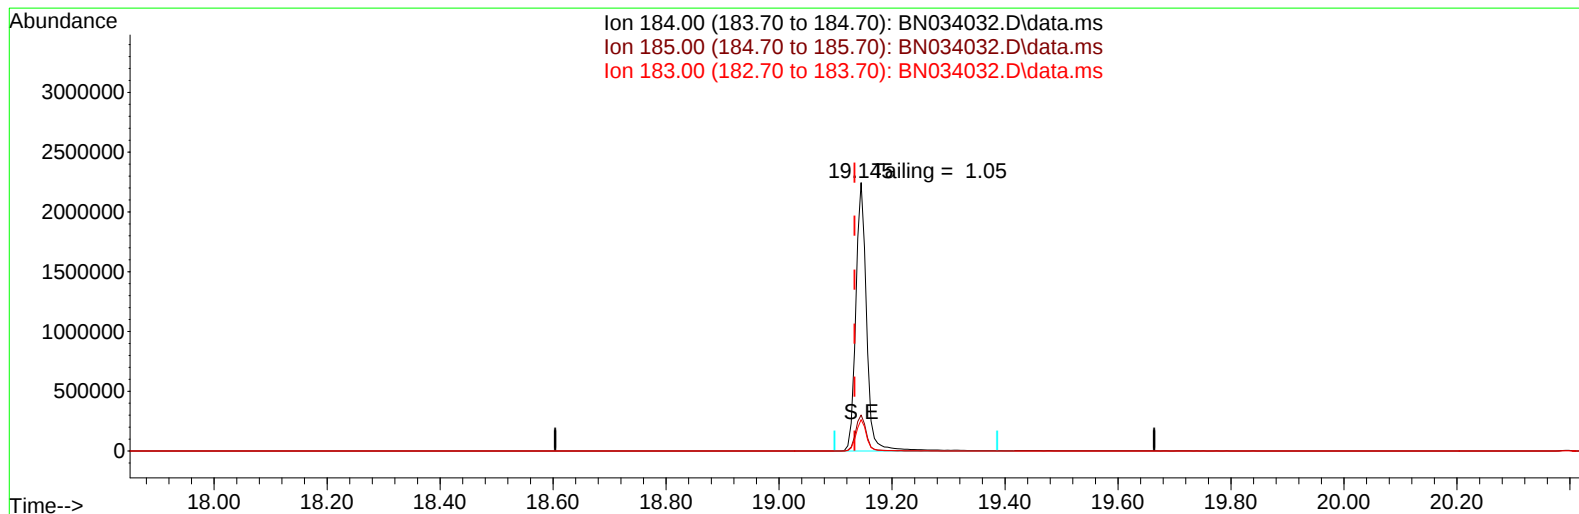

TIC: BN034032.D\data.ms

(77) Benzidine

19.145min (+ 0.011) 0.00 ng

response 3004968

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.44
183.00	13.20	11.67
0.00	0.00	0.00