
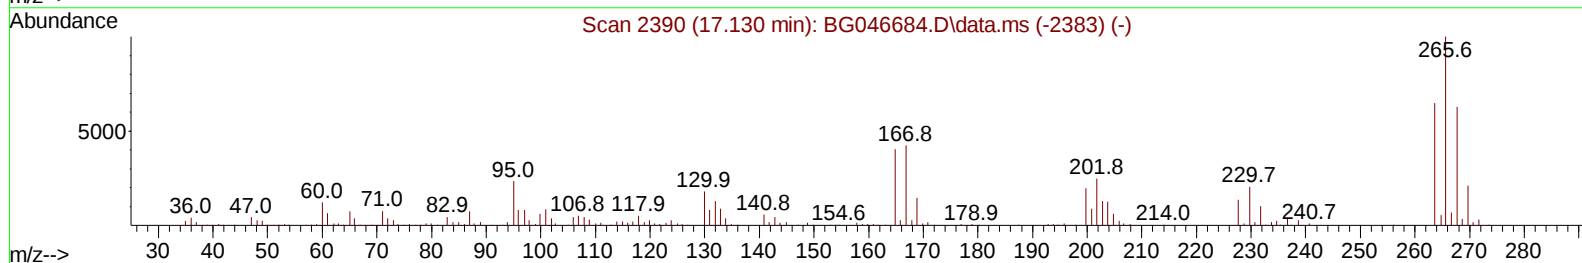
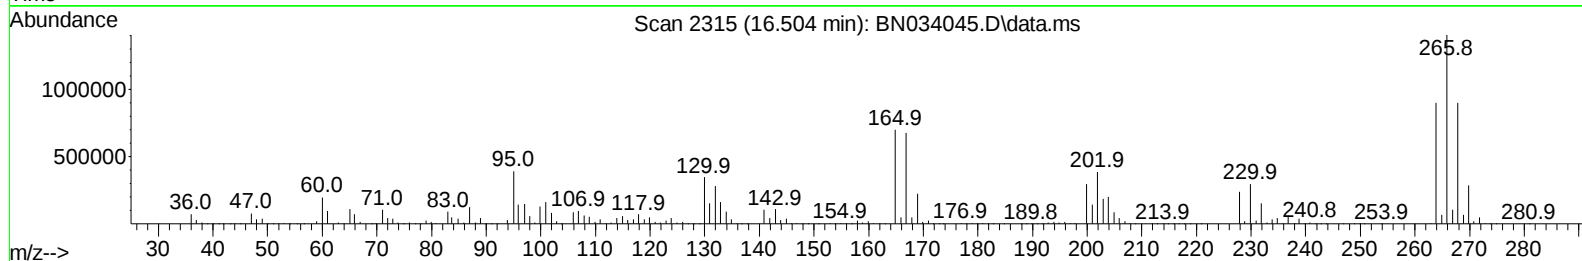


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034045.D
Acq On : 19 Sep 2024 08:54
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 04:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

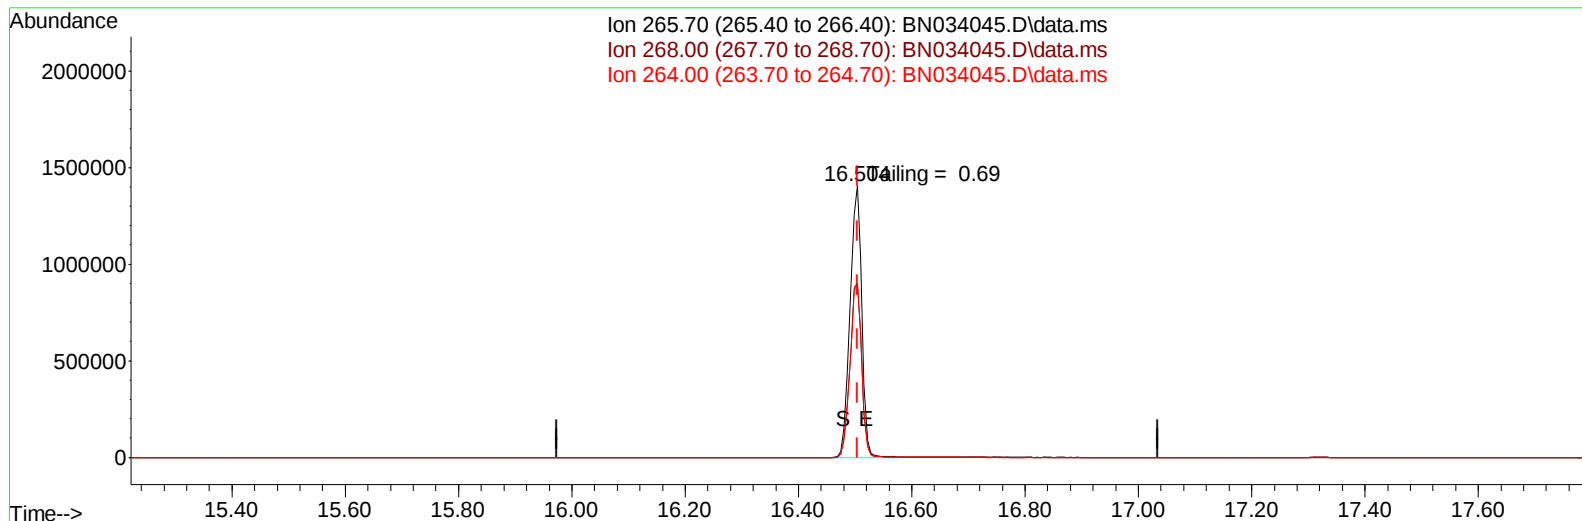




TIC: BN034045.D\data.ms

(70) Pentachlorophenol (C)**16.504min (0.000) 33339.48 ng****response 2034773**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.08
264.00	61.60	63.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091924\
Data File : BN034045.D
Acq On : 19 Sep 2024 08:54
Operator : JU/RC
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 04:53:49 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 20 04:53:44 2024
Response via : Initial Calibration

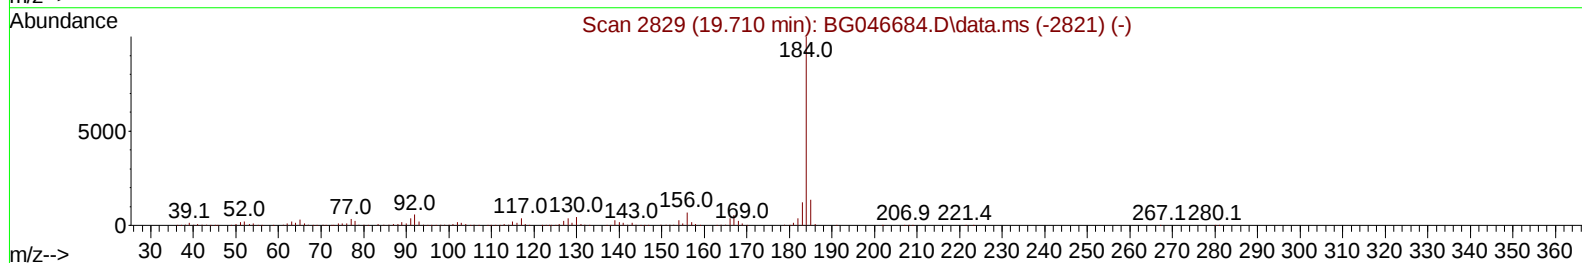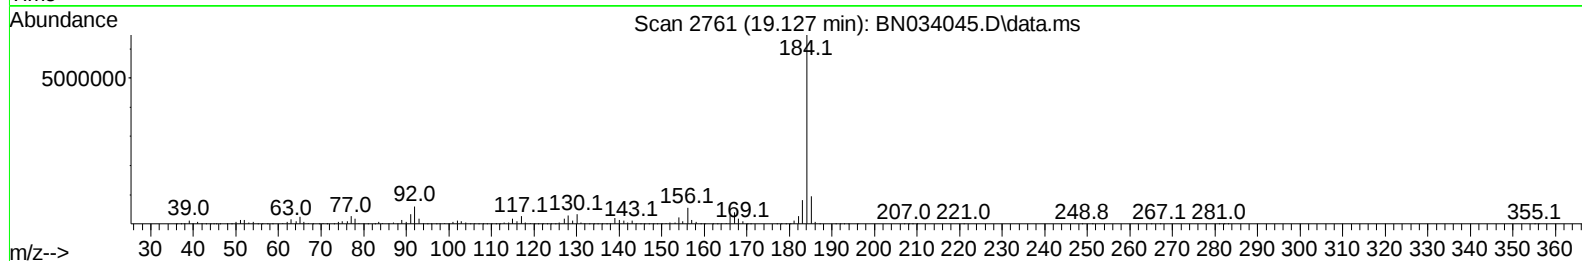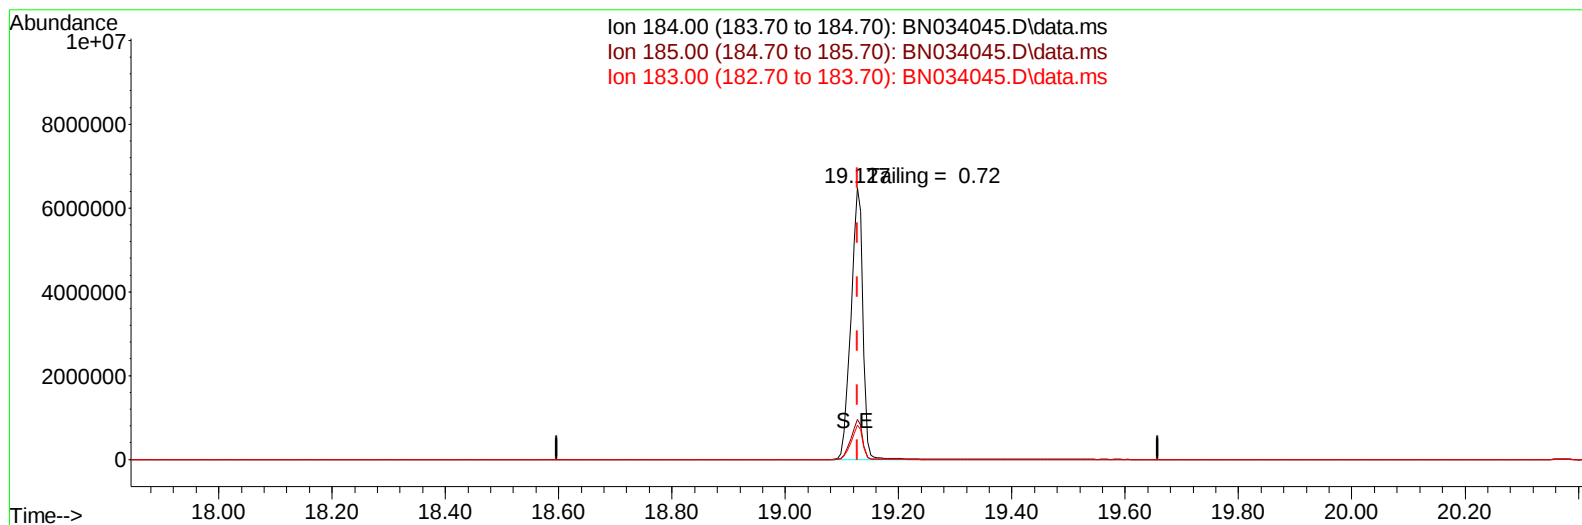

TIC: BN034045.D\data.ms

(77) Benzidine

19.127min (0.000) 0.00 ng

response 9558562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.69
183.00	13.20	12.59
0.00	0.00	0.00