

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
 Data File : BN037818.D
 Acq On : 19 Sep 2025 17:21
 Operator : RC/JU
 Sample : Q3097-19DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :

Quant Time: Sep 19 18:01:02 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 11 14:20:01 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.833	152	8131	0.400	ng	0.00
7) Naphthalene-d8	10.637	136	21334	0.400	ng	-0.01
13) Acenaphthene-d10	14.484	164	9041	0.400	ng	-0.01
19) Phenanthrene-d10	17.235	188	15081	0.400	ng	# 0.00
29) Chrysene-d12	21.411	240	11372	0.400	ng	0.00
35) Perylene-d12	23.744	264	11377	0.400	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.392	112	836	0.045	ng	0.00
5) Phenol-d6	6.988	99	601	0.025	ng	0.00
8) Nitrobenzene-d5	8.982	82	1832	0.117	ng	-0.01
11) 2-Methylnaphthalene-d10	12.227	152	2602	0.092	ng	-0.02
14) 2,4,6-Tribromophenol	15.982	330	298	0.126	ng	0.00
15) 2-Fluorobiphenyl	13.105	172	4101	0.108	ng	-0.01
27) Fluoranthene-d10	19.262	212	4190	0.111	ng	0.00
31) Terphenyl-d14	19.861	244	3082	0.134	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.297	88	21691	2.561	ng	96
34) Bis(2-ethylhexyl)phtha...	21.331	149	479	0.041	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037818.D
Acq On : 19 Sep 2025 17:21
Operator : RC/JU
Sample : Q3097-19DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :


Quant Time: Sep 19 18:01:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN091125.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 11 14:20:01 2025
Response via : Initial Calibration

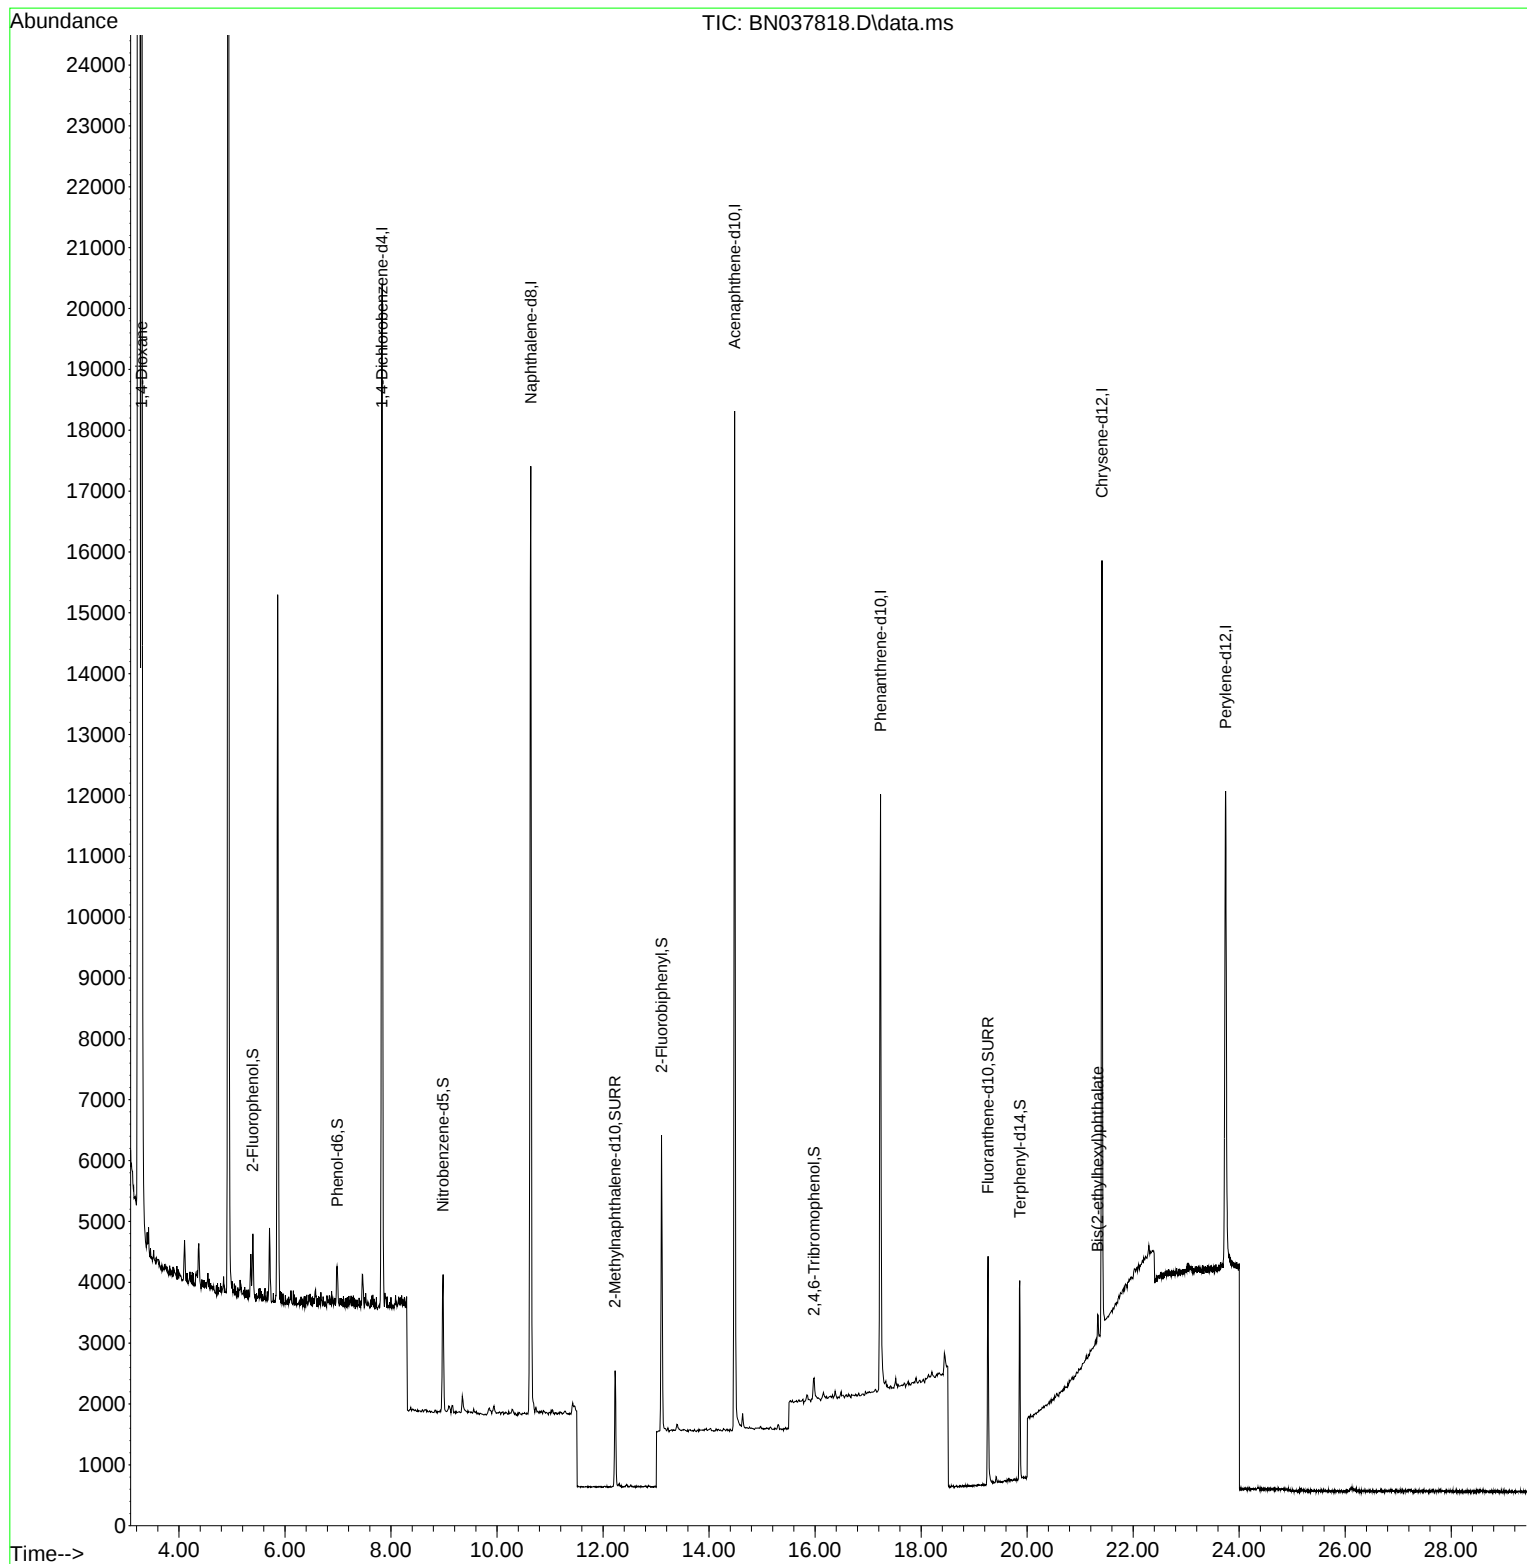





#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.833 min Scan# 61
 Delta R.T. -0.007 min
 Lab File: BN037818.D
 Acq: 19 Sep 2025 17:21


Instrument :
 BNA_N
 ClientSampleId :

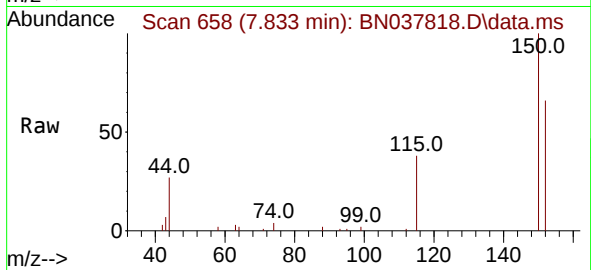



Tgt Ion:152 Resp: 8131
 Ion Ratio Lower Upper
 152 100
 150 151.6 124.5 186.7
 115 58.1 49.2 73.8

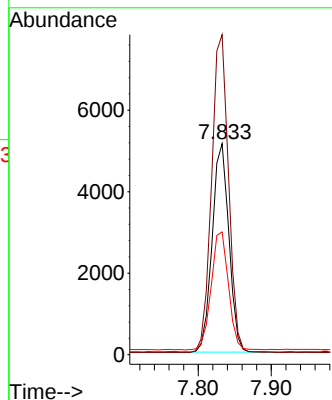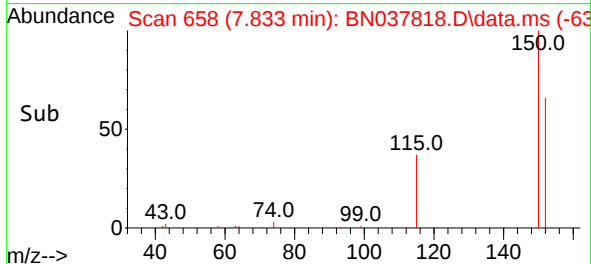

#2
 1,4-Dioxane
 Concen: 2.561 ng
 RT: 3.297 min Scan# 30
 Delta R.T. -0.007 min
 Lab File: BN037818.D
 Acq: 19 Sep 2025 17:21

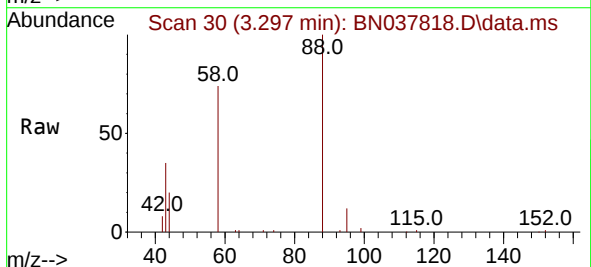

Tgt Ion: 88 Resp: 21691
 Ion Ratio Lower Upper
 88 100
 43 31.2 26.8 40.2
 58 73.4 61.9 92.9


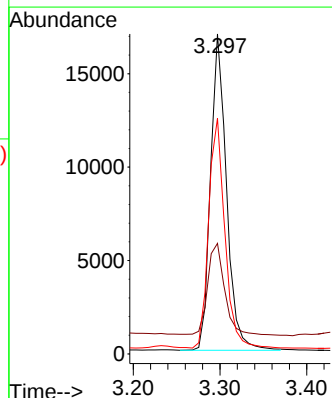
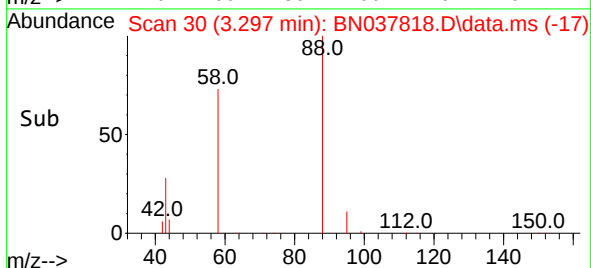




#4
2-Fluorophenol
Concen: 0.045 ng
RT: 5.392 min Scan# 31
Delta R.T. -0.007 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21




Instrument :
BNA_N
ClientSampleId :


Tgt Ion:112 Resp: 836
Ion Ratio Lower Upper
112 100
64 61.2 44.9 67.3
63 36.5 24.7 37.1

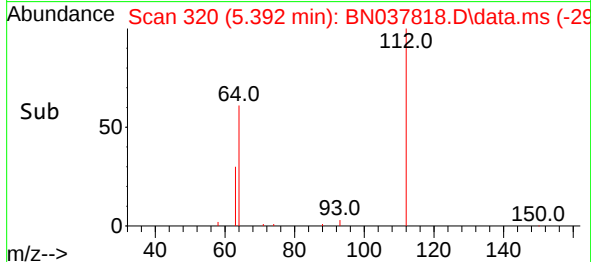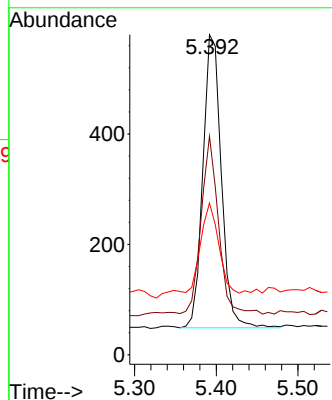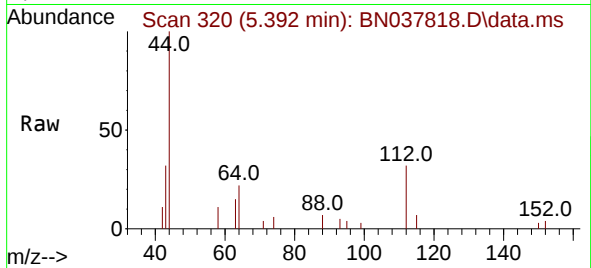

#5
Phenol-d6
Concen: 0.025 ng
RT: 6.988 min Scan# 541
Delta R.T. -0.000 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21


Tgt Ion: 99 Resp: 601
Ion Ratio Lower Upper
99 100
42 23.0 16.6 24.8
71 41.3 26.7 40.1#

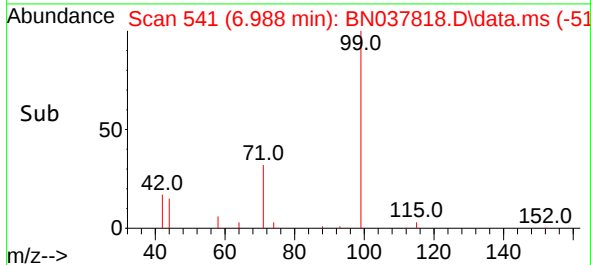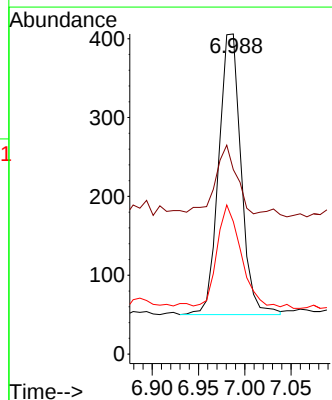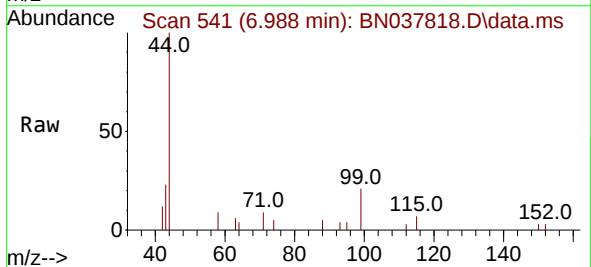


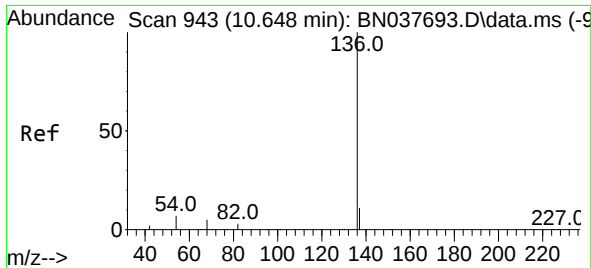


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.637 min Scan# 94
Delta R.T. -0.011 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Instrument :
BNA_N
ClientSampleId :



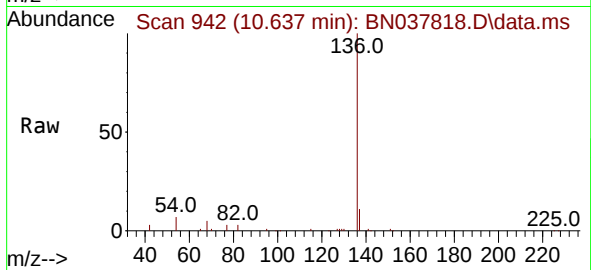


Tgt Ion:136 Resp: 21334
Ion Ratio Lower Upper
136 100
137 11.2 9.1 13.7
54 6.6 6.3 9.5
68 5.3 5.0 7.4

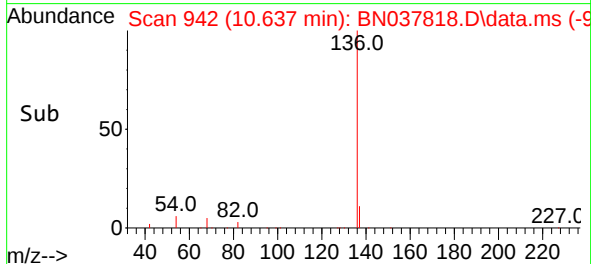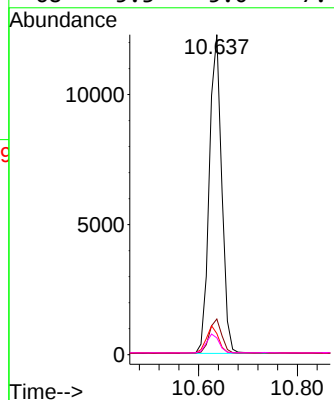

#8
Nitrobenzene-d5
Concen: 0.117 ng
RT: 8.982 min Scan# 787
Delta R.T. -0.011 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Tgt Ion: 82 Resp: 1832
Ion Ratio Lower Upper
82 100
128 50.6 38.3 57.5
54 52.4 41.4 62.2

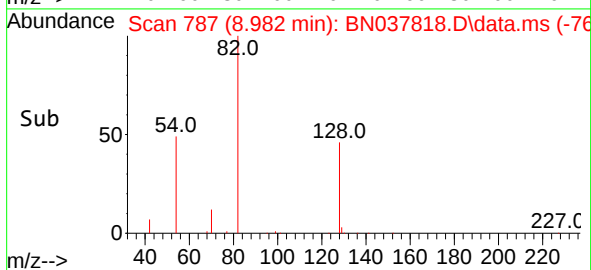
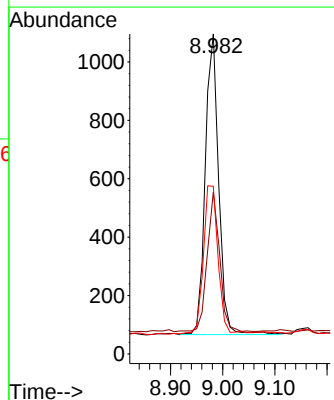
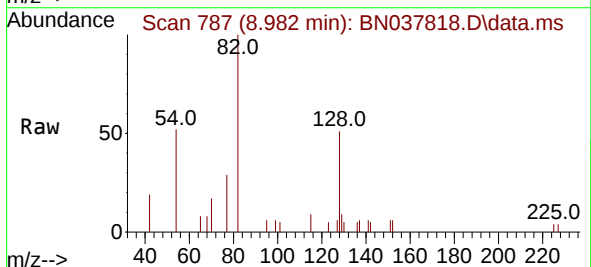




#11
2-Methylnaphthalene-d10
Concen: 0.092 ng
RT: 12.227 min Scan# 1165
Delta R.T. -0.015 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:152 Resp: 2602
Ion Ratio Lower Upper
152 100
151 21.5 17.0 25.6

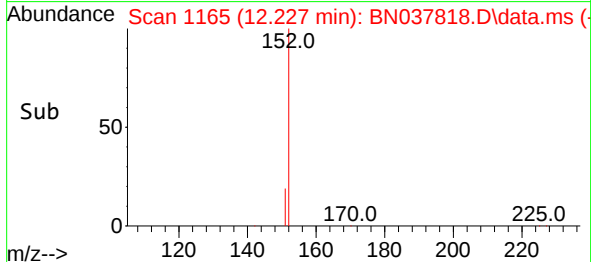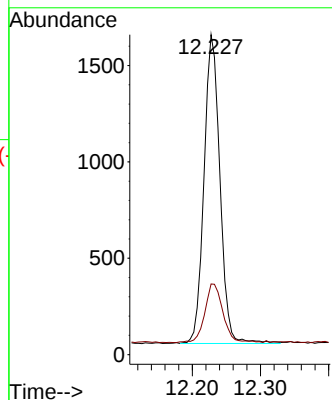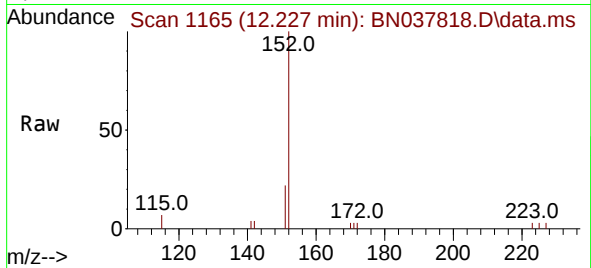

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.484 min Scan# 1457
Delta R.T. -0.011 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Tgt Ion:164 Resp: 9041
Ion Ratio Lower Upper
164 100
162 106.6 83.1 124.7
160 56.5 44.3 66.5

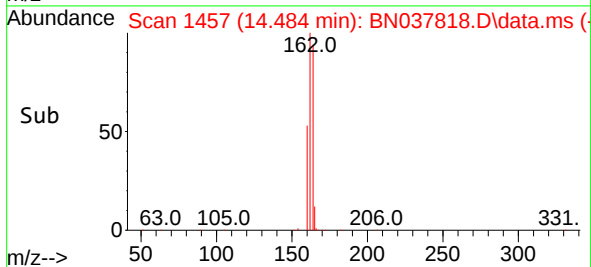
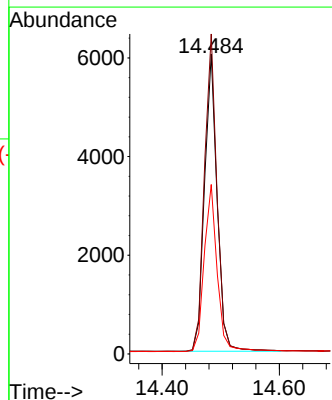
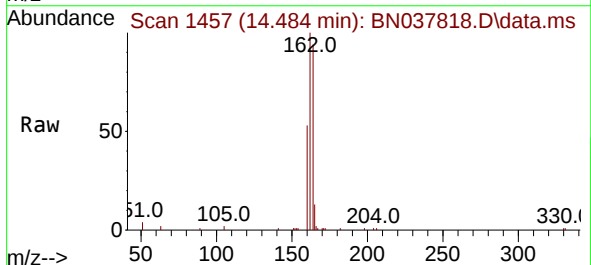




#14
2,4,6-Tribromophenol
Concen: 0.126 ng
RT: 15.982 min Scan# 1591
Delta R.T. -0.000 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:330 Resp: 298
Ion Ratio Lower Upper
330 100
332 91.6 75.3 112.9
141 46.0 35.0 52.4

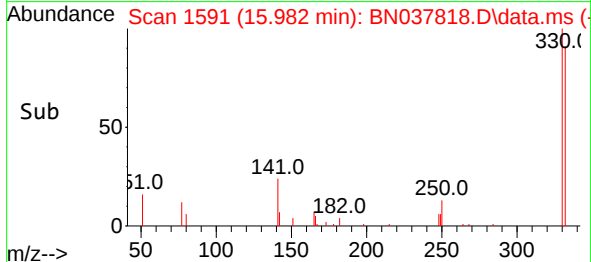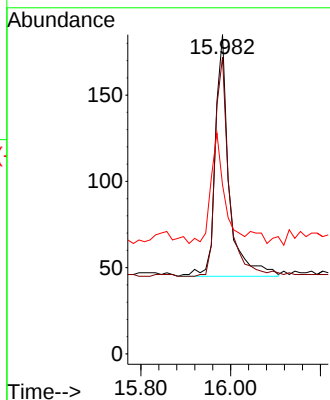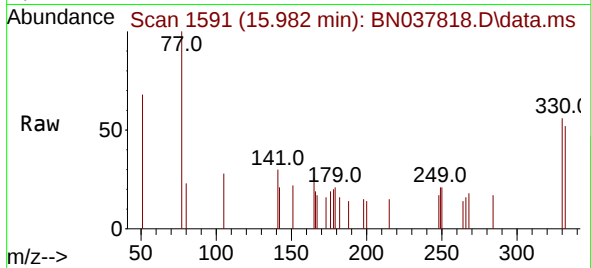

#15
2-Fluorobiphenyl
Concen: 0.108 ng
RT: 13.105 min Scan# 1328
Delta R.T. -0.011 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Tgt Ion:172 Resp: 4101
Ion Ratio Lower Upper
172 100
171 36.2 28.6 43.0
170 24.9 19.8 29.8

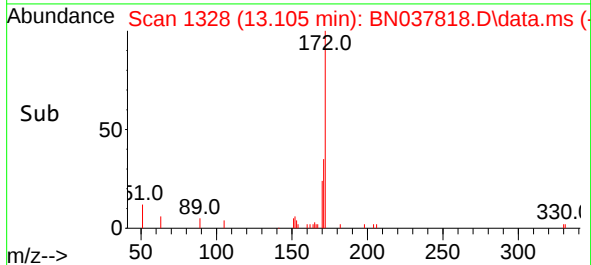
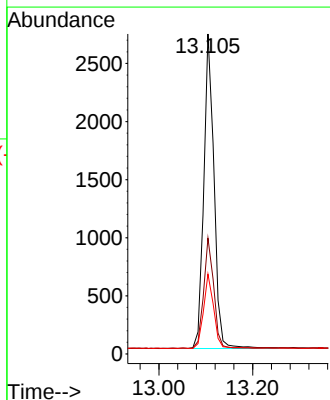
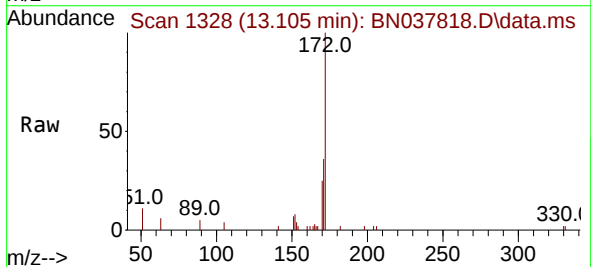




#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.235 min Scan# 1692
Delta R.T. -0.000 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21




Instrument :
BNA_N
ClientSampleId :

Tgt Ion:188 Resp: 15081
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 9.3 10.6 15.8#

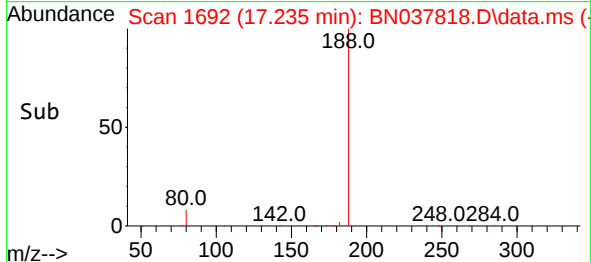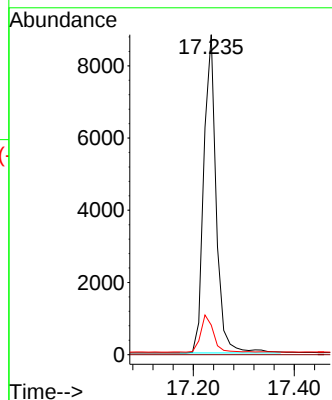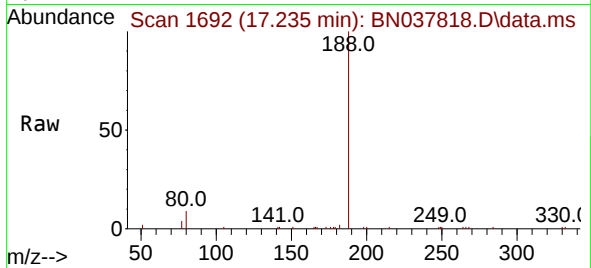

#27
Fluoranthene-d10
Concen: 0.111 ng
RT: 19.262 min Scan# 1956
Delta R.T. -0.009 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21


Tgt Ion:212 Resp: 4190
Ion Ratio Lower Upper
212 100
106 16.1 12.2 18.2
104 9.2 6.9 10.3

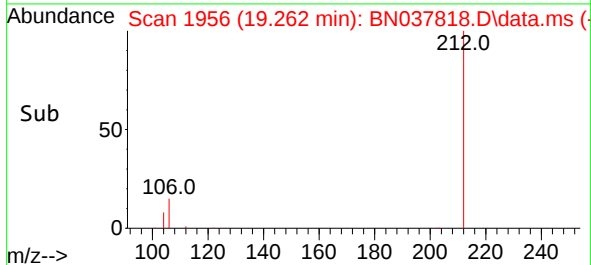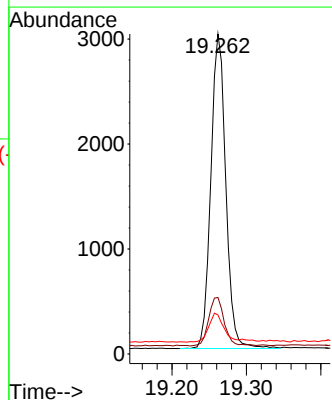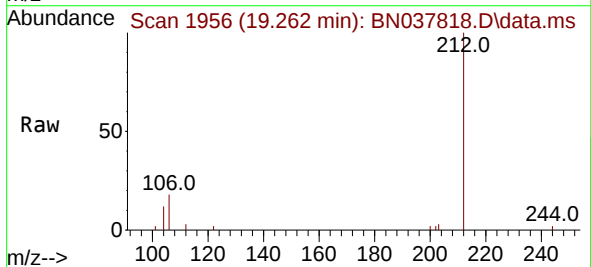





#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.411 min Scan# 21
Delta R.T. -0.009 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21


Instrument :
BNA_N
ClientSampleId :

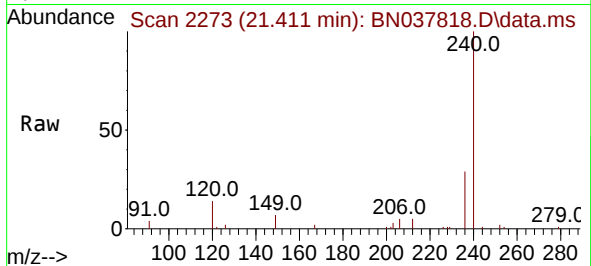



Tgt Ion:240 Resp: 11372
Ion Ratio Lower Upper
240 100
120 13.8 9.2 13.8
236 28.8 22.6 33.8

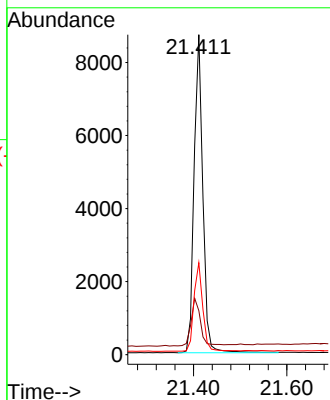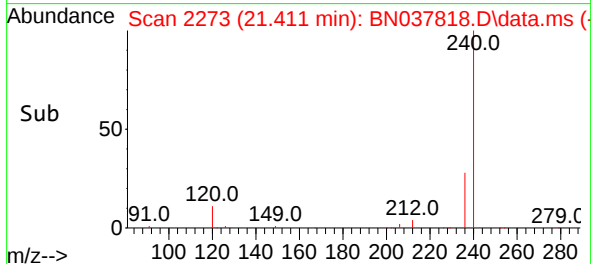

#31
Terphenyl-d14
Concen: 0.134 ng
RT: 19.861 min Scan# 2085
Delta R.T. -0.009 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

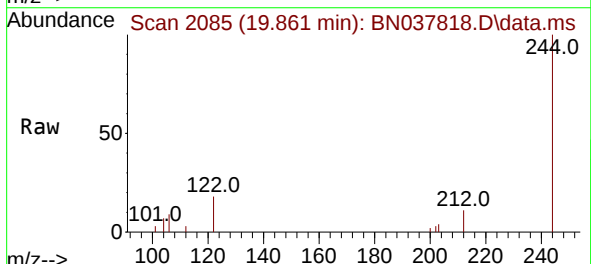


Tgt Ion:244 Resp: 3082
Ion Ratio Lower Upper
244 100
212 10.8 7.5 11.3
122 18.1 13.2 19.8

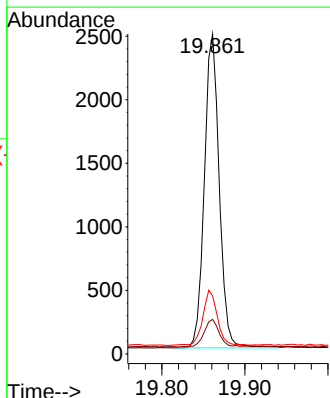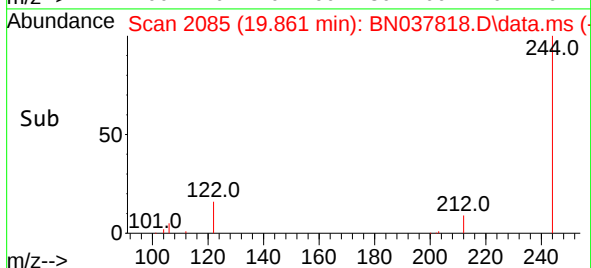





#34
Bis(2-ethylhexyl)phthalate
Concen: 0.041 ng
RT: 21.331 min Scan# 2133
Delta R.T. -0.018 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Instrument :
BNA_N
ClientSampleId :

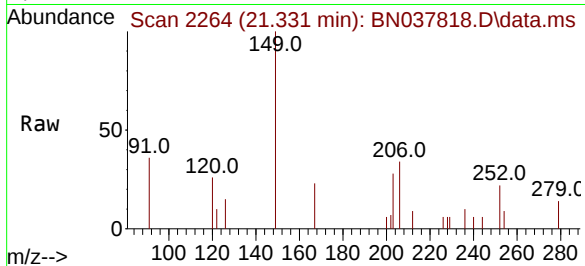

Tgt Ion:149 Resp: 479
Ion Ratio Lower Upper
149 100
167 25.9 20.8 31.2
279 13.8 3.3 4.9#

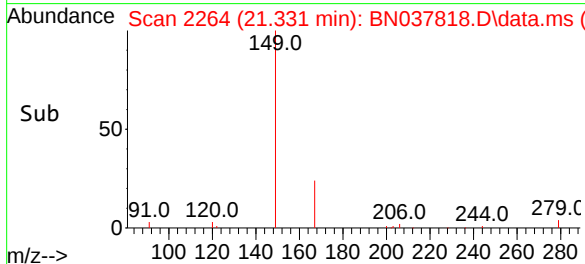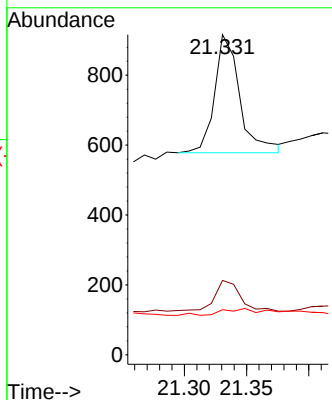

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.744 min Scan# 2842
Delta R.T. -0.009 min
Lab File: BN037818.D
Acq: 19 Sep 2025 17:21

Tgt Ion:264 Resp: 11377
Ion Ratio Lower Upper
264 100
260 27.1 21.8 32.8
265 71.1 39.4 59.2#

