
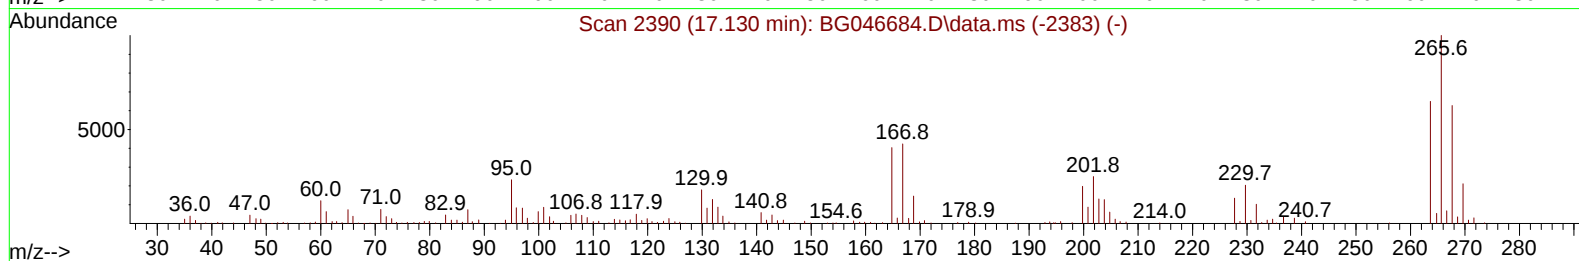
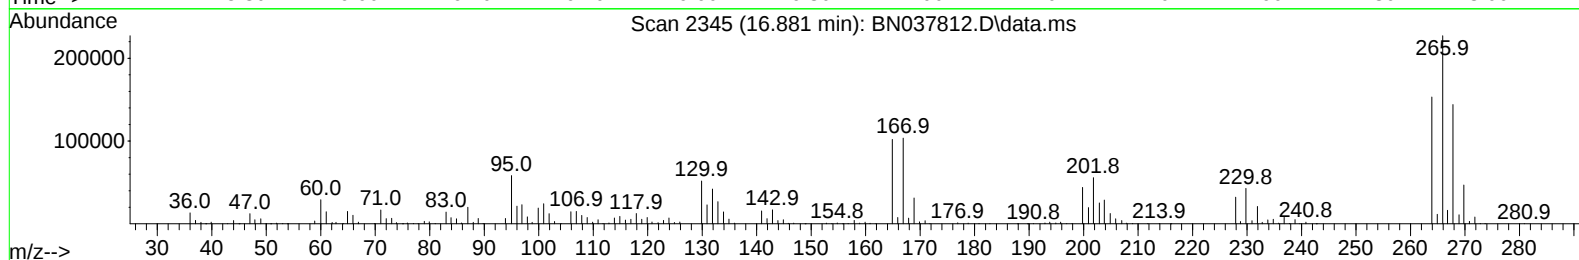


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037812.D
Acq On : 19 Sep 2025 13:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 20:01:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

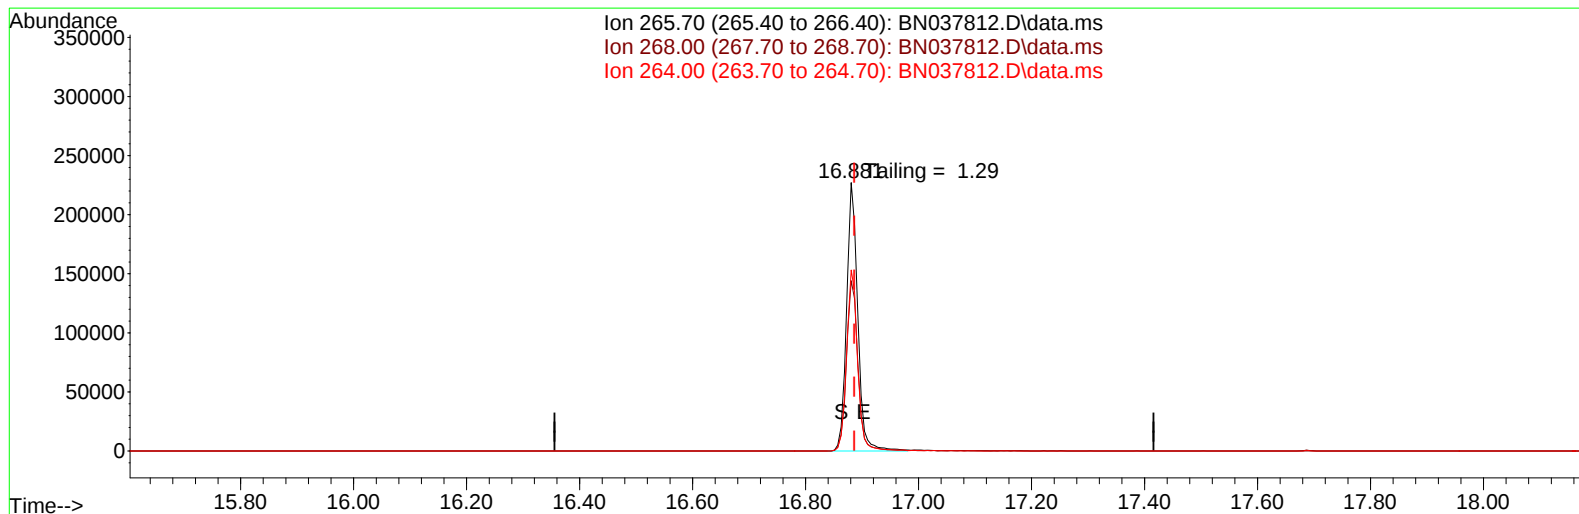

TIC: BN037812.D\data.ms

(70) Pentachlorophenol (C)




16.881min (-0.005) 23824.83 ng

response 312055

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.43
264.00	61.60	67.43
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN091925\
Data File : BN037812.D
Acq On : 19 Sep 2025 13:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 22 20:01:10 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 20 01:53:13 2025
Response via : Initial Calibration

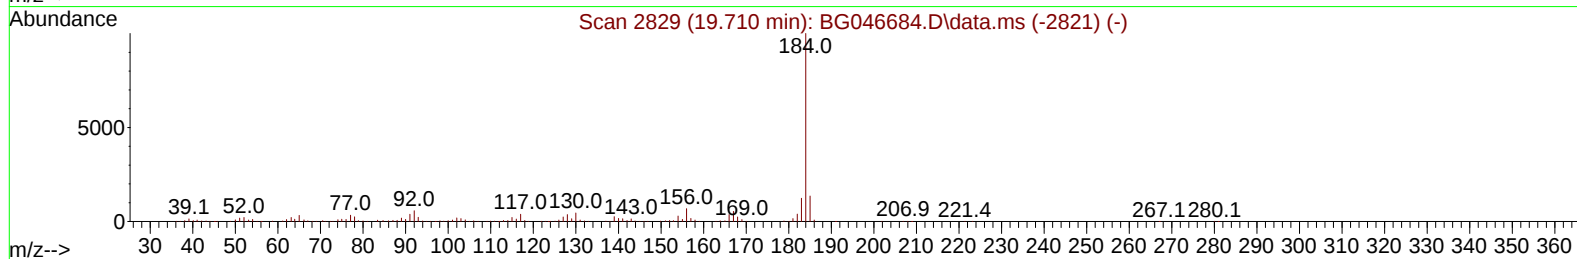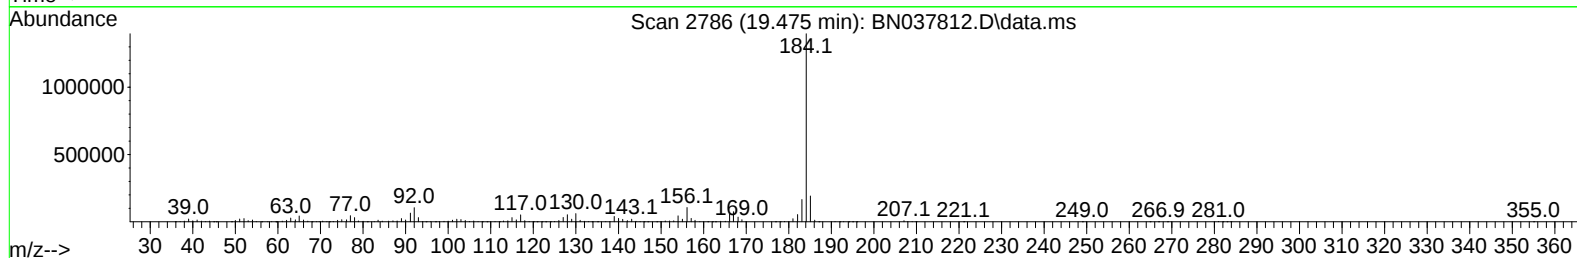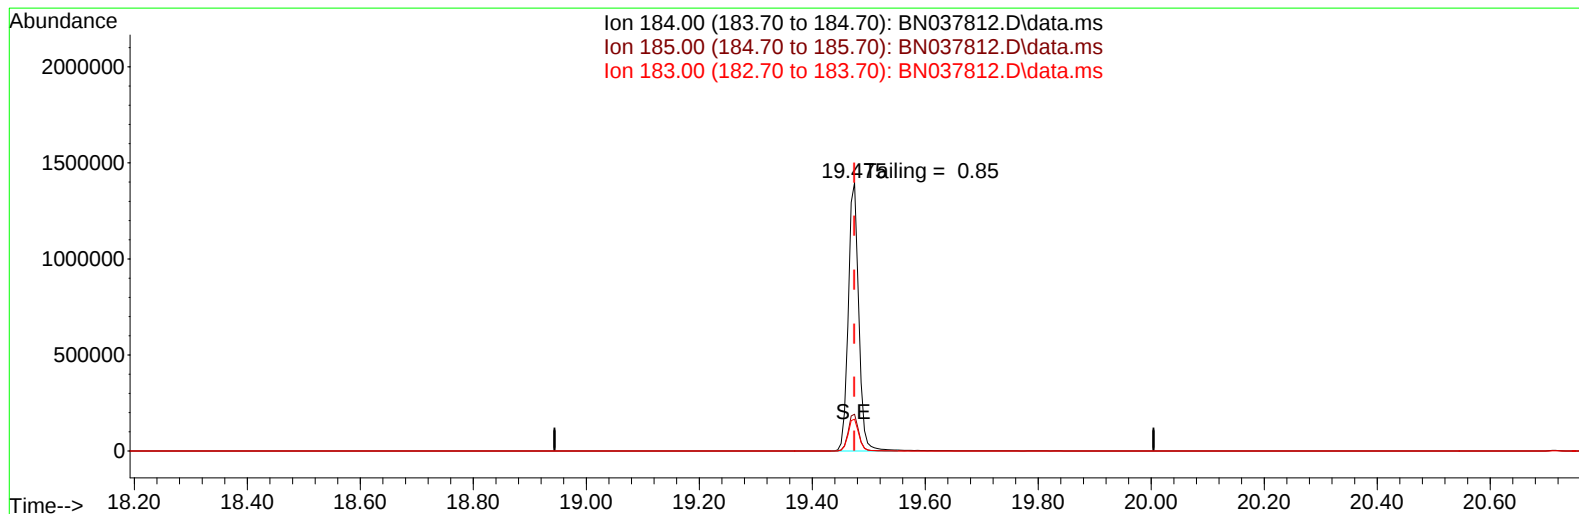

TIC: BN037812.D\data.ms

(77) Benizidine

19.475min (+ 0.001) 0.00 ng

response 1812303

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.75
183.00	13.20	11.88
0.00	0.00	0.00