

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
 Data File : BN007769.D
 Acq On : 20 Sep 2019 18:08
 Operator : HP/JU
 Sample : K4975-08
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE134D4-20190918

Quant Time: Sep 20 22:48:37 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	6198	0.40	ng	0.00
7) Naphthalene-d8	10.46	136	23196	0.40	ng	-0.01
13) Acenaphthene-d10	14.32	164	13594	0.40	ng	0.00
19) Phenanthrene-d10	17.06	188	31093	0.40	ng	-0.01
27) Chrysene-d12	21.25	240	36330	0.40	ng	-0.02
34) Perylene-d12	23.47	264	38438	0.40	ng	-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	1946	0.09	ng	0.00
5) Phenol-d6	6.87	99	1438	0.05	ng	0.00
8) Nitrobenzene-d5	8.83	82	5540	0.27	ng	0.00
11) 2-Methylnaphthalene-d10	12.05	152	12604	0.32	ng	0.00
14) 2,4,6-Tribromophenol	15.80	330	1462	0.20	ng	-0.02
15) 2-Fluorobiphenyl	12.94	172	18589	0.33	ng	0.00
25) Fluoranthene-d10	19.10	212	34574	0.33	ng	-0.01
29) Terphenyl-d14	19.70	244	35908	0.40	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.29	88	9112	1.319	ng	# 88
3) n-Nitrosodimethylamine	3.00	42	189684	59.948	ng	# 67
32) Bis(2-ethylhexyl)phthalate	21.19	149	7452	0.108	ng	# 89

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
Data File : BN007769.D
Acq On : 20 Sep 2019 18:08
Operator : HP/JU
Sample : K4975-08
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE134D4-20190918

Quant Time: Sep 20 22:48:37 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

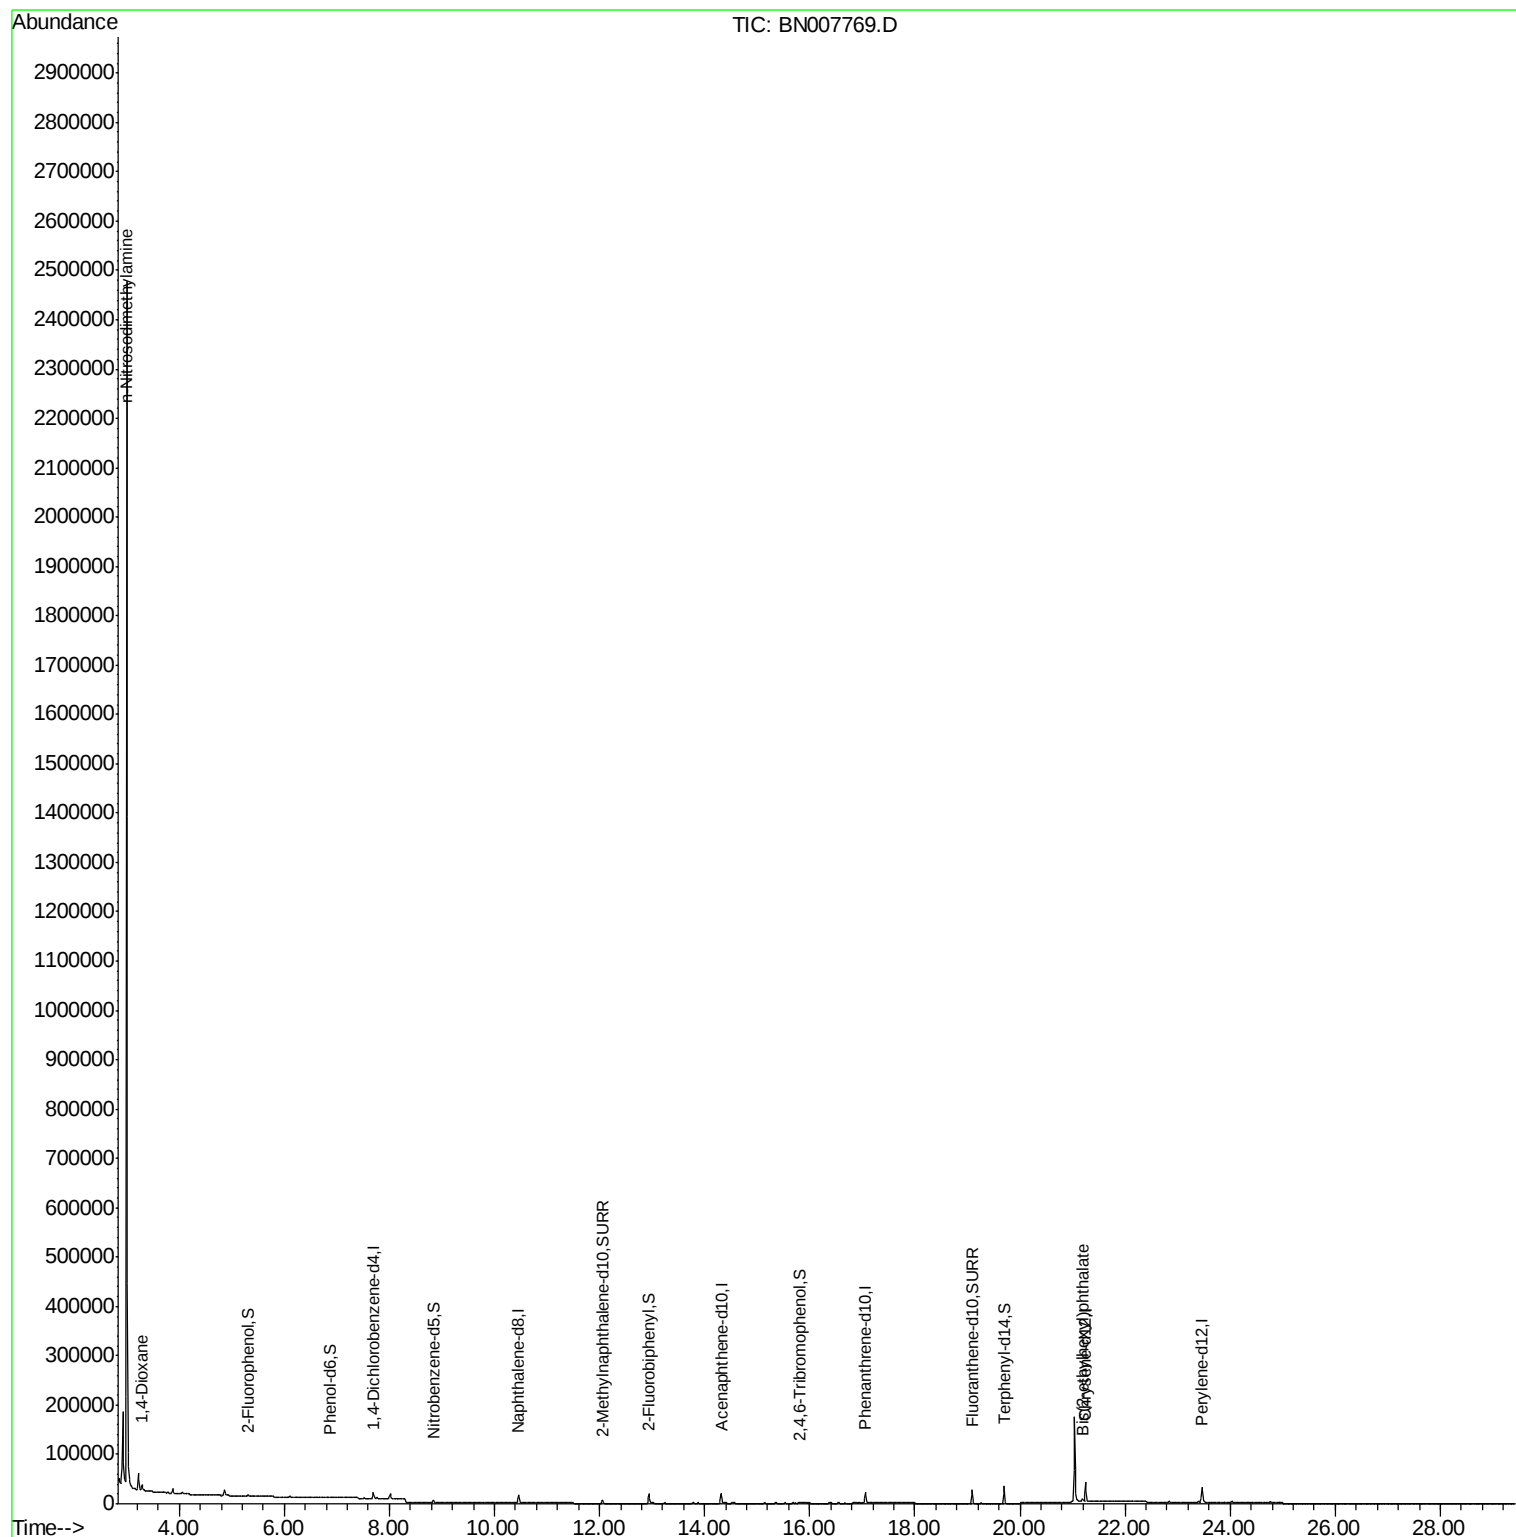



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.69 min Scan# 604

Delta R.T. -0.01 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918


Tot Ion:152 Resp: 6198

Ion Ratio Lower Upper

152 100

150 153.2 125.6 188.4

115 63.5 53.3 79.9



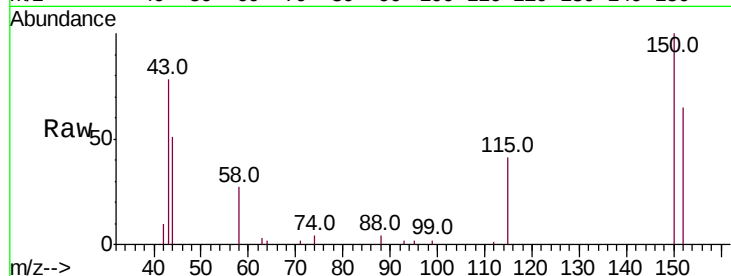


Abundance

Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

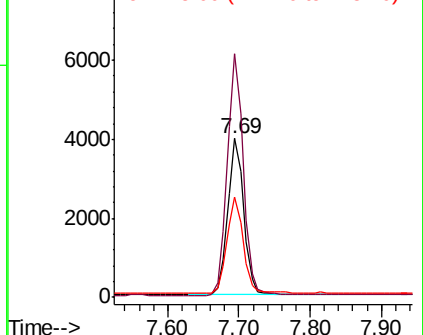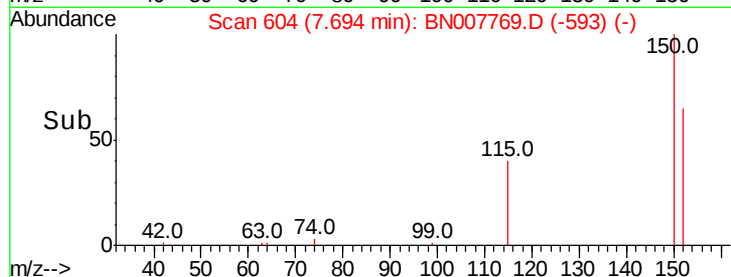

#2

1,4-Dioxane

Concen: 1.319 ng

RT: 3.29 min Scan# 57

Delta R.T. -0.02 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08


Tgt Ion: 88 Resp: 9112

Ion Ratio Lower Upper

88 100

58 59.8 44.6 66.8

43 32.0 14.4 21.6#





Abundance

Ion 88.00 (87.70 to 88.70): BNC

Ion 58.00 (57.70 to 58.70): BNC

Ion 43.00 (42.70 to 43.70): BNC

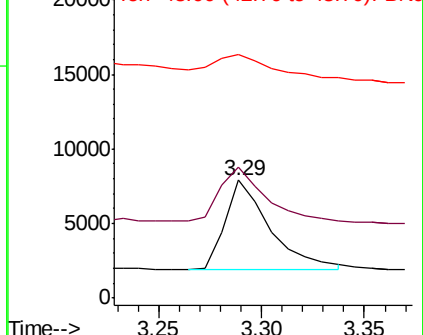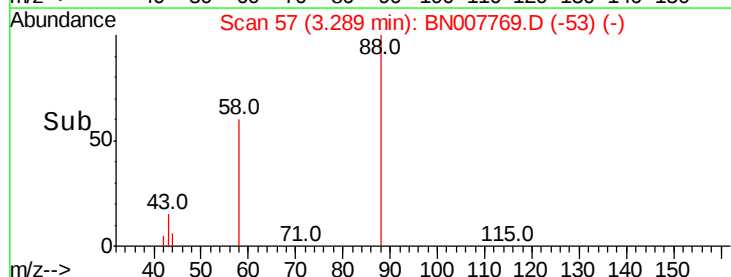



#3

n-Nitrosodimethylamine

Concen: 59.948 ng

RT: 3.00 min Scan# 21

Delta R.T. -0.01 min





Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :
BNA_N
ClientSampleId :
RE134D4-20190918

Tot Ion: 42 Resp: 189684

Ion	Ratio	Lower	Upper
42	100		
74	150.9	87.9	131.9#
44	26.8	29.4	44.0#

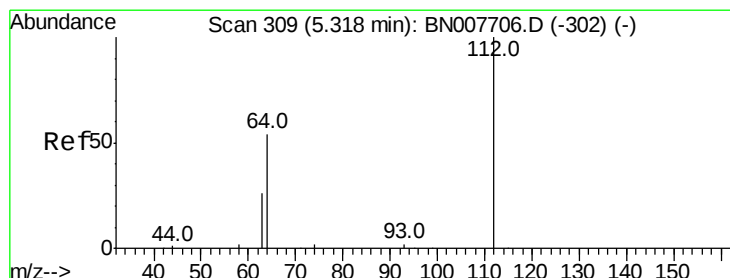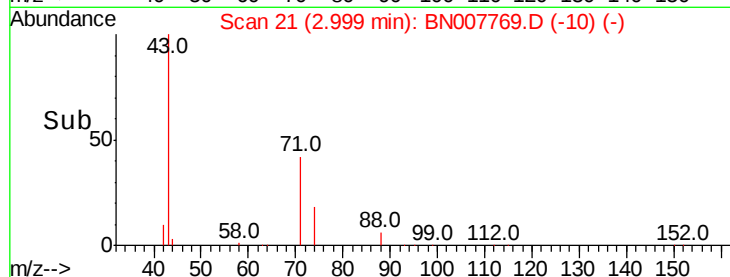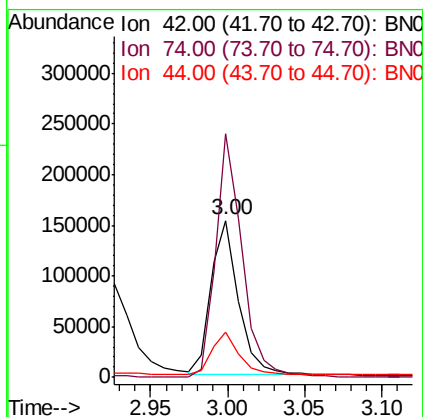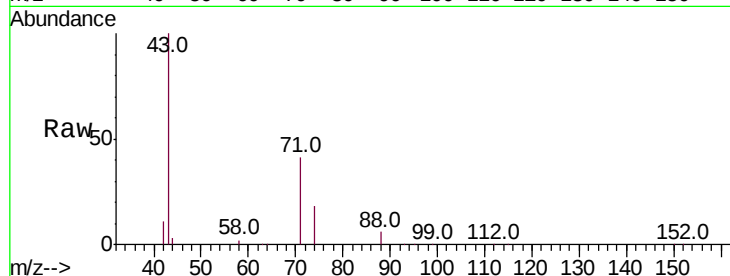

#4

2-Fluorophenol

Concen: 0.091 ng

RT: 5.31 min Scan# 308




Delta R.T. -0.01 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Tgt Ion: 112 Resp: 1946

Ion	Ratio	Lower	Upper
112	100		
64	59.7	46.6	70.0
63	28.6	23.1	34.7

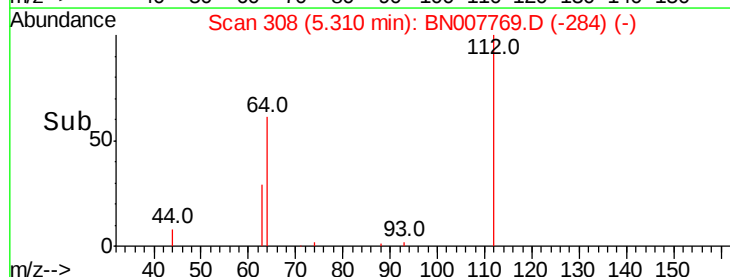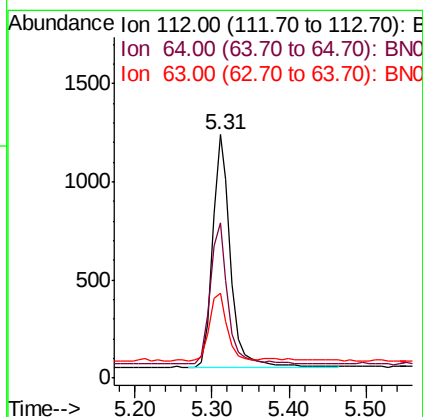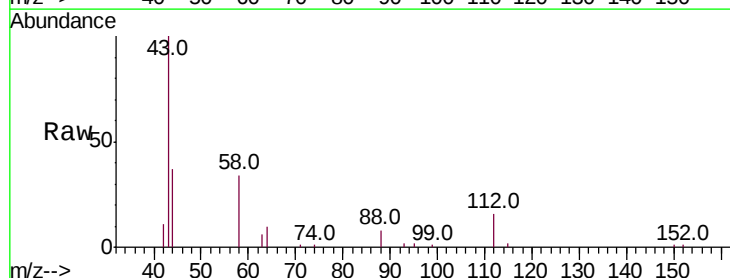



#5

Phenol-d6

Concen: 0.049 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918


Tot Ion: 99 Resp: 1438

Ion Ratio Lower Upper

99 100

42 22.5 12.8 19.2#




71 43.2 27.6 41.4#

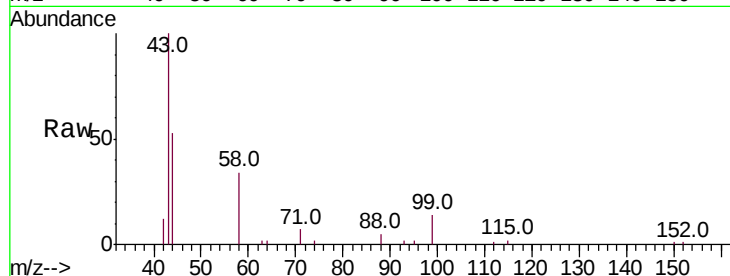

Abundance Ion 99.00 (98.70 to 99.70): BN007706.D (-493) (-)

Ion 42.00 (41.70 to 42.70): BN007706.D (-493) (-)

Ion 71.00 (70.70 to 71.70): BN007706.D (-493) (-)

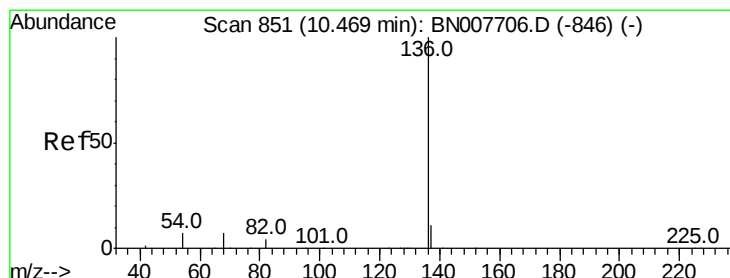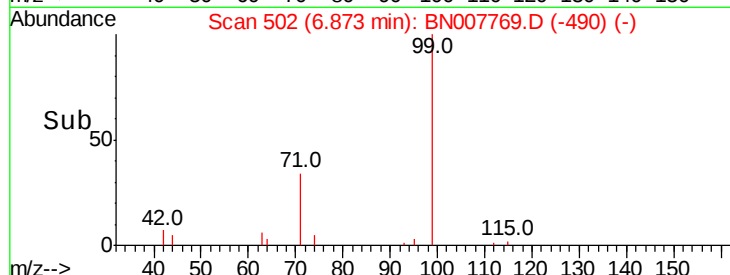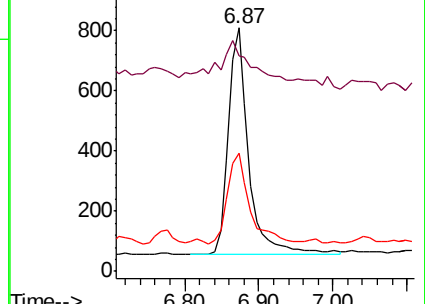

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Tgt Ion: 136 Resp: 23196


Ion Ratio Lower Upper

136 100

137 11.3 9.2 13.8

54 8.5 5.8 8.8

68 9.1 6.5 9.7


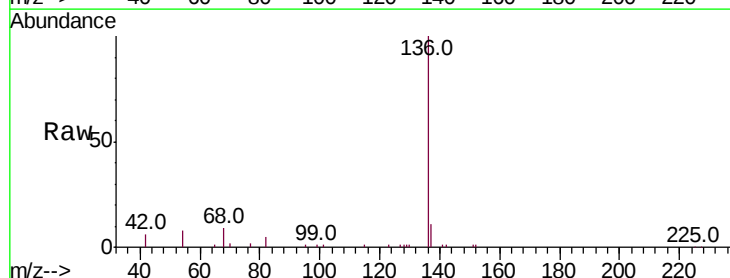


Abundance Ion 136.00 (135.70 to 136.70): BN007706.D (-846) (-)

Ion 137.00 (136.70 to 137.70): BN007706.D (-846) (-)

Ion 54.00 (53.70 to 54.70): BN007706.D (-846) (-)

Ion 68.00 (67.70 to 68.70): BN007706.D (-846) (-)



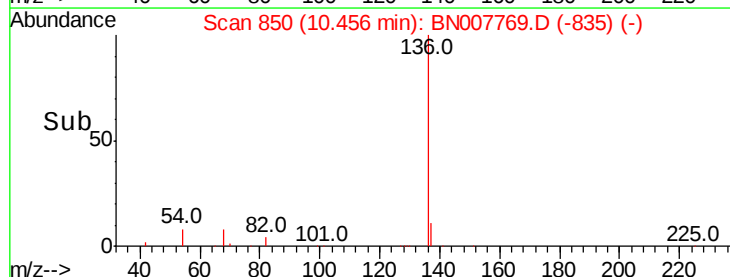
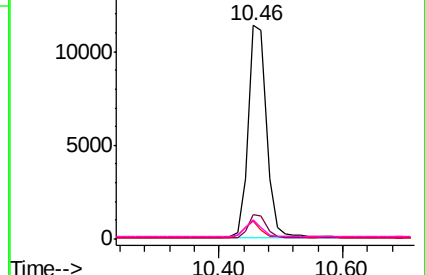




#8
 Nitrobenzene-d5
 Concen: 0.273 ng
 RT: 8.83 min Scan# 722
 Delta R.T. 0.00 min
 Lab File: BN007769.D
 Acq: 20 Sep 2019 18:08




Instrument :
 BNA_N
 ClientSampleId :
 RE134D4-20190918


Tot Ion	82	Resp	5540
Ion	Ratio	Lower	Upper
82	100		
128	36.5	24.5	36.7
54	38.6	35.2	52.8

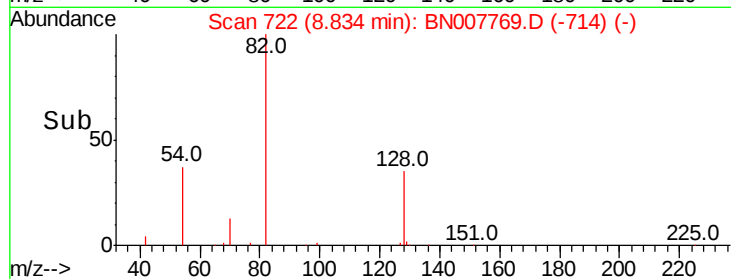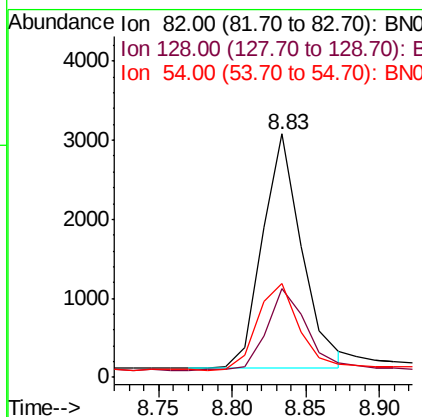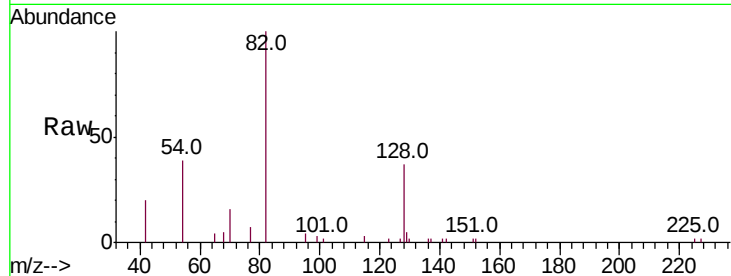

#11
 2-Methylnaphthalene-d10
 Concen: 0.323 ng
 RT: 12.05 min Scan# 1056
 Delta R.T. -0.01 min
 Lab File: BN007769.D
 Acq: 20 Sep 2019 18:08

Tgt Ion	152	Resp	12604
Ion	Ratio	Lower	Upper
152	100		
151	19.1	15.4	23.2

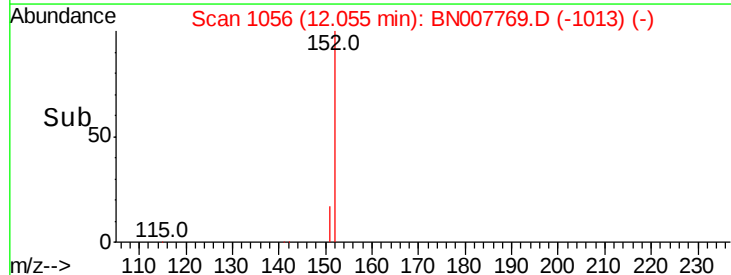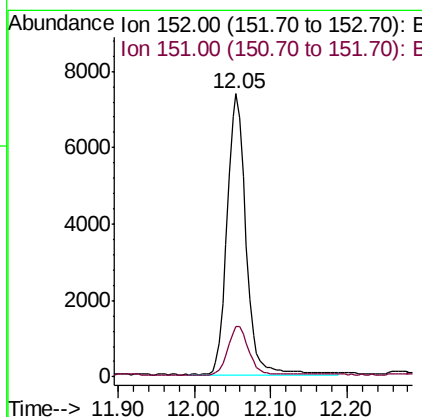

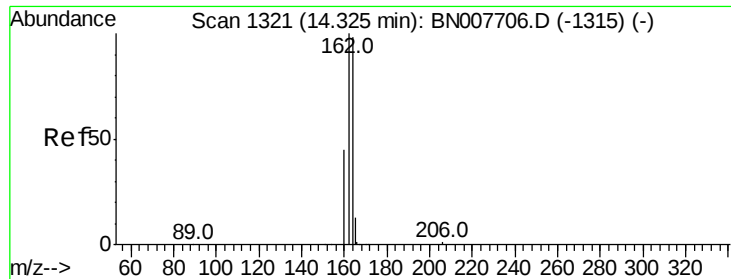

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.32 min Scan# 1320

Delta R.T. -0.00 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918


Tot Ion:164 Resp: 13594

Ion Ratio Lower Upper

164 100

162 98.8 81.7 122.5

160 44.7 37.0 55.4






Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

14.32

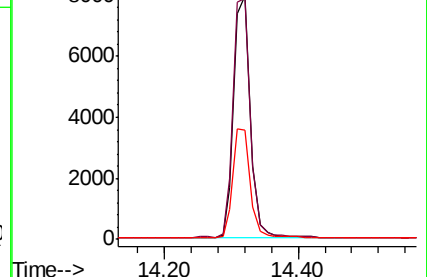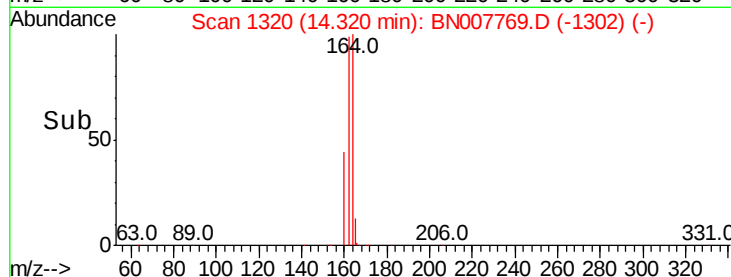

#14

2,4,6-Tribromophenol

Concen: 0.197 ng

RT: 15.80 min Scan# 1453

Delta R.T. -0.02 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08


Tgt Ion:330 Resp: 1462

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0

141 35.5 28.7 43.1





Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

15.80



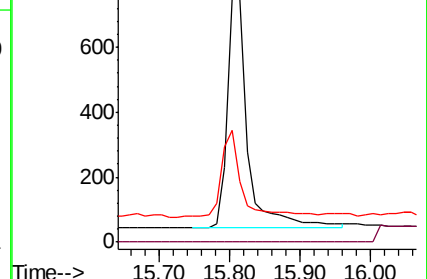
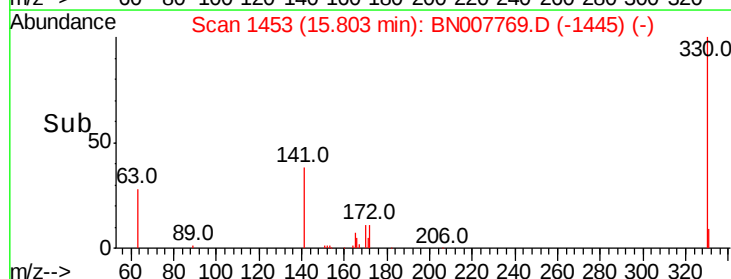




#15
 2-Fluorobiphenyl
 Concen: 0.332 ng
 RT: 12.94 min Scan# 1196
 Delta R.T. -0.00 min
 Lab File: BN007769.D
 Acq: 20 Sep 2019 18:08




Instrument :
 BNA_N
 ClientSampleId :
 RE134D4-20190918


Tot Ion:172 Resp: 18589
 Ion Ratio Lower Upper
 172 100
 171 35.1 28.8 43.2
 170 22.8 19.5 29.3

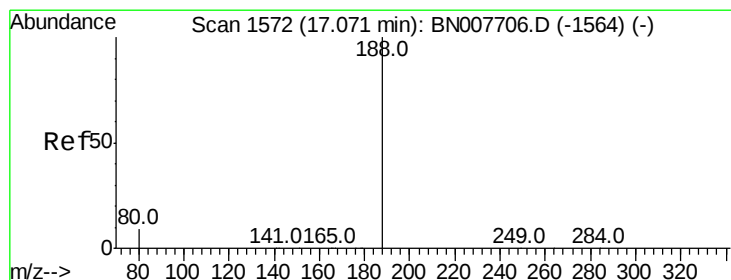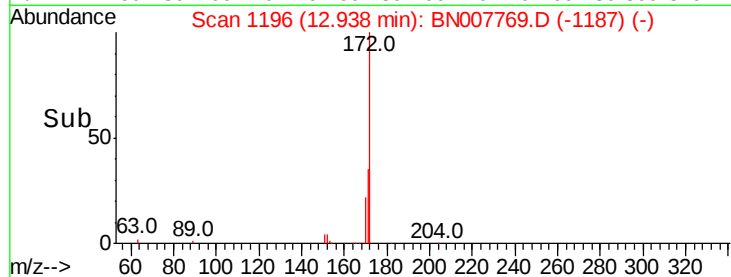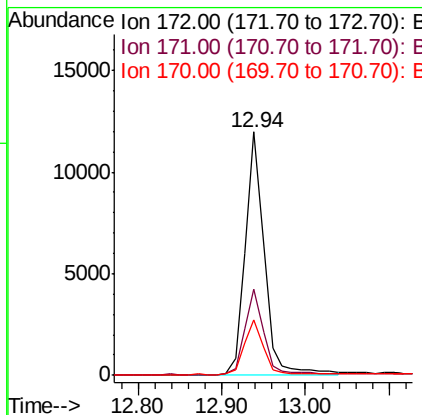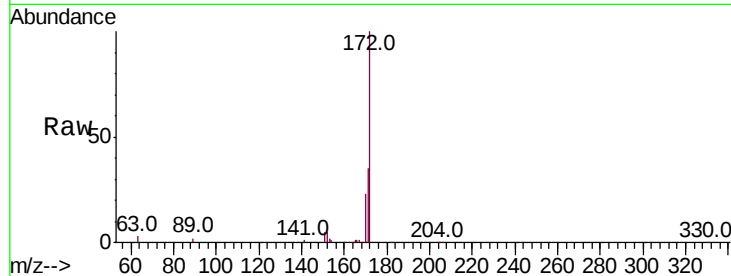

#19
 Phenanthrene-d10
 Concen: 0.400 ng
 RT: 17.06 min Scan# 1570
 Delta R.T. -0.01 min
 Lab File: BN007769.D
 Acq: 20 Sep 2019 18:08

Tgt Ion:188 Resp: 31093
 Ion Ratio Lower Upper
 188 100
 94 0.0 0.0 0.0
 80 11.8 7.4 11.2#

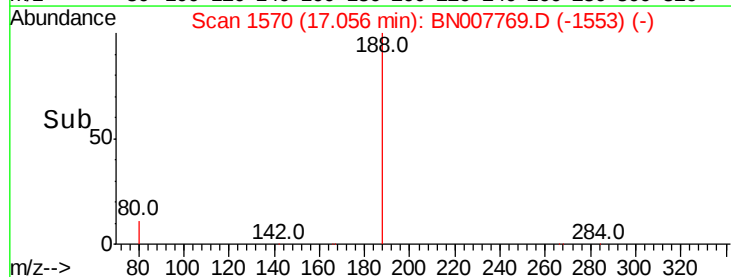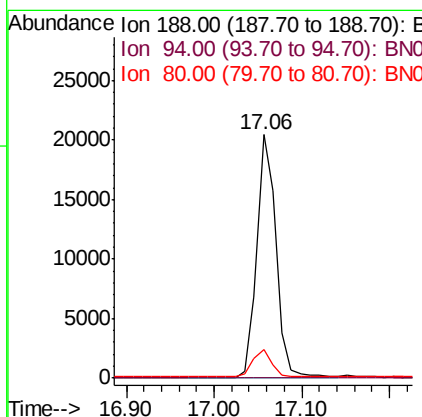

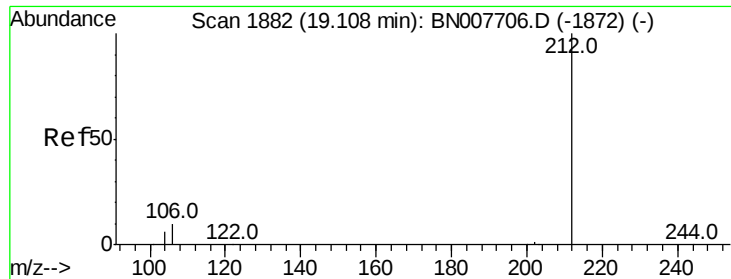

#25

Fluoranthene-d10

Concen: 0.330 ng

RT: 19.10 min Scan# 1878

Delta R.T. -0.01 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918


Tot Ion:212 Resp: 34574

Ion Ratio Lower Upper

212 100

106 11.8 9.4 14.0




104 6.8 5.3 7.9

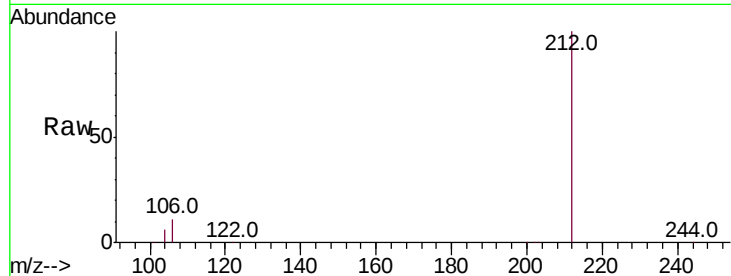

Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

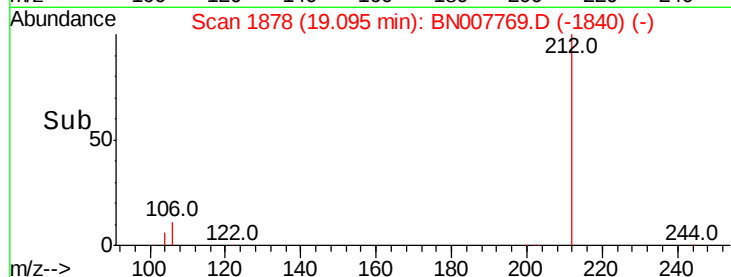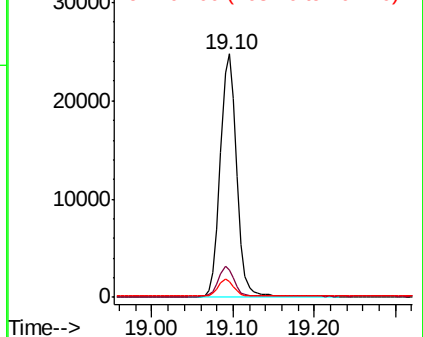

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.25 min Scan# 2179

Delta R.T. -0.02 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08


Tgt Ion:240 Resp: 36330

Ion Ratio Lower Upper

240 100

120 9.4 5.4 8.2#



236 26.1 21.0 31.4




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

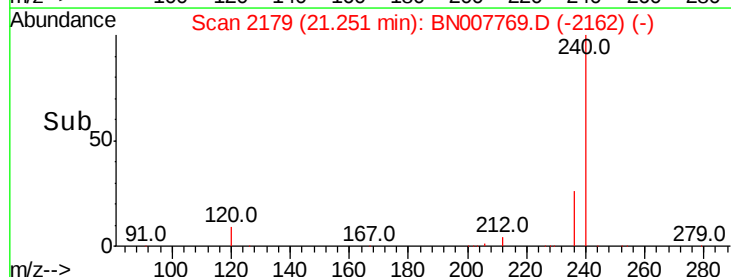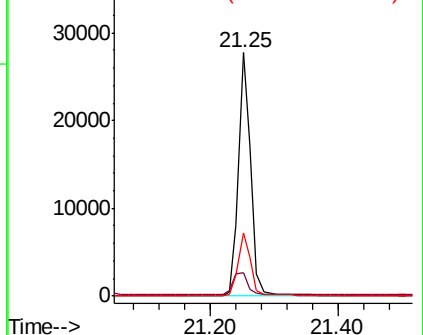

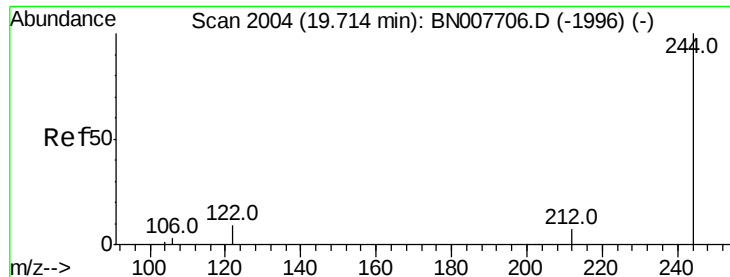

#29

Terphenyl-d14

Concen: 0.402 ng

RT: 19.70 min Scan# 2000

Delta R.T. -0.01 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918


Tot Ion:244 Resp: 35908

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9




122 9.5 7.4 11.2

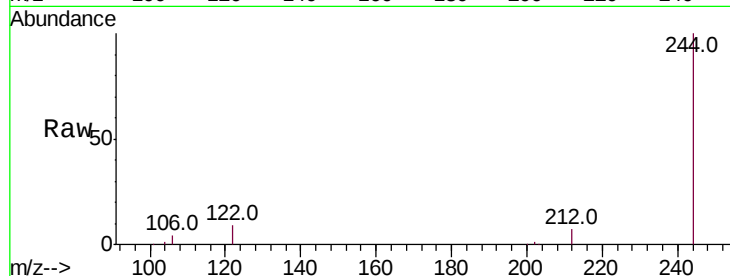

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

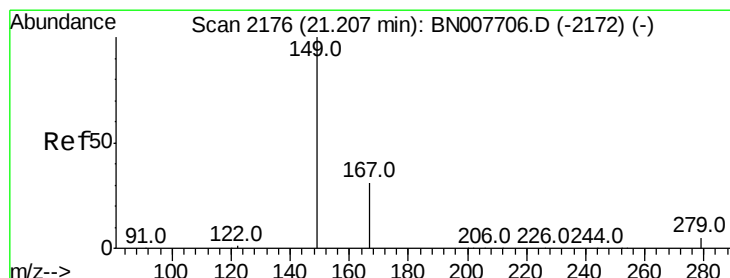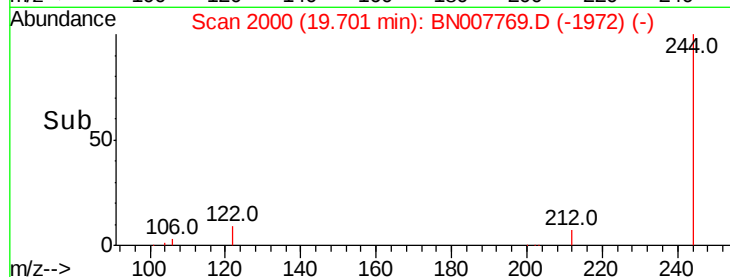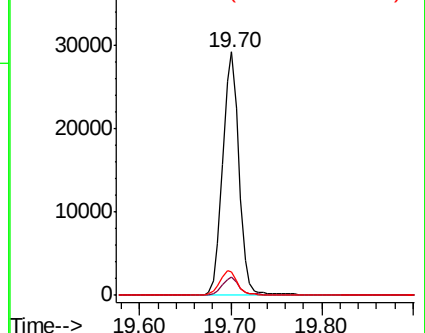

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.108 ng

RT: 21.19 min Scan# 2173

Delta R.T. -0.02 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08


Tgt Ion:149 Resp: 7452

Ion Ratio Lower Upper

149 100

167 22.8 23.7 35.5#



279 4.0 4.2 6.2#



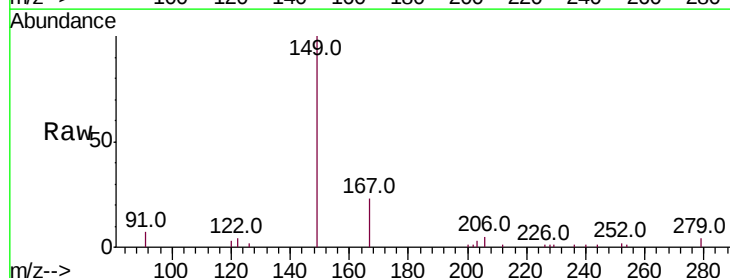


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

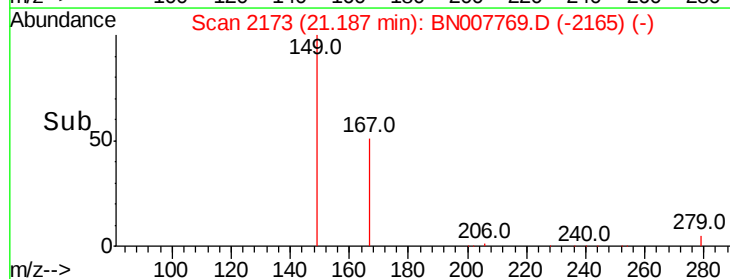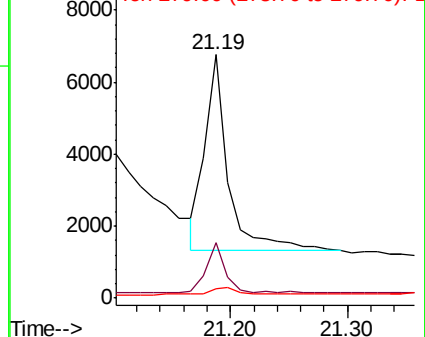

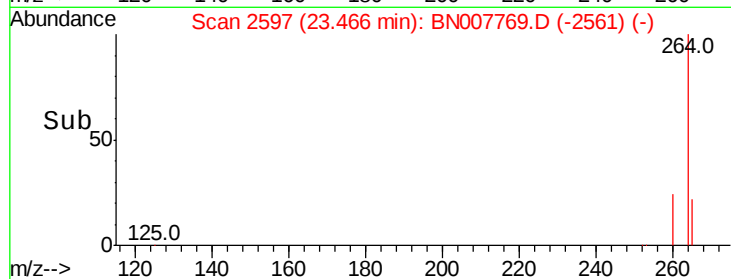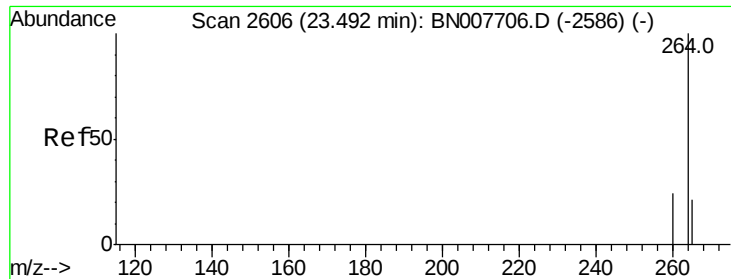

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.47 min Scan# 2597

Delta R.T. -0.03 min

Lab File: BN007769.D

Acq: 20 Sep 2019 18:08

Instrument :

BNA_N

ClientSampleId :

RE134D4-20190918

Tot Ion: 264 Resp: 38438

Ion Ratio Lower Upper

264 100

260 24.2 19.3 28.9

265 32.1 26.9 40.3

