

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
 Data File : BN007779.D
 Acq On : 21 Sep 2019 01:18
 Operator : HP/JU
 Sample : PB122993BL
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 PB122993BL

Quant Time: Sep 21 03:34:38 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	6898	0.40	ng	0.00
7) Naphthalene-d8	10.46	136	26293	0.40	ng	-0.01
13) Acenaphthene-d10	14.31	164	15252	0.40	ng	-0.01
19) Phenanthrene-d10	17.06	188	34615	0.40	ng	-0.01
27) Chrysene-d12	21.25	240	33248	0.40	ng	-0.02
34) Perylene-d12	23.46	264	33686	0.40	ng	-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	5940	0.25	ng	0.00
5) Phenol-d6	6.87	99	7353	0.25	ng	0.00
8) Nitrobenzene-d5	8.83	82	6153	0.27	ng	0.00
11) 2-Methylnaphthalene-d10	12.05	152	14394	0.32	ng	0.00
14) 2,4,6-Tribromophenol	15.81	330	1579	0.19	ng	-0.01
15) 2-Fluorobiphenyl	12.94	172	19511	0.31	ng	0.00
25) Fluoranthene-d10	19.09	212	35897	0.31	ng	-0.01
29) Terphenyl-d14	19.70	244	29891	0.37	ng	-0.01
Target Compounds						
3) n-Nitrosodimethylamine	3.00	42	7262	2.062	ng	# 87
32) Bis(2-ethylhexyl)phthalate	21.19	149	1394	0.022	ng	# 82

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
Data File : BN007779.D
Acq On : 21 Sep 2019 01:18
Operator : HP/JU
Sample : PB122993BL
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
PB122993BL

Quant Time: Sep 21 03:34:38 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

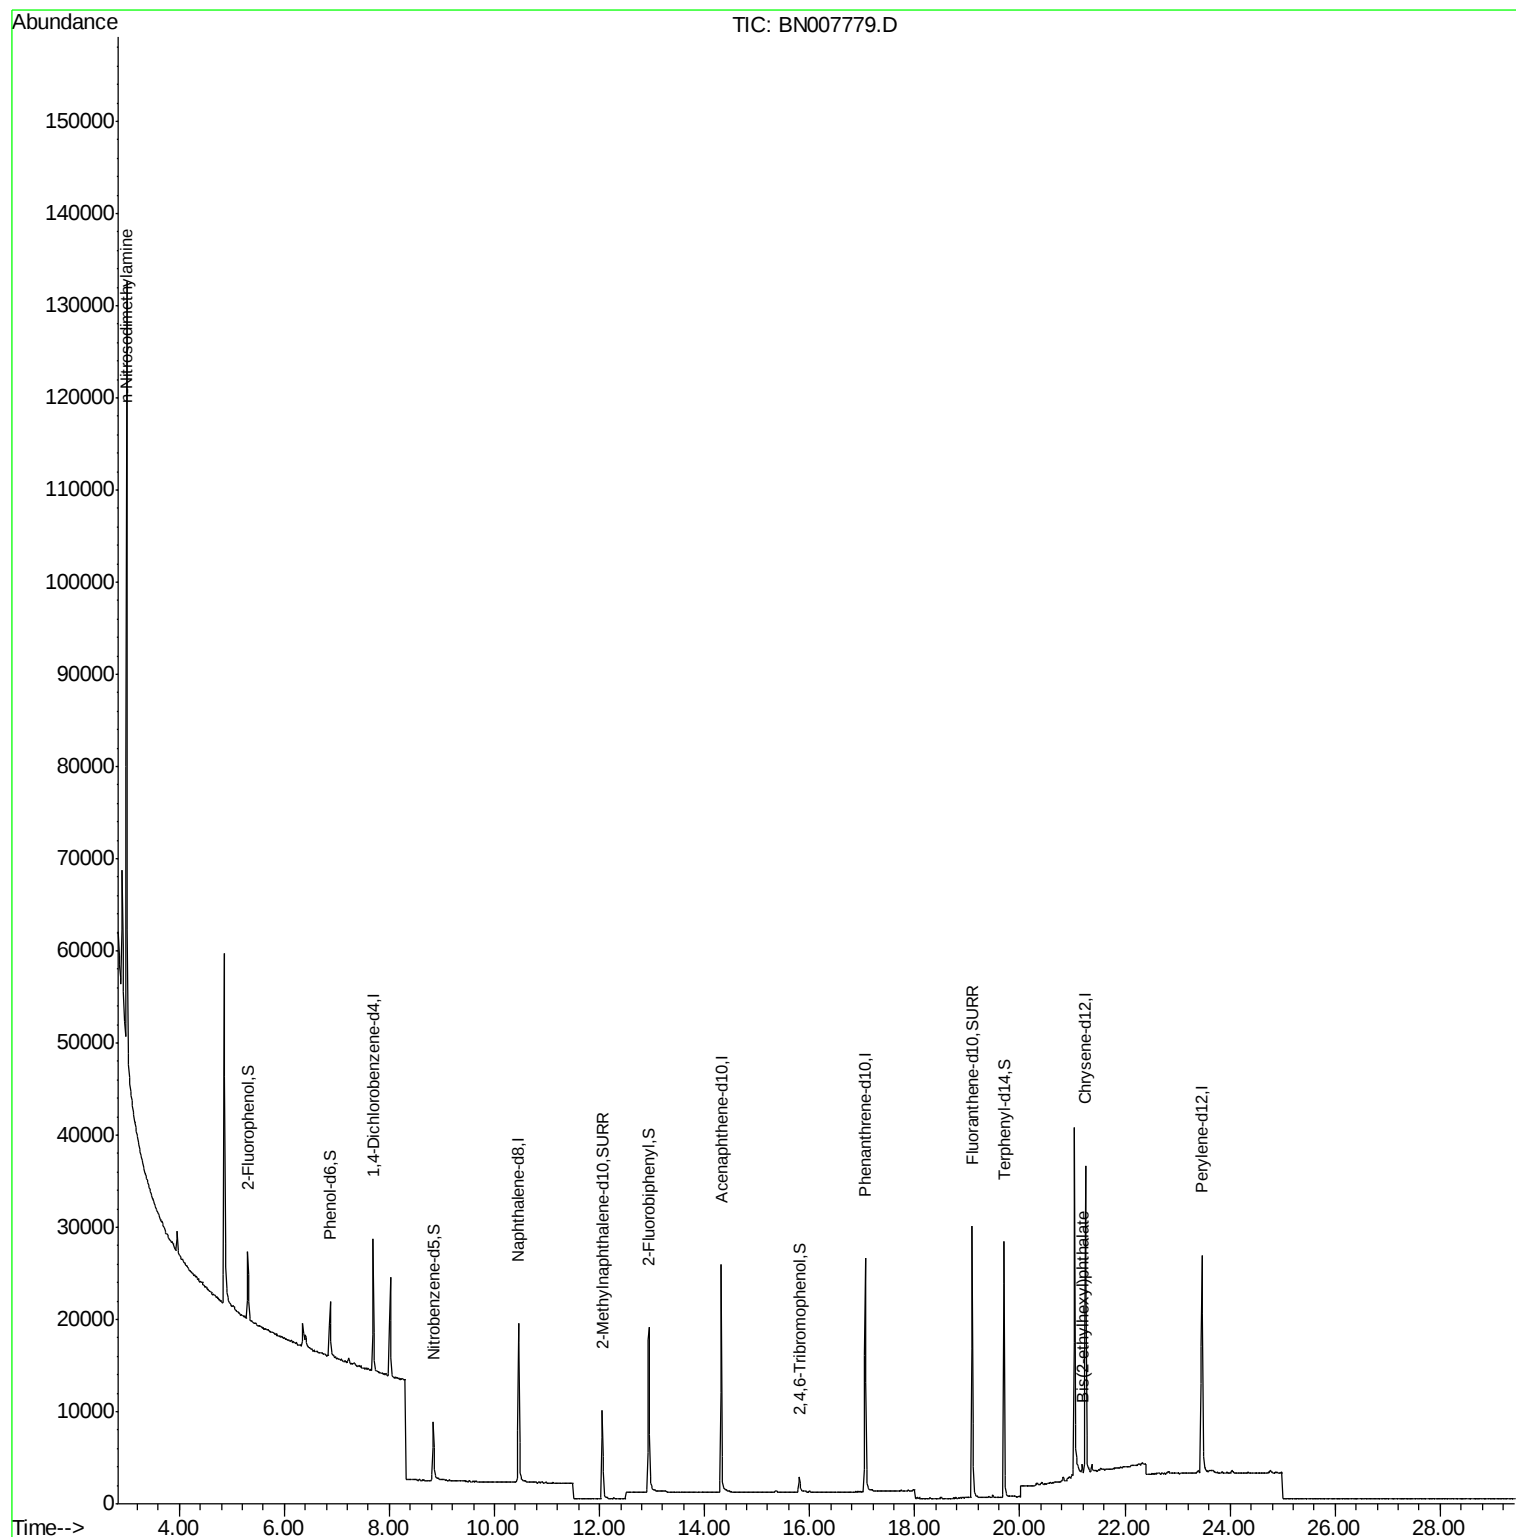



#1

1,4-Dichlorobenzene-d4

Concen: 0.400 ng

RT: 7.69 min Scan# 604

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL


Tot Ion:152 Resp: 6898

Ion Ratio Lower Upper

152 100

150 156.7 125.6 188.4




115 65.1 53.3 79.9

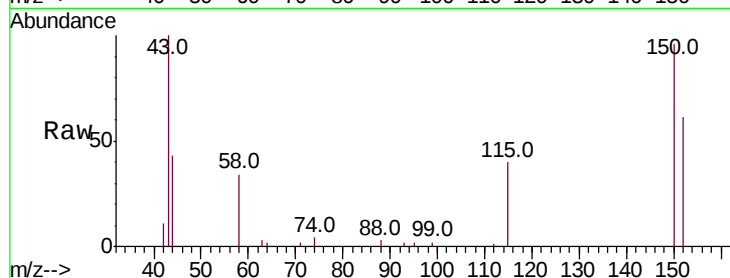

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

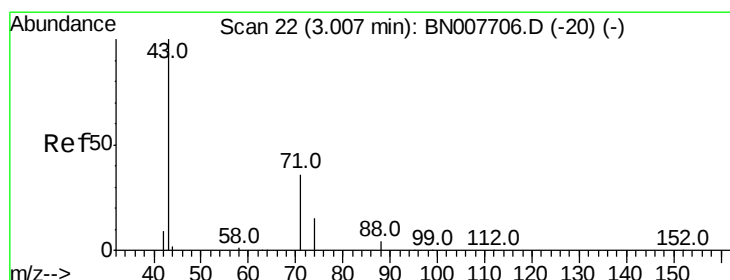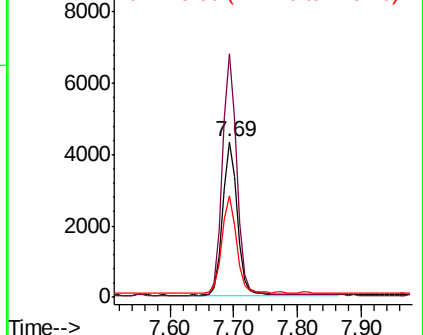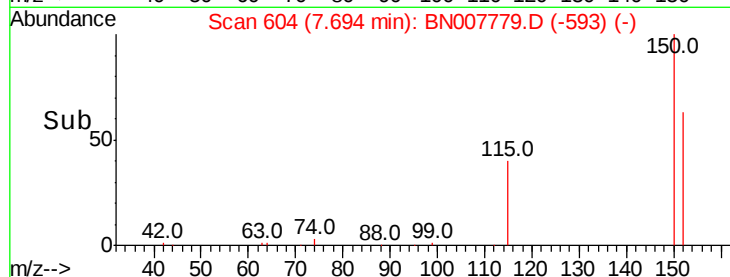

#3

n-Nitrosodimethylamine

Concen: 2.062 ng

RT: 3.00 min Scan# 21

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion: 42 Resp: 7262

Ion Ratio Lower Upper

42 100

74 123.4 87.9 131.9



44 28.4 29.4 44.0#

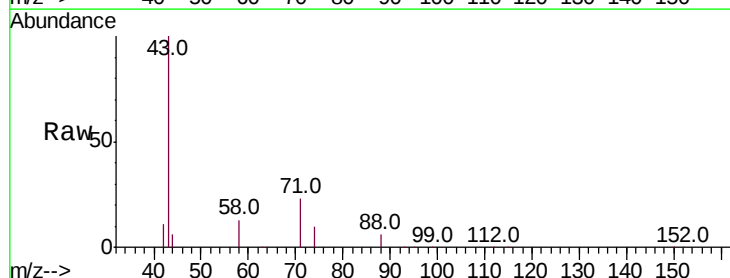


Abundance Ion 42.00 (41.70 to 42.70): BNC

Ion 74.00 (73.70 to 74.70): BNC

Ion 44.00 (43.70 to 44.70): BNC

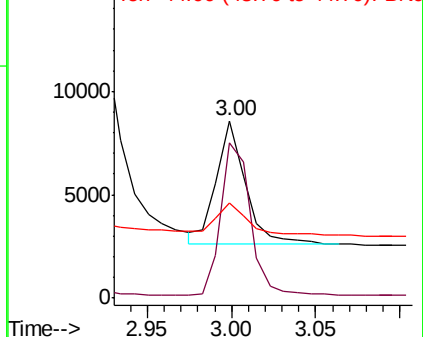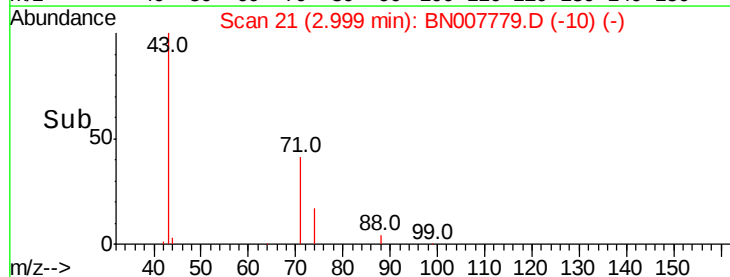

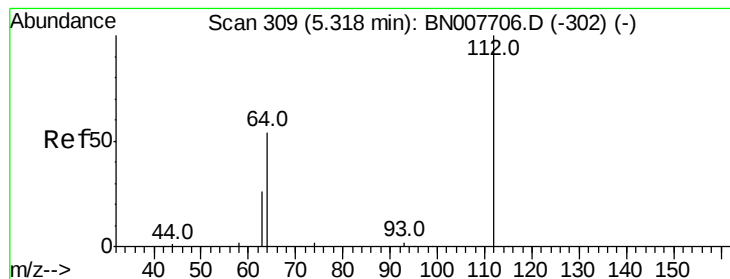

#4

2-Fluorophenol

Concen: 0.250 ng

RT: 5.31 min Scan# 308

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL


Tot Ion:112 Resp: 5940

Ion Ratio Lower Upper

112 100

64 59.5 46.6 70.0




63 30.6 23.1 34.7

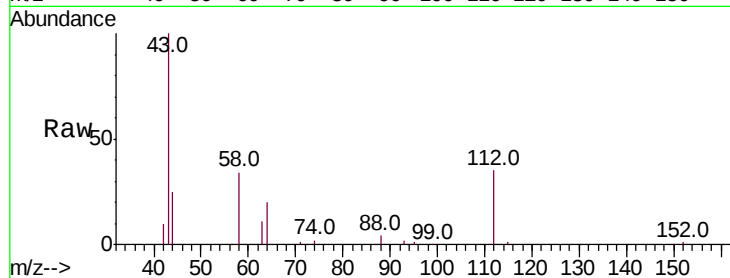

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

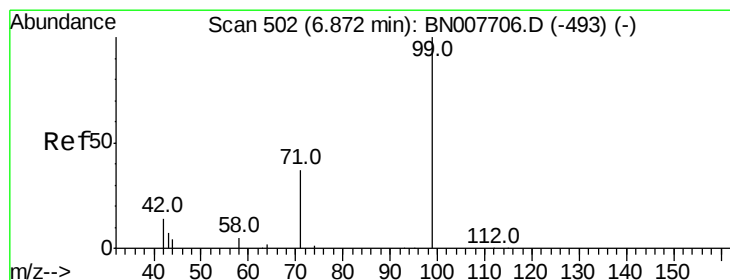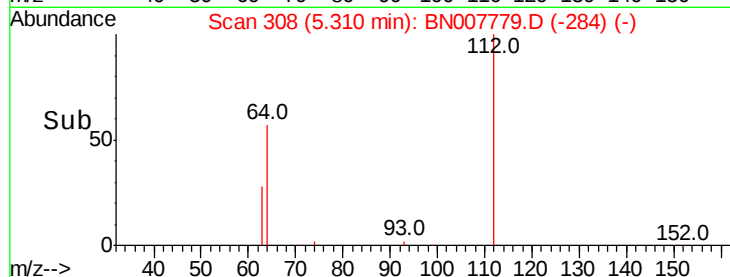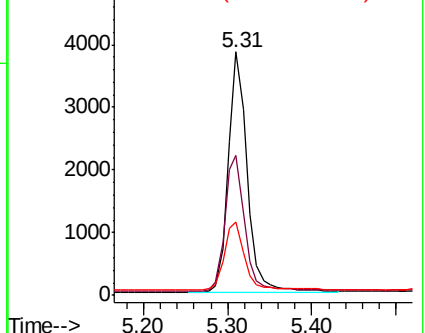

#5

Phenol-d6

Concen: 0.246 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion: 99 Resp: 7353

Ion Ratio Lower Upper

99 100

42 13.6 12.8 19.2



71 34.6 27.6 41.4

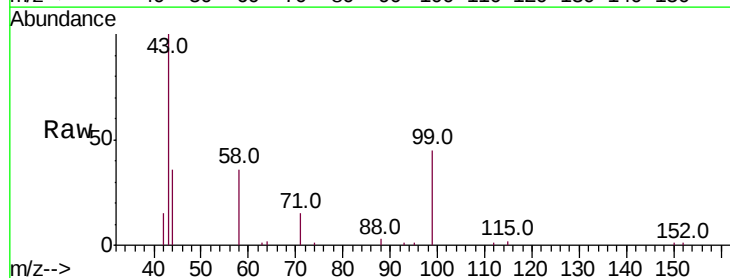


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

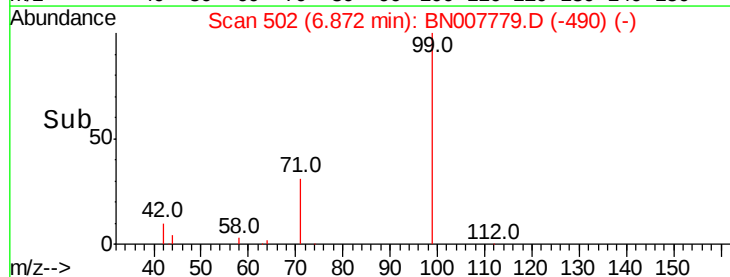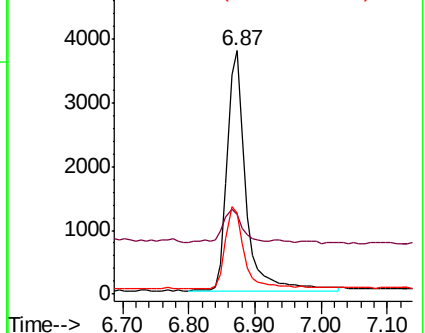



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL

Tot Ion:136 Resp: 26293


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 8.5 5.8 8.8

68 9.0 6.5 9.7



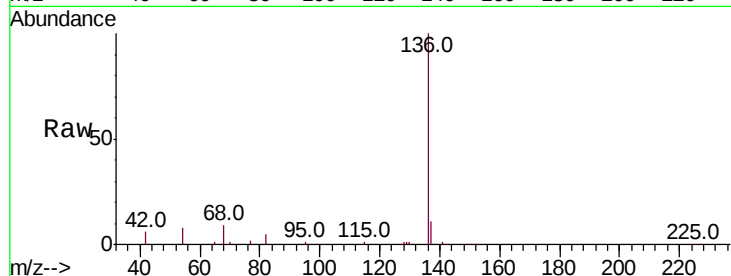


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

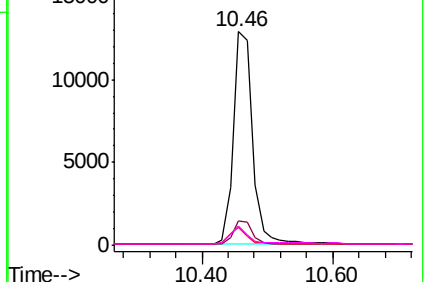

#8

Nitrobenzene-d5

Concen: 0.268 ng

RT: 8.83 min Scan# 722

Delta R.T. 0.00 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion: 82 Resp: 6153

Ion Ratio Lower Upper

82 100

128 36.4 24.5 36.7



54 39.0 35.2 52.8




Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC

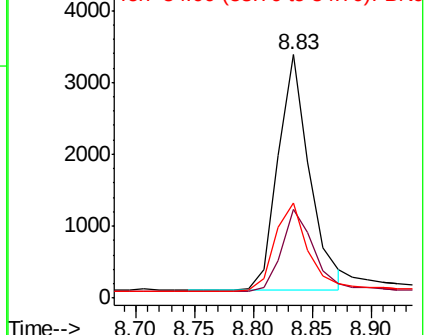

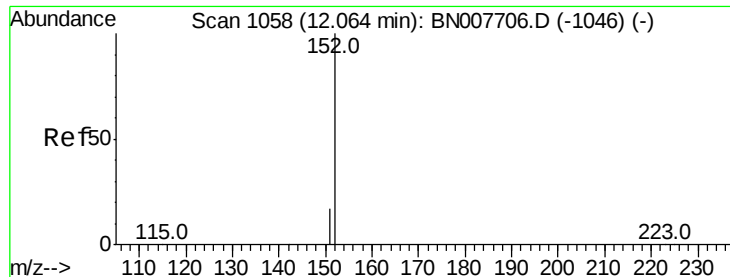

#11

2-Methylnaphthalene-d10

Concen: 0.325 ng

RT: 12.05 min Scan# 1056

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :


PB122993BL

Tot Ion:152 Resp: 14394

Ion Ratio Lower Upper




152 100

151 18.9 15.4 23.2

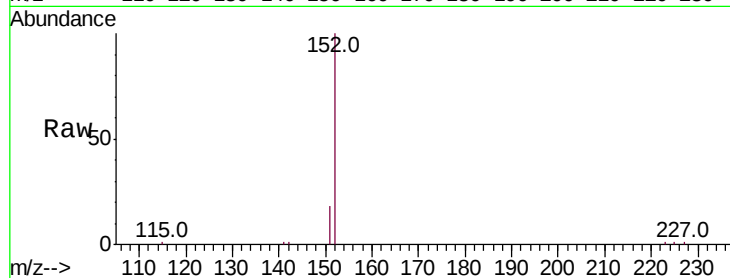

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

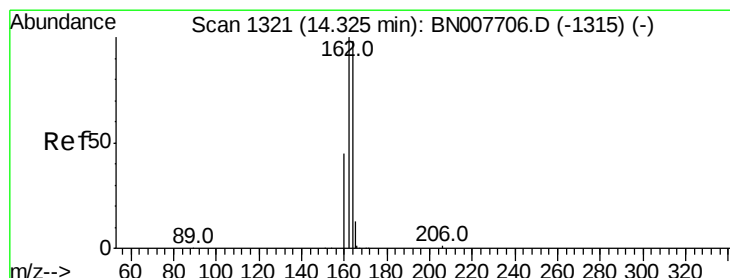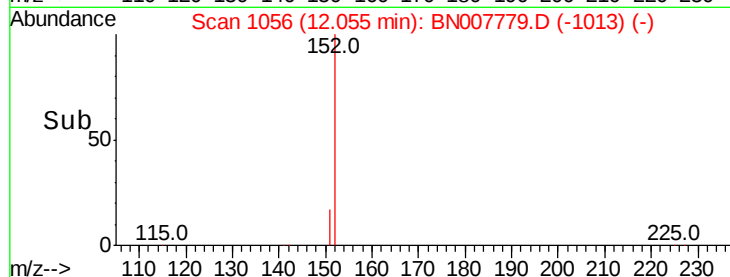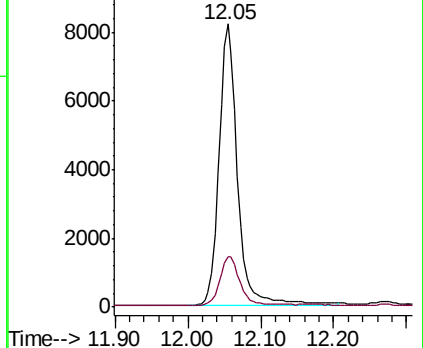

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.31 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion:164 Resp: 15252

Ion Ratio Lower Upper

164 100

162 102.7 81.7 122.5



160 47.0 37.0 55.4

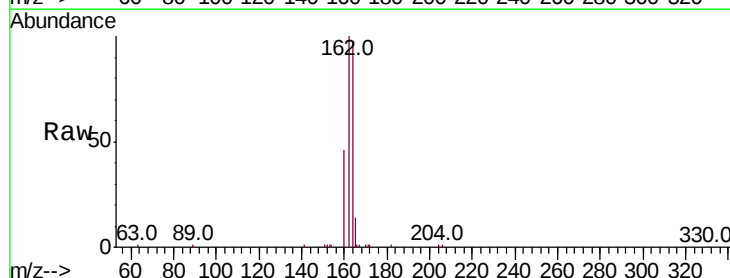


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

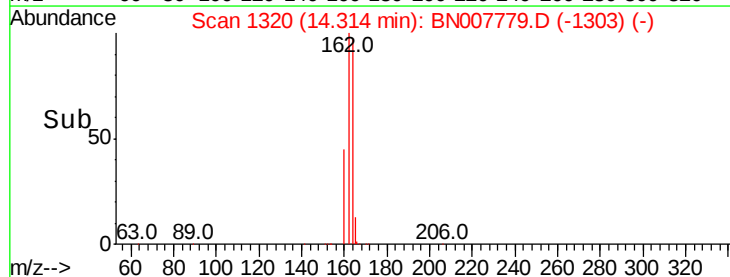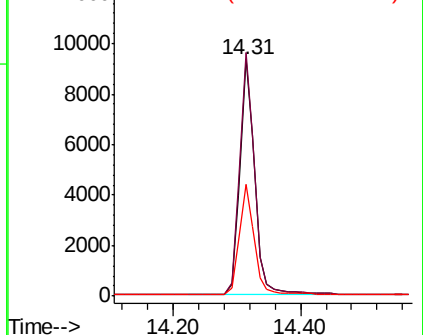







#14
 2,4,6-Tribromophenol
 Concen: 0.190 ng
 RT: 15.81 min Scan# 1454
 Delta R.T. -0.01 min
 Lab File: BN007779.D
 Acq: 21 Sep 2019 01:18

Instrument :
 BNA_N
 ClientSampleId :
 PB122993BL

Tot Ion:330 Resp: 1579
 Ion Ratio Lower Upper
 330 100
 332 0.0 0.0 0.0
 141 32.3 28.7 43.1

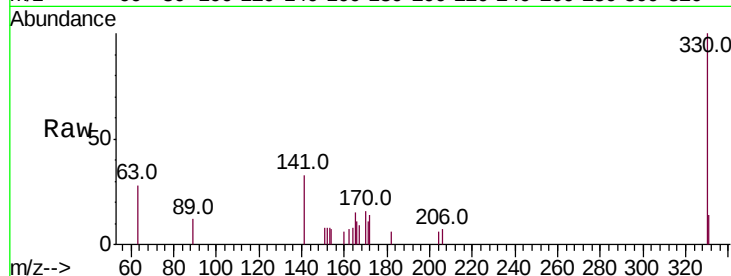


Abundance Ion 330.00 (329.70 to 330.70): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


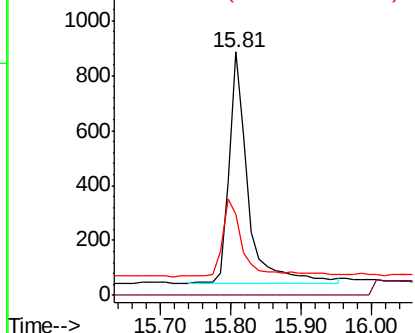



#15
 2-Fluorobiphenyl
 Concen: 0.311 ng
 RT: 12.94 min Scan# 1197
 Delta R.T. 0.00 min
 Lab File: BN007779.D
 Acq: 21 Sep 2019 01:18

Tgt Ion:172 Resp: 19511
 Ion Ratio Lower Upper
 172 100
 171 33.7 28.8 43.2
 170 21.8 19.5 29.3



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

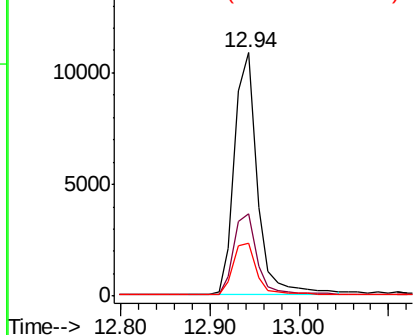



#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.06 min Scan# 1571

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL





Tot Ion:188 Resp: 34615

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0

80 9.5 7.4 11.2

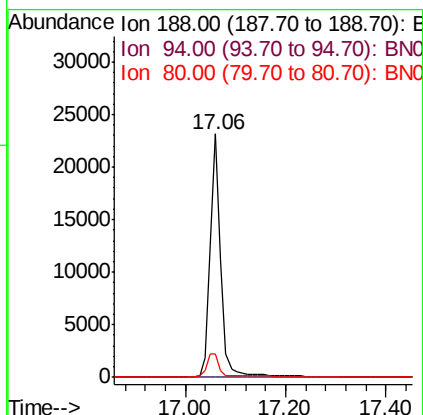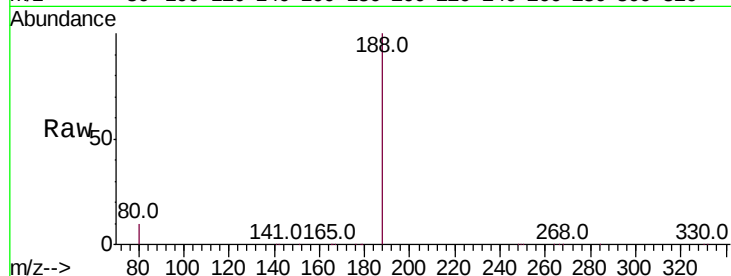

#25

Fluoranthene-d10

Concen: 0.308 ng

RT: 19.09 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18




Tgt Ion:212 Resp: 35897


Ion Ratio Lower Upper

212 100

106 11.9 9.4 14.0

104 6.6 5.3 7.9

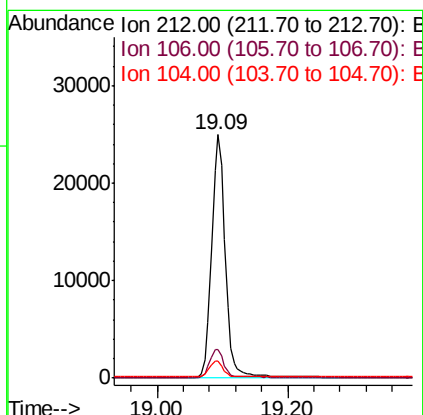



#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.25 min Scan# 2180

Delta R.T. -0.02 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL


Tot Ion:240 Resp: 33248

Ion Ratio Lower Upper

240 100

120 10.4 5.4 8.2#




236 26.9 21.0 31.4



Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

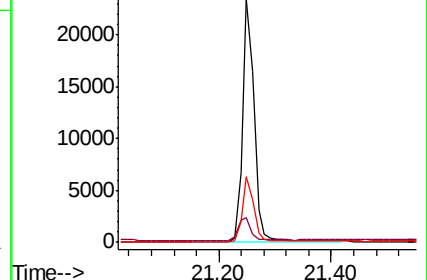

#29

Terphenyl-d14

Concen: 0.366 ng

RT: 19.70 min Scan# 2001

Delta R.T. -0.01 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion:244 Resp: 29891

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9



122 9.8 7.4 11.2




Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

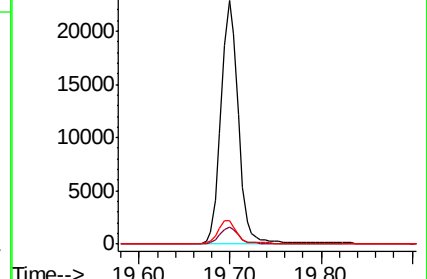



#32

Bis(2-ethylhexyl)phthalate

Concen: 0.022 ng

RT: 21.19 min Scan# 2174

Delta R.T. -0.02 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18

Instrument :

BNA_N

ClientSampleId :

PB122993BL


Tot Ion:149 Resp: 1394

Ion Ratio Lower Upper

149 100

167 18.1 23.7 35.5#




279 5.5 4.2 6.2



Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

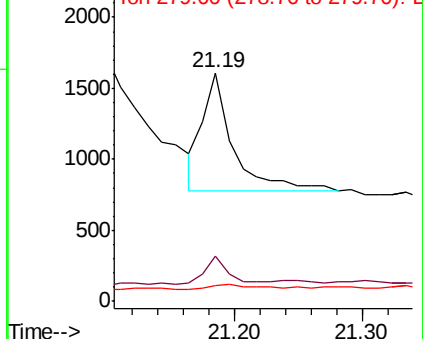

#34

Perylene-d12

Concen: 0.400 ng

RT: 23.46 min Scan# 2598

Delta R.T. -0.03 min

Lab File: BN007779.D

Acq: 21 Sep 2019 01:18


Tgt Ion:264 Resp: 33686

Ion Ratio Lower Upper

264 100

260 23.8 19.3 28.9

265 34.2 26.9 40.3



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

