

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
 Data File : BN007765.D
 Acq On : 20 Sep 2019 15:45
 Operator : HP/JU
 Sample : K4975-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE120D1-20190917

Quant Time: Sep 21 04:16:10 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	6363	0.40	ng	0.00
7) Naphthalene-d8	10.46	136	24576	0.40	ng	-0.01
13) Acenaphthene-d10	14.31	164	14691	0.40	ng	-0.01
19) Phenanthrene-d10	17.06	188	32534	0.40	ng	-0.01
27) Chrysene-d12	21.26	240	37218	0.40	ng	-0.01
34) Perylene-d12	23.47	264	41061	0.40	ng	-0.02
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	2113	0.10	ng	0.00
5) Phenol-d6	6.87	99	1554	0.05	ng	0.00
8) Nitrobenzene-d5	8.83	82	5955	0.28	ng	0.00
11) 2-Methylnaphthalene-d10	12.05	152	14004	0.34	ng	0.00
14) 2,4,6-Tribromophenol	15.81	330	1682	0.21	ng	-0.01
15) 2-Fluorobiphenyl	12.94	172	23168	0.38	ng	0.00
25) Fluoranthene-d10	19.09	212	38318	0.35	ng	-0.01
29) Terphenyl-d14	19.70	244	36599	0.40	ng	0.00
Target Compounds						
2) 1,4-Dioxane	3.28	88	50020	7.053	ng	Qvalue 95
6) bis(2-Chloroethyl)ether	7.14	93	529	0.029	ng	# 85
32) Bis(2-ethylhexyl)phthalate	21.19	149	12466	0.177	ng	# 86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
Data File : BN007765.D
Acq On : 20 Sep 2019 15:45
Operator : HP/JU
Sample : K4975-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE120D1-20190917

Quant Time: Sep 21 04:16:10 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

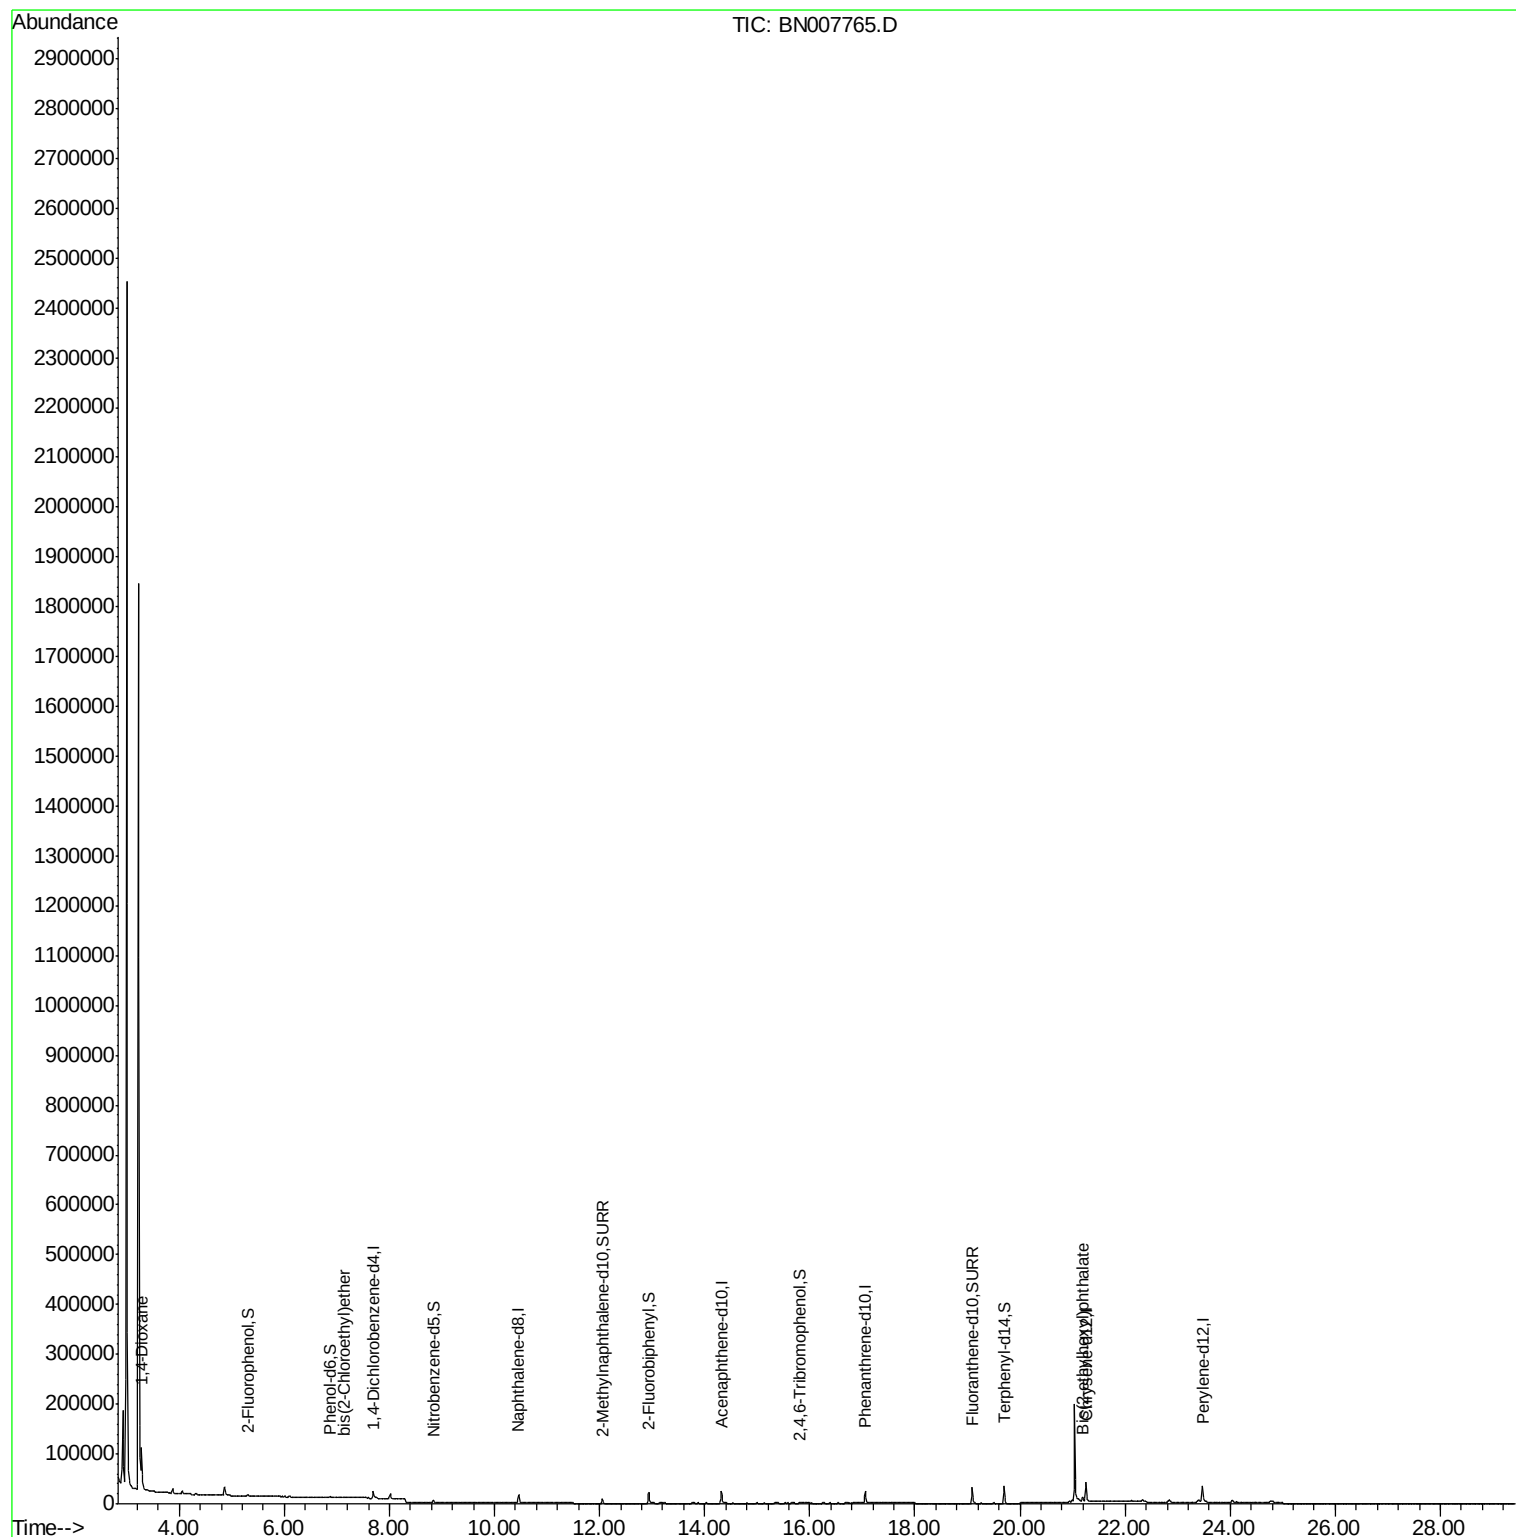




#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.69 min Scan# 604
Delta R.T. -0.01 min
Lab File: BN007765.D
Acq: 20 Sep 2019 15:45

Instrument :
BNA_N
ClientSampleId :
RE120D1-20190917

Tot Ion:152 Resp: 6363
Ion Ratio Lower Upper
152 100
150 154.8 125.6 188.4
115 63.9 53.3 79.9

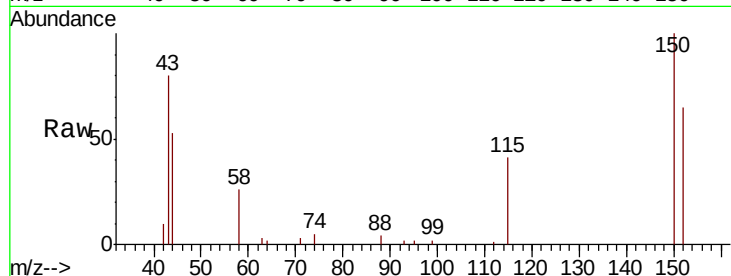


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

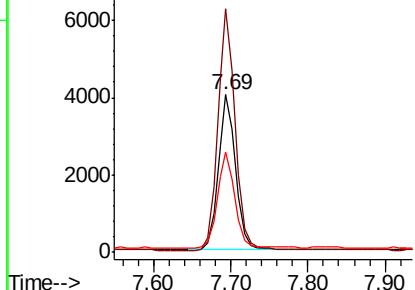



#2


1,4-Dioxane
Concen: 7.053 ng
RT: 3.28 min Scan# 56
Delta R.T. -0.02 min
Lab File: BN007765.D
Acq: 20 Sep 2019 15:45

Tgt Ion: 88 Resp: 50020
Ion Ratio Lower Upper
88 100
58 58.4 44.6 66.8
43 21.4 14.4 21.6



Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

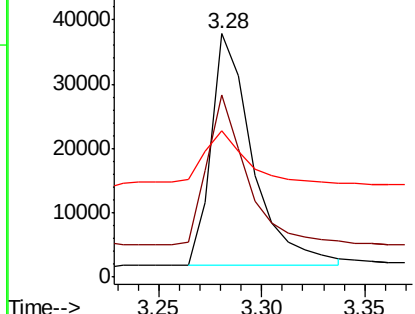

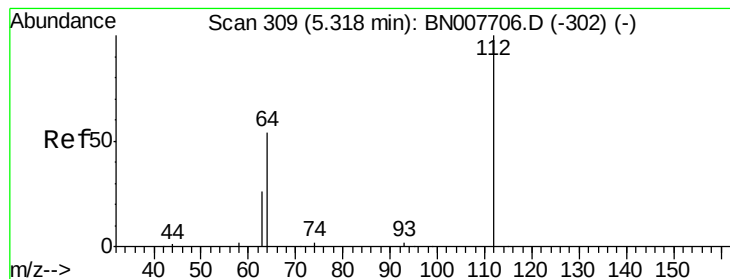

#4

2-Fluorophenol

Concen: 0.096 ng

RT: 5.31 min Scan# 308

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45

Instrument :

BNA_N

ClientSampleId :

RE120D1-20190917


Tot Ion: 112 Resp: 2113

Ion Ratio Lower Upper

112 100

64 59.3 46.6 70.0




63 30.0 23.1 34.7

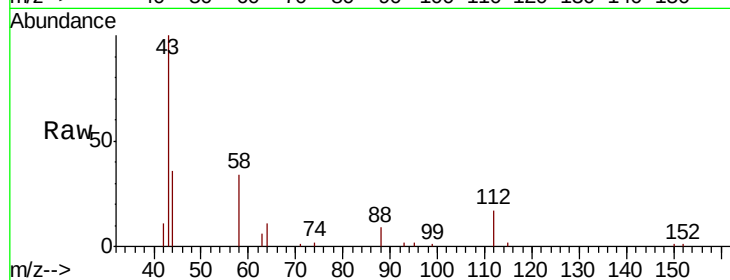

Abundance Ion 112.00 (111.70 to 112.70): B

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

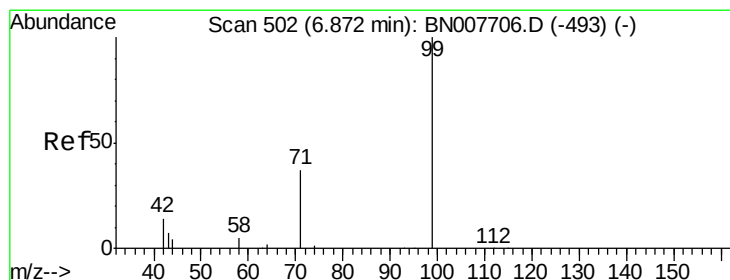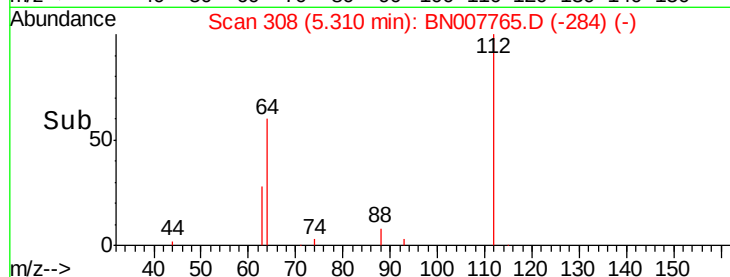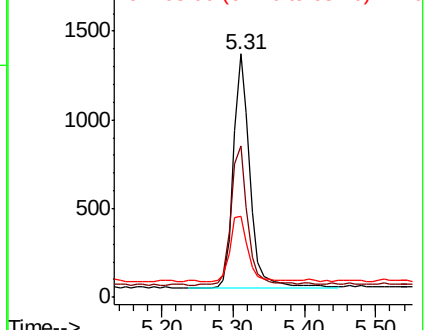

#5

Phenol-d6

Concen: 0.051 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45


Tgt Ion: 99 Resp: 1554

Ion Ratio Lower Upper

99 100

42 21.7 12.8 19.2#



71 41.8 27.6 41.4#

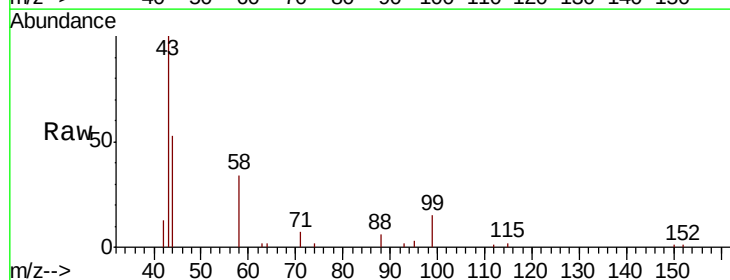


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

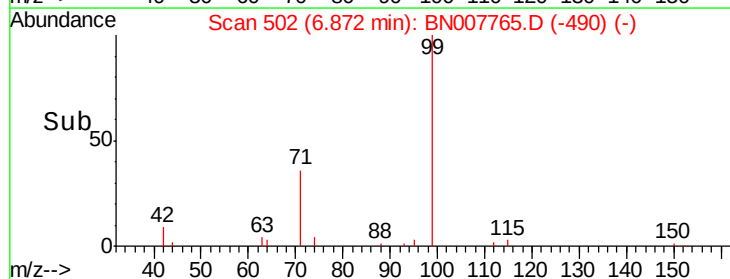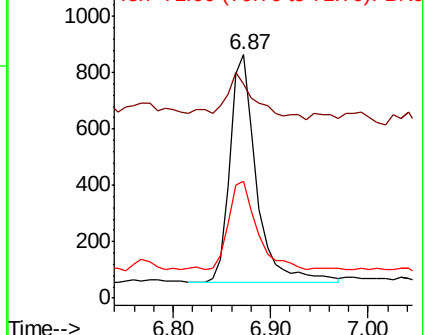

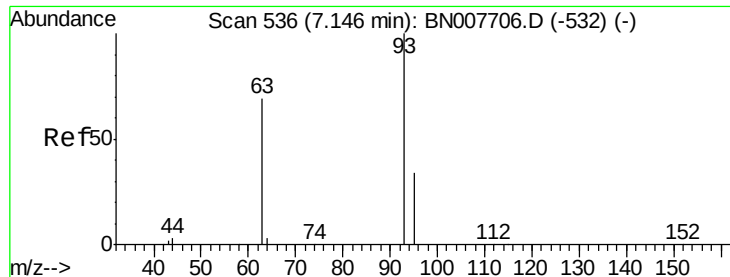

#6

bis(2-Chloroethyl)ether

Concen: 0.029 ng

RT: 7.14 min Scan# 535

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45

Instrument :

BNA_N

ClientSampleId :

RE120D1-20190917


Tot Ion: 93 Resp: 529

Ion Ratio Lower Upper

93 100

63 56.7 59.3 88.9#

95 37.2 31.4 47.0



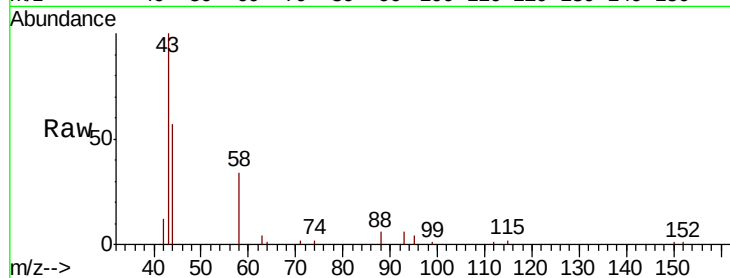


Abundance Ion 93.00 (92.70 to 93.70): BN007706.D (-532) (-)

Ion 63.00 (62.70 to 63.70): BN007706.D (-532) (-)

Ion 95.00 (94.70 to 95.70): BN007706.D (-532) (-)

Time-->

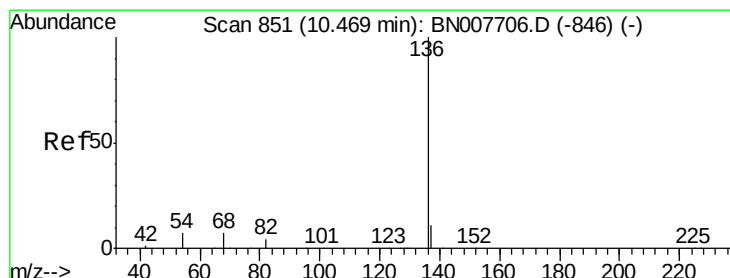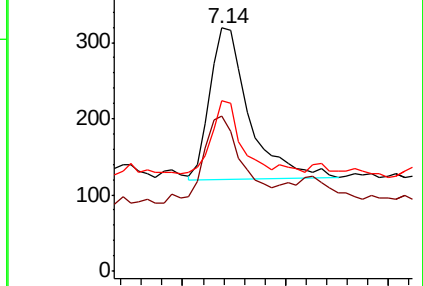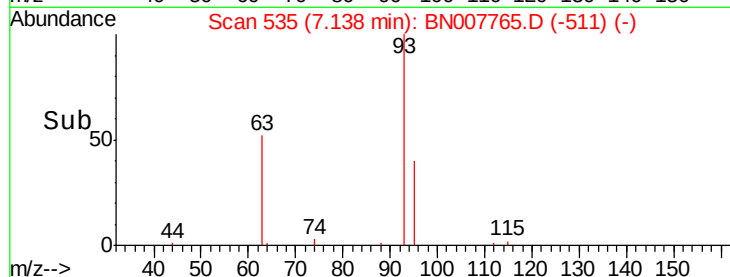

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45

Tgt Ion: 136 Resp: 24576


Ion Ratio Lower Upper

136 100

137 11.2 9.2 13.8

54 8.5 5.8 8.8

68 9.2 6.5 9.7

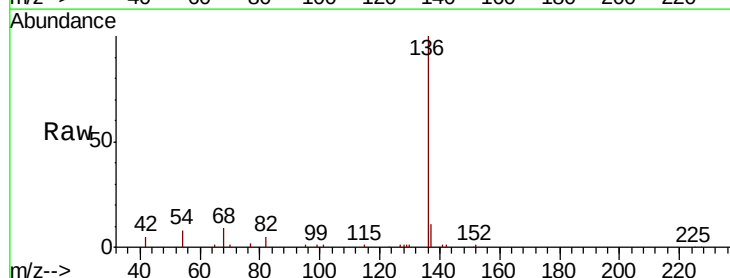



Abundance Ion 136.00 (135.70 to 136.70): BN007706.D (-846) (-)


Ion 137.00 (136.70 to 137.70): BN007706.D (-846) (-)

Ion 54.00 (53.70 to 54.70): BN007706.D (-846) (-)

Ion 68.00 (67.70 to 68.70): BN007706.D (-846) (-)

Time-->

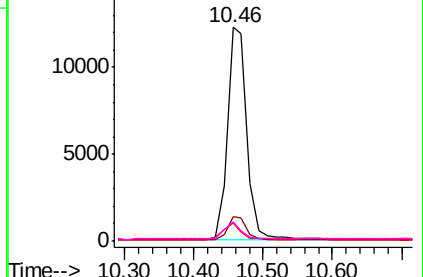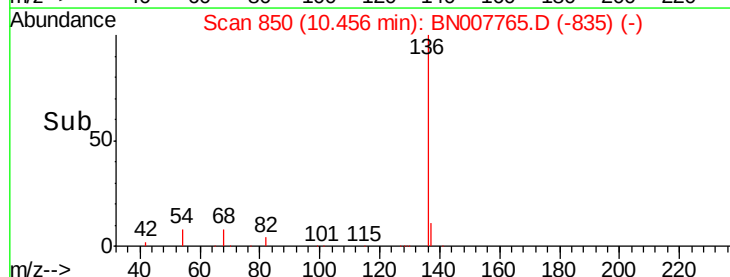







#8
 Nitrobenzene-d5
 Concen: 0.277 ng
 RT: 8.83 min Scan# 722
 Delta R.T. -0.00 min
 Lab File: BN007765.D
 Acq: 20 Sep 2019 15:45

Instrument :
 BNA_N
 ClientSampleId :
 RE120D1-20190917

Tot Ion	82	Resp	5955
Ion Ratio	Lower	Upper	
82	100		
128	36.9	24.5	36.7#
54	38.4	35.2	52.8

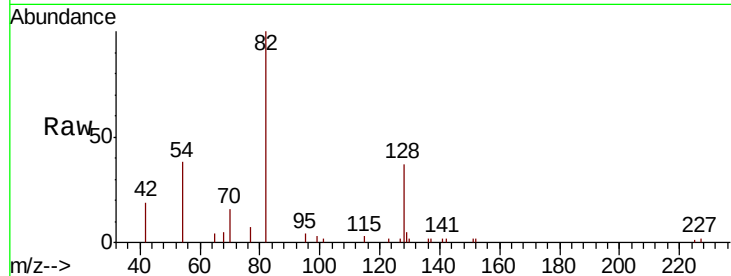


Abundance Ion 82.00 (81.70 to 82.70): BN0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BN0


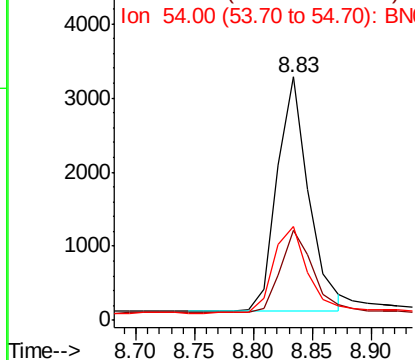



#11
 2-Methylnaphthalene-d10
 Concen: 0.338 ng
 RT: 12.05 min Scan# 1056
 Delta R.T. -0.01 min
 Lab File: BN007765.D
 Acq: 20 Sep 2019 15:45

Tgt Ion	152	Resp	14004
Ion Ratio	Lower	Upper	
152	100		
151	18.9	15.4	23.2



Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 151.00 (150.70 to 151.70): E

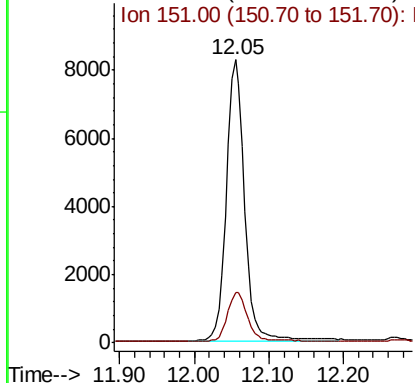

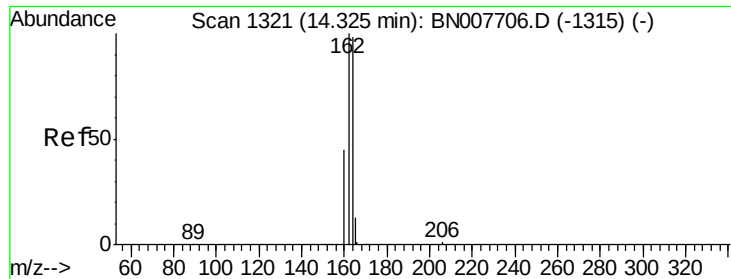

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.31 min Scan# 1320

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45

Instrument :

BNA_N

ClientSampleId :

RE120D1-20190917


Tot Ion:164 Resp: 14691

Ion Ratio Lower Upper

164 100

162 103.6 81.7 122.5




160 47.3 37.0 55.4



Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

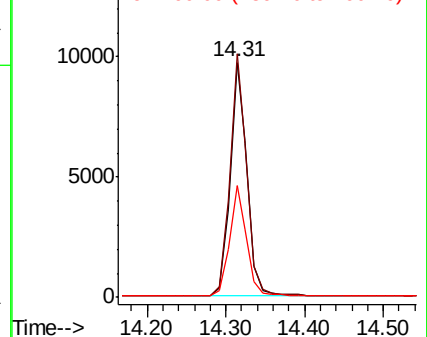

#14

2,4,6-Tribromophenol

Concen: 0.210 ng

RT: 15.81 min Scan# 1454

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45


Tgt Ion:330 Resp: 1682

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0



141 35.3 28.7 43.1




Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E




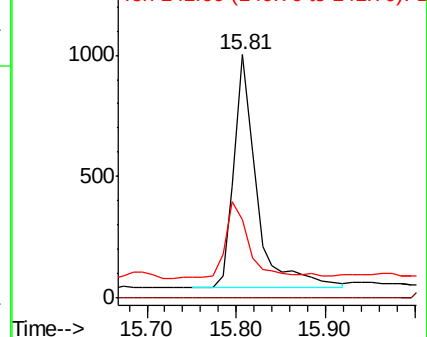


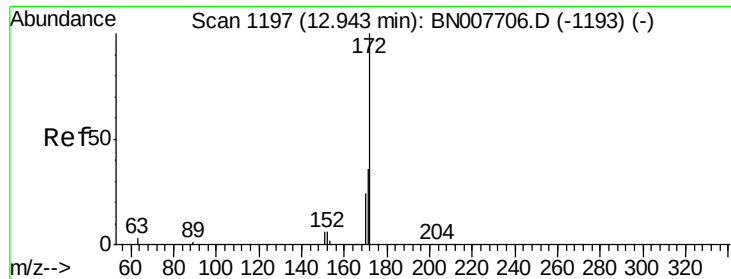

#15
2-Fluorobiphenyl
Concen: 0.383 ng
RT: 12.94 min Scan# 1197
Delta R.T. -0.00 min
Lab File: BN007765.D
Acq: 20 Sep 2019 15:45




Instrument :
BNA_N
ClientSampleId :
RE120D1-20190917


Tot Ion:172 Resp: 23168
Ion Ratio Lower Upper
172 100
171 34.3 28.8 43.2
170 21.7 19.5 29.3

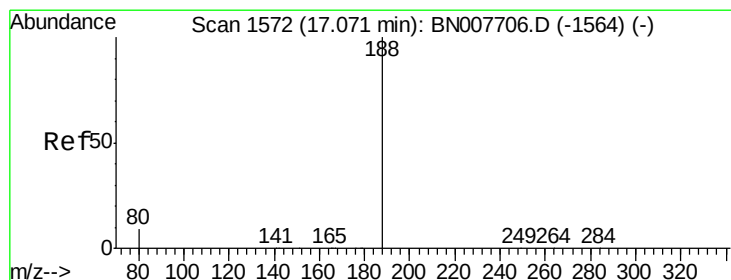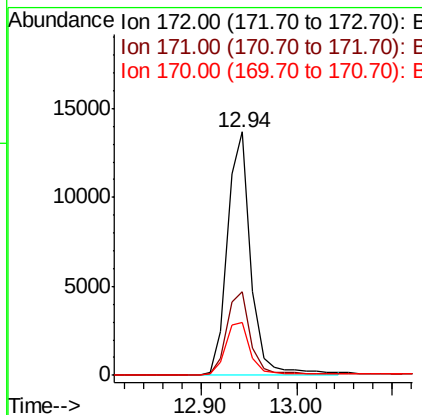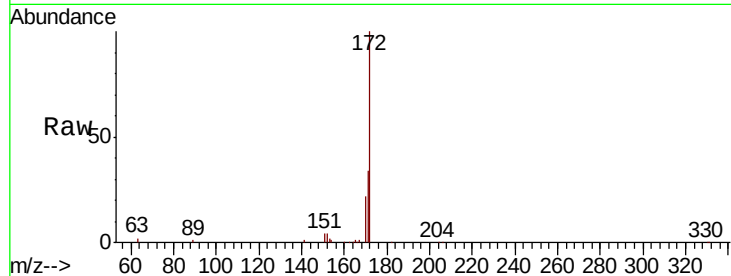

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.06 min Scan# 1571
Delta R.T. -0.01 min
Lab File: BN007765.D
Acq: 20 Sep 2019 15:45

Tgt Ion:188 Resp: 32534
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 10.1 7.4 11.2


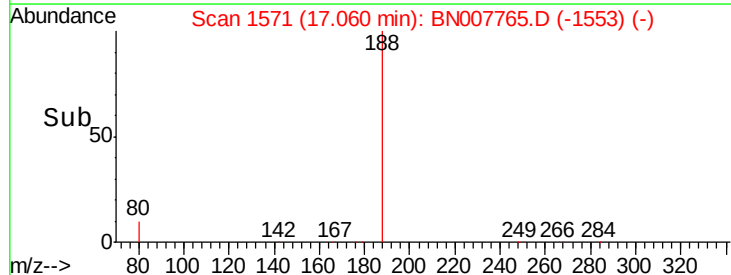
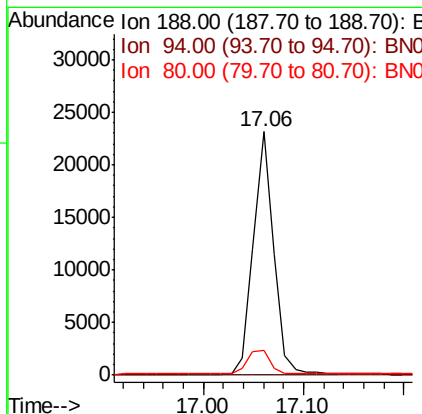



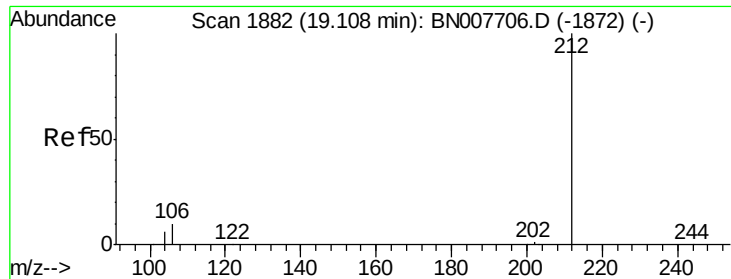

#25
 Fluoranthene-d10
 Concen: 0.349 ng
 RT: 19.09 min Scan# 1879
 Delta R.T. -0.01 min
 Lab File: BN007765.D
 Acq: 20 Sep 2019 15:45




Instrument :
 BNA_N
 ClientSampleId :
 RE120D1-20190917


Tot Ion:212 Resp: 38318
 Ion Ratio Lower Upper
 212 100
 106 12.0 9.4 14.0
 104 6.7 5.3 7.9

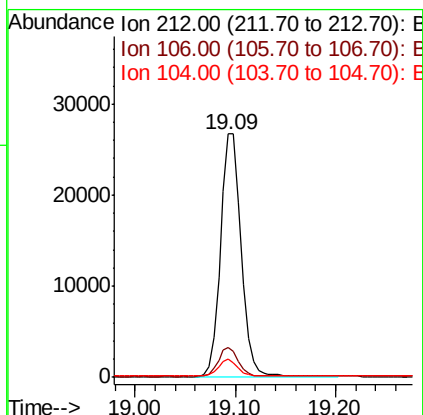

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.26 min Scan# 2181
 Delta R.T. -0.01 min
 Lab File: BN007765.D
 Acq: 20 Sep 2019 15:45

Tgt Ion:240 Resp: 37218
 Ion Ratio Lower Upper
 240 100
 120 6.1 5.4 8.2
 236 26.0 21.0 31.4

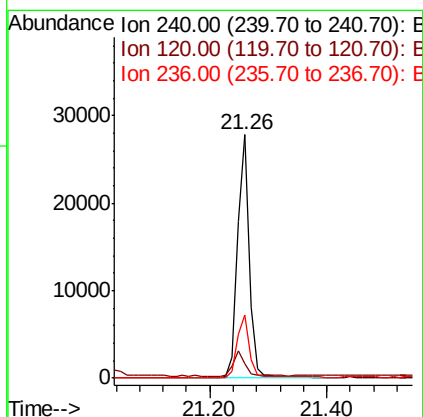

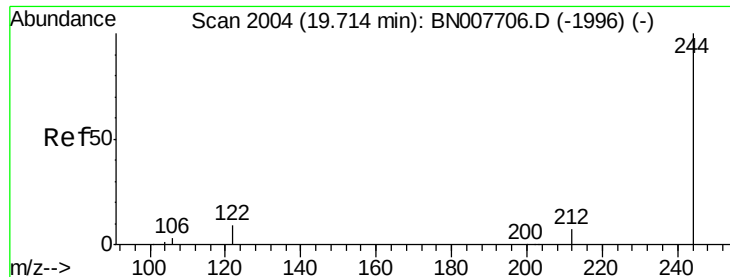

#29

Terphenyl-d14

Concen: 0.400 ng

RT: 19.70 min Scan# 2002

Delta R.T. -0.01 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45

Instrument :

BNA_N

ClientSampleId :

RE120D1-20190917


Tot Ion:244 Resp: 36599

Ion Ratio Lower Upper

244 100

212 7.3 5.9 8.9




122 9.2 7.4 11.2

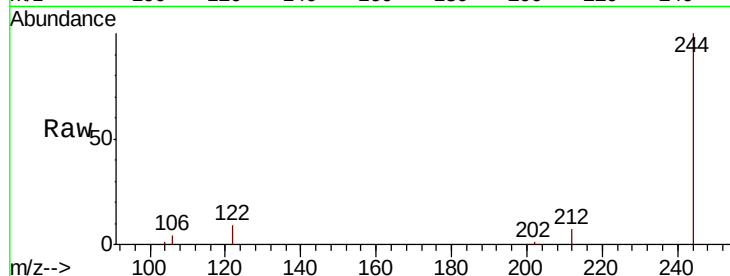

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

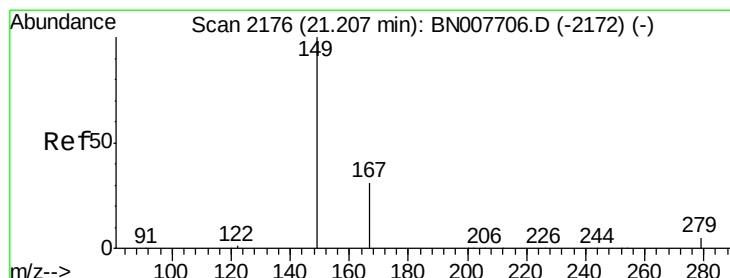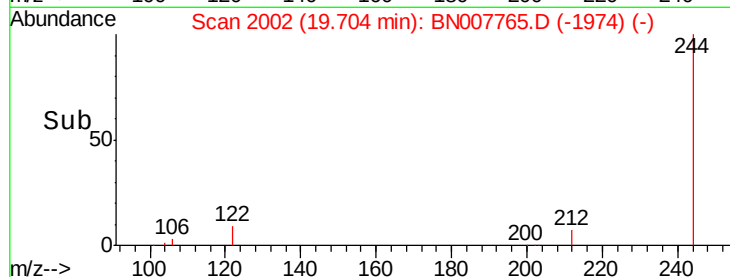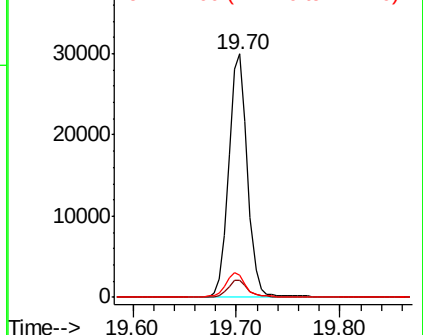

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.177 ng

RT: 21.19 min Scan# 2174

Delta R.T. -0.02 min

Lab File: BN007765.D

Acq: 20 Sep 2019 15:45


Tgt Ion:149 Resp: 12466

Ion Ratio Lower Upper

149 100

167 21.1 23.7 35.5#



279 3.4 4.2 6.2#



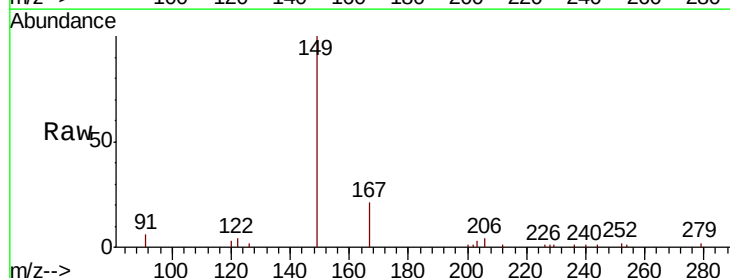


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

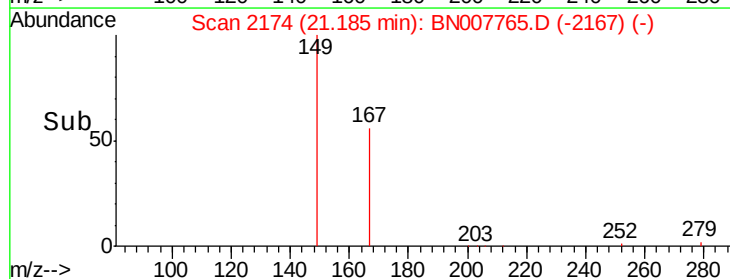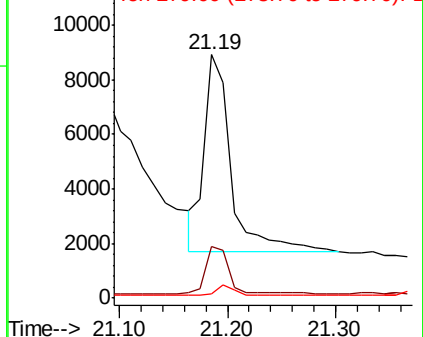

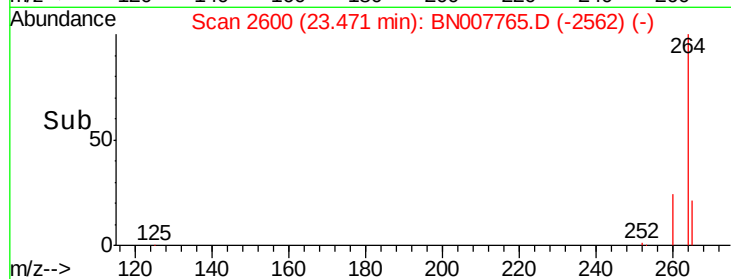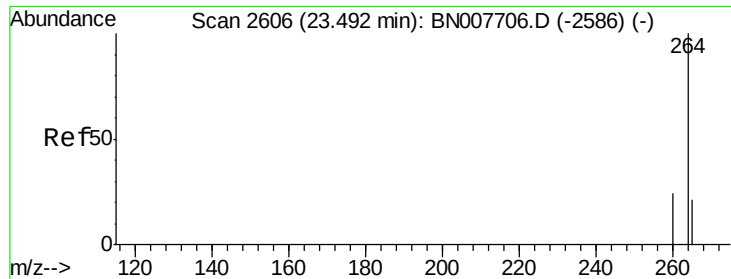

#34
 Pervlene-d12
 Concen: 0.400 ng
 RT: 23.47 min Scan# 2600
 Delta R.T. -0.02 min
 Lab File: BN007765.D
 Acq: 20 Sep 2019 15:45

Instrument :
 BNA_N
 ClientSampleId :
 RE120D1-20190917

Tot Ion: 264 Resp: 41061
 Ion Ratio Lower Upper
 264 100
 260 24.4 19.3 28.9
 265 32.0 26.9 40.3

