

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
 Data File : BN007788.D
 Acq On : 21 Sep 2019 06:40
 Operator : HP/JU
 Sample : K4974-06
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20190916

Quant Time: Sep 23 02:08:40 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 18 18:24:40 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.69	152	6466	0.40	ng	0.00
7) Naphthalene-d8	10.46	136	24053	0.40	ng	-0.01
13) Acenaphthene-d10	14.31	164	14644	0.40	ng	-0.01
19) Phenanthrene-d10	17.06	188	31766	0.40	ng	-0.01
27) Chrysene-d12	21.25	240	36083	0.40	ng	-0.02
34) Perylene-d12	23.46	264	41526	0.40	ng	-0.03
System Monitoring Compounds						
4) 2-Fluorophenol	5.31	112	2082	0.09	ng	0.00
5) Phenol-d6	6.87	99	1651	0.05	ng	0.00
8) Nitrobenzene-d5	8.83	82	5555	0.26	ng	0.00
11) 2-Methylnaphthalene-d10	12.05	152	13002	0.32	ng	0.00
14) 2,4,6-Tribromophenol	15.81	330	1218	0.15	ng	-0.01
15) 2-Fluorobiphenyl	12.94	172	18797	0.31	ng	0.00
25) Fluoranthene-d10	19.09	212	34669	0.32	ng	-0.01
29) Terphenyl-d14	19.70	244	30498	0.34	ng	-0.01
Target Compounds						
2) 1,4-Dioxane	3.30	88	3247	0.451	ng	Qvalue # 79
32) Bis(2-ethylhexyl)phthalate	21.19	149	3553	0.052	ng	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN092019\
Data File : BN007788.D
Acq On : 21 Sep 2019 06:40
Operator : HP/JU
Sample : K4974-06
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
RE134D1-20190916

Quant Time: Sep 23 02:08:40 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN091819.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 18 18:24:40 2019
Response via : Initial Calibration

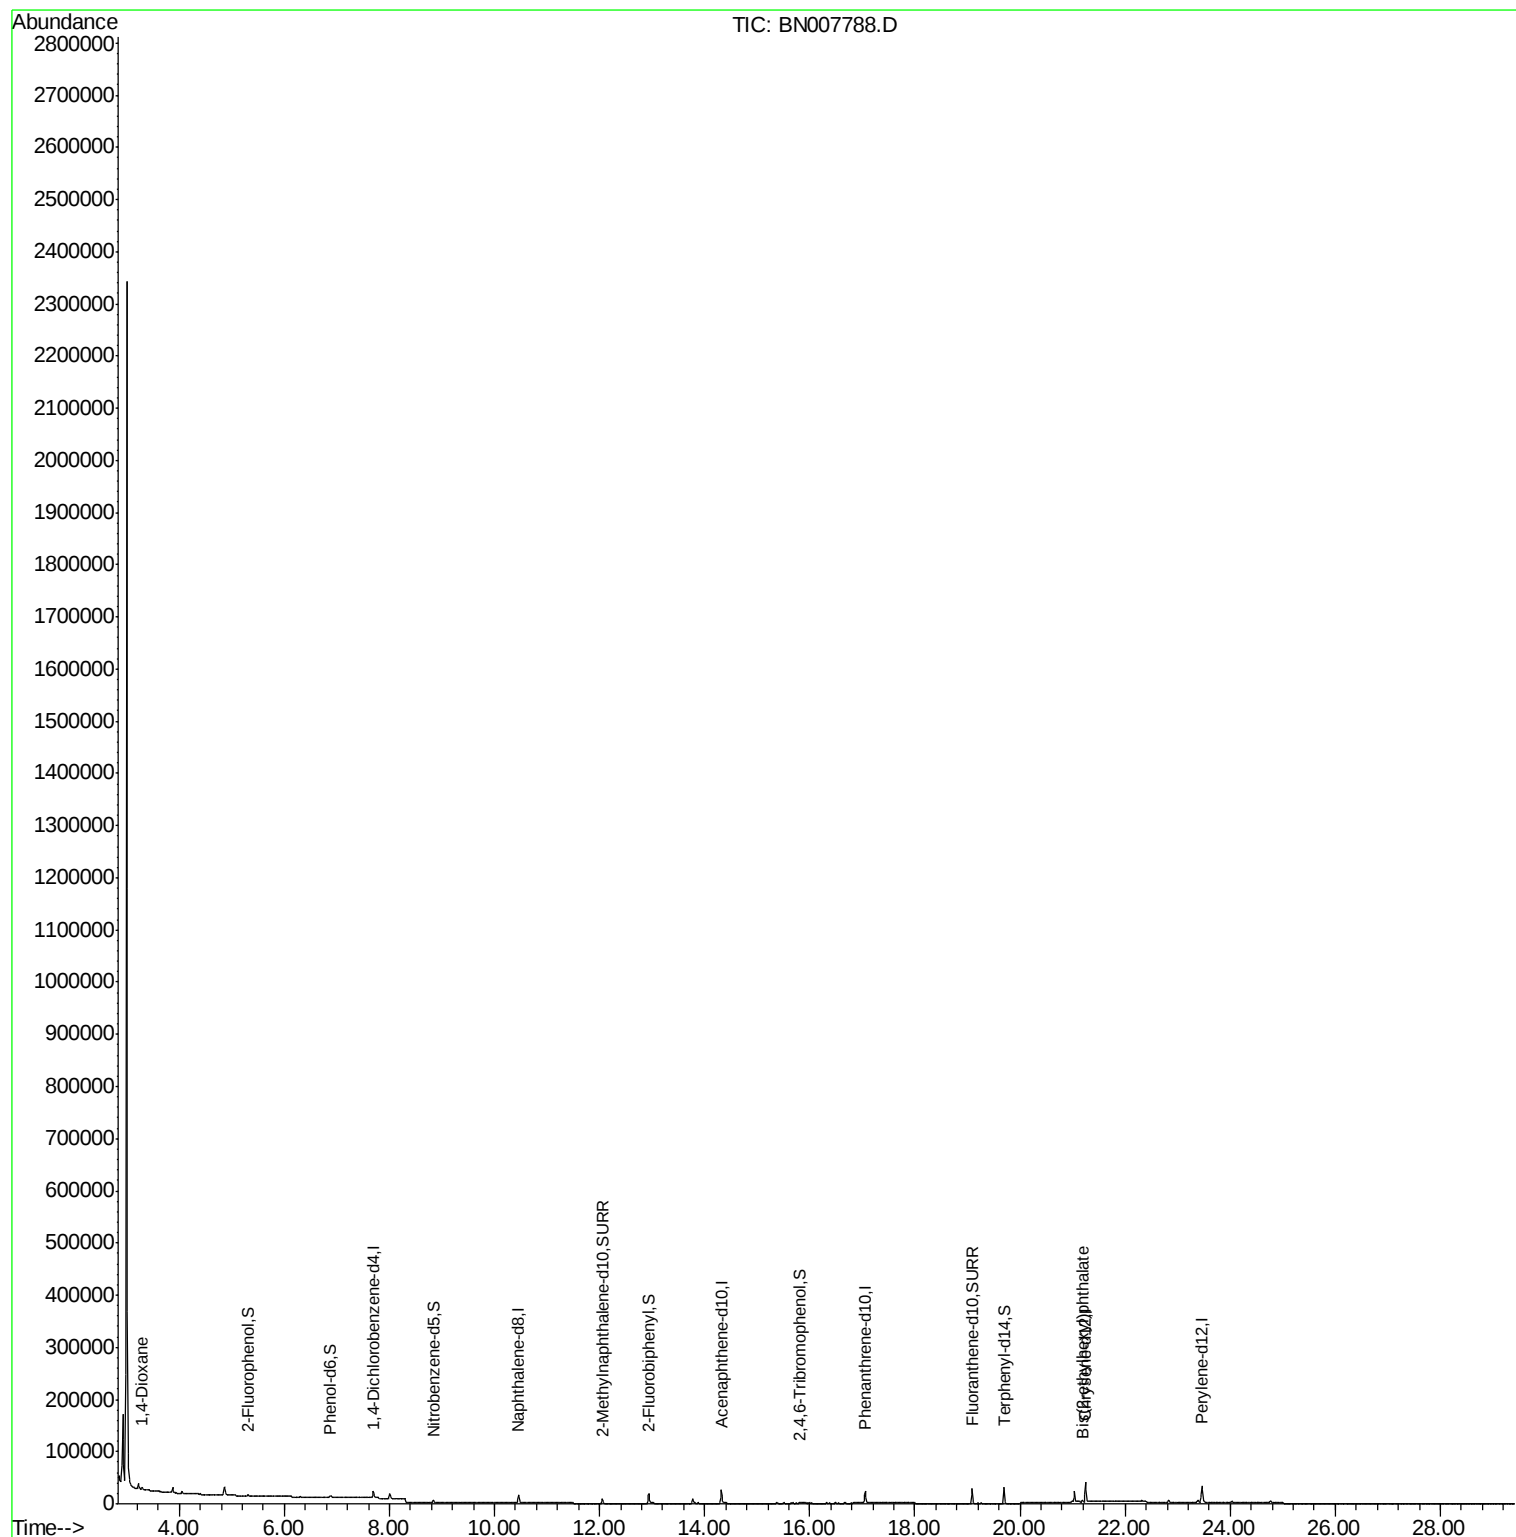




#1



1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.69 min Scan# 604
Delta R.T. -0.01 min
Lab File: BN007788.D
Acq: 21 Sep 2019 06:40

Instrument :
BNA_N
ClientSampleId :
RE134D1-20190916

Tot Ion:152 Resp: 6466
Ion Ratio Lower Upper
152 100
150 155.5 125.6 188.4
115 64.3 53.3 79.9

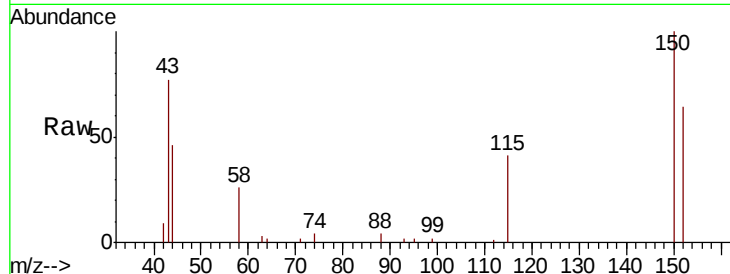


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

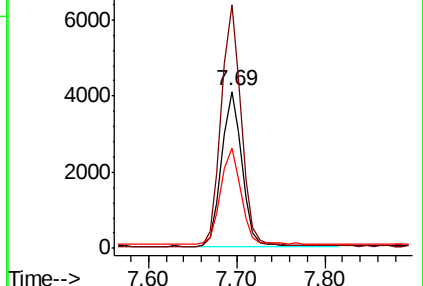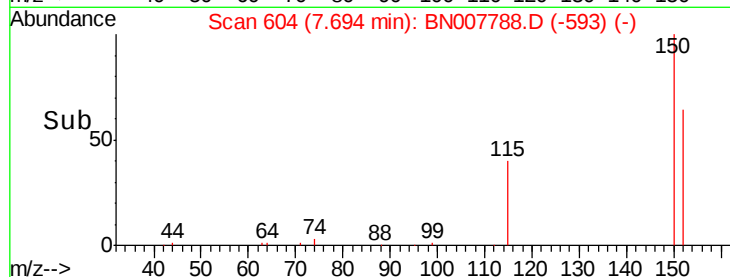



#2

1,4-Dioxane
Concen: 0.451 ng
RT: 3.30 min Scan# 58
Delta R.T. -0.01 min
Lab File: BN007788.D
Acq: 21 Sep 2019 06:40

Tgt Ion: 88 Resp: 3247
Ion Ratio Lower Upper
88 100
58 59.7 44.6 66.8
43 49.4 14.4 21.6#

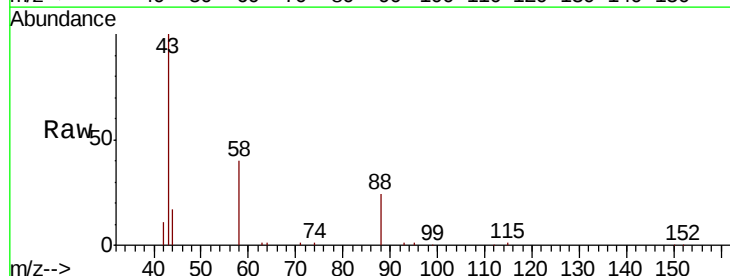

Abundance Ion 88.00 (87.70 to 88.70): BNC
Ion 58.00 (57.70 to 58.70): BNC
Ion 43.00 (42.70 to 43.70): BNC

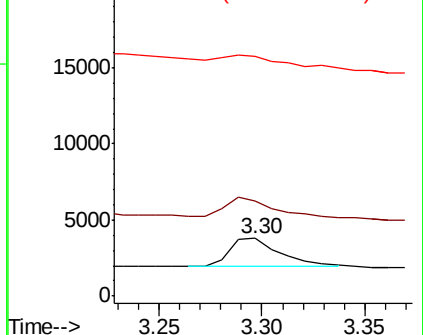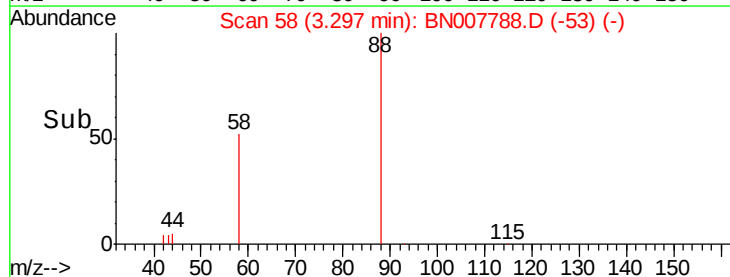



#4

2-Fluorophenol

Concen: 0.094 ng

RT: 5.31 min Scan# 308

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40

Instrument :

BNA_N

ClientSampleId :

RE134D1-20190916


Tot Ion: 112 Resp: 2082

Ion Ratio Lower Upper

112 100

64 59.6 46.6 70.0



63 29.7 23.1 34.7

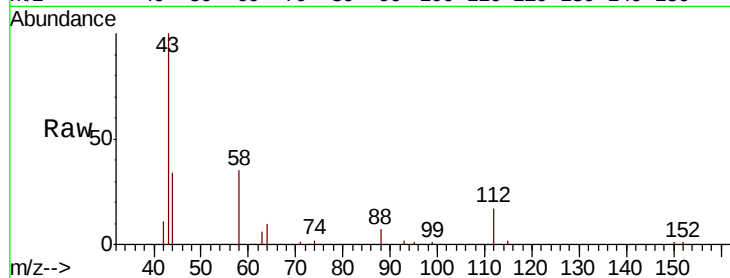

Abundance Ion 112.00 (111.70 to 112.70): BNC

Ion 64.00 (63.70 to 64.70): BNC

Ion 63.00 (62.70 to 63.70): BNC

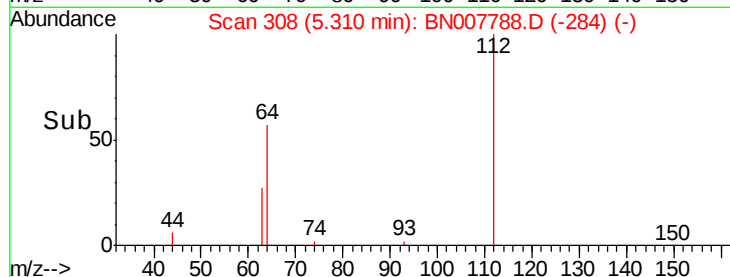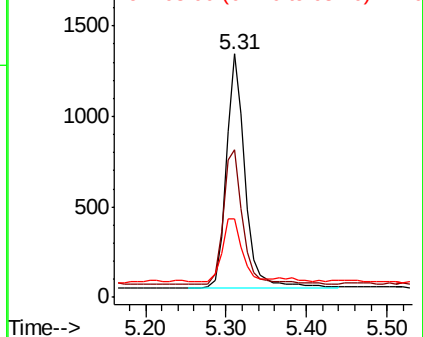

#5

Phenol-d6

Concen: 0.054 ng

RT: 6.87 min Scan# 502

Delta R.T. 0.00 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40


Tgt Ion: 99 Resp: 1651

Ion Ratio Lower Upper

99 100

42 25.0 12.8 19.2#



71 41.2 27.6 41.4

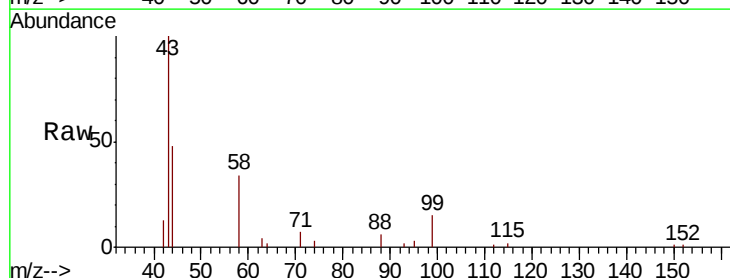


Abundance Ion 99.00 (98.70 to 99.70): BNC

Ion 42.00 (41.70 to 42.70): BNC

Ion 71.00 (70.70 to 71.70): BNC

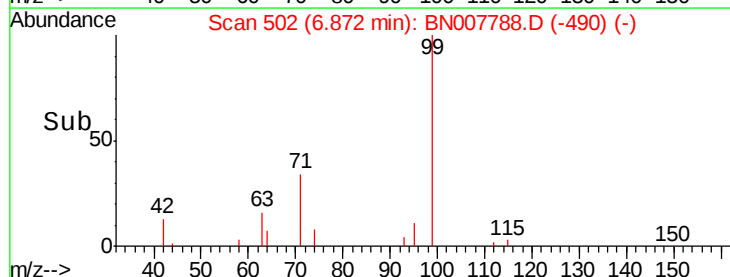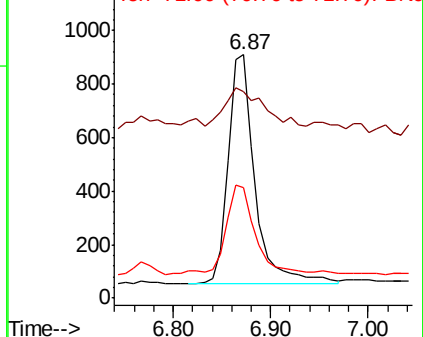

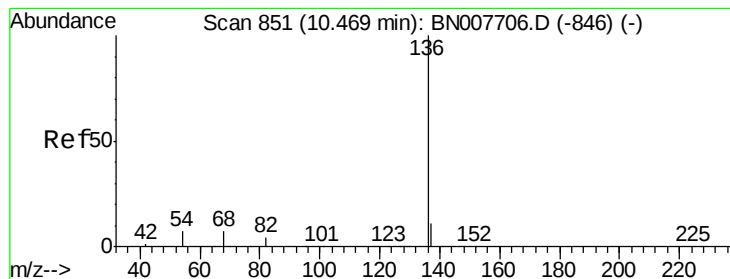

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.46 min Scan# 850

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40

Instrument :

BNA_N

ClientSampleId :

RE134D1-20190916

Tot Ion:136 Resp: 24053


Ion Ratio Lower Upper

136 100

137 11.3 9.2 13.8

54 8.3 5.8 8.8

68 8.9 6.5 9.7



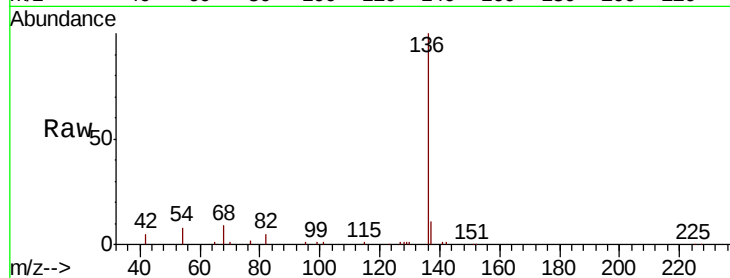


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BNC

Ion 68.00 (67.70 to 68.70): BNC

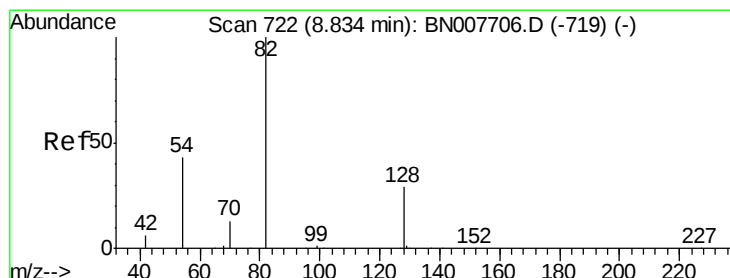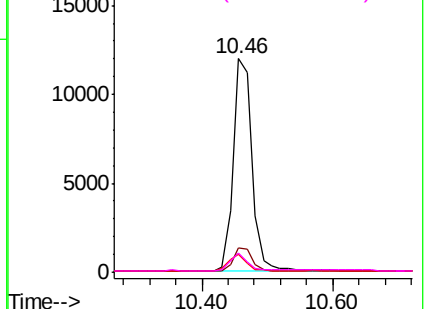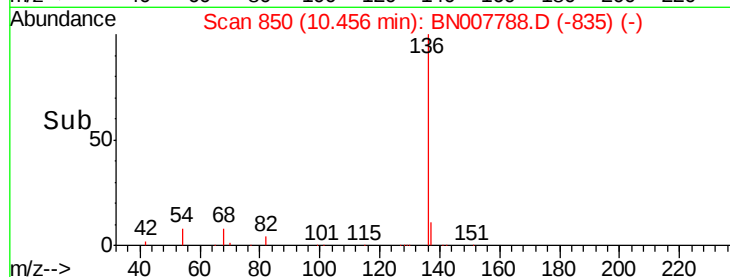

#8

Nitrobenzene-d5

Concen: 0.264 ng

RT: 8.83 min Scan# 722

Delta R.T. -0.00 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40


Tgt Ion: 82 Resp: 5555

Ion Ratio Lower Upper

82 100

128 36.9 24.5 36.7#



54 38.5 35.2 52.8

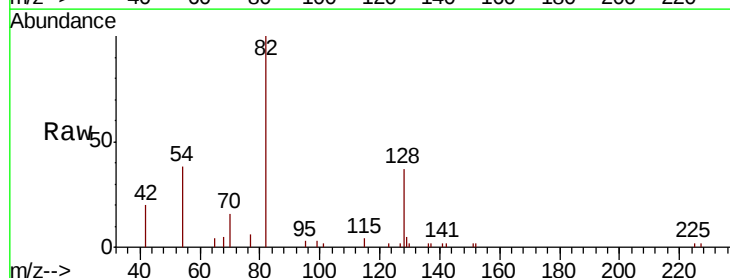

Abundance Ion 82.00 (81.70 to 82.70): BNC

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BNC



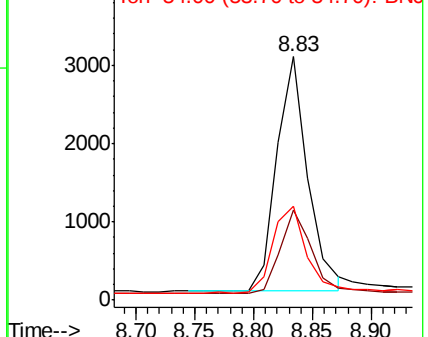
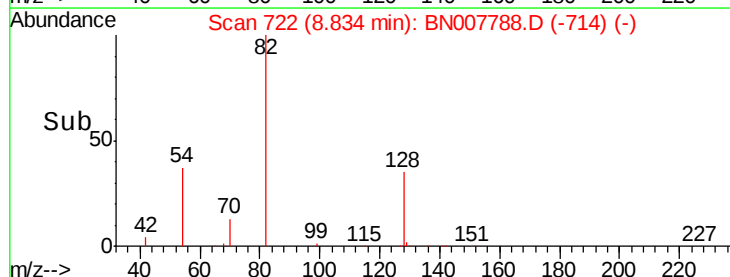




#11
2-Methylnaphthalene-d10
Concen: 0.321 ng
RT: 12.05 min Scan# 1056
Delta R.T. -0.01 min
Lab File: BN007788.D
Acq: 21 Sep 2019 06:40




Instrument :
BNA_N
ClientSampleId :
RE134D1-20190916


Tot Ion:152 Resp: 13002
Ion Ratio Lower Upper
152 100
151 19.1 15.4 23.2

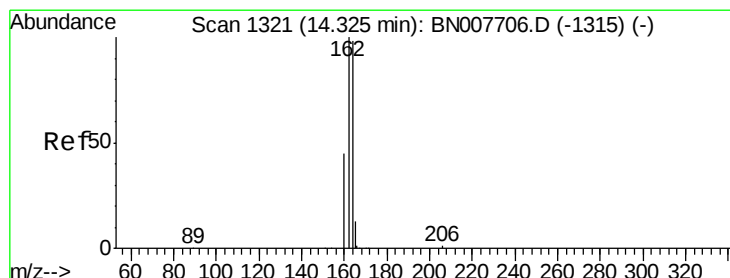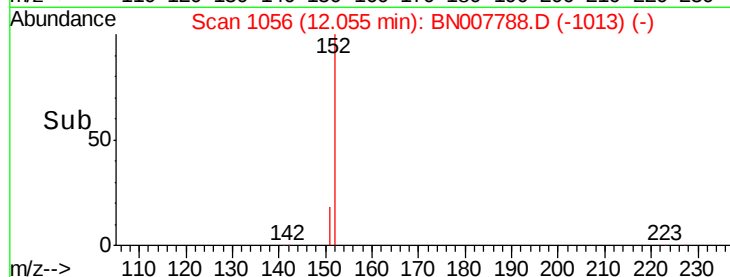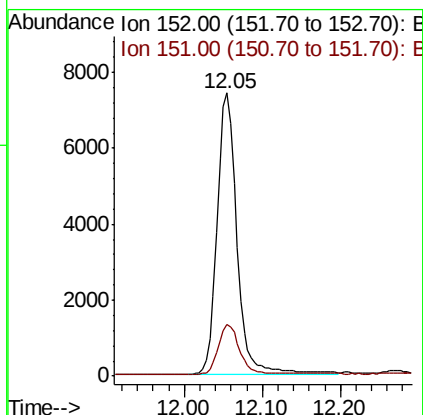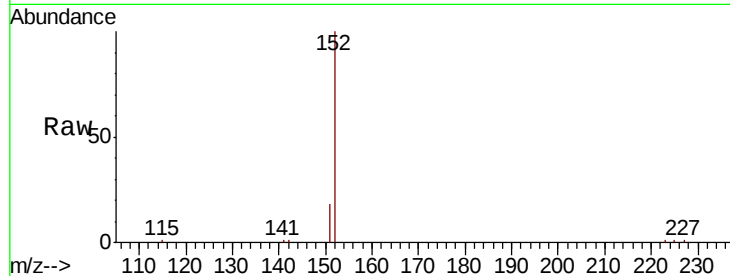

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.31 min Scan# 1320
Delta R.T. -0.01 min
Lab File: BN007788.D
Acq: 21 Sep 2019 06:40

Tgt Ion:164 Resp: 14644
Ion Ratio Lower Upper
164 100
162 103.7 81.7 122.5
160 46.8 37.0 55.4

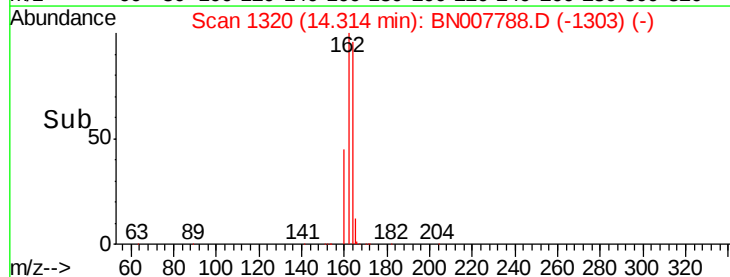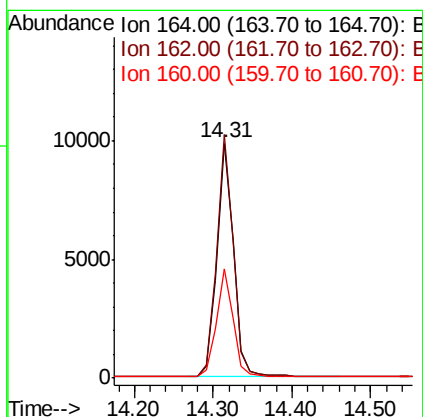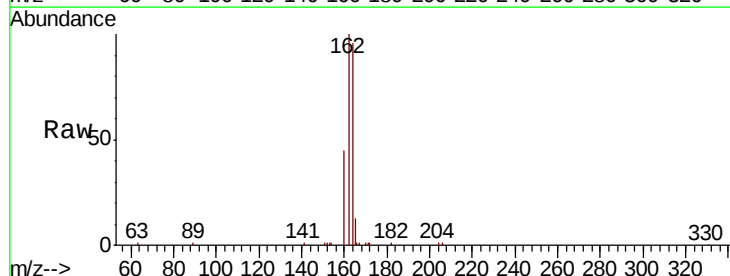



#14

2,4,6-Tribromophenol

Concen: 0.153 ng

RT: 15.81 min Scan# 1454

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40

Instrument :

BNA_N

ClientSampleId :

RE134D1-20190916


Tot Ion:330 Resp: 1218

Ion Ratio Lower Upper

330 100

332 0.0 0.0 0.0




141 36.9 28.7 43.1

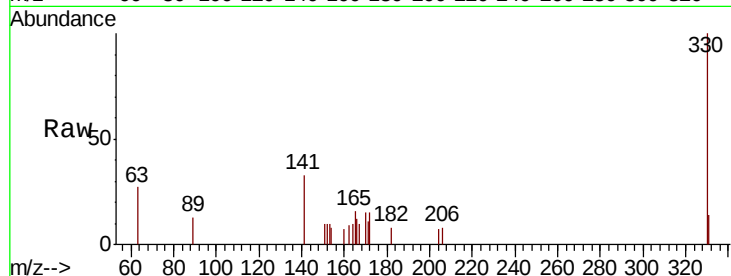

Abundance Ion 330.00 (329.70 to 330.70): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

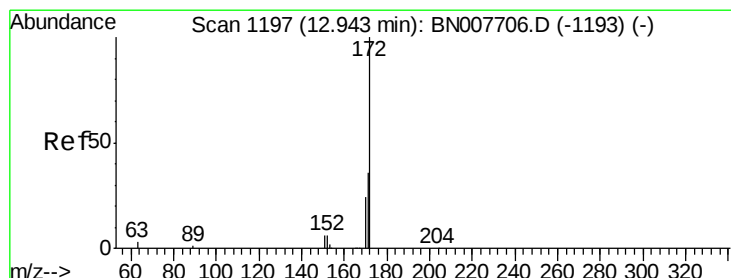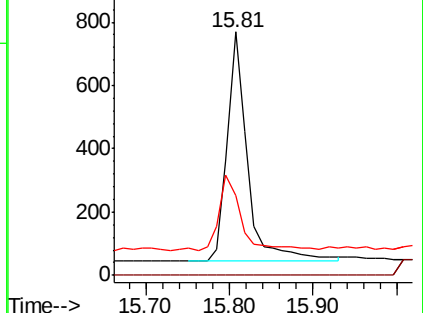

#15

2-Fluorobiphenyl

Concen: 0.312 ng

RT: 12.94 min Scan# 1197

Delta R.T. -0.00 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40


Tgt Ion:172 Resp: 18797

Ion Ratio Lower Upper

172 100

171 33.9 28.8 43.2



170 22.1 19.5 29.3

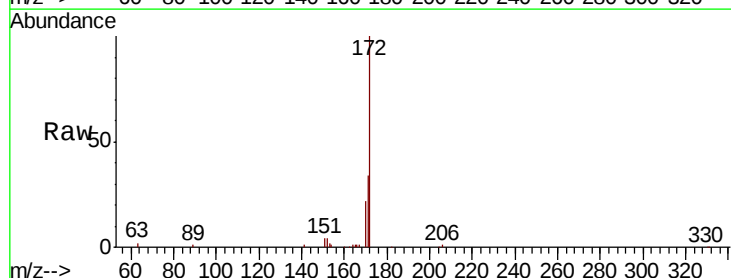


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

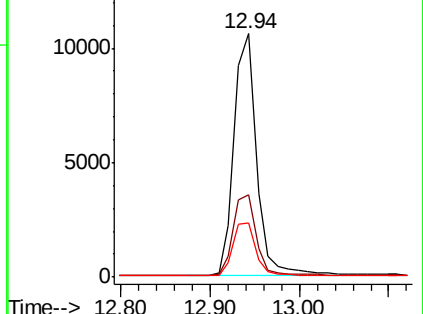

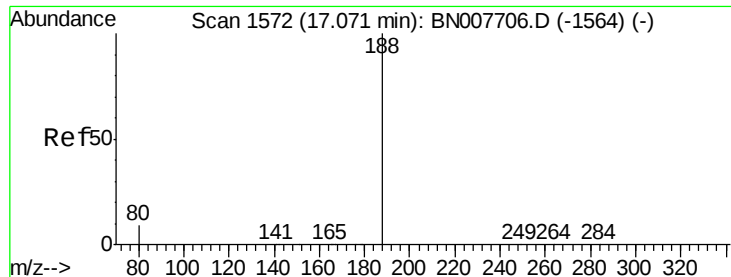

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.06 min Scan# 1571

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40

Instrument :

BNA_N

ClientSampleId :

RE134D1-20190916


Tot Ion:188 Resp: 31766

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 9.8 7.4 11.2

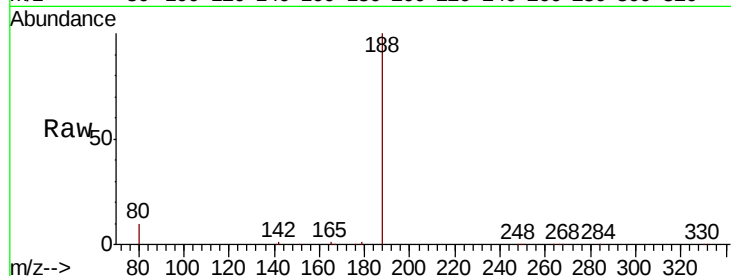

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BNC

Ion 80.00 (79.70 to 80.70): BNC

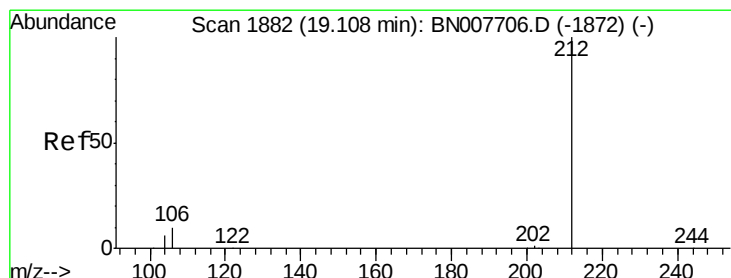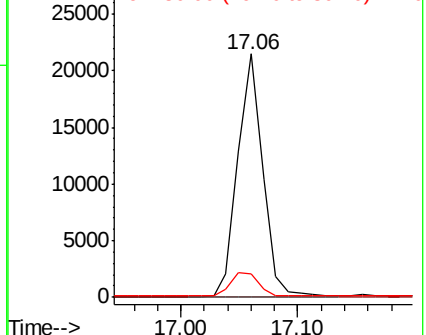

#25

Fluoranthene-d10

Concen: 0.324 ng

RT: 19.09 min Scan# 1879

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40


Tgt Ion:212 Resp: 34669

Ion Ratio Lower Upper

212 100

106 11.7 9.4 14.0



104 6.8 5.3 7.9

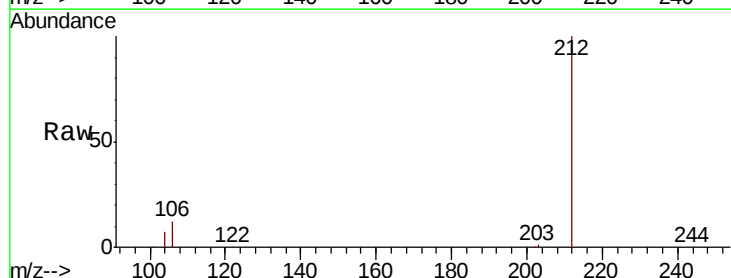


Abundance Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

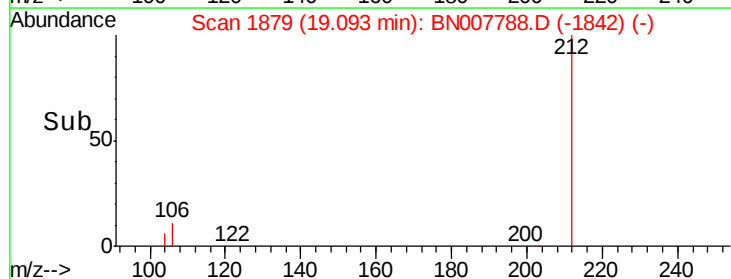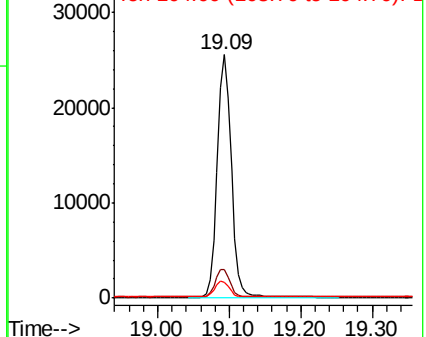

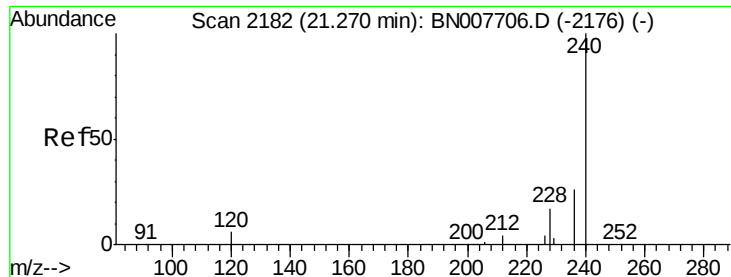

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.25 min Scan# 2180

Delta R.T. -0.02 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40

Instrument :

BNA_N

ClientSampleId :

RE134D1-20190916


Tot Ion:240 Resp: 36083

Ion Ratio Lower Upper

240 100

120 10.6 5.4 8.2#




236 26.8 21.0 31.4

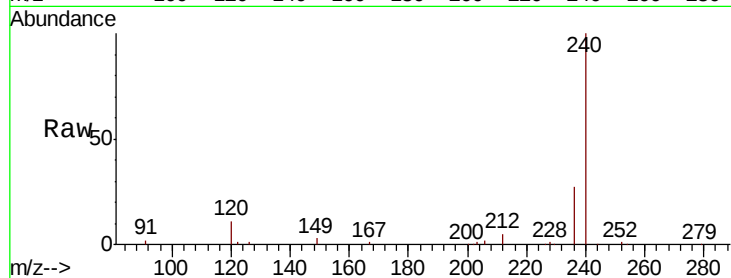

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

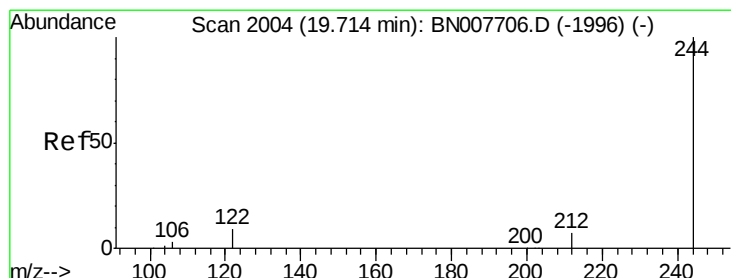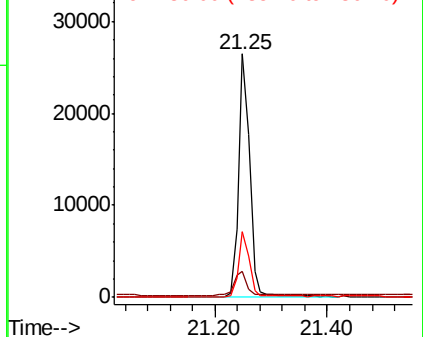

#29

Terphenyl-d14

Concen: 0.344 ng

RT: 19.70 min Scan# 2001

Delta R.T. -0.01 min

Lab File: BN007788.D

Acq: 21 Sep 2019 06:40


Tgt Ion:244 Resp: 30498

Ion Ratio Lower Upper

244 100

212 7.2 5.9 8.9



122 9.7 7.4 11.2

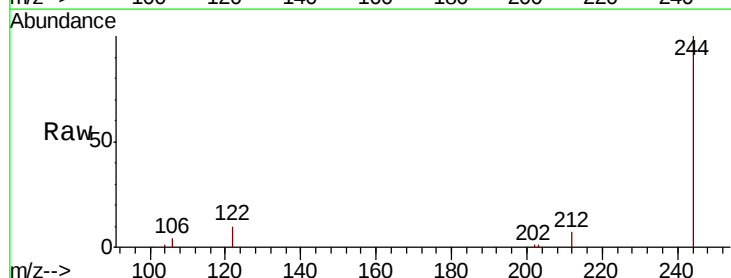


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

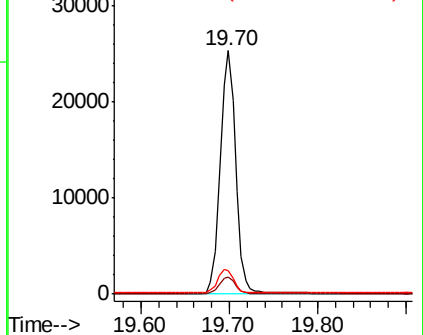







#32
 Bis(2-ethylhexyl)phthalate
 Concen: 0.052 ng
 RT: 21.19 min Scan# 2174
 Delta R.T. -0.02 min
 Lab File: BN007788.D
 Acq: 21 Sep 2019 06:40

Instrument :
 BNA_N
 ClientSampleId :
 RE134D1-20190916

Tot Ion:149 Resp: 3553
 Ion Ratio Lower Upper
 149 100
 167 26.1 23.7 35.5
 279 5.3 4.2 6.2

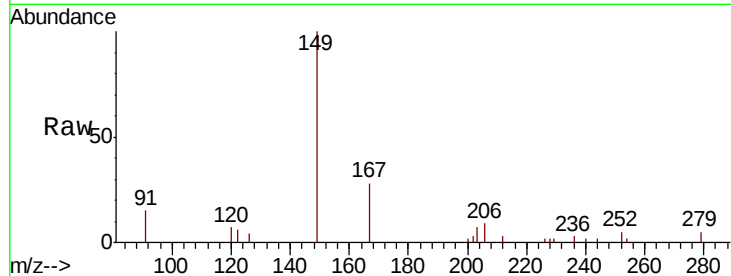


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

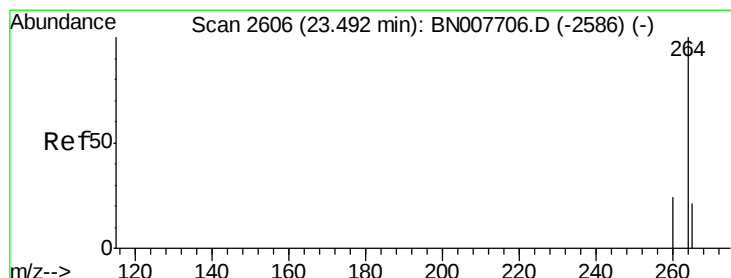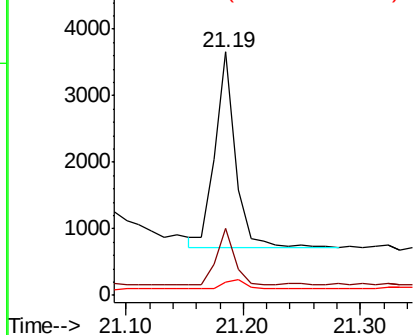

#34
 Perylene-d12
 Concen: 0.400 ng
 RT: 23.46 min Scan# 2597
 Delta R.T. -0.03 min
 Lab File: BN007788.D
 Acq: 21 Sep 2019 06:40

Tgt Ion:264 Resp: 41526
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.3 28.9
 265 30.3 26.9 40.3

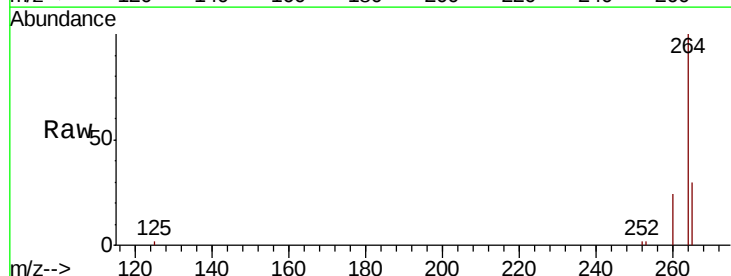

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

