


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092019\
 Data File : BN007759.D
 Acq On : 20 Sep 2019 11:30
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

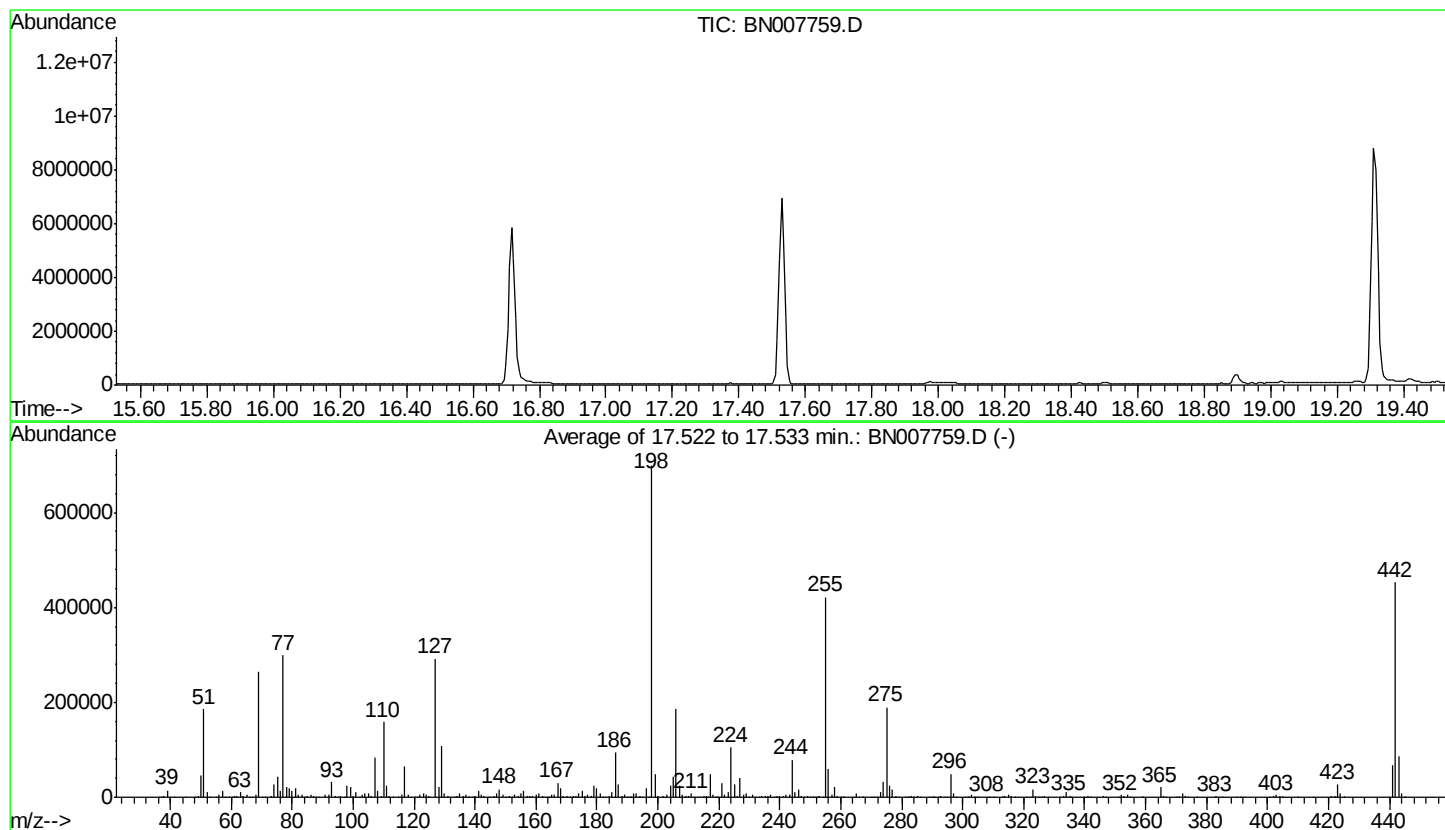

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	185653	PASS
68	69	0.00	2	1.7	4614	PASS
69	198	0.00	100	38.0	265676	PASS
70	69	0.00	2	0.5	1217	PASS
127	198	10	80	41.8	292096	PASS
197	198	0.00	2	0.2	1275	PASS
198	198	100	100	100.0	698730	PASS
199	198	5	9	7.0	48866	PASS
275	198	10	60	27.1	189354	PASS
365	198	1	100	3.0	21161	PASS
441	198	0.01	100	9.8	68664	PASS
442	198	50	100	64.8	452629	PASS
443	442	15	24	18.8	85197	PASS