


Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN092019\
 Data File : BN007777.D
 Acq On : 21 Sep 2019 00:07
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091819.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 18 18:24:40 2019

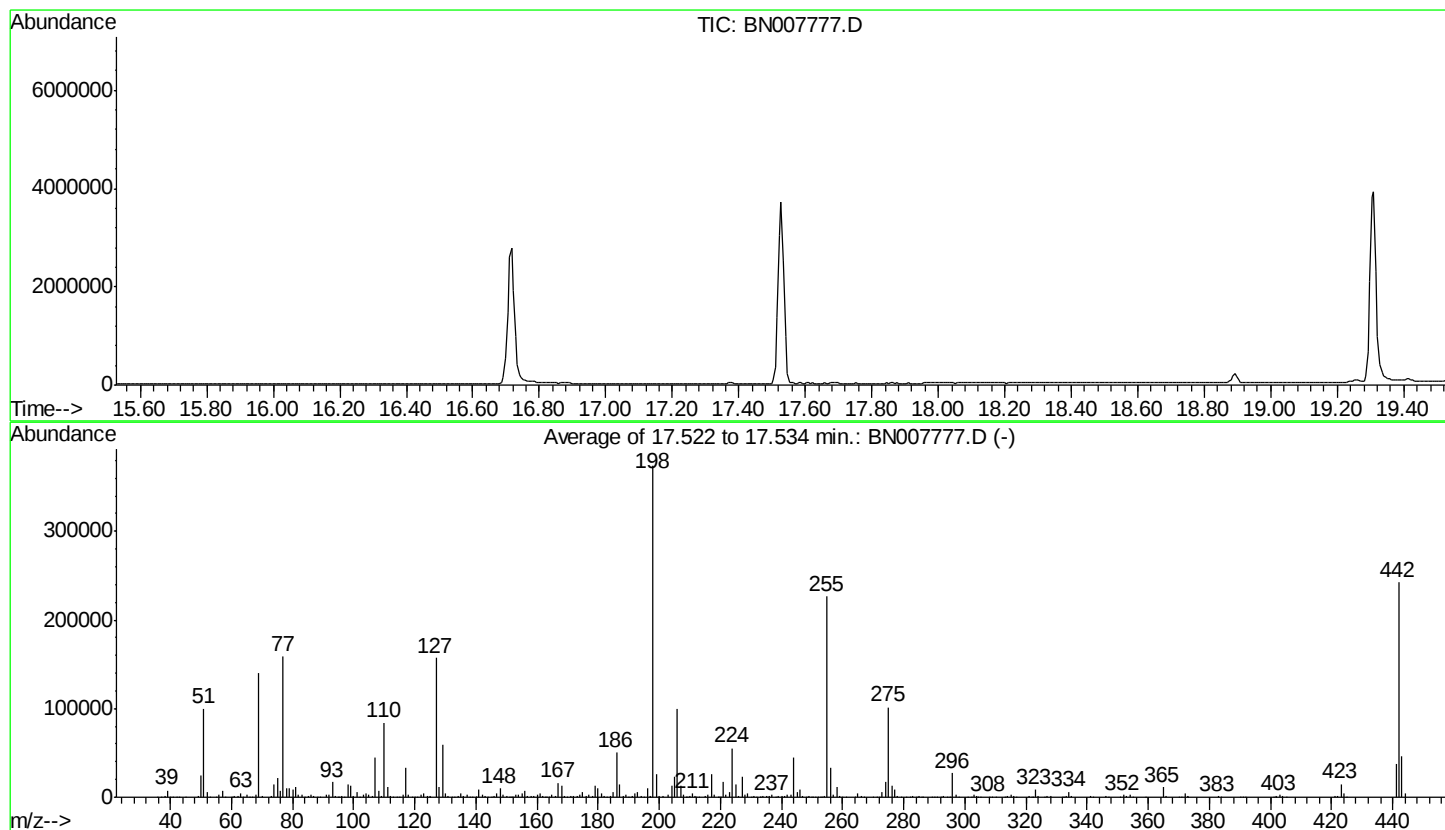

AutoFind: Scans 2471, 2472, 2473; Background Corrected with Scan 2464

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.7	99872	PASS
68	69	0.00	2	1.7	2358	PASS
69	198	0.00	100	37.3	139597	PASS
70	69	0.00	2	0.6	867	PASS
127	198	10	80	42.1	157416	PASS
197	198	0.00	2	0.5	1774	PASS
198	198	100	100	100.0	374186	PASS
199	198	5	9	6.9	25816	PASS
275	198	10	60	27.2	101642	PASS
365	198	1	100	3.1	11458	PASS
441	198	0.01	100	10.2	38034	PASS
442	198	50	100	64.7	242282	PASS
443	442	15	24	19.2	46560	PASS