
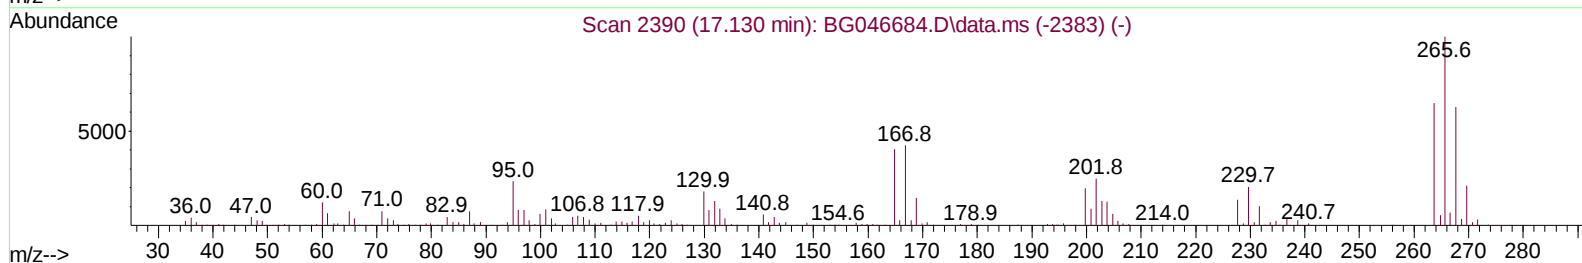
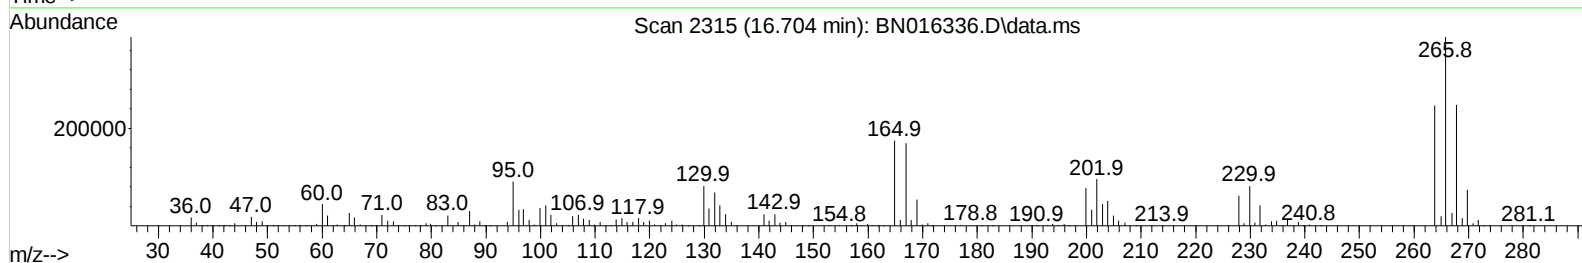


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016336.D
Acq On : 20 Sep 2021 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 10:45:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 20 10:45:20 2021
Response via : Initial Calibration

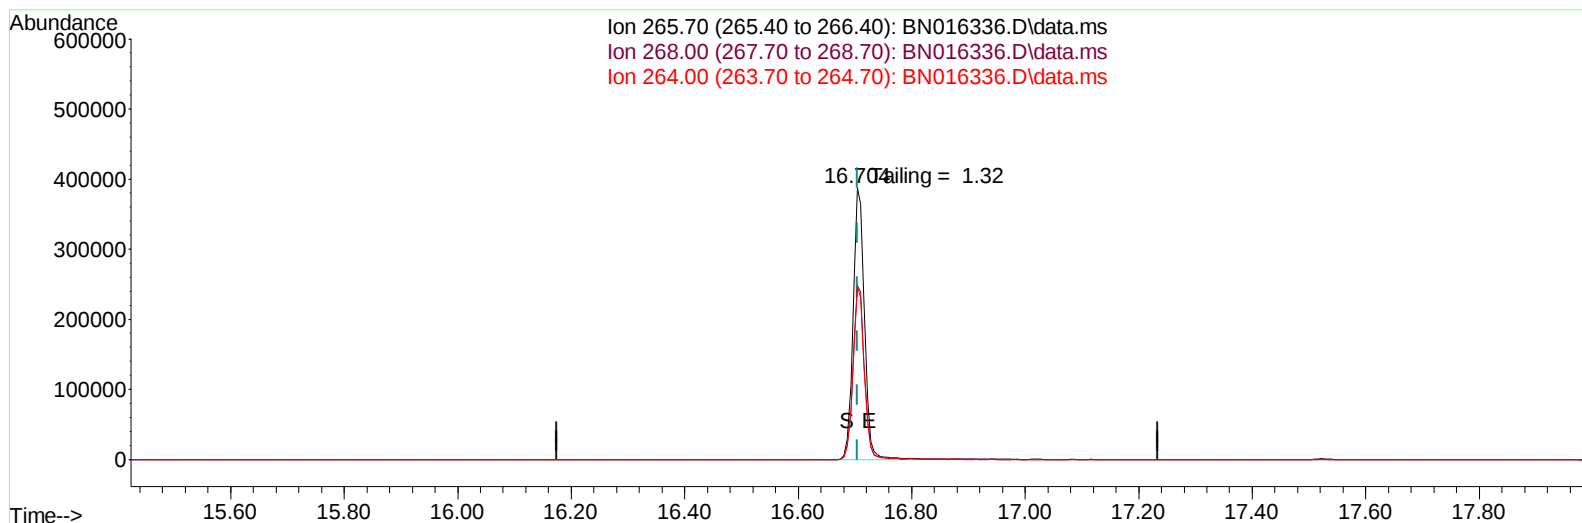

TIC: BN016336.D\data.ms

(70) Pentachloropheno1 (C)




16.704min (0.000) 22490.36 ng

response 545028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.95
264.00	61.60	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016336.D
Acq On : 20 Sep 2021 09:32
Operator : CG/JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 20 10:45:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 20 10:45:20 2021
Response via : Initial Calibration

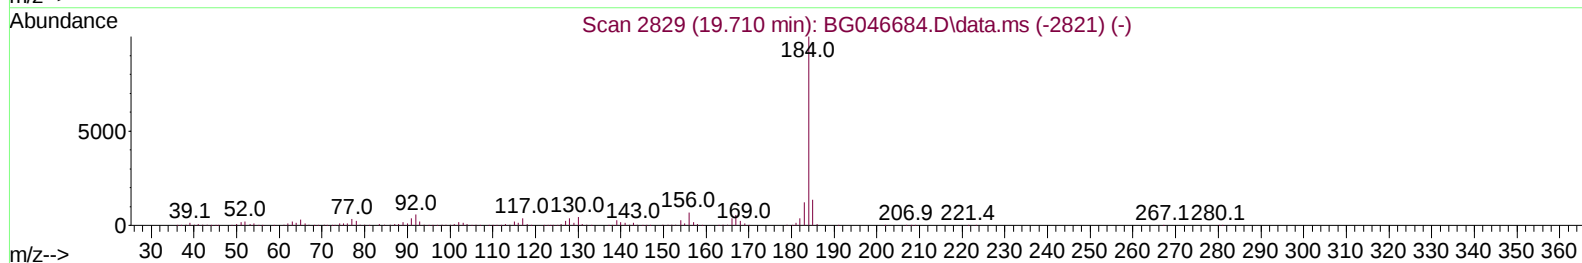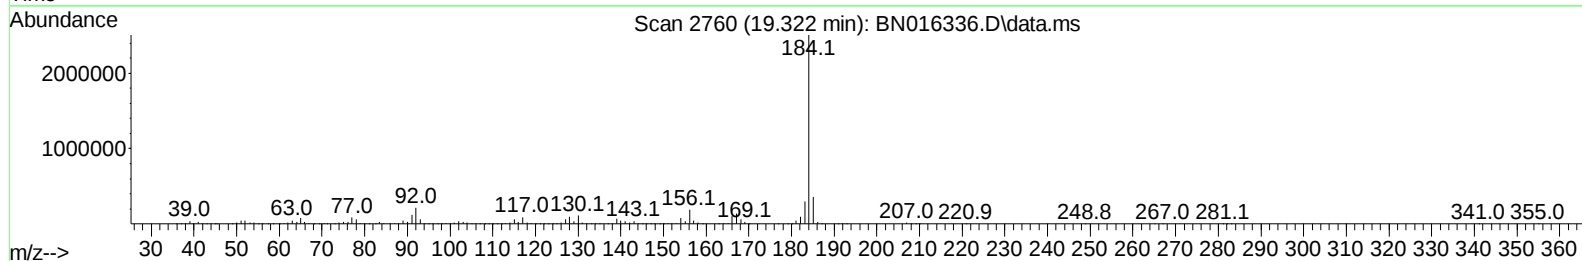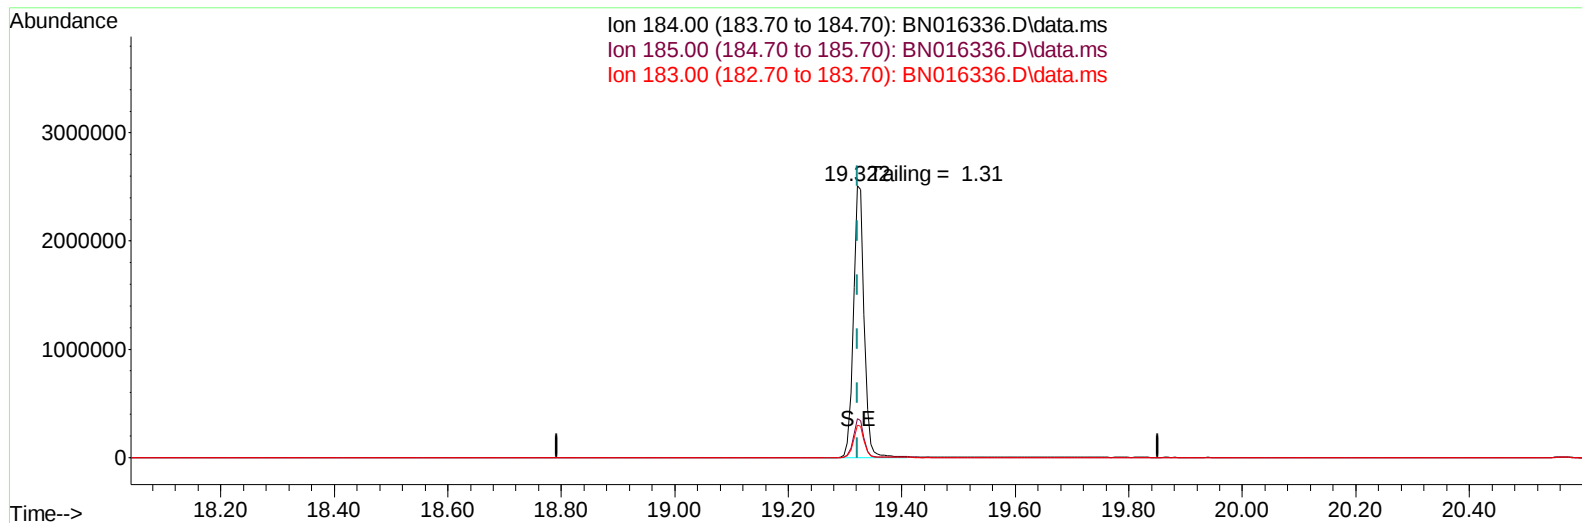

TIC: BN016336.D\data.ms

(77) Benzidine**19.322min (0.000) 0.00 ng****response 3349376**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	11.90
0.00	0.00	0.00