


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
 Data File : BN016336.D
 Acq On : 20 Sep 2021 09:32
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN091721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 20 11:09:23 2021

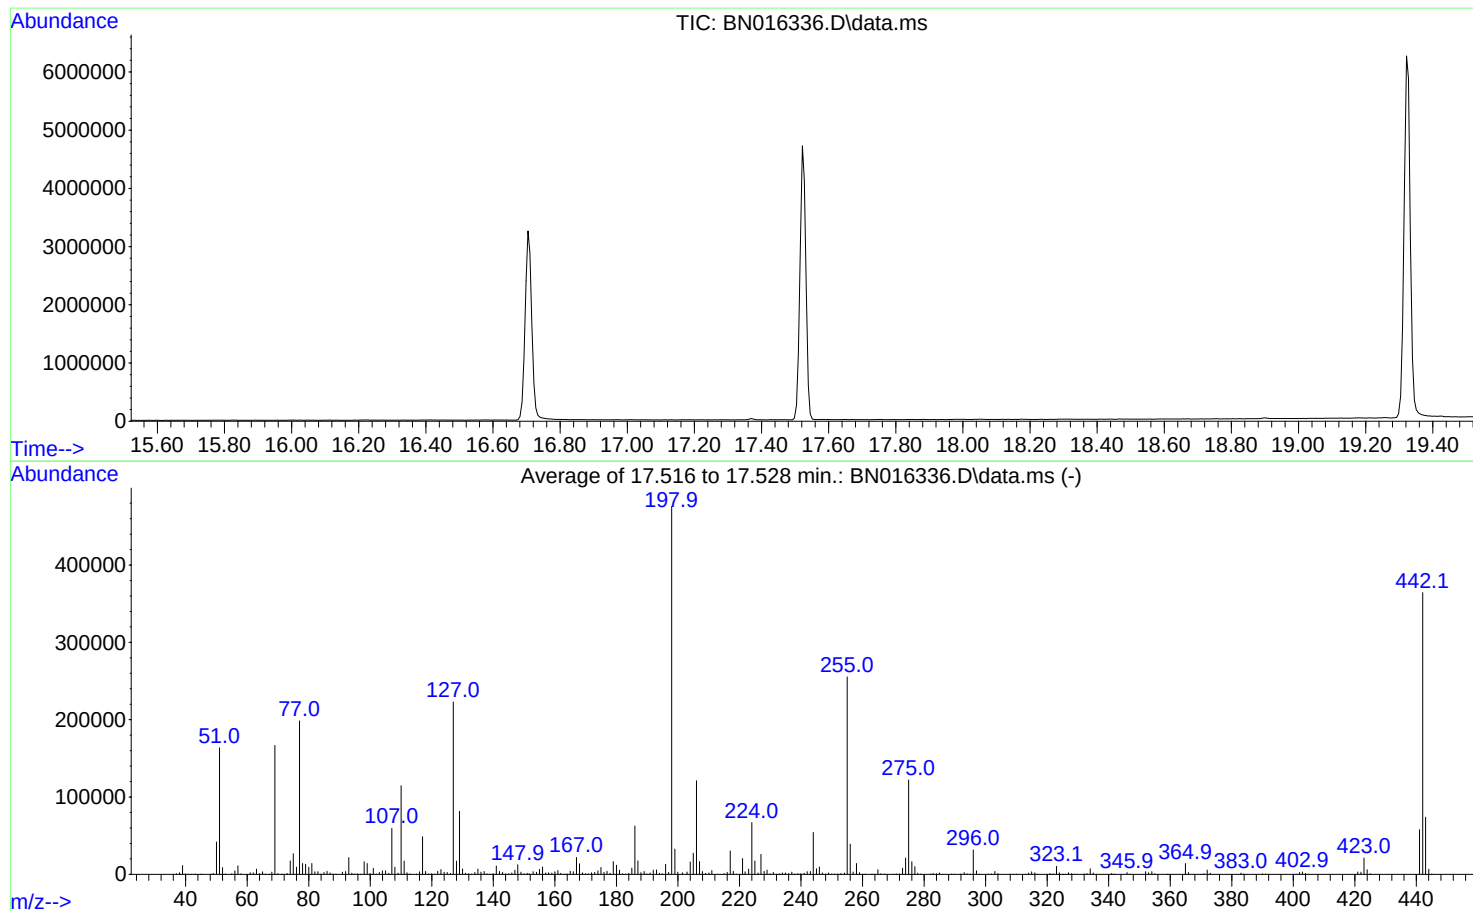




AutoFind: Scans 2453, 2454, 2455; Background Corrected with Scan 2447

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.4	163698	PASS
68	69	0.00	2	1.8	2975	PASS
69	198	0.00	100	35.1	166790	PASS
70	69	0.00	2	0.6	994	PASS
127	198	10	80	46.9	223019	PASS
197	198	0.00	2	0.5	2540	PASS
198	198	100	100	100.0	475712	PASS
199	198	5	9	6.9	32637	PASS
275	198	10	60	25.7	122101	PASS
365	198	1	100	2.9	13986	PASS
441	198	0.01	100	12.1	57781	PASS
442	442	50	100	100.0	364373	PASS
443	442	15	24	20.3	73819	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016336.D
Acq On : 20 Sep 2021 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 10:45:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 20 10:45:20 2021
Response via : Initial Calibration

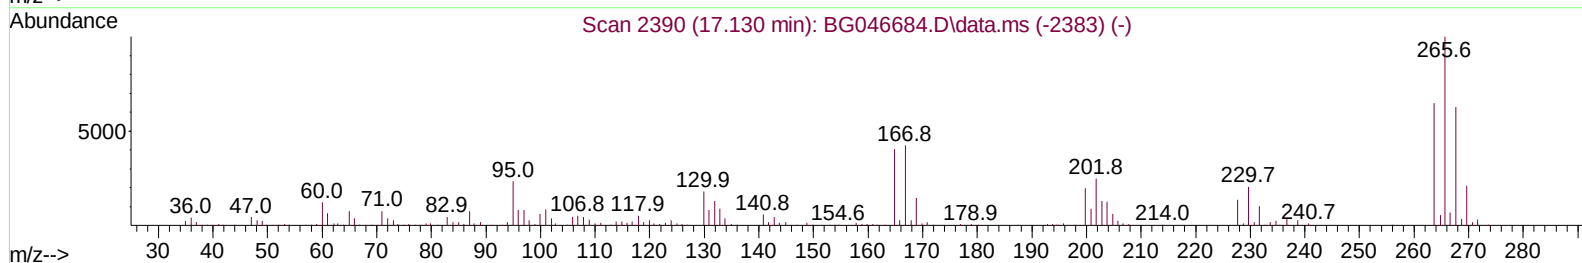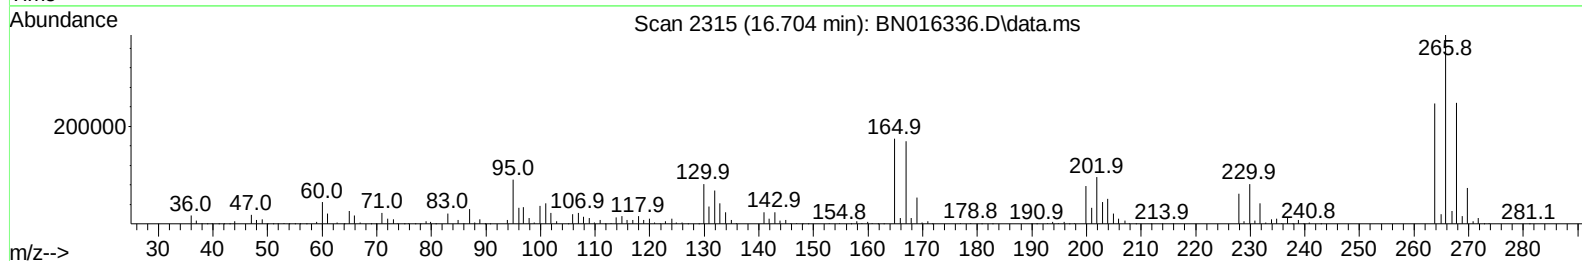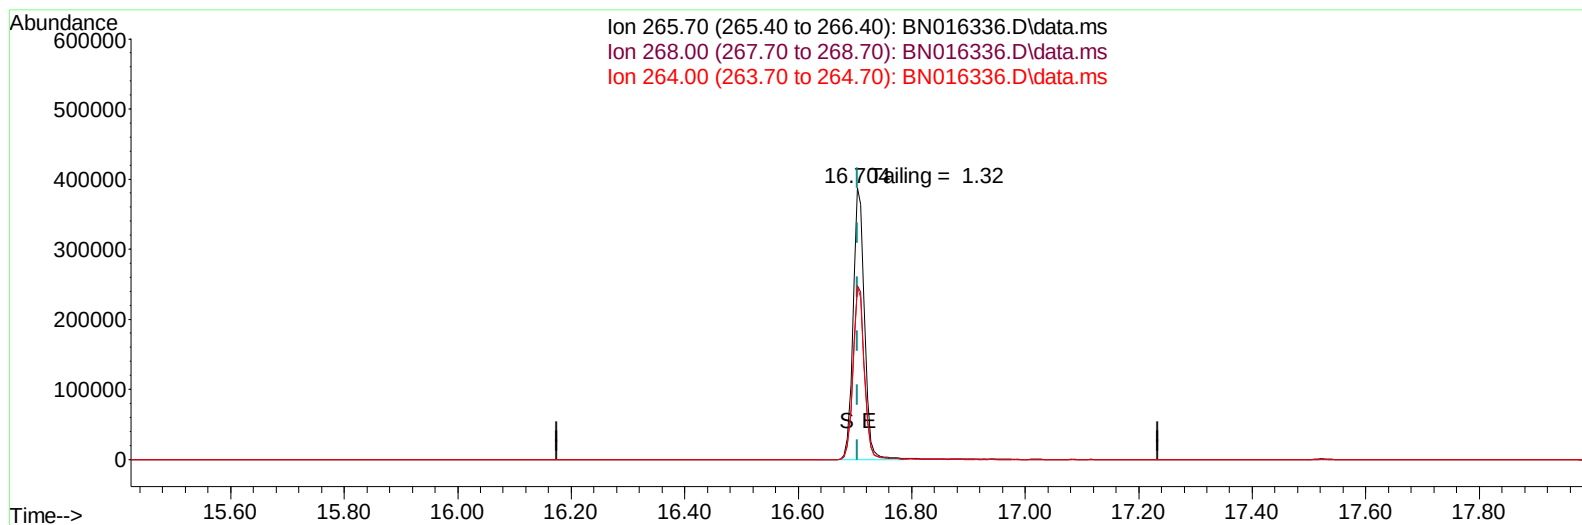

TIC: BN016336.D\data.ms

(70) Pentachlorophenol (C)

16.704min (0.000) 22490.36 ng




response 545028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.95
264.00	61.60	63.79
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN092021\
Data File : BN016336.D
Acq On : 20 Sep 2021 09:32
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Sep 20 10:45:26 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Sep 20 10:45:20 2021
Response via : Initial Calibration

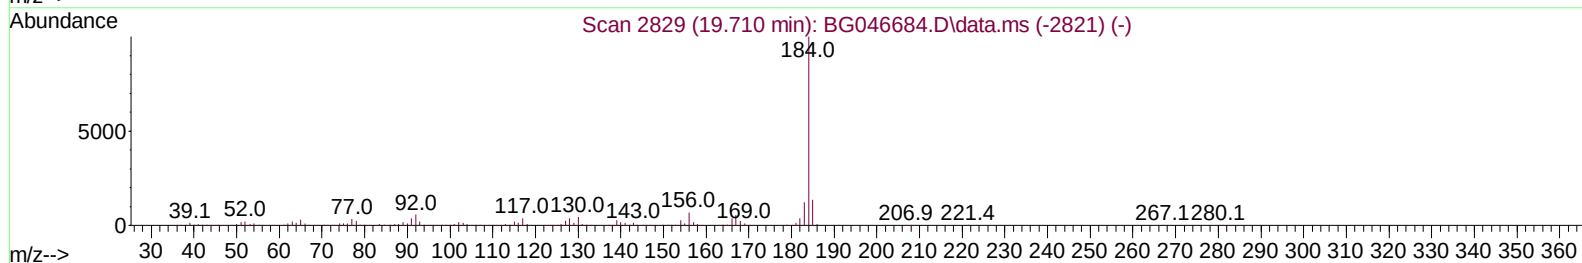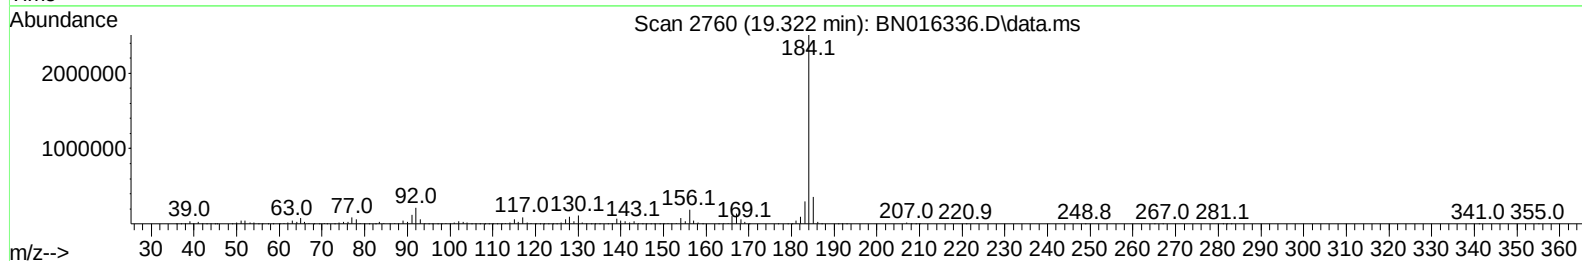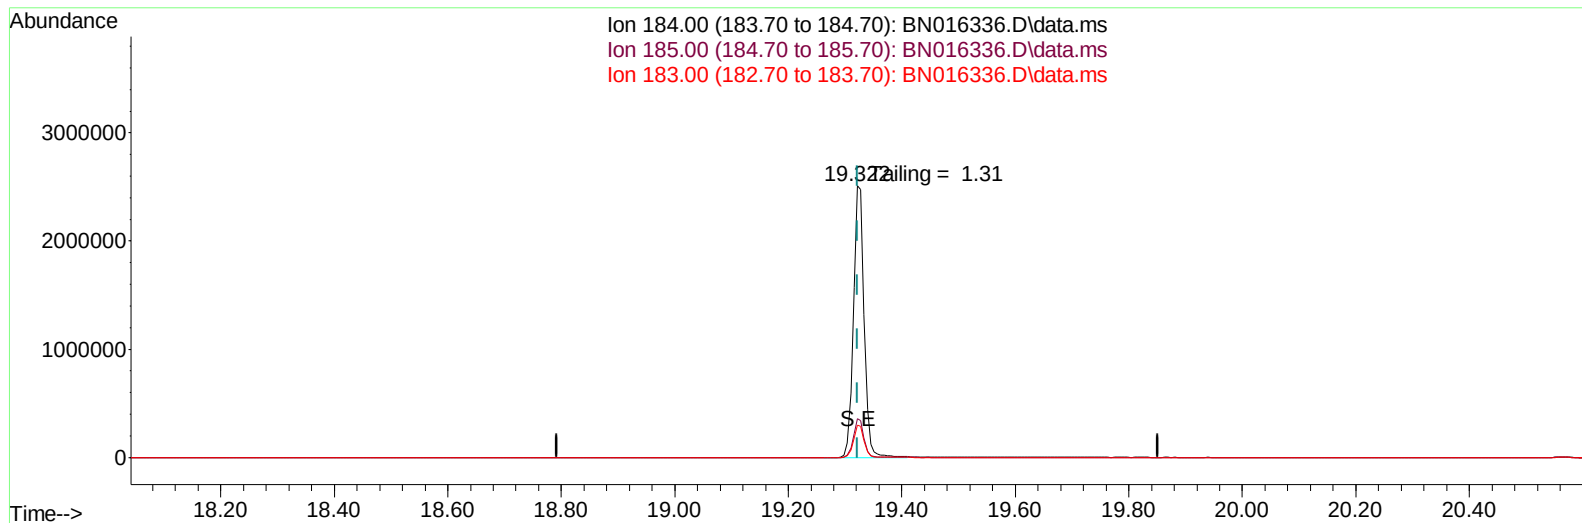

TIC: BN016336.D\data.ms

(77) Benzidine

19.322min (0.000) 0.00 ng

response 3349376

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.36
183.00	13.20	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/20/2021	BNA_N	<u>BN016336.D</u>
Compound Name	Response	Retention Time
DDT	1515070	20.569
DDD	33731	20.122
DDE	3334	19.616
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
37065	1552135	2.39

Instrument :
BNA_N
ClientSampleId :
DFTPP